

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061223\
 Data File : BP015470.D
 Acq On : 12 Jun 2023 12:34
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020745

Quant Time: Jun 12 13:08:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	153672	20.000	ng/u1	0.00
20) Naphthalene-d8	10.928	136	711048	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.740	164	490802	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.498	188	1149474	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	1126886	20.000	ng/u1	0.00
88) Perylene-d12	24.133	264	1197696	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	33181	7.996	ng/uL	0.00
4) Pyridine-d5	3.846	84	227289	21.085	ng/u1	0.00
7) Phenol-d5	7.246	99	283249	20.007	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	179129	21.186	ng/u1	0.00
11) 2-Chlorophenol-d4	7.622	132	211552	20.610	ng/u1	0.00
15) 4-Methylphenol-d8	8.811	113	235758	20.291	ng/u1	0.00
21) Nitrobenzene-d5	9.275	128	111838	20.034	ng/u1	0.00
24) 2-Nitrophenol-d4	10.005	143	126086	19.778	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	242356	20.840	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	346183	20.739	ng/u1	0.00
46) Dimethylphthalate-d6	14.146	166	787587	20.350	ng/u1	0.00
49) Acenaphthylene-d8	14.440	160	871244	20.587	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	112338	16.209	ng/u1	0.00
60) Fluorene-d10	15.734	176	670200	20.535	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	126485	17.370	ng/u1	0.00
73) Anthracene-d10	17.598	188	1076092	20.576	ng/u1	0.00
81) Pyrene-d10	19.822	212	1291887	21.420	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.969	264	1214949	20.217	ng/u1	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.446	88	35653	8.133	ng/uL	91
5) Pyridine	3.870	79	233434	20.888	ng/u1	96
6) Benzaldehyde	7.228	77	95918	17.725	ng/u1	96
8) Phenol	7.275	94	300157	20.551	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.511	93	235341	20.380	ng/u1	97
12) 2-Chlorophenol	7.652	128	223487	20.608	ng/u1	98
13) 2-Methylphenol	8.546	108	227872	20.277	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.622	45	327180	21.380	ng/u1	100
16) Acetophenone	8.934	105	393912	21.243	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.911	70	211107	21.094	ng/u1	99
18) 4-Methylphenol	8.875	108	256558	20.750	ng/u1	99
19) Hexachloroethane	9.187	117	93752	20.457	ng/u1	98
22) Nitrobenzene	9.316	77	312542	21.111	ng/u1	99
23) Isophorone	9.846	82	594452	20.059	ng/u1	99
25) 2-Nitrophenol	10.034	139	140977	20.482	ng/u1	98
26) 2,4-Dimethylphenol	10.087	107	299010	20.485	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.328	93	354458	20.573	ng/u1	99
29) 2,4-Dichlorophenol	10.569	162	244525	21.148	ng/u1	96
30) Naphthalene	10.975	128	784961	20.372	ng/u1	99
32) 4-Chloroaniline	11.093	127	360163	20.853	ng/u1	100
33) Hexachlorobutadiene	11.252	225	160341	20.562	ng/u1	99
34) Caprolactam	11.869	113	80801	18.564	ng/u1	88
35) 4-Chloro-3-methylphenol	12.204	107	296359	21.154	ng/u1	98
36) 2-Methylnaphthalene	12.575	142	553043	20.417	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061223\
 Data File : BP015470.D
 Acq On : 12 Jun 2023 12:34
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020745

Quant Time: Jun 12 13:08:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.793	142	557919	20.457	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.940	216	314418	20.573	ng/ul	99
40) Hexachlorocyclopentadiene	12.916	237	129066	20.602	ng/ul	97
41) 2,4,6-Trichlorophenol	13.181	196	213135	20.953	ng/ul	99
42) 2,4,5-Trichlorophenol	13.257	196	230815	20.823	ng/ul	100
43) 1,1'-Biphenyl	13.575	154	777931	20.496	ng/ul	99
44) 2-Chloronaphthalene	13.622	162	611833	20.546	ng/ul	98
45) 2-Nitroaniline	13.834	65	199370	20.919	ng/ul	97
47) Dimethylphthalate	14.193	163	809765	20.264	ng/ul	99
48) 2,6-Dinitrotoluene	14.322	165	165139	20.171	ng/ul	98
50) Acenaphthylene	14.469	152	956729	20.414	ng/ul	98
51) 3-Nitroaniline	14.657	138	113805	16.839	ng/ul	97
52) Acenaphthene	14.804	153	665896	20.555	ng/ul	100
53) 2,4-Dinitrophenol	14.869	184	64253	13.047	ng/ul	99
55) 4-Nitrophenol	14.957	109	114845	17.179	ng/ul	98
56) Dibenzofuran	15.140	168	951538	20.724	ng/ul	99
57) 2,4-Dinitrotoluene	15.110	165	246389	20.462	ng/ul	96
58) 2,3,4,6-Tetrachlorophenol	15.369	232	208306	20.813	ng/ul	97
59) Diethylphthalate	15.551	149	837742	20.455	ng/ul	98
61) Fluorene	15.793	166	773677	20.670	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.781	204	392184	20.790	ng/ul	99
63) 4-Nitroaniline	15.816	138	105066	16.389	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.875	198	132607	17.855	ng/ul	96
67) N-Nitrosodiphenylamine	15.993	169	671246	20.584	ng/ul	99
68) 4-Bromophenyl-phenylether	16.681	248	252605	20.541	ng/ul	100
69) Hexachlorobenzene	16.798	284	297228	20.490	ng/ul	96
70) Atrazine	16.951	200	263685	20.249	ng/ul	100
71) Pentachlorophenol	17.145	266	163688	19.964	ng/ul	98
72) Phenanthrene	17.539	178	1269894	20.587	ng/ul	100
74) Anthracene	17.634	178	1291338	20.632	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.546	216	326125	20.557	ng/uL	98
76) Pentachlorobenzene	15.057	250	341016	20.531	ng/uL	99
77) Carbazole	17.904	167	1167248	20.712	ng/ul	100
78) Di-n-butylphthalate	18.428	149	1494884	20.907	ng/ul	99
80) Fluoranthene	19.492	202	1574534	21.432	ng/ul	99
82) Pyrene	19.851	202	1631627	21.467	ng/ul	99
83) Butylbenzylphthalate	20.704	149	725475	21.595	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.492	252	488172	18.337	ng/ul	99
85) Benzo(a)anthracene	21.563	228	1633153	20.731	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.457	149	1100525	22.163	ng/ul	98
87) Chrysene	21.622	228	1547204	20.778	ng/ul	99
89) Di-n-octyl phthalate	22.433	149	1911159	24.279	ng/ul	100
90) Benzo(b)fluoranthene	23.345	252	1590897	20.578	ng/ul	99
91) Benzo(k)fluoranthene	23.398	252	1591495	21.296	ng/ul	99
93) Benzo(a)pyrene	24.022	252	1364687	20.246	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.839	276	1572690	18.029	ng/ul	99
95) Dibenzo(a,h)anthracene	26.857	278	1290307	18.156	ng/ul	100
96) Benzo(g,h,i)perylene	27.674	276	1299352	18.075	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061223\
 Data File : BP015470.D
 Acq On : 12 Jun 2023 12:34
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020745

Quant Time: Jun 12 13:08:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration




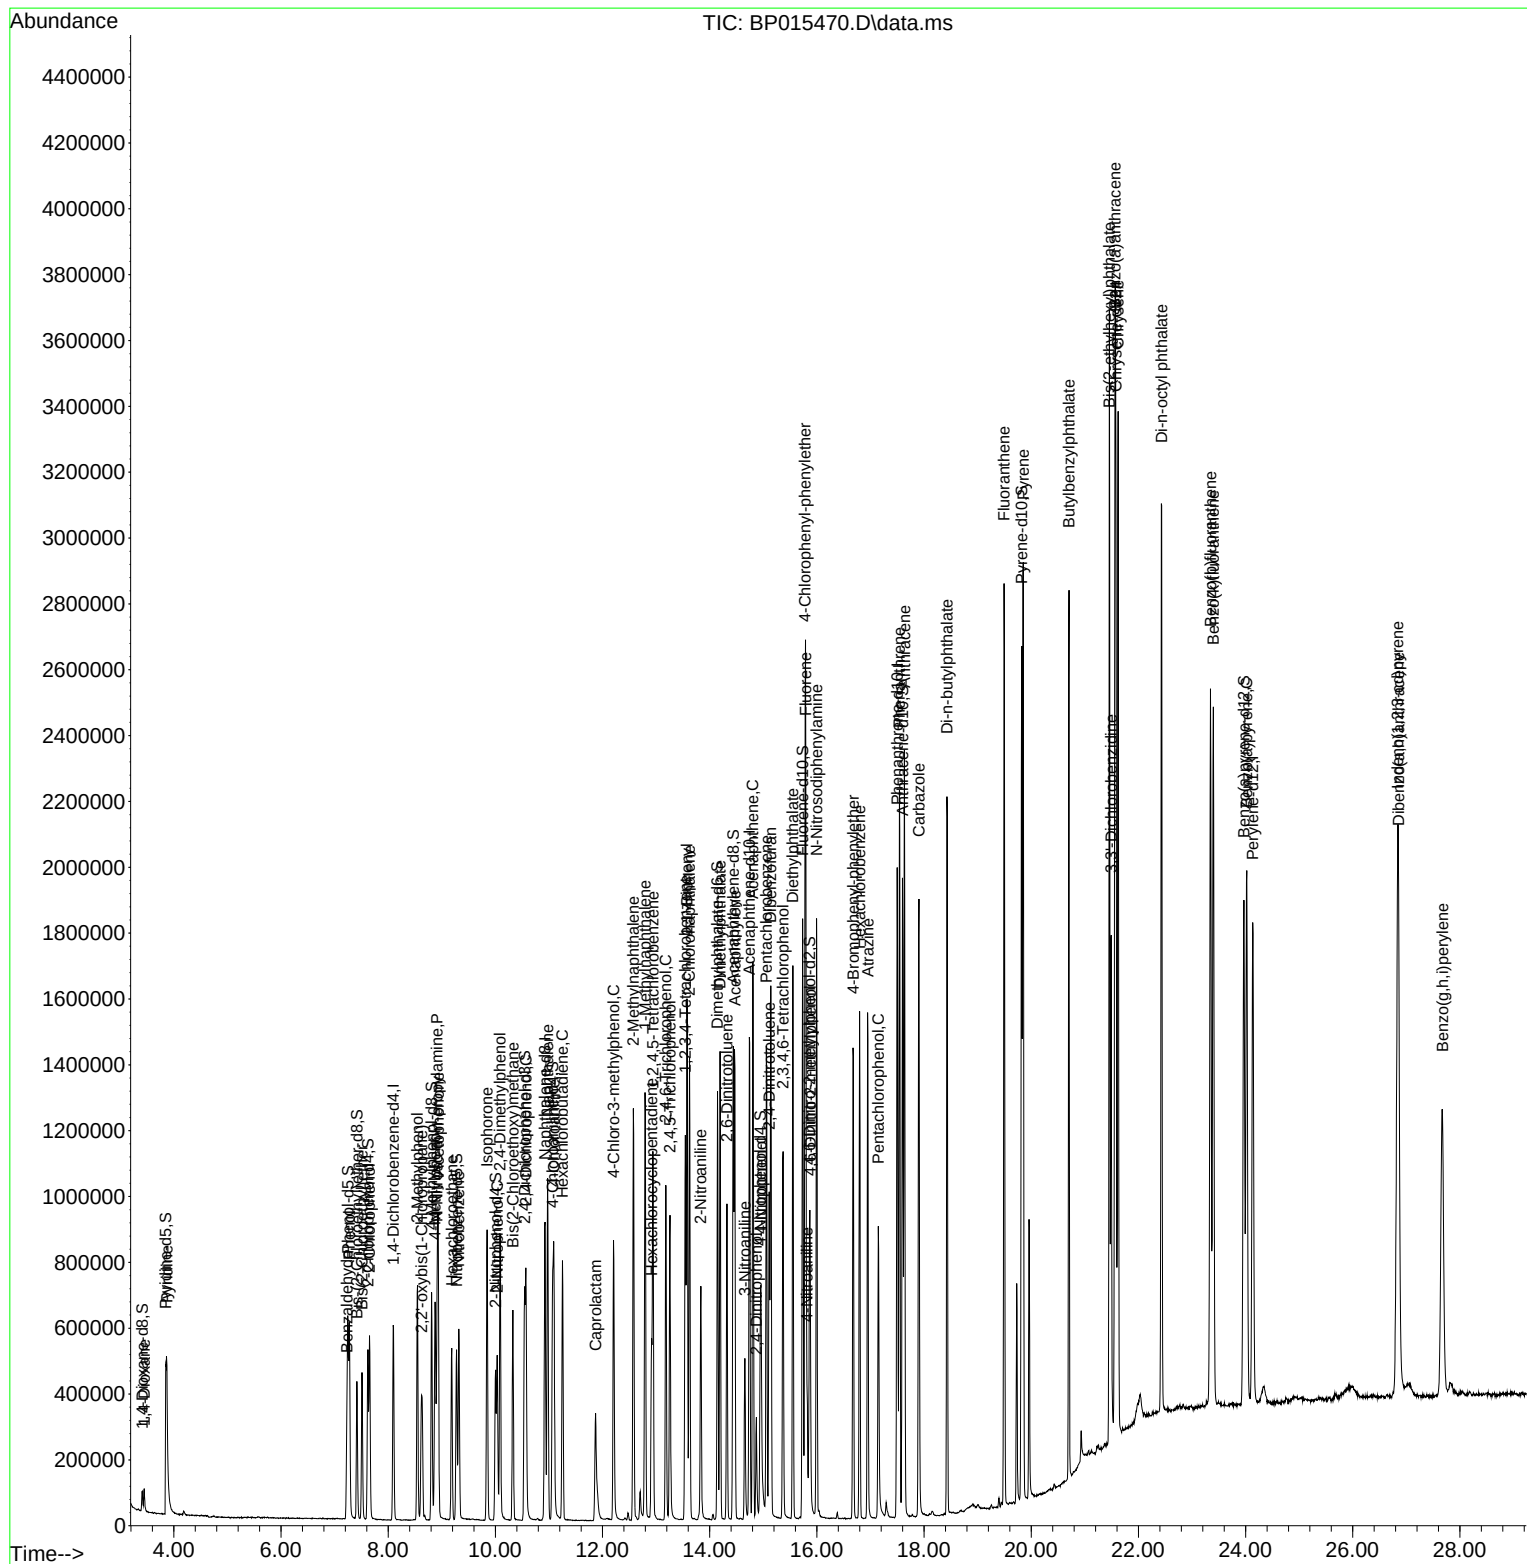


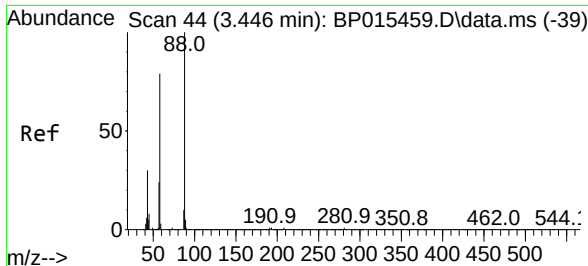

#2
1,4-Dioxane
Concen: 8.133 ng/uL
RT: 3.446 min Scan# 44
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion: 88	Resp: 35653
Ion Ratio	Lower Upper
88 100	
43 33.6	23.9 35.9
58 71.7	51.4 77.2

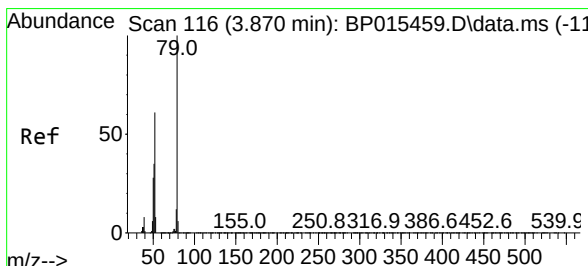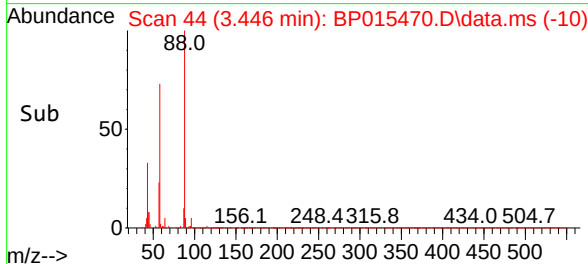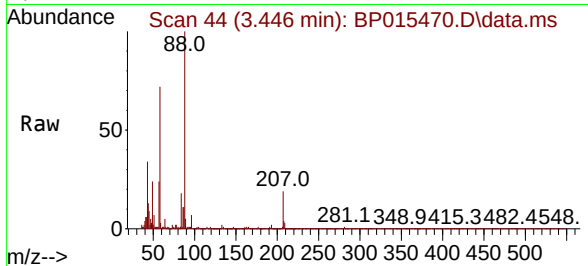

#5
Pyridine
Concen: 20.888 ng/uL
RT: 3.870 min Scan# 116
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion: 79	Resp: 233434
Ion Ratio	Lower Upper
79 100	
52 78.2	59.5 89.3
51 38.5	29.8 44.6


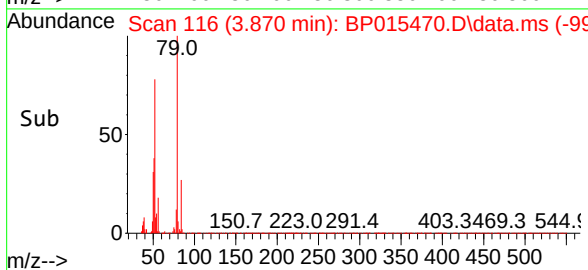

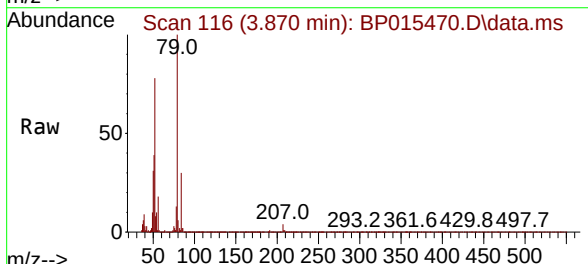




#6
Benzaldehyde
Concen: 17.725 ng/ul
RT: 7.228 min Scan# 687
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:	77	Resp:	95918
Ion	Ratio	Lower	Upper
77	100		
105	91.6	77.3	115.9
106	89.2	73.3	109.9



#8
Phenol
Concen: 20.551 ng/ul
RT: 7.275 min Scan# 695
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:	94	Resp:	300157
Ion	Ratio	Lower	Upper
94	100		
65	32.3	23.5	35.3
66	44.0	34.2	51.4



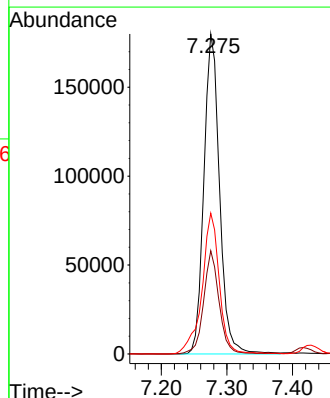
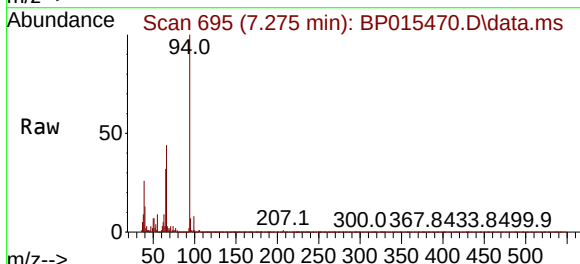




#10
Bis(2-Chloroethyl)ether
Concen: 20.380 ng/ul
RT: 7.511 min Scan# 735
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion: 93 Resp: 235341
Ion Ratio Lower Upper
93 100
63 81.0 62.6 93.8
95 31.3 25.5 38.3



#12
2-Chlorophenol
Concen: 20.608 ng/ul
RT: 7.652 min Scan# 759
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:128 Resp: 223487
Ion Ratio Lower Upper
128 100
64 51.4 40.2 60.4
130 31.9 24.5 36.7





#13

2-Methylphenol

Concen: 20.277 ng/ul

RT: 8.546 min Scan# 910

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :





SSTD020745

Tgt Ion:108 Resp: 227872

Ion Ratio Lower Upper

108 100

107 87.8 71.2 106.8



#14

2,2'-oxybis(1-Chloropropane)

Concen: 21.380 ng/ul

RT: 8.622 min Scan# 924

Delta R.T. 0.000 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion: 45 Resp: 327180


Ion Ratio Lower Upper

45 100

77 14.6 11.8 17.8

79 11.0 8.7 13.1


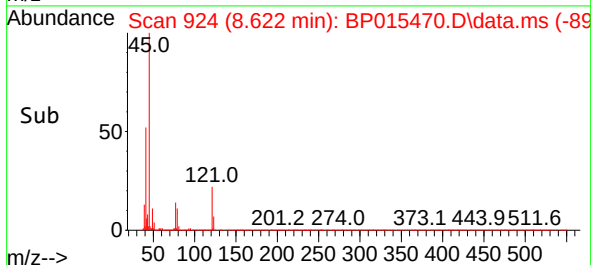
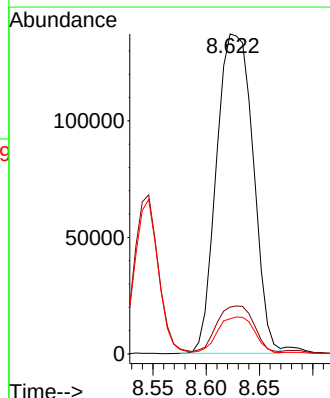
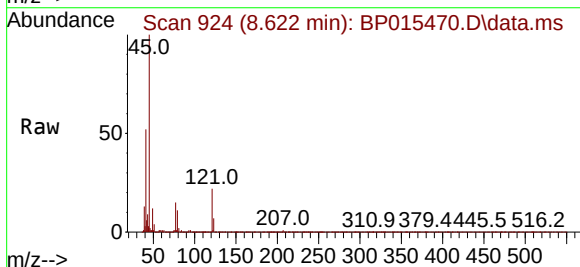




#16
Acetophenone
Concen: 21.243 ng/ul
RT: 8.934 min Scan# 91
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:105 Resp: 393912
Ion Ratio Lower Upper
105 100
77 81.0 64.9 97.3
51 30.1 23.5 35.3



#17
N-Nitroso-di-n-propylamine
Concen: 21.094 ng/ul
RT: 8.911 min Scan# 973
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion: 70 Resp: 211107
Ion Ratio Lower Upper
70 100
42 58.9 46.6 69.8
101 9.8 7.8 11.6
130 19.1 15.9 23.9



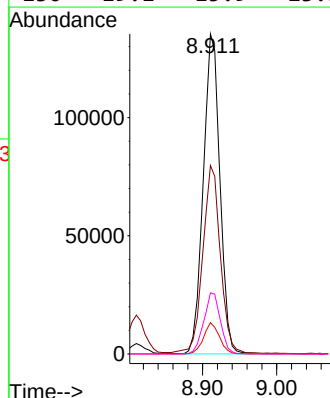





#18
4-Methylphenol
Concen: 20.750 ng/ul
RT: 8.875 min Scan# 967
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:108 Resp: 256558
Ion Ratio Lower Upper
108 100
107 112.3 89.3 133.9



#19
Hexachloroethane
Concen: 20.457 ng/ul
RT: 9.187 min Scan# 1020
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:117 Resp: 93752
Ion Ratio Lower Upper
117 100
201 101.6 82.8 124.2
199 62.3 50.6 76.0







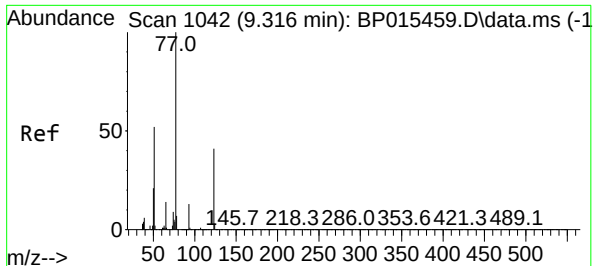

#22
Nitrobenzene
Concen: 21.111 ng/ul
RT: 9.316 min Scan# 1042
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion: 77 Resp: 312542
Ion Ratio Lower Upper
77 100
123 41.0 33.5 50.3
65 13.8 11.6 17.4

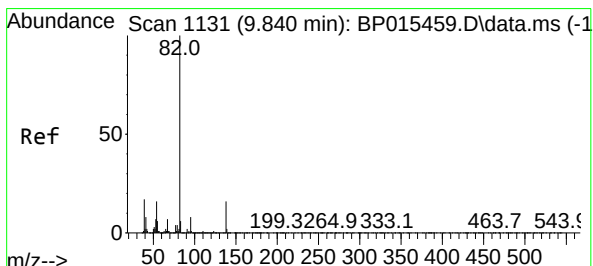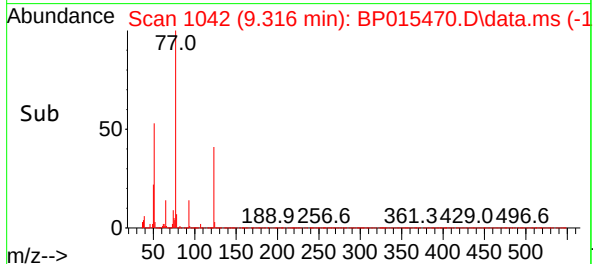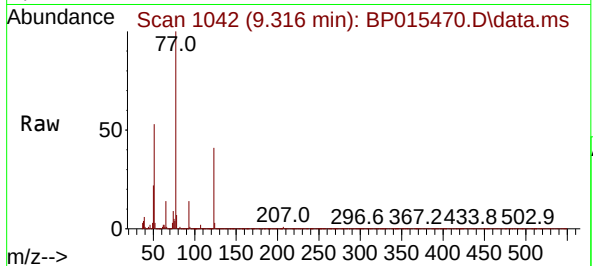

#23
Isophorone
Concen: 20.059 ng/ul
RT: 9.846 min Scan# 1132
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion: 82 Resp: 594452
Ion Ratio Lower Upper
82 100
95 7.9 5.8 8.8
138 16.0 13.1 19.7


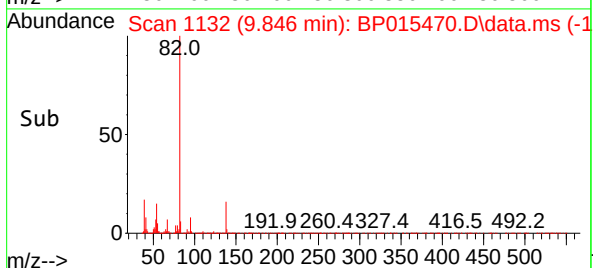
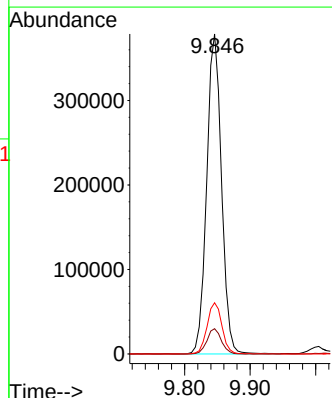
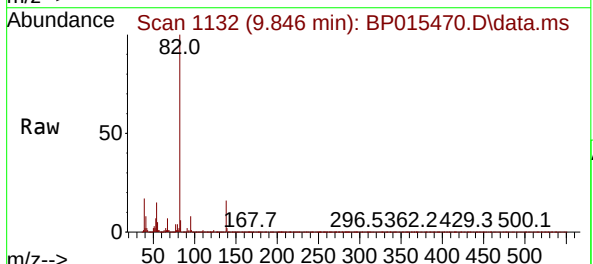




#25
2-Nitrophenol
Concen: 20.482 ng/ul
RT: 10.034 min Scan# 1164
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:139 Resp: 140977
Ion Ratio Lower Upper
139 100
65 58.8 46.9 70.3
109 35.3 30.2 45.2

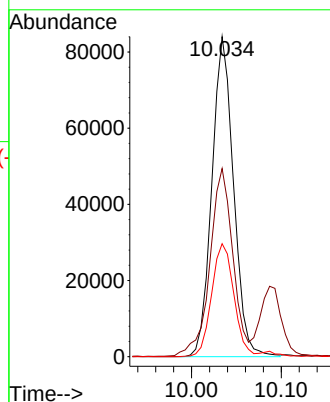

#26
2,4-Dimethylphenol
Concen: 20.485 ng/ul
RT: 10.087 min Scan# 1173
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:107 Resp: 299010
Ion Ratio Lower Upper
107 100
121 47.2 39.0 58.6
122 79.6 64.8 97.2


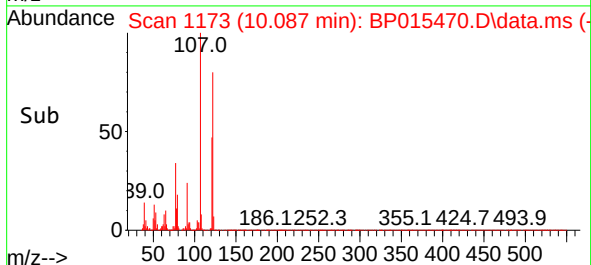

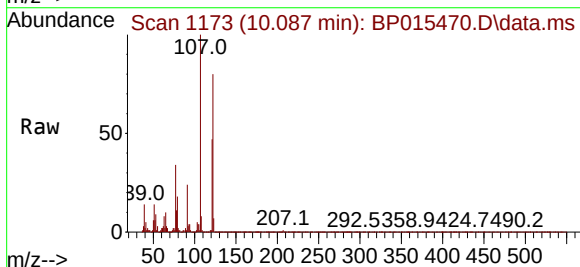




#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.573 ng/ul
 RT: 10.328 min Scan# 1214
 Delta R.T. 0.006 min
 Lab File: BP015470.D
 Acq: 12 Jun 2023 12:34




Instrument :
 BNA_P
 ClientSampleId :
 SST020745


Tgt Ion: 93 Resp: 354458
 Ion Ratio Lower Upper
 93 100
 95 32.8 25.7 38.5
 123 9.9 8.6 13.0



#29
 2,4-Dichlorophenol
 Concen: 21.148 ng/ul
 RT: 10.569 min Scan# 1255
 Delta R.T. 0.000 min
 Lab File: BP015470.D
 Acq: 12 Jun 2023 12:34

Tgt Ion: 162 Resp: 244525
 Ion Ratio Lower Upper
 162 100
 164 67.7 50.6 76.0
 98 38.6 30.2 45.2


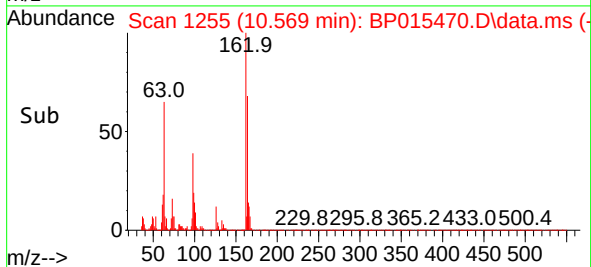

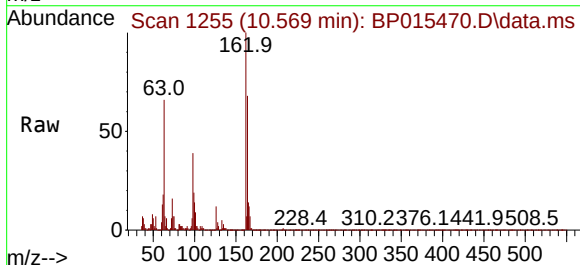




#30
Naphthalene
Concen: 20.372 ng/ul
RT: 10.975 min Scan# 1324
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:128 Resp: 784961
Ion Ratio Lower Upper
128 100
129 10.7 8.6 13.0
127 13.5 10.5 15.7

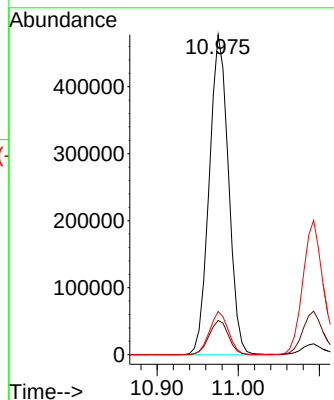

#32
4-Chloroaniline
Concen: 20.853 ng/ul
RT: 11.093 min Scan# 1344
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:127 Resp: 360163
Ion Ratio Lower Upper
127 100
129 32.3 26.1 39.1

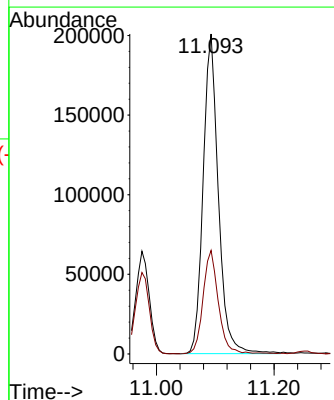



#33

Hexachlorobutadiene

Concen: 20.562 ng/ul

RT: 11.252 min Scan# 1371

Delta R.T. 0.000 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:225 Resp: 160341

Ion Ratio Lower Upper

225 100

223 63.0 52.0 78.0

227 63.3 50.6 75.8

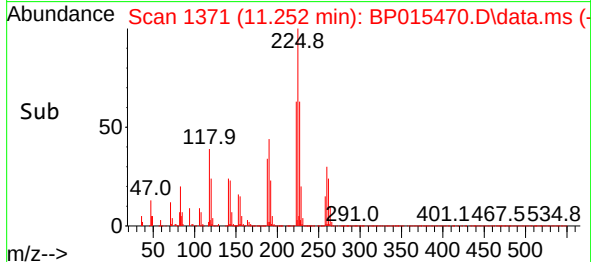

#34

Caprolactam

Concen: 18.564 ng/ul

RT: 11.869 min Scan# 1476

Delta R.T. 0.000 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:113 Resp: 80801


Ion Ratio Lower Upper

113 100

55 177.1 127.9 191.9

56 138.2 101.1 151.7


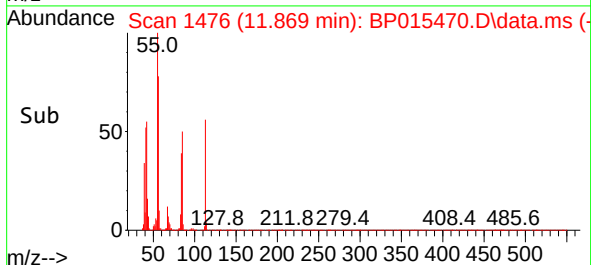
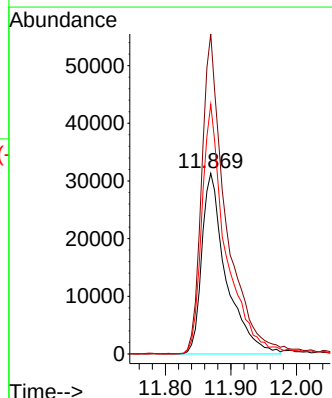
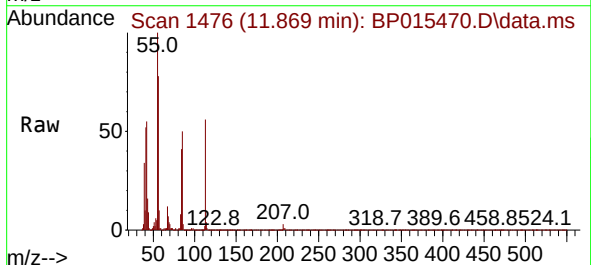




#35
4-Chloro-3-methylphenol
Concen: 21.154 ng/ul
RT: 12.204 min Scan# 1533
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:107 Resp: 296359
Ion Ratio Lower Upper
107 100
144 24.5 19.4 29.0
142 73.0 60.4 90.6

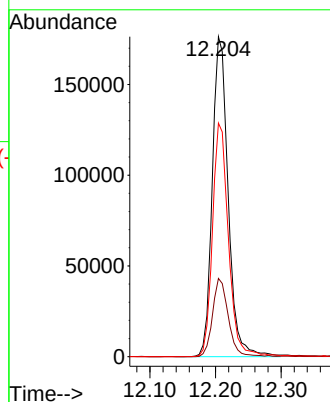

#36
2-Methylnaphthalene
Concen: 20.417 ng/ul
RT: 12.575 min Scan# 1596
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:142 Resp: 553043
Ion Ratio Lower Upper
142 100
141 89.7 72.0 108.0





#37

1-Methylnaphthalene

Concen: 20.457 ng/ul

RT: 12.793 min Scan# 1633

Delta R.T. 0.000 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:142 Resp: 557919

Ion Ratio Lower Upper

142 100

141 92.3 71.9 107.9

116 4.4 3.4 5.2



#39

1,2,4,5-Tetrachlorobenzene

Concen: 20.573 ng/ul

RT: 12.940 min Scan# 1658

Delta R.T. 0.000 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Tgt Ion:216 Resp: 314418




Ion Ratio Lower Upper


216 100

214 78.9 62.2 93.2

179 22.1 17.4 26.2

108 18.9 14.2 21.4





#40

Hexachlorocyclopentadiene

Concen: 20.602 ng/ul

RT: 12.916 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:237 Resp: 129066

Ion Ratio Lower Upper

237 100

235 63.2 48.2 72.2

272 13.0 10.3 15.5



#41

2,4,6-Trichlorophenol

Concen: 20.953 ng/ul

RT: 13.181 min Scan# 1699

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:196 Resp: 213135


Ion Ratio Lower Upper

196 100

198 96.4 77.8 116.6

200 31.7 25.8 38.6









#42
2,4,5-Trichlorophenol
Concen: 20.823 ng/ul
RT: 13.257 min Scan# 1711
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:196 Resp: 230815
Ion Ratio Lower Upper
196 100
198 94.7 75.5 113.3
200 31.2 24.7 37.1

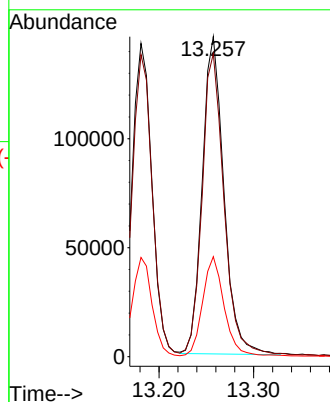

#43
1,1'-Biphenyl
Concen: 20.496 ng/ul
RT: 13.575 min Scan# 1766
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:154 Resp: 777931
Ion Ratio Lower Upper
154 100
153 40.0 32.2 48.2
76 13.4 10.4 15.6









#44
2-Chloronaphthalene
Concen: 20.546 ng/ul
RT: 13.622 min Scan# 11
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:162 Resp: 611833
Ion Ratio Lower Upper
162 100
164 32.7 27.0 40.6
127 41.1 32.2 48.4



#45
2-Nitroaniline
Concen: 20.919 ng/ul
RT: 13.834 min Scan# 1810
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion: 65 Resp: 199370
Ion Ratio Lower Upper
65 100
92 66.0 55.4 83.2
138 96.4 78.8 118.2




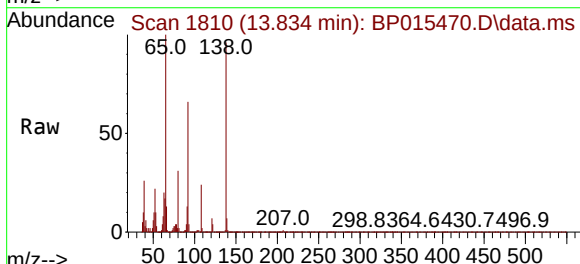




#47
Dimethylphthalate
Concen: 20.264 ng/ul
RT: 14.193 min Scan# 1871
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:163 Resp: 809765
Ion Ratio Lower Upper
163 100
194 3.9 3.2 4.8
164 9.9 8.2 12.2

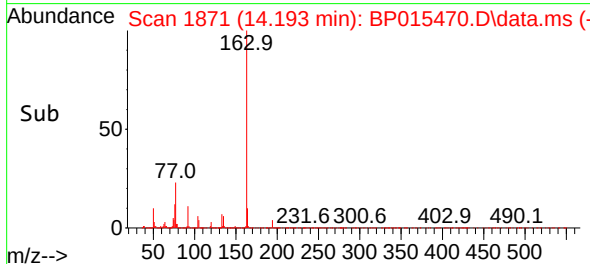

#48
2,6-Dinitrotoluene
Concen: 20.171 ng/ul
RT: 14.322 min Scan# 1893
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:165 Resp: 165139
Ion Ratio Lower Upper
165 100
89 65.9 51.5 77.3
121 21.4 17.3 25.9

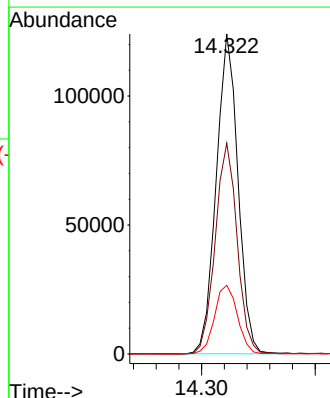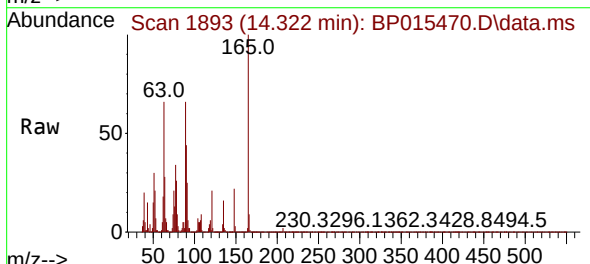



#50

Acenaphthylene

Concen: 20.414 ng/ul

RT: 14.469 min Scan# 1917

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:152 Resp: 956729

Ion Ratio Lower Upper

152 100

151 19.2 16.0 24.0

153 12.7 10.6 15.8



#51

3-Nitroaniline

Concen: 16.839 ng/ul

RT: 14.657 min Scan# 1950

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:138 Resp: 113805


Ion Ratio Lower Upper

138 100

108 11.8 8.4 12.6

92 125.7 98.0 147.0





#52

Acenaphthene

Concen: 20.555 ng/ul

RT: 14.804 min Scan# 1975

Delta R.T. 0.000 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:153 Resp: 665896

Ion Ratio Lower Upper

153 100

152 47.6 38.3 57.5

154 87.1 69.8 104.6

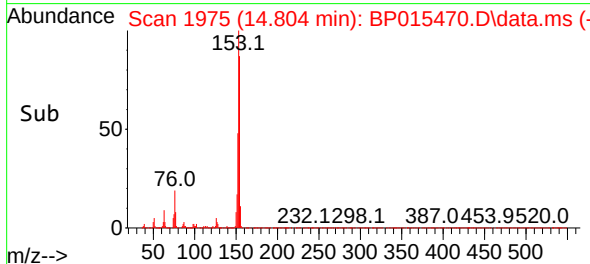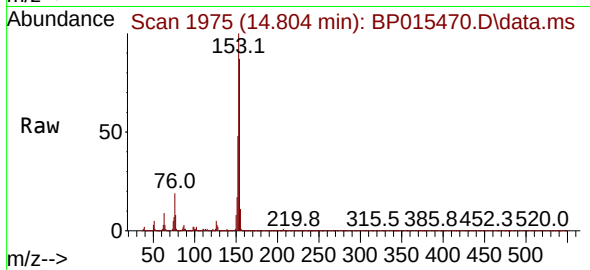

#53

2,4-Dinitrophenol

Concen: 13.047 ng/ul

RT: 14.869 min Scan# 1986

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:184 Resp: 64253


Ion Ratio Lower Upper

184 100

63 75.5 59.0 88.4

154 72.3 57.6 86.4


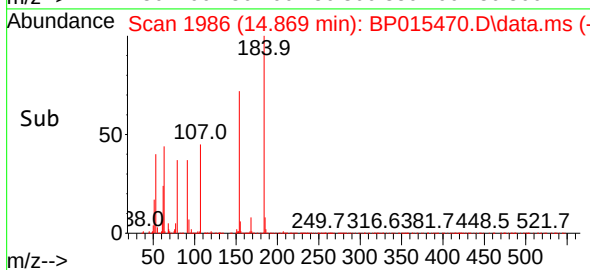

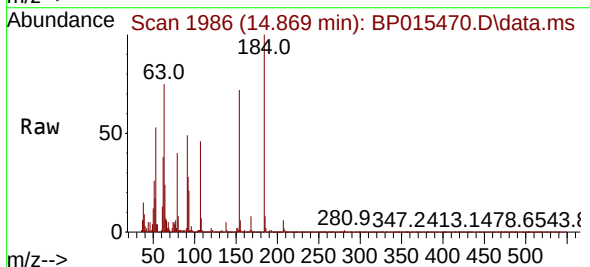




#55
4-Nitrophenol
Concen: 17.179 ng/ul
RT: 14.957 min Scan# 2000
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:109 Resp: 114845
Ion Ratio Lower Upper
109 100
139 113.0 89.1 133.7
65 126.6 103.1 154.7



#56
Dibenzofuran
Concen: 20.724 ng/ul
RT: 15.140 min Scan# 2032
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:168 Resp: 951538
Ion Ratio Lower Upper
168 100
139 39.7 31.2 46.8

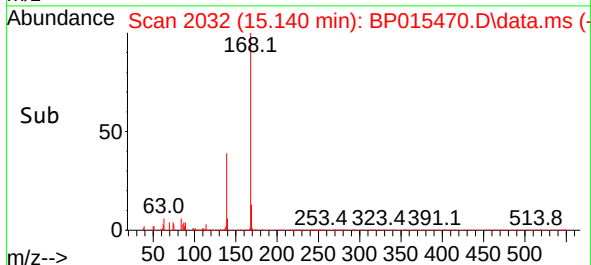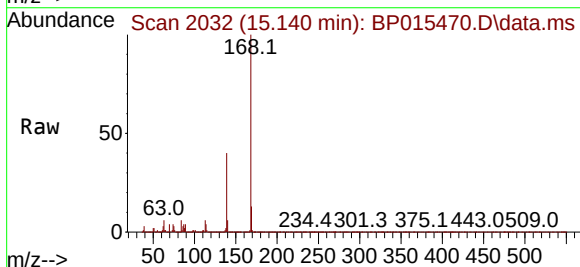



#57

2,4-Dinitrotoluene

Concen: 20.462 ng/ul

RT: 15.110 min Scan# 2026

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:165 Resp: 246389

Ion Ratio Lower Upper

165 100

63 51.5 39.1 58.7

182 2.9 2.2 3.4



#58

2,3,4,6-Tetrachlorophenol

Concen: 20.813 ng/ul

RT: 15.369 min Scan# 2071

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Tgt Ion:232 Resp: 208306




Ion Ratio Lower Upper


232 100

131 44.7 37.8 56.8

130 2.5 1.9 2.9

166 32.1 26.2 39.2









#59
Diethylphthalate
Concen: 20.455 ng/ul
RT: 15.551 min Scan# 2102
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:149 Resp: 837742
Ion Ratio Lower Upper
149 100
177 21.0 17.8 26.8
150 12.4 10.1 15.1



#61
Fluorene
Concen: 20.670 ng/ul
RT: 15.793 min Scan# 2143
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:166 Resp: 773677
Ion Ratio Lower Upper
166 100
165 97.7 79.1 118.7
167 13.3 10.6 16.0




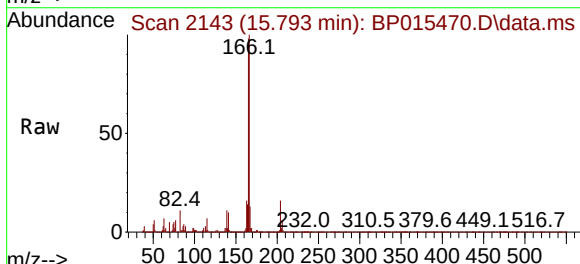




#62
4-Chlorophenyl-phenylether
Concen: 20.790 ng/ul
RT: 15.781 min Scan# 2140
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:204 Resp: 392184
Ion Ratio Lower Upper
204 100
206 32.7 26.6 40.0
141 63.1 49.8 74.8



#63
4-Nitroaniline
Concen: 16.389 ng/ul
RT: 15.816 min Scan# 2147
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:138 Resp: 105066
Ion Ratio Lower Upper
138 100
92 56.0 44.6 67.0
108 97.0 78.4 117.6









#66
4,6-Dinitro-2-methylphenol
Concen: 17.855 ng/ul
RT: 15.875 min Scan# 2156
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:198 Resp: 132607
Ion Ratio Lower Upper
198 100
182 4.4 3.0 4.4
77 27.9 20.5 30.7



#67
N-Nitrosodiphenylamine
Concen: 20.584 ng/ul
RT: 15.993 min Scan# 2177
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:169 Resp: 671246
Ion Ratio Lower Upper
169 100
168 65.4 53.0 79.4
167 35.4 28.9 43.3


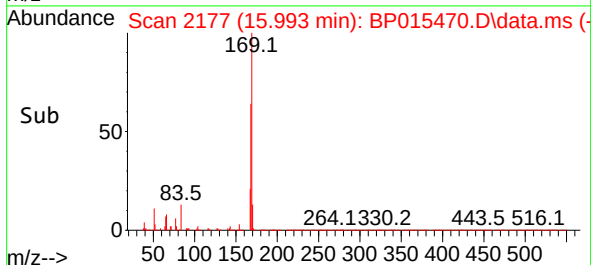

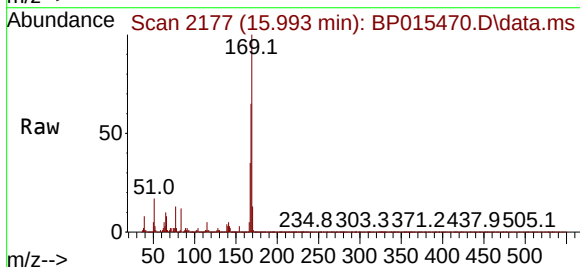




#68
4-Bromophenyl-phenylether
Concen: 20.541 ng/ul
RT: 16.681 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:248 Resp: 252605
Ion Ratio Lower Upper
248 100
250 98.3 78.3 117.5
141 76.8 61.1 91.7



#69
Hexachlorobenzene
Concen: 20.490 ng/ul
RT: 16.798 min Scan# 2314
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:284 Resp: 297228
Ion Ratio Lower Upper
284 100
142 35.3 25.4 38.2
249 32.3 24.8 37.2

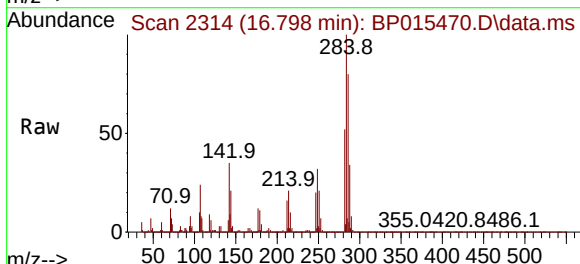



#70

Atrazine

Concen: 20.249 ng/ul

RT: 16.951 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:200 Resp: 263685

Ion Ratio Lower Upper

200 100

173 24.5 19.8 29.6

215 46.8 37.4 56.0



#71

Pentachlorophenol

Concen: 19.964 ng/ul

RT: 17.145 min Scan# 2373

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:266 Resp: 163688


Ion Ratio Lower Upper

266 100

264 61.9 49.6 74.4

268 61.5 51.0 76.6





#72

Phenanthrene

Concen: 20.587 ng/ul

RT: 17.539 min Scan# 2440

Delta R.T. 0.000 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:178 Resp: 1269894

Ion Ratio Lower Upper

178 100

179 15.4 12.3 18.5

176 19.2 15.4 23.0



#74

Anthracene

Concen: 20.632 ng/ul

RT: 17.634 min Scan# 2456

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:178 Resp: 1291338


Ion Ratio Lower Upper

178 100

179 15.5 12.4 18.6

176 18.9 15.0 22.4

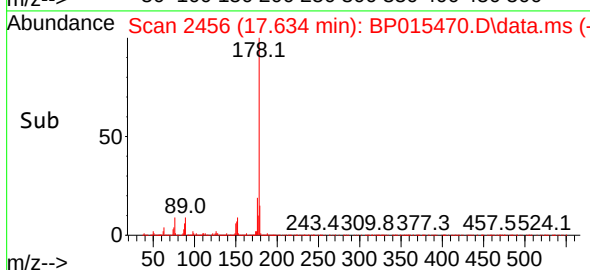



#75

1,2,3,4-Tetrachlorobenzene

Concen: 20.557 ng/uL

RT: 13.546 min Scan# 1761

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:216 Resp: 326125

Ion Ratio Lower Upper

216 100

214 75.6 62.1 93.1

218 47.6 39.0 58.4

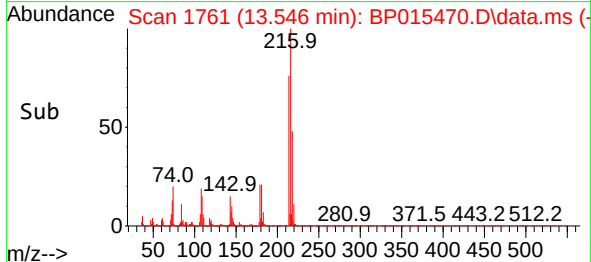

#76

Pentachlorobenzene

Concen: 20.531 ng/uL

RT: 15.057 min Scan# 2018

Delta R.T. 0.000 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:250 Resp: 341016


Ion Ratio Lower Upper

250 100

248 62.2 49.0 73.4

252 63.0 49.9 74.9

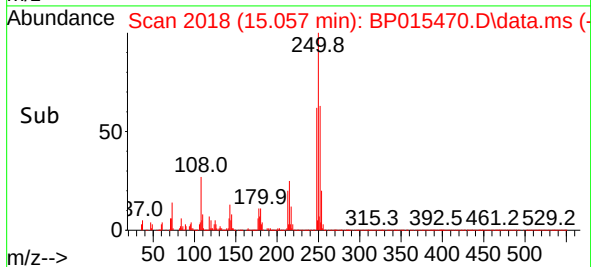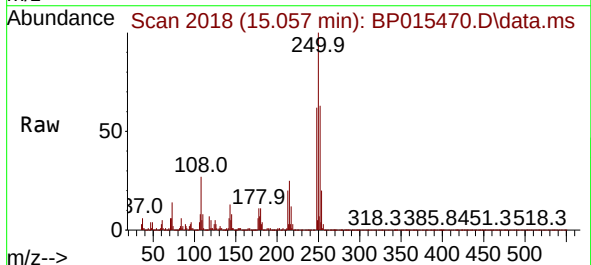



#77

Carbazole

Concen: 20.712 ng/ul

RT: 17.904 min Scan# 2502

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:167 Resp: 1167248

Ion Ratio Lower Upper

167 100

166 21.3 17.2 25.8

139 13.2 10.6 16.0

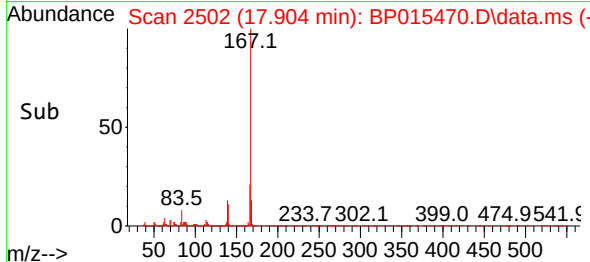

#78

Di-n-butylphthalate

Concen: 20.907 ng/ul

RT: 18.428 min Scan# 2591

Delta R.T. 0.000 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:149 Resp: 1494884


Ion Ratio Lower Upper

149 100

150 9.1 7.1 10.7

104 5.7 4.5 6.7


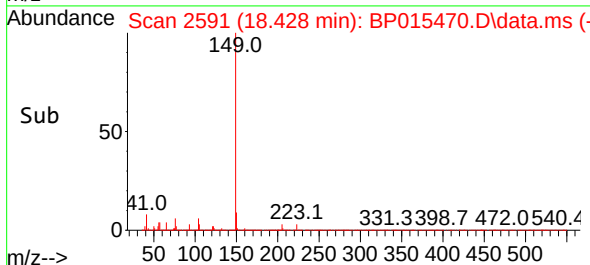
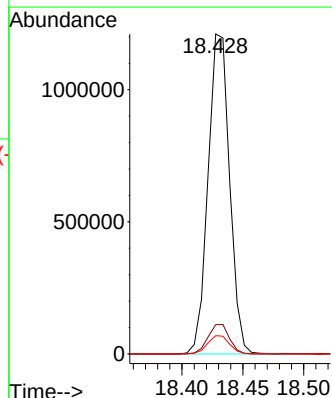
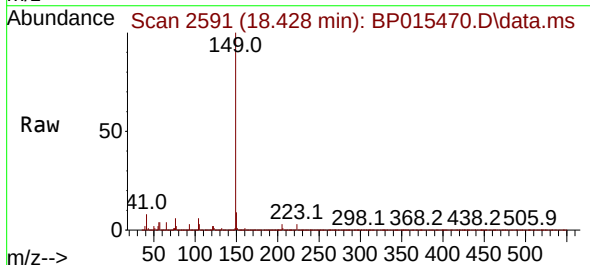




#80
Fluoranthene
Concen: 21.432 ng/u1
RT: 19.492 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:202 Resp: 1574534
Ion Ratio Lower Upper
202 100
101 11.5 8.6 13.0
100 8.6 6.6 9.8

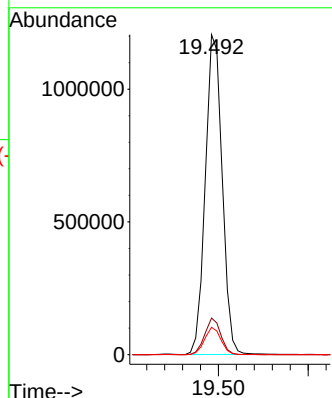

#82
Pyrene
Concen: 21.467 ng/u1
RT: 19.851 min Scan# 2833
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:202 Resp: 1631627
Ion Ratio Lower Upper
202 100
101 12.0 9.9 14.9
100 9.9 8.4 12.6

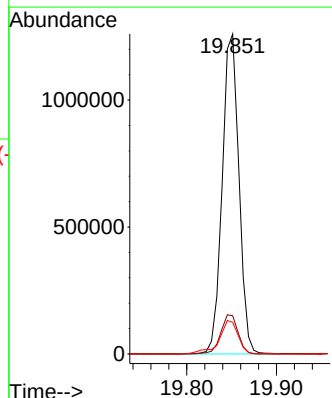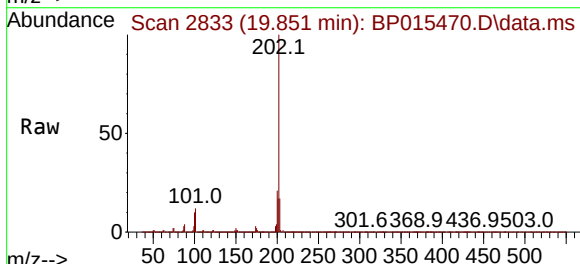



#83

Butylbenzylphthalate

Concen: 21.595 ng/ul

RT: 20.704 min Scan# 2978

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:149 Resp: 725475

Ion Ratio Lower Upper

149 100

91 74.3 60.4 90.6

206 21.4 16.4 24.6



#84

3,3'-Dichlorobenzidine

Concen: 18.337 ng/ul

RT: 21.492 min Scan# 3112

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:252 Resp: 488172


Ion Ratio Lower Upper

252 100

254 63.7 51.6 77.4

126 10.9 8.5 12.7





#85

Benzo(a)anthracene

Concen: 20.731 ng/ul

RT: 21.563 min Scan# 3123

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:228 Resp: 1633153

Ion Ratio Lower Upper

228 100

229 19.7 15.8 23.6

226 27.0 21.8 32.6



#86

Bis(2-ethylhexyl)phthalate

Concen: 22.163 ng/ul

RT: 21.457 min Scan# 3106

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:149 Resp: 1100525


Ion Ratio Lower Upper

149 100

167 26.2 21.8 32.8

279 3.9 3.7 5.5









#87
Chrysene
Concen: 20.778 ng/ul
RT: 21.622 min Scan# 3133
Delta R.T. 0.006 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34




Instrument :
BNA_P
ClientSampleId :
SSTD020745


Tgt Ion:228 Resp: 1547204
Ion Ratio Lower Upper
228 100
226 30.4 23.9 35.9
229 19.6 15.1 22.7

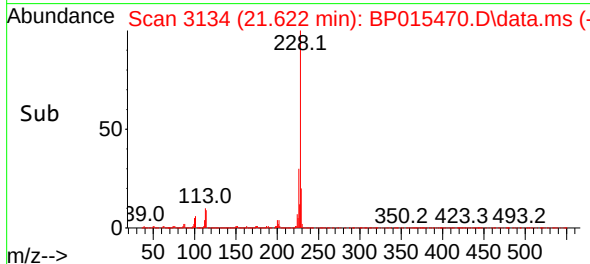

#89
Di-n-octyl phthalate
Concen: 24.279 ng/ul
RT: 22.433 min Scan# 3272
Delta R.T. 0.012 min
Lab File: BP015470.D
Acq: 12 Jun 2023 12:34

Tgt Ion:149 Resp: 1911159

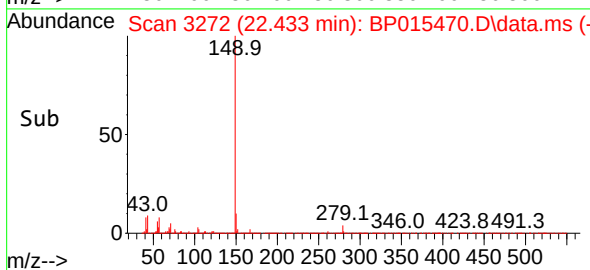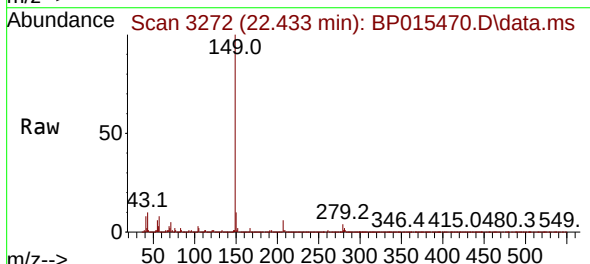



#90

Benzo(b)fluoranthene

Concen: 20.578 ng/ul

RT: 23.345 min Scan# 3426

Delta R.T. 0.006 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:252 Resp: 1590897

Ion Ratio Lower Upper

252 100

253 21.9 17.4 26.2

125 9.6 7.3 10.9



#91

Benzo(k)fluoranthene

Concen: 21.296 ng/ul

RT: 23.398 min Scan# 3436

Delta R.T. 0.012 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:252 Resp: 1591495


Ion Ratio Lower Upper

252 100

253 21.2 17.7 26.5

125 9.2 7.3 10.9





#93

Benzo(a)pyrene

Concen: 20.246 ng/ul

RT: 24.022 min Scan# 3

Delta R.T. 0.012 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:252 Resp: 1364687

Ion Ratio Lower Upper

252 100

253 21.8 17.8 26.6

125 10.2 8.1 12.1



#94

Indeno(1,2,3-cd)pyrene

Concen: 18.029 ng/ul

RT: 26.839 min Scan# 4021

Delta R.T. 0.012 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34




Tgt Ion:276 Resp: 1572690


Ion Ratio Lower Upper

276 100

138 22.4 17.3 25.9

277 25.3 20.2 30.2

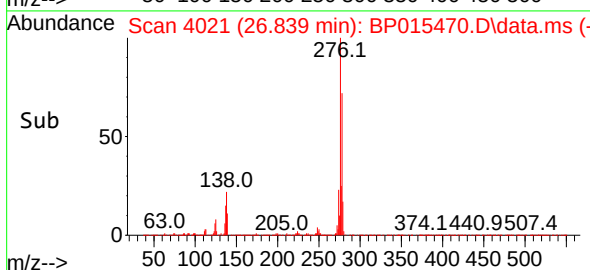



#95

Dibenzo(a,h)anthracene

Concen: 18.156 ng/ul

RT: 26.857 min Scan# 4021

Delta R.T. 0.018 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Instrument :

BNA_P

ClientSampleId :

SSTD020745





Tgt Ion:278 Resp: 1290307

Ion Ratio Lower Upper

278 100

139 14.6 11.4 17.0

279 23.5 18.7 28.1

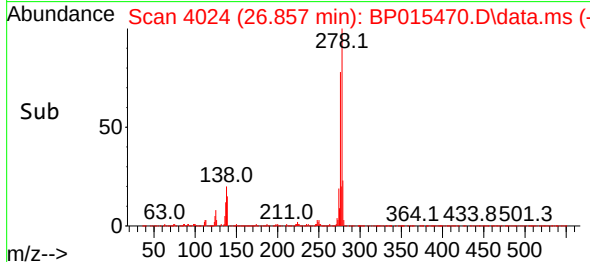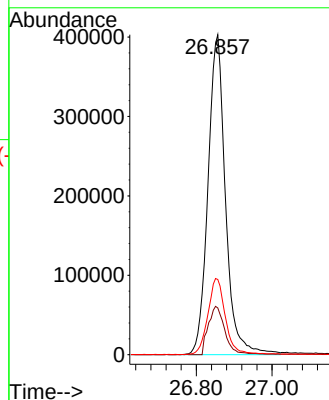

#96

Benzo(g,h,i)perylene

Concen: 18.075 ng/ul

RT: 27.674 min Scan# 4163

Delta R.T. 0.018 min

Lab File: BP015470.D

Acq: 12 Jun 2023 12:34

Tgt Ion:276 Resp: 1299352

Ion Ratio Lower Upper

276 100

138 19.8 15.6 23.4

277 24.1 19.0 28.6

