

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061223\
 Data File : BP015482.D
 Acq On : 12 Jun 2023 20:52
 Operator : MA/JU
 Sample : PB153305BS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS305

Quant Time: Jun 12 23:23:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	139521	20.000	ng/u1	0.00
20) Naphthalene-d8	10.922	136	656806	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.733	164	448334	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.492	188	1042227	20.000	ng/u1	0.00
79) Chrysene-d12	21.574	240	997828	20.000	ng/u1	0.00
88) Perylene-d12	24.121	264	1101727	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	24006	6.371	ng/uL	0.00
4) Pyridine-d5	3.846	84	311082	31.786	ng/u1	0.00
7) Phenol-d5	7.246	99	438237	34.095	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	275756	35.923	ng/u1	0.00
11) 2-Chlorophenol-d4	7.616	132	347441	37.282	ng/u1	0.00
15) 4-Methylphenol-d8	8.810	113	377068	35.744	ng/u1	0.00
21) Nitrobenzene-d5	9.269	128	181543	35.206	ng/u1	0.00
24) 2-Nitrophenol-d4	9.998	143	210497	35.745	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.539	165	380885	35.457	ng/u1	0.00
31) 4-Chloroaniline-d4	11.063	131	486136	31.528	ng/u1	0.00
46) Dimethylphthalate-d6	14.139	166	1242928	35.157	ng/u1	0.00
49) Acenaphthylene-d8	14.433	160	1380074	35.700	ng/u1	0.00
54) 4-Nitrophenol-d4	14.939	143	215741	34.076	ng/u1	0.00
60) Fluorene-d10	15.727	176	1036773	34.776	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	228654	34.631	ng/u1	0.00
73) Anthracene-d10	17.592	188	1632097	34.418	ng/u1	0.00
81) Pyrene-d10	19.815	212	2015470	37.739	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.956	264	2079334	37.615	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.446	88	48576	12.205	ng/uL	89
5) Pyridine	3.869	79	308844	30.439	ng/u1	96
6) Benzaldehyde	7.228	77	203430	41.406	ng/u1	96
8) Phenol	7.275	94	459533	34.654	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.510	93	362941	34.617	ng/u1	100
12) 2-Chlorophenol	7.651	128	347197	35.262	ng/u1	99
13) 2-Methylphenol	8.540	108	356482	34.939	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.622	45	495966	35.697	ng/u1	98
16) Acetophenone	8.928	105	588101	34.933	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.910	70	314680	34.632	ng/u1	98
18) 4-Methylphenol	8.875	108	395440	35.226	ng/u1	99
19) Hexachloroethane	9.181	117	142712	34.299	ng/u1	98
22) Nitrobenzene	9.316	77	469707	34.348	ng/u1	99
23) Isophorone	9.839	82	916253	33.471	ng/u1	99
25) 2-Nitrophenol	10.028	139	218439	34.356	ng/u1	97
26) 2,4-Dimethylphenol	10.087	107	442415	32.812	ng/u1	96
27) Bis(2-Chloroethoxy)met...	10.322	93	539514	33.899	ng/u1	100
29) 2,4-Dichlorophenol	10.569	162	376682	35.268	ng/u1	98
30) Naphthalene	10.969	128	1185318	33.304	ng/u1	99
32) 4-Chloroaniline	11.086	127	367252	23.019	ng/u1	99
33) Hexachlorobutadiene	11.245	225	242843	33.715	ng/u1	98
34) Caprolactam	11.869	113	127820	31.791	ng/u1	92
35) 4-Chloro-3-methylphenol	12.198	107	448974	34.695	ng/u1	98
36) 2-Methylnaphthalene	12.569	142	830675	33.199	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061223\
 Data File : BP015482.D
 Acq On : 12 Jun 2023 20:52
 Operator : MA/JU
 Sample : PB153305BS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS305

Quant Time: Jun 12 23:23:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.786	142	837383	33.240	ng/ul	97
39) 1,2,4,5-Tetrachloroben...	12.933	216	472068	33.814	ng/ul	97
40) Hexachlorocyclopentadiene	12.910	237	201205	35.160	ng/ul	97
41) 2,4,6-Trichlorophenol	13.175	196	316069	34.016	ng/ul	98
42) 2,4,5-Trichlorophenol	13.251	196	347889	34.358	ng/ul	98
43) 1,1'-Biphenyl	13.569	154	1159646	33.447	ng/ul	100
44) 2-Chloronaphthalene	13.616	162	915068	33.639	ng/ul	98
45) 2-Nitroaniline	13.828	65	315513	36.241	ng/ul	97
47) Dimethylphthalate	14.186	163	1217023	33.341	ng/ul	99
48) 2,6-Dinitrotoluene	14.316	165	262602	35.114	ng/ul	99
50) Acenaphthylene	14.463	152	1420696	33.186	ng/ul	99
51) 3-Nitroaniline	14.651	138	244619	39.623	ng/ul	99
52) Acenaphthene	14.798	153	986777	33.346	ng/ul	99
53) 2,4-Dinitrophenol	14.863	184	141185	31.383	ng/ul	99
55) 4-Nitrophenol	14.951	109	200042	32.757	ng/ul	95
56) Dibenzofuran	15.133	168	1409333	33.602	ng/ul	98
57) 2,4-Dinitrotoluene	15.104	165	381890	34.719	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.363	232	300775	32.899	ng/ul	97
59) Diethylphthalate	15.545	149	1281166	34.246	ng/ul	99
61) Fluorene	15.786	166	1145572	33.505	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.774	204	581176	33.727	ng/ul	100
63) 4-Nitroaniline	15.816	138	255326	43.601	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.869	198	224257	33.302	ng/ul	93
67) N-Nitrosodiphenylamine	15.986	169	989533	33.466	ng/ul	100
68) 4-Bromophenyl-phenylether	16.669	248	376793	33.793	ng/ul	96
69) Hexachlorobenzene	16.792	284	449075	34.144	ng/ul	97
70) Atrazine	16.939	200	155309	13.154	ng/ul	99
71) Pentachlorophenol	17.139	266	245921	33.081	ng/ul	100
72) Phenanthrene	17.533	178	1900320	33.977	ng/ul	99
74) Anthracene	17.627	178	1887990	33.269	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.539	216	491013	34.136	ng/ul	100
76) Pentachlorobenzene	15.057	250	492435	32.698	ng/ul	98
77) Carbazole	17.898	167	1768278	34.606	ng/ul	99
78) Di-n-butylphthalate	18.421	149	2293885	35.382	ng/ul	99
80) Fluoranthene	19.486	202	2381292	36.605	ng/ul	99
82) Pyrene	19.845	202	2422488	35.994	ng/ul	98
83) Butylbenzylphthalate	20.698	149	1132800	38.081	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.480	252	824781	34.987	ng/ul	98
85) Benzo(a)anthracene	21.557	228	2470157	35.411	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.451	149	1691840	38.479	ng/ul	99
87) Chrysene	21.615	228	2311845	35.063	ng/ul	98
89) Di-n-octyl phthalate	22.421	149	2959037	40.866	ng/ul	100
90) Benzo(b)fluoranthene	23.339	252	2564401	36.059	ng/ul	100
91) Benzo(k)fluoranthene	23.386	252	2466253	35.875	ng/ul	99
93) Benzo(a)pyrene	24.009	252	2172216	35.034	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.815	276	2597799	32.374	ng/ul	99
95) Dibenzo(a,h)anthracene	26.833	278	2133255	32.632	ng/ul	99
96) Benzo(g,h,i)perylene	27.644	276	2094327	31.671	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061223\
Data File : BP015482.D
Acq On : 12 Jun 2023 20:52
Operator : MA/JU
Sample : PB153305BS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLCS305

Quant Time: Jun 12 23:23:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 09 23:33:38 2023
Response via : Initial Calibration




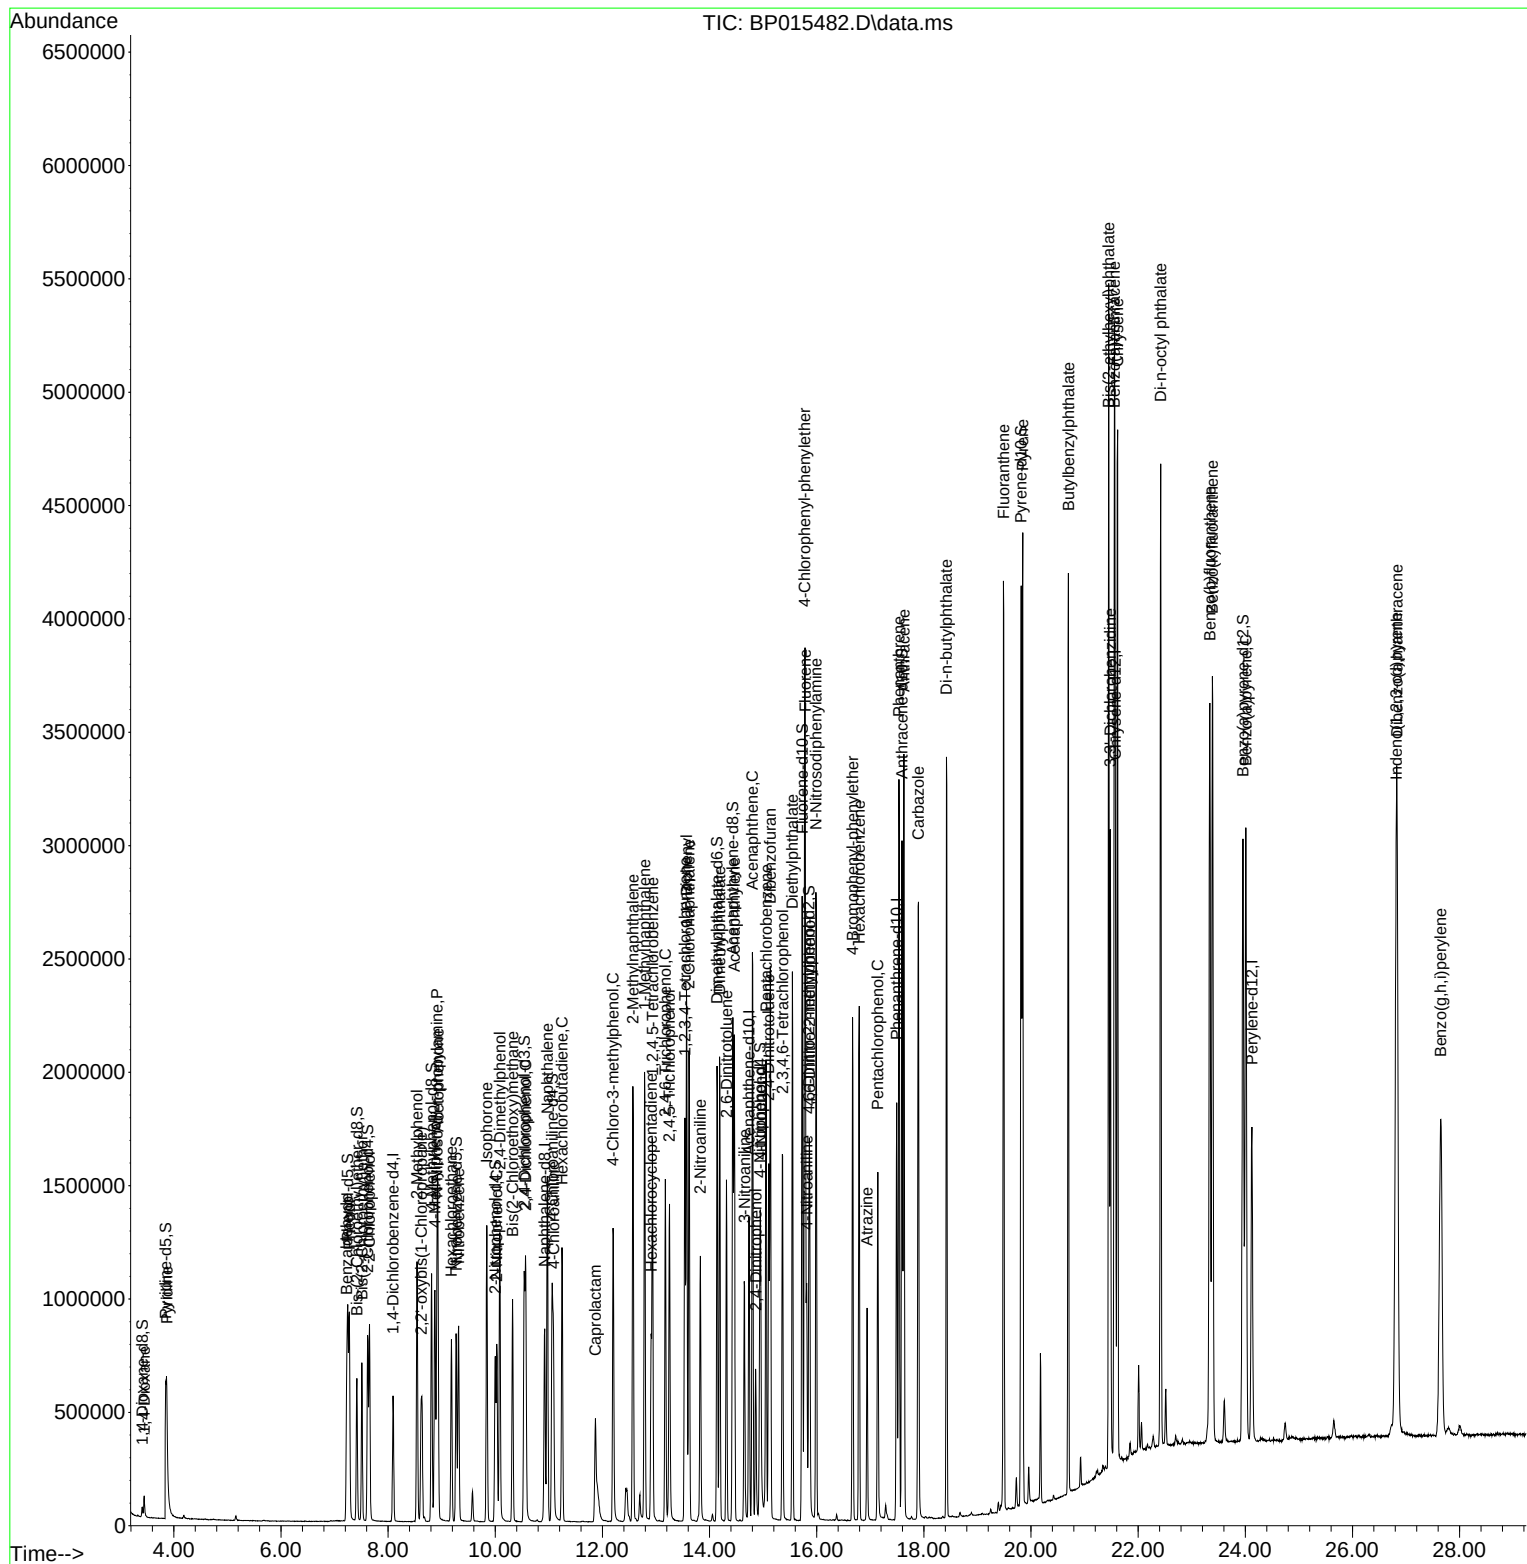




#2
 1,4-Dioxane
 Concen: 12.205 ng/uL
 RT: 3.446 min Scan# 44
 Delta R.T. -0.000 min
 Lab File: BP015482.D
 Acq: 12 Jun 2023 20:52




Instrument :
 BNA_P
 ClientSampleId :
 SLCS305


Tgt Ion:	88	Resp:	48576
Ion	Ratio	Lower	Upper
88	100		
43	31.8	23.9	35.9
58	76.1	51.4	77.2

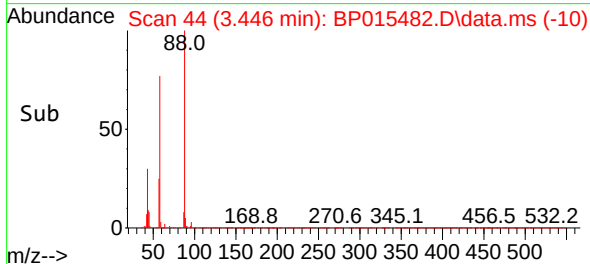

#5
 Pyridine
 Concen: 30.439 ng/uL
 RT: 3.869 min Scan# 116
 Delta R.T. -0.000 min
 Lab File: BP015482.D
 Acq: 12 Jun 2023 20:52

Tgt Ion:	79	Resp:	308844
Ion	Ratio	Lower	Upper
79	100		
52	78.9	59.5	89.3
51	37.0	29.8	44.6


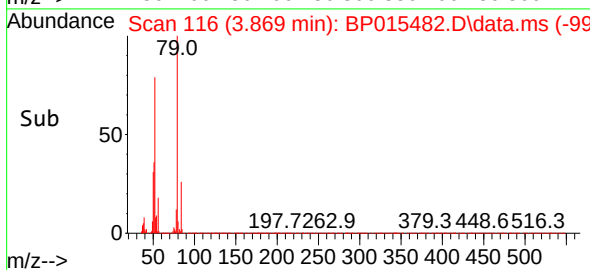

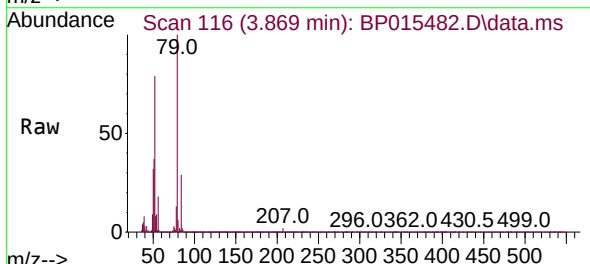




#6
Benzaldehyde
Concen: 41.406 ng/ul
RT: 7.228 min Scan# 610
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion: 77 Resp: 203430
Ion Ratio Lower Upper
77 100
105 92.1 77.3 115.9
106 88.1 73.3 109.9



#8
Phenol
Concen: 34.654 ng/ul
RT: 7.275 min Scan# 695
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion: 94 Resp: 459533
Ion Ratio Lower Upper
94 100
65 31.5 23.5 35.3
66 43.7 34.2 51.4



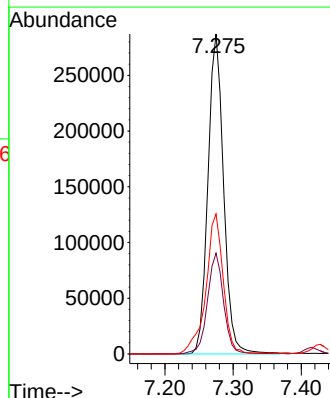





#10
Bis(2-Chloroethyl)ether
Concen: 34.617 ng/ul
RT: 7.510 min Scan# 735
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion: 93 Resp: 362941
Ion Ratio Lower Upper
93 100
63 78.4 62.6 93.8
95 32.1 25.5 38.3



#12
2-Chlorophenol
Concen: 35.262 ng/ul
RT: 7.651 min Scan# 759
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:128 Resp: 347197
Ion Ratio Lower Upper
128 100
64 50.0 40.2 60.4
130 32.2 24.5 36.7









#13
2-Methylphenol
Concen: 34.939 ng/ul
RT: 8.540 min Scan# 911
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:108 Resp: 356482
Ion Ratio Lower Upper
108 100
107 88.5 71.2 106.8



#14
2,2'-oxybis(1-Chloropropane)
Concen: 35.697 ng/ul
RT: 8.622 min Scan# 924
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion: 45 Resp: 495966
Ion Ratio Lower Upper
45 100
77 15.7 11.8 17.8
79 11.3 8.7 13.1









#16
Acetophenone
Concen: 34.933 ng/ul
RT: 8.928 min Scan# 91
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:105 Resp: 588101
Ion Ratio Lower Upper
105 100
77 81.1 64.9 97.3
51 29.6 23.5 35.3



#17
N-Nitroso-di-n-propylamine
Concen: 34.632 ng/ul
RT: 8.910 min Scan# 973
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion: 70 Resp: 314680
Ion Ratio Lower Upper
70 100
42 59.6 46.6 69.8
101 10.0 7.8 11.6
130 19.5 15.9 23.9



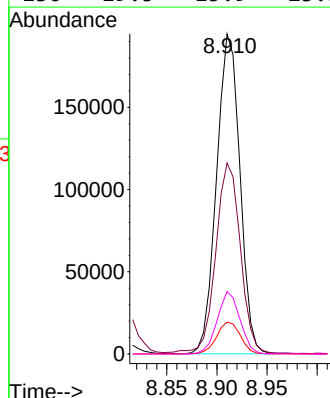





#18
4-Methylphenol
Concen: 35.226 ng/ul
RT: 8.875 min Scan# 90
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:108 Resp: 395440
Ion Ratio Lower Upper
108 100
107 112.3 89.3 133.9



#19
Hexachloroethane
Concen: 34.299 ng/ul
RT: 9.181 min Scan# 1019
Delta R.T. -0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:117 Resp: 142712
Ion Ratio Lower Upper
117 100
201 104.6 82.8 124.2
199 66.2 50.6 76.0


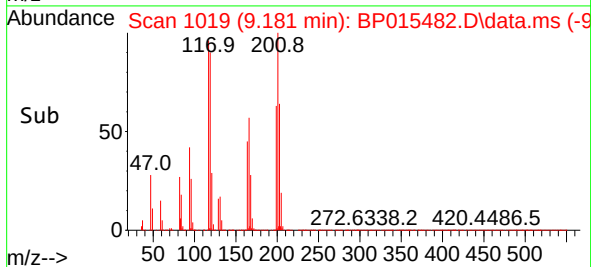

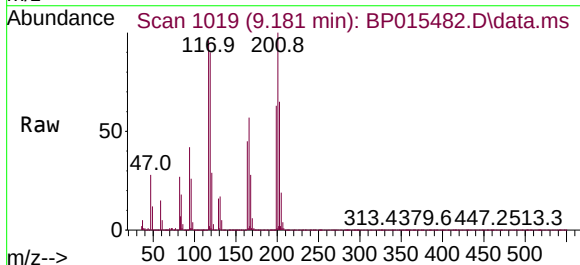




#22
Nitrobenzene
Concen: 34.348 ng/ul
RT: 9.316 min Scan# 1042
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion: 77 Resp: 469707
Ion Ratio Lower Upper
77 100
123 41.2 33.5 50.3
65 14.2 11.6 17.4



#23
Isophorone
Concen: 33.471 ng/ul
RT: 9.839 min Scan# 1131
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion: 82 Resp: 916253
Ion Ratio Lower Upper
82 100
95 7.5 5.8 8.8
138 16.0 13.1 19.7









#25
2-Nitrophenol
Concen: 34.356 ng/ul
RT: 10.028 min Scan# 1163
Delta R.T. -0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:139 Resp: 218439
Ion Ratio Lower Upper
139 100
65 61.1 46.9 70.3
109 36.9 30.2 45.2

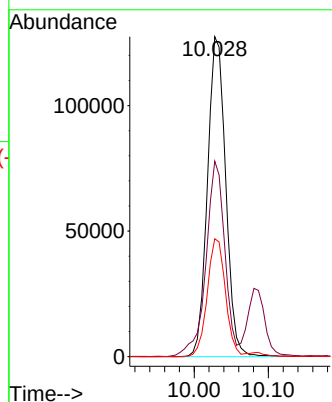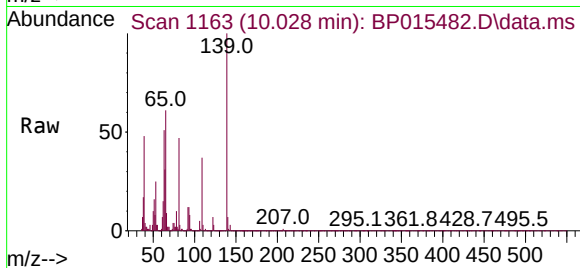

#26
2,4-Dimethylphenol
Concen: 32.812 ng/ul
RT: 10.087 min Scan# 1173
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:107 Resp: 442415
Ion Ratio Lower Upper
107 100
121 47.3 39.0 58.6
122 76.6 64.8 97.2



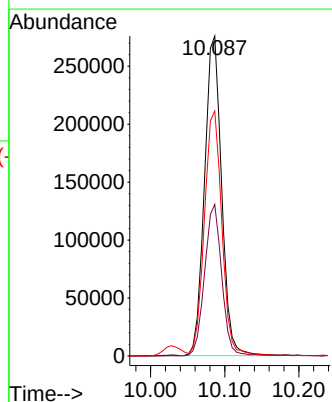





#27
 Bis(2-Chloroethoxy)methane
 Concen: 33.899 ng/ul
 RT: 10.322 min Scan# 1213
 Delta R.T. -0.000 min
 Lab File: BP015482.D
 Acq: 12 Jun 2023 20:52




Instrument :
 BNA_P
 ClientSampleId :
 SLCS305


Tgt Ion: 93 Resp: 539514
 Ion Ratio Lower Upper
 93 100
 95 32.3 25.7 38.5
 123 10.4 8.6 13.0



#29
 2,4-Dichlorophenol
 Concen: 35.268 ng/ul
 RT: 10.569 min Scan# 1255
 Delta R.T. -0.000 min
 Lab File: BP015482.D
 Acq: 12 Jun 2023 20:52

Tgt Ion: 162 Resp: 376682
 Ion Ratio Lower Upper
 162 100
 164 65.0 50.6 76.0
 98 37.1 30.2 45.2


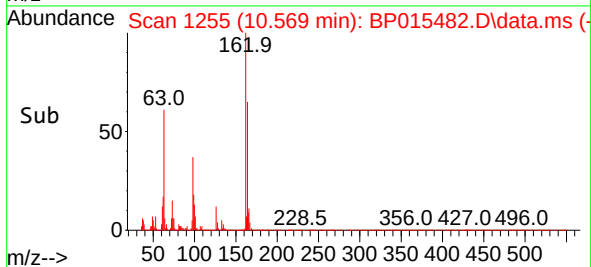

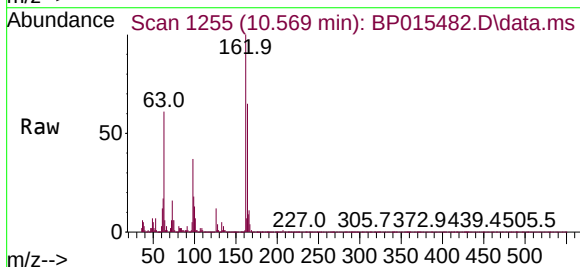




#30
Naphthalene
Concen: 33.304 ng/ul
RT: 10.969 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:128 Resp: 1185318
Ion Ratio Lower Upper
128 100
129 10.8 8.6 13.0
127 13.9 10.5 15.7



#32
4-Chloroaniline
Concen: 23.019 ng/ul
RT: 11.086 min Scan# 1343
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:127 Resp: 367252
Ion Ratio Lower Upper
127 100
129 32.9 26.1 39.1

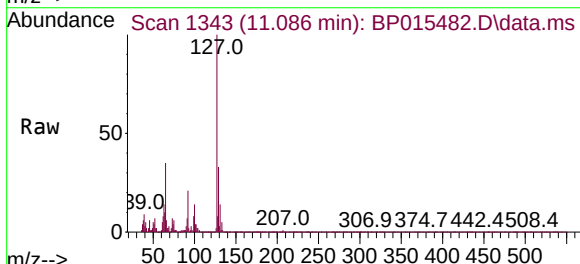



#33

Hexachlorobutadiene

Concen: 33.715 ng/ul

RT: 11.245 min Scan# 11

Delta R.T. -0.006 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:225 Resp: 242843

Ion Ratio Lower Upper

225 100

223 62.6 52.0 78.0

227 63.2 50.6 75.8

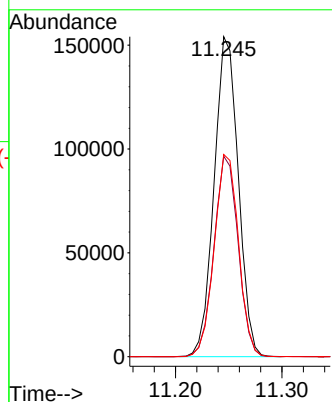

#34

Caprolactam

Concen: 31.791 ng/ul

RT: 11.869 min Scan# 1476

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52




Tgt Ion:113 Resp: 127820


Ion Ratio Lower Upper

113 100

55 172.2 127.9 191.9

56 132.6 101.1 151.7


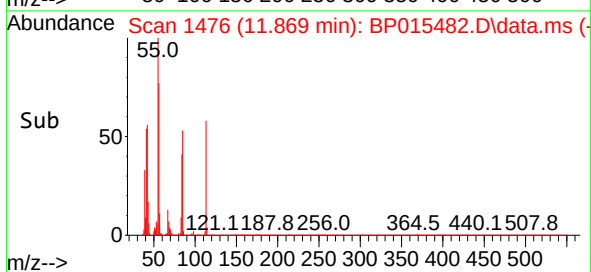
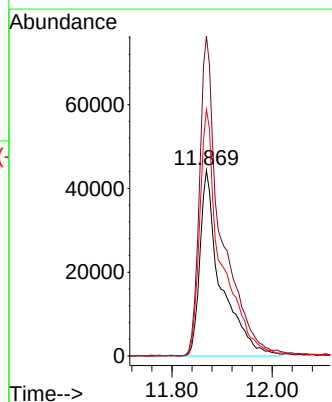





#35
4-Chloro-3-methylphenol
Concen: 34.695 ng/ul
RT: 12.198 min Scan# 1532
Delta R.T. -0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:107 Resp: 448974
Ion Ratio Lower Upper
107 100
144 23.8 19.4 29.0
142 73.9 60.4 90.6

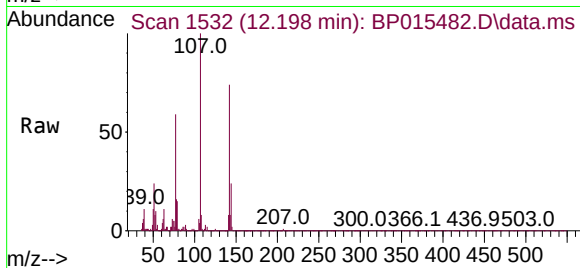

#36
2-Methylnaphthalene
Concen: 33.199 ng/ul
RT: 12.569 min Scan# 1595
Delta R.T. -0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:142 Resp: 830675
Ion Ratio Lower Upper
142 100
141 88.3 72.0 108.0

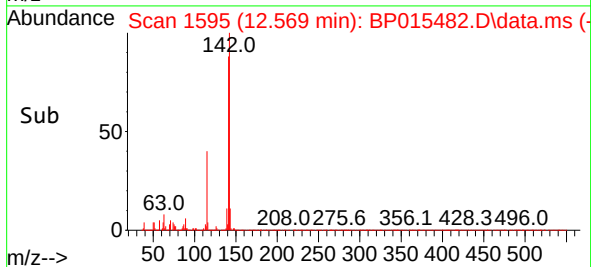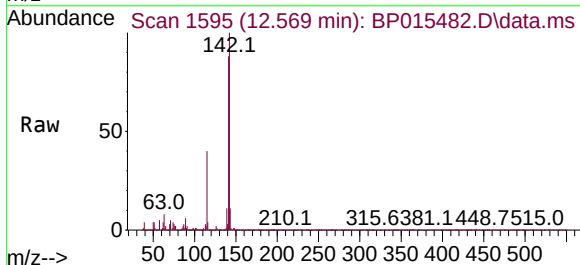



#37

1-Methylnaphthalene

Concen: 33.240 ng/ul

RT: 12.786 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:142 Resp: 837383

Ion Ratio Lower Upper

142 100

141 93.1 71.9 107.9

116 4.4 3.4 5.2

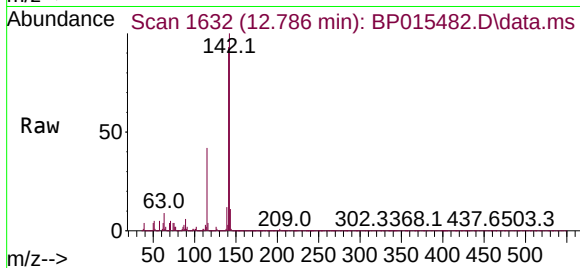

#39

1,2,4,5-Tetrachlorobenzene

Concen: 33.814 ng/ul

RT: 12.933 min Scan# 1657

Delta R.T. -0.006 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Tgt Ion:216 Resp: 472068




Ion Ratio Lower Upper


216 100

214 80.2 62.2 93.2

179 22.7 17.4 26.2

108 18.9 14.2 21.4



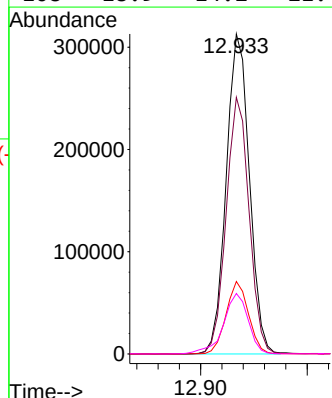





#40
Hexachlorocyclopentadiene
Concen: 35.160 ng/ul
RT: 12.910 min Scan# 1653
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:237 Resp: 201205
Ion Ratio Lower Upper
237 100
235 62.4 48.2 72.2
272 12.5 10.3 15.5



#41
2,4,6-Trichlorophenol
Concen: 34.016 ng/ul
RT: 13.175 min Scan# 1698
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:196 Resp: 316069
Ion Ratio Lower Upper
196 100
198 95.3 77.8 116.6
200 30.4 25.8 38.6




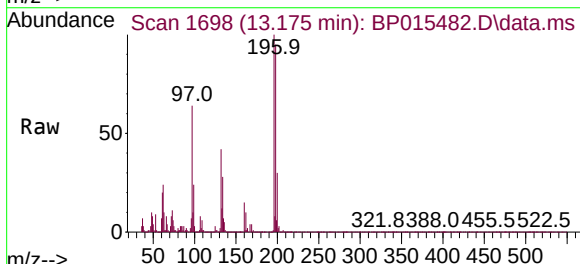




#42
2,4,5-Trichlorophenol
Concen: 34.358 ng/ul
RT: 13.251 min Scan# 1711
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:196 Resp: 347889
Ion Ratio Lower Upper
196 100
198 96.7 75.5 113.3
200 31.0 24.7 37.1

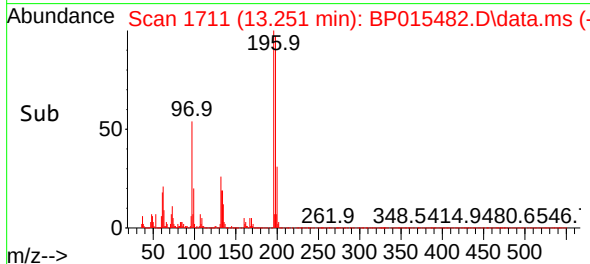

#43
1,1'-Biphenyl
Concen: 33.447 ng/ul
RT: 13.569 min Scan# 1765
Delta R.T. -0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:154 Resp: 1159646
Ion Ratio Lower Upper
154 100
153 40.2 32.2 48.2
76 13.6 10.4 15.6

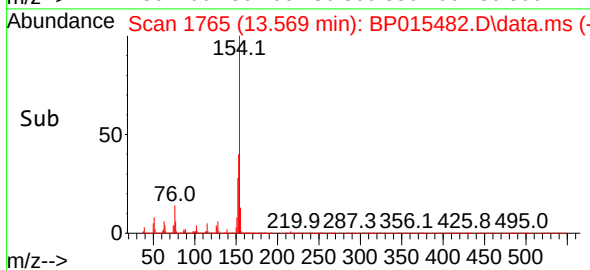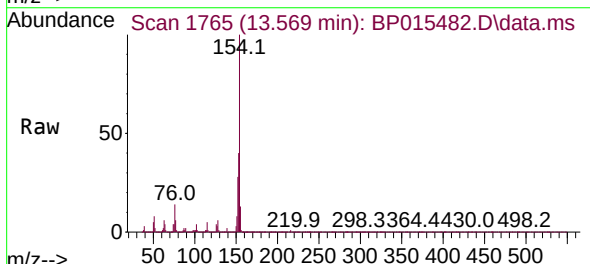



#44

2-Chloronaphthalene

Concen: 33.639 ng/ul

RT: 13.616 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:162 Resp: 915068

Ion Ratio Lower Upper

162 100

164 32.8 27.0 40.6

127 41.1 32.2 48.4

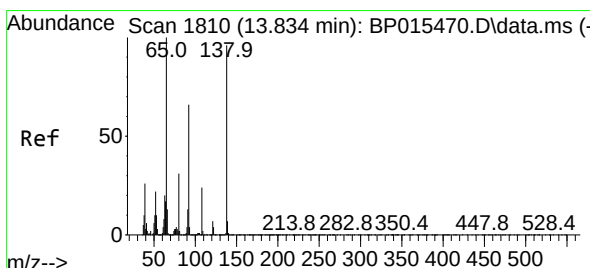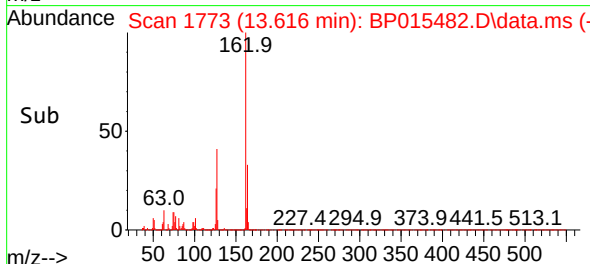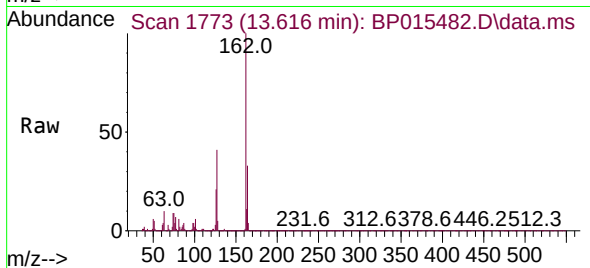

#45

2-Nitroaniline

Concen: 36.241 ng/ul

RT: 13.828 min Scan# 1809

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52




Tgt Ion: 65 Resp: 315513


Ion Ratio Lower Upper

65 100

92 65.9 55.4 83.2

138 96.5 78.8 118.2


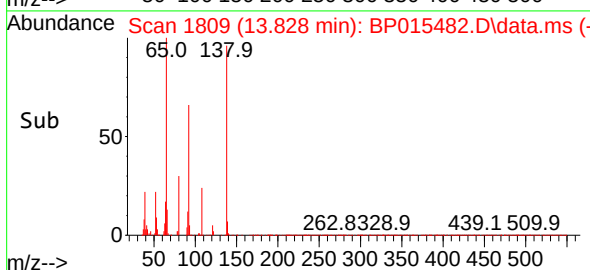






#47
Dimethylphthalate
Concen: 33.341 ng/ul
RT: 14.186 min Scan# 1870
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:163 Resp: 1217023
Ion Ratio Lower Upper
163 100
194 3.9 3.2 4.8
164 10.7 8.2 12.2

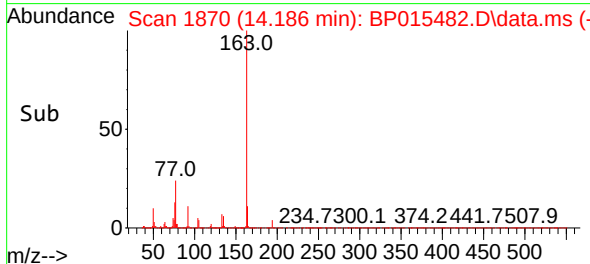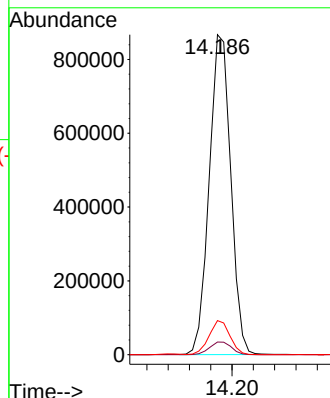

#48
2,6-Dinitrotoluene
Concen: 35.114 ng/ul
RT: 14.316 min Scan# 1892
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:165 Resp: 262602
Ion Ratio Lower Upper
165 100
89 65.2 51.5 77.3
121 22.1 17.3 25.9


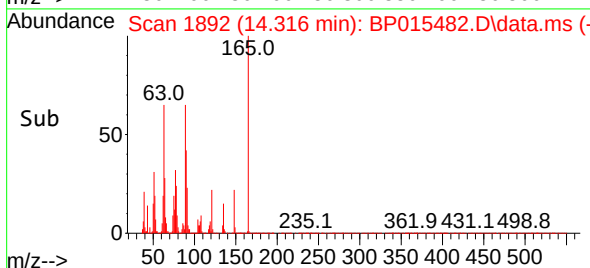
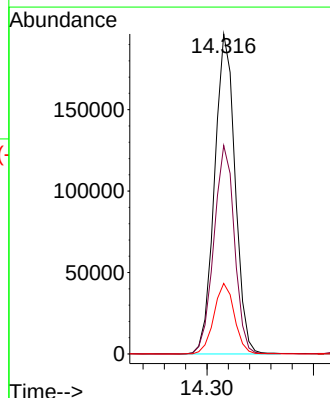
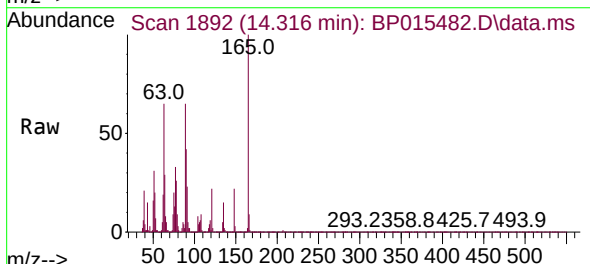




#50
Acenaphthylene
Concen: 33.186 ng/ul
RT: 14.463 min Scan# 1917
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:152 Resp: 1420696
Ion Ratio Lower Upper
152 100
151 20.3 16.0 24.0
153 12.9 10.6 15.8



#51
3-Nitroaniline
Concen: 39.623 ng/ul
RT: 14.651 min Scan# 1949
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:138 Resp: 244619
Ion Ratio Lower Upper
138 100
108 11.8 8.4 12.6
92 123.8 98.0 147.0




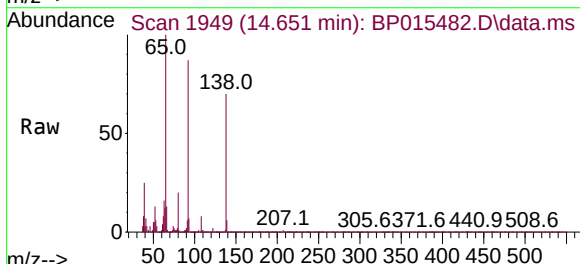




#52
Acenaphthene
Concen: 33.346 ng/ul
RT: 14.798 min Scan# 1974
Delta R.T. -0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:153 Resp: 986777
Ion Ratio Lower Upper
153 100
152 46.7 38.3 57.5
154 87.6 69.8 104.6



#53
2,4-Dinitrophenol
Concen: 31.383 ng/ul
RT: 14.863 min Scan# 1985
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:184 Resp: 141185
Ion Ratio Lower Upper
184 100
63 72.2 59.0 88.4
154 71.9 57.6 86.4




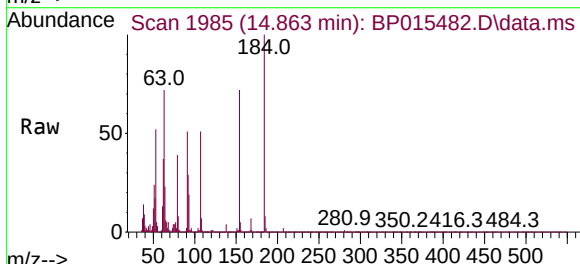




#55
4-Nitrophenol
Concen: 32.757 ng/ul
RT: 14.951 min Scan# 2000
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:109 Resp: 200042
Ion Ratio Lower Upper
109 100
139 105.5 89.1 133.7
65 124.4 103.1 154.7



#56
Dibenzofuran
Concen: 33.602 ng/ul
RT: 15.133 min Scan# 2031
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:168 Resp: 1409333
Ion Ratio Lower Upper
168 100
139 40.4 31.2 46.8


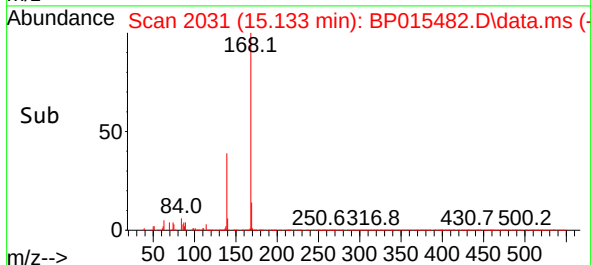
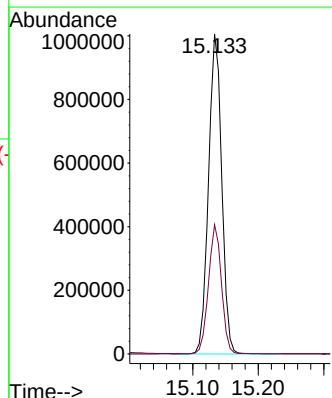
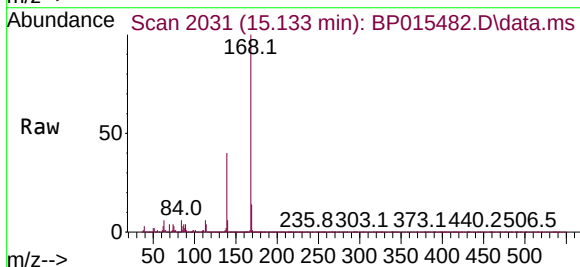




#57
2,4-Dinitrotoluene
Concen: 34.719 ng/ul
RT: 15.104 min Scan# 2027
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:165 Resp: 381890
Ion Ratio Lower Upper
165 100
63 50.4 39.1 58.7
182 2.9 2.2 3.4



#58
2,3,4,6-Tetrachlorophenol
Concen: 32.899 ng/ul
RT: 15.363 min Scan# 2070
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:232 Resp: 300775
Ion Ratio Lower Upper
232 100
131 44.5 37.8 56.8
130 2.6 1.9 2.9
166 32.0 26.2 39.2









#59
Diethylphthalate
Concen: 34.246 ng/ul
RT: 15.545 min Scan# 2101
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:149 Resp: 1281166
Ion Ratio Lower Upper
149 100
177 21.6 17.8 26.8
150 12.5 10.1 15.1



#61
Fluorene
Concen: 33.505 ng/ul
RT: 15.786 min Scan# 2142
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:166 Resp: 1145572
Ion Ratio Lower Upper
166 100
165 98.9 79.1 118.7
167 13.1 10.6 16.0


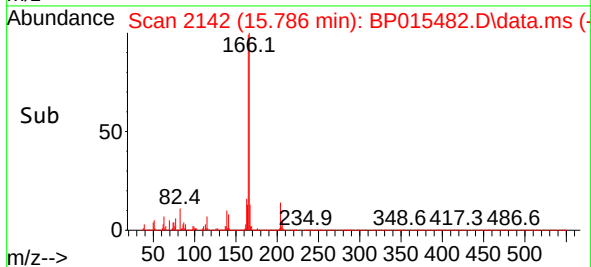

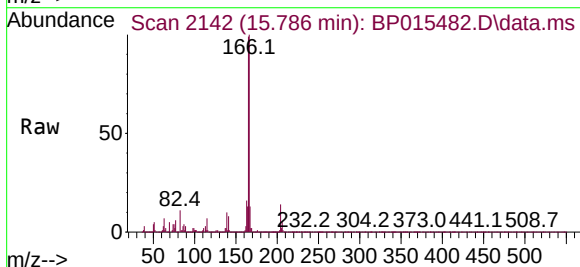




#62
4-Chlorophenyl-phenylether
Concen: 33.727 ng/ul
RT: 15.774 min Scan# 2140
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:204 Resp: 581176
Ion Ratio Lower Upper
204 100
206 32.9 26.6 40.0
141 62.4 49.8 74.8



#63
4-Nitroaniline
Concen: 43.601 ng/ul
RT: 15.816 min Scan# 2147
Delta R.T. 0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:138 Resp: 255326
Ion Ratio Lower Upper
138 100
92 55.7 44.6 67.0
108 98.8 78.4 117.6


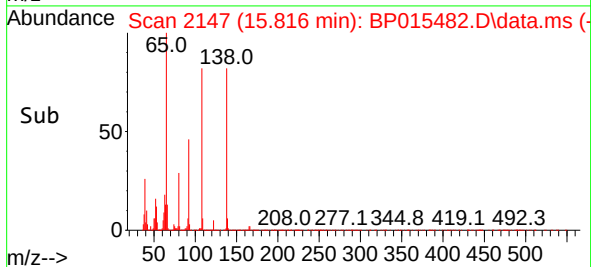

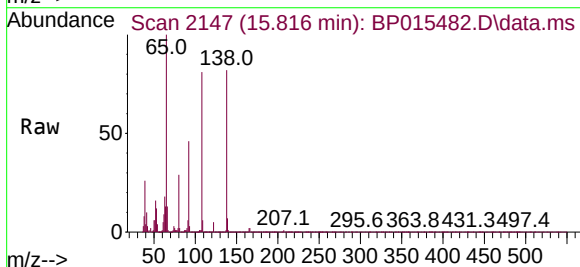




#66
4,6-Dinitro-2-methylphenol
Concen: 33.302 ng/ul
RT: 15.869 min Scan# 2156
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:198 Resp: 224257
Ion Ratio Lower Upper
198 100
182 4.3 3.0 4.4
77 29.7 20.5 30.7



#67
N-Nitrosodiphenylamine
Concen: 33.466 ng/ul
RT: 15.986 min Scan# 2176
Delta R.T. -0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:169 Resp: 989533
Ion Ratio Lower Upper
169 100
168 66.4 53.0 79.4
167 36.2 28.9 43.3




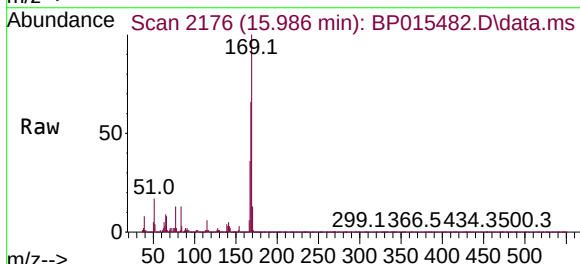




#68
4-Bromophenyl-phenylether
Concen: 33.793 ng/ul
RT: 16.669 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:248 Resp: 376793
Ion Ratio Lower Upper
248 100
250 99.3 78.3 117.5
141 83.4 61.1 91.7



#69
Hexachlorobenzene
Concen: 34.144 ng/ul
RT: 16.792 min Scan# 2313
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:284 Resp: 449075
Ion Ratio Lower Upper
284 100
142 34.6 25.4 38.2
249 31.6 24.8 37.2

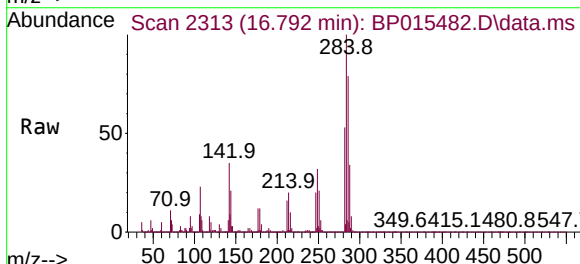



#70

Atrazine

Concen: 13.154 ng/ul

RT: 16.939 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:200 Resp: 155309

Ion Ratio Lower Upper

200 100

173 25.2 19.8 29.6

215 45.9 37.4 56.0

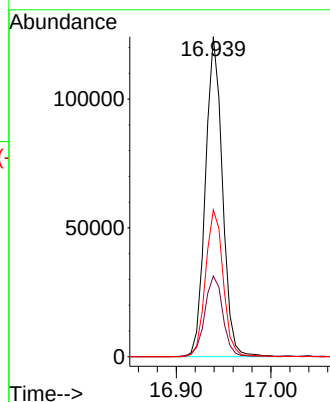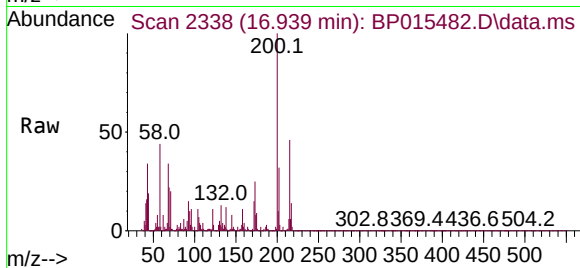

#71

Pentachlorophenol

Concen: 33.081 ng/ul

RT: 17.139 min Scan# 2372

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52




Tgt Ion:266 Resp: 245921


Ion Ratio Lower Upper

266 100

264 62.7 49.6 74.4

268 63.9 51.0 76.6





#72

Phenanthrene

Concen: 33.977 ng/ul

RT: 17.533 min Scan# 2440

Delta R.T. -0.006 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:178 Resp: 1900320

Ion Ratio Lower Upper

178 100

179 15.7 12.3 18.5

176 19.4 15.4 23.0

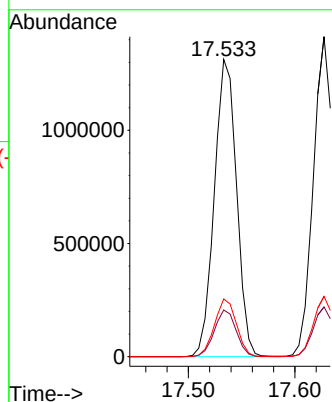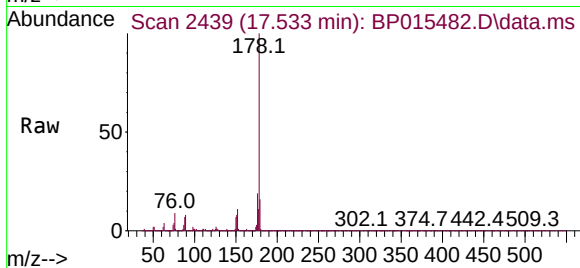

#74

Anthracene

Concen: 33.269 ng/ul

RT: 17.627 min Scan# 2455

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52




Tgt Ion:178 Resp: 1887990


Ion Ratio Lower Upper

178 100

179 15.6 12.4 18.6

176 18.9 15.0 22.4

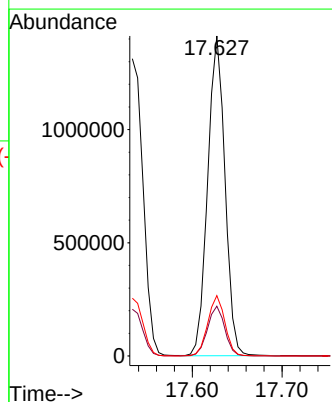



#75

1,2,3,4-Tetrachlorobenzene

Concen: 34.136 ng/uL

RT: 13.539 min Scan# 1760

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:216 Resp: 491013

Ion Ratio Lower Upper

216 100

214 77.6 62.1 93.1

218 48.6 39.0 58.4



#76

Pentachlorobenzene

Concen: 32.698 ng/uL

RT: 15.057 min Scan# 2018

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52




Tgt Ion:250 Resp: 492435


Ion Ratio Lower Upper

250 100

248 62.5 49.0 73.4

252 63.8 49.9 74.9

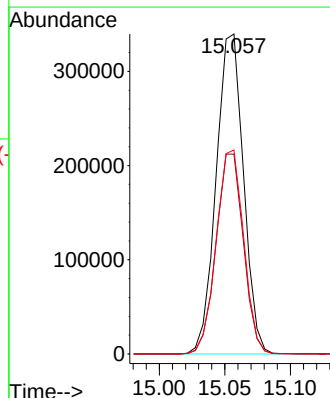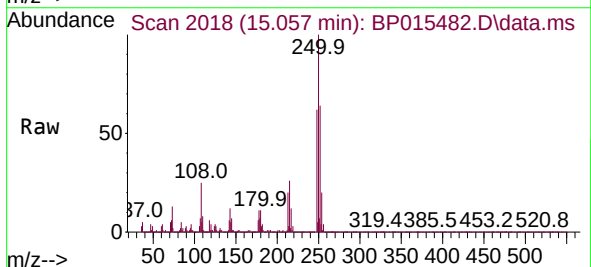



#77

Carbazole

Concen: 34.606 ng/ul

RT: 17.898 min Scan# 2501

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:167 Resp: 1768278

Ion Ratio Lower Upper

167 100

166 21.1 17.2 25.8

139 13.0 10.6 16.0



#78

Di-n-butylphthalate

Concen: 35.382 ng/ul

RT: 18.421 min Scan# 2590

Delta R.T. -0.006 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52




Tgt Ion:149 Resp: 2293885


Ion Ratio Lower Upper

149 100

150 9.3 7.1 10.7

104 5.9 4.5 6.7



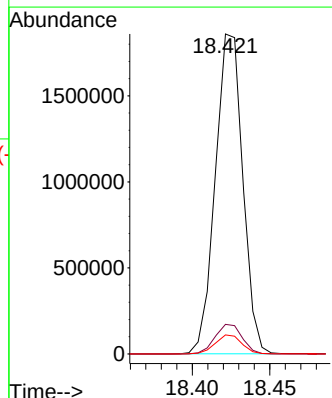
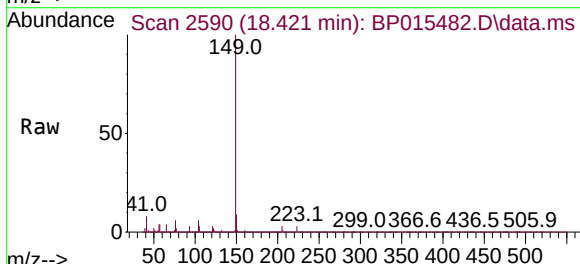




#80
Fluoranthene
Concen: 36.605 ng/u1
RT: 19.486 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:202 Resp: 2381292
Ion Ratio Lower Upper
202 100
101 11.2 8.6 13.0
100 8.4 6.6 9.8

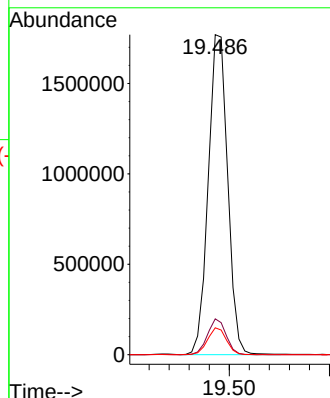

#82
Pyrene
Concen: 35.994 ng/u1
RT: 19.845 min Scan# 2832
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:202 Resp: 2422488
Ion Ratio Lower Upper
202 100
101 11.8 9.9 14.9
100 9.9 8.4 12.6

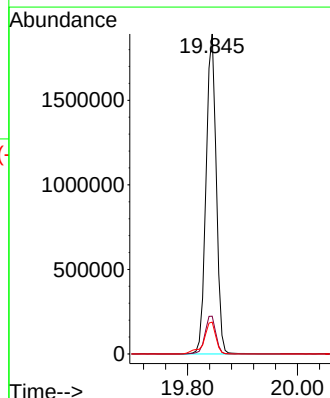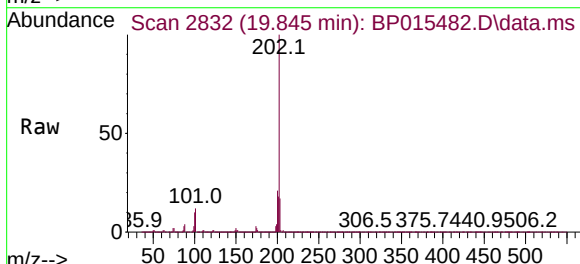



#83

Butylbenzylphthalate

Concen: 38.081 ng/ul

RT: 20.698 min Scan# 2977

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:149 Resp: 1132800

Ion Ratio Lower Upper

149 100

91 72.3 60.4 90.6

206 20.7 16.4 24.6

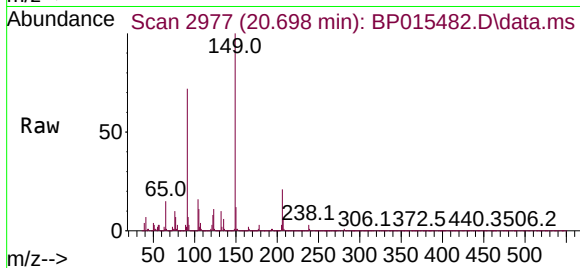

#84

3,3'-Dichlorobenzidine

Concen: 34.987 ng/ul

RT: 21.480 min Scan# 3110

Delta R.T. -0.006 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52




Tgt Ion:252 Resp: 824781


Ion Ratio Lower Upper

252 100

254 63.2 51.6 77.4

126 11.1 8.5 12.7





#85

Benzo(a)anthracene

Concen: 35.411 ng/ul

RT: 21.557 min Scan# 31

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:228 Resp: 2470157

Ion Ratio Lower Upper

228 100

229 19.6 15.8 23.6

226 27.1 21.8 32.6

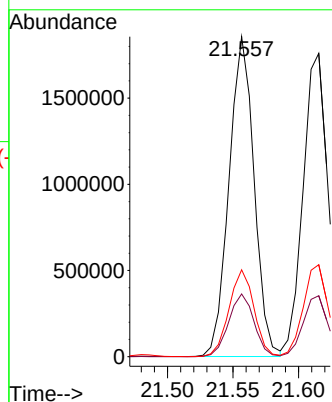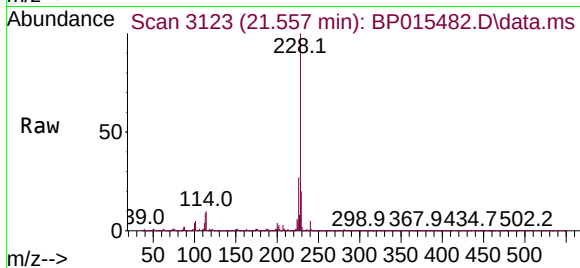

#86

Bis(2-ethylhexyl)phthalate

Concen: 38.479 ng/ul

RT: 21.451 min Scan# 3105

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52




Tgt Ion:149 Resp: 1691840


Ion Ratio Lower Upper

149 100

167 26.9 21.8 32.8

279 4.2 3.7 5.5



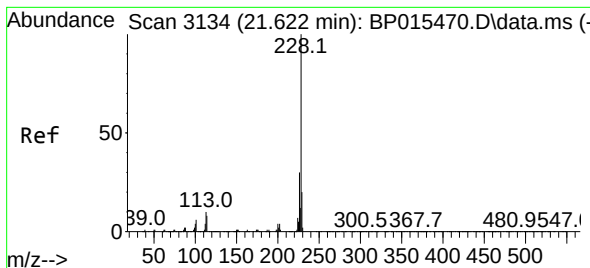

#87

Chrysene

Concen: 35.063 ng/ul

RT: 21.615 min Scan# 31

Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:228 Resp: 2311845

Ion Ratio Lower Upper

228 100

226 30.4 23.9 35.9

229 20.1 15.1 22.7

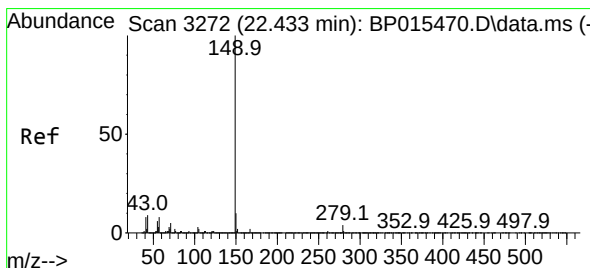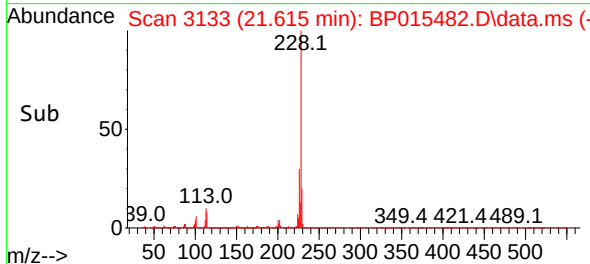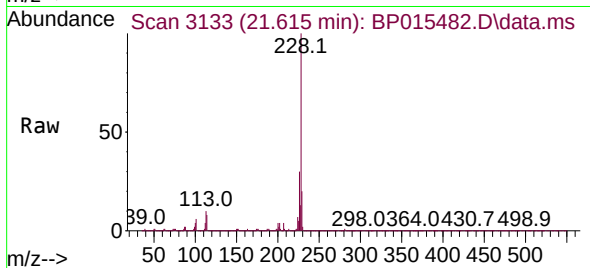

#89

Di-n-octyl phthalate

Concen: 40.866 ng/ul




RT: 22.421 min Scan# 3270


Delta R.T. -0.000 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Tgt Ion:149 Resp: 2959037


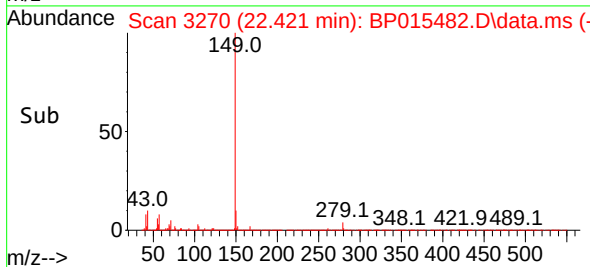

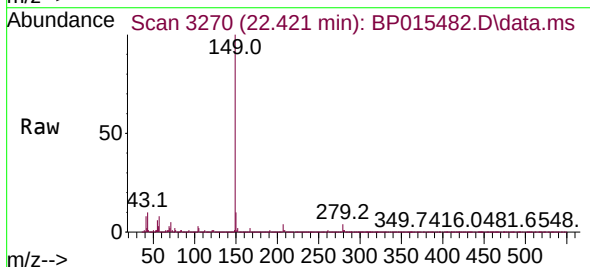




#90
Benzo(b)fluoranthene
Concen: 36.059 ng/ul
RT: 23.339 min Scan# 34
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:252 Resp: 2564401
Ion Ratio Lower Upper
252 100
253 22.0 17.4 26.2
125 9.3 7.3 10.9



#91
Benzo(k)fluoranthene
Concen: 35.875 ng/ul
RT: 23.386 min Scan# 3434
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:252 Resp: 2466253
Ion Ratio Lower Upper
252 100
253 21.9 17.7 26.5
125 9.5 7.3 10.9









#93
Benzo(a)pyrene
Concen: 35.034 ng/ul
RT: 24.009 min Scan# 31
Delta R.T. -0.000 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52




Instrument :
BNA_P
ClientSampleId :
SLCS305


Tgt Ion:252 Resp: 2172216
Ion Ratio Lower Upper
252 100
253 21.8 17.8 26.6
125 10.3 8.1 12.1

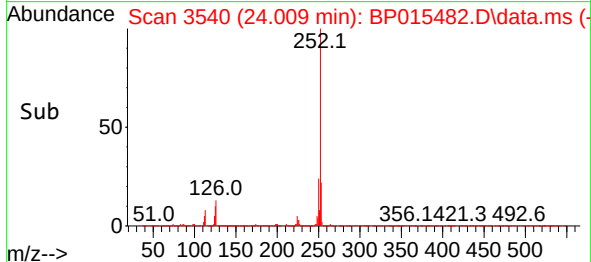

#94
Indeno(1,2,3-cd)pyrene
Concen: 32.374 ng/ul
RT: 26.815 min Scan# 4017
Delta R.T. -0.012 min
Lab File: BP015482.D
Acq: 12 Jun 2023 20:52

Tgt Ion:276 Resp: 2597799
Ion Ratio Lower Upper
276 100
138 21.8 17.3 25.9
277 24.2 20.2 30.2

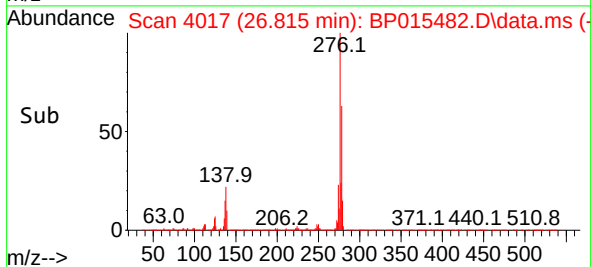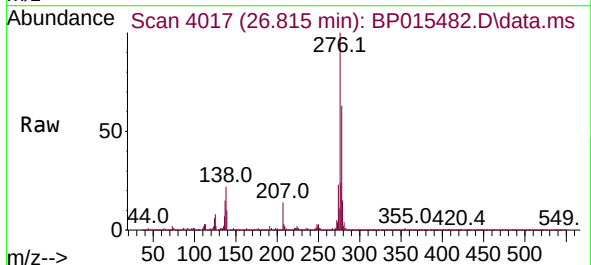



#95

Dibenzo(a,h)anthracene

Concen: 32.632 ng/ul

RT: 26.833 min Scan# 4158

Delta R.T. -0.006 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Instrument :

BNA_P

ClientSampleId :

SLCS305





Tgt Ion:278 Resp: 2133255

Ion Ratio Lower Upper

278 100

139 15.0 11.4 17.0

279 23.7 18.7 28.1

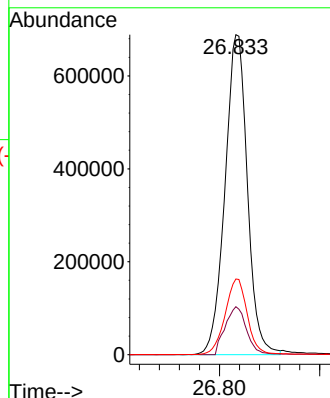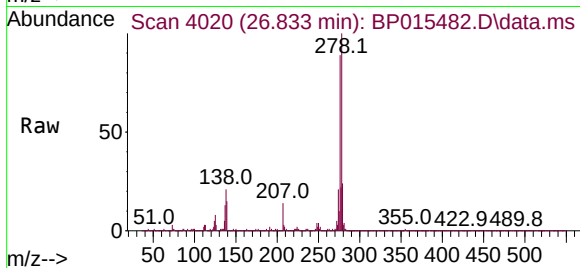

#96

Benzo(g,h,i)perylene

Concen: 31.671 ng/ul

RT: 27.644 min Scan# 4158

Delta R.T. -0.012 min

Lab File: BP015482.D

Acq: 12 Jun 2023 20:52

Tgt Ion:276 Resp: 2094327

Ion Ratio Lower Upper

276 100

138 20.4 15.6 23.4

277 23.3 19.0 28.6

