

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061323\
 Data File : BP015489.D
 Acq On : 13 Jun 2023 11:03
 Operator : MA/JU
 Sample : 03078-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQX2

Quant Time: Jun 14 00:12:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	160587	20.000	ng/ul	0.00
20) Naphthalene-d8	10.916	136	753122	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.734	164	539417	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.492	188	1243166	20.000	ng/ul	0.00
79) Chrysene-d12	21.569	240	1211454	20.000	ng/ul	0.00
88) Perylene-d12	24.121	264	1271734	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	11868	2.737	ng/uL	0.00
4) Pyridine-d5	3.840	84	536	0.048	ng/ul	0.00
7) Phenol-d5	7.246	99	210179	14.207	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.410	67	146679	16.601	ng/ul	0.00
11) 2-Chlorophenol-d4	7.616	132	170904	15.933	ng/ul	0.00
15) 4-Methylphenol-d8	8.804	113	151513	12.479	ng/ul	0.00
21) Nitrobenzene-d5	9.269	128	90877	15.370	ng/ul	0.00
24) 2-Nitrophenol-d4	9.999	143	101133	14.978	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	175480	14.247	ng/ul	0.00
31) 4-Chloroaniline-d4	11.069	131	140640	7.955	ng/ul	0.00
46) Dimethylphthalate-d6	14.139	166	701393	16.489	ng/ul	0.00
49) Acenaphthylene-d8	14.428	160	752378	16.176	ng/ul	0.00
54) 4-Nitrophenol-d4	14.957	143	52615	6.907	ng/ul	0.02
60) Fluorene-d10	15.728	176	602320	16.792	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	76681	9.737	ng/ul	0.00
73) Anthracene-d10	17.592	188	969515	17.141	ng/ul	0.00
81) Pyrene-d10	19.810	212	1216977	18.769	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	1091106	17.099	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.928	105	61991	3.199	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061323\
Data File : BP015489.D
Acq On : 13 Jun 2023 11:03
Operator : MA/JU
Sample : 03078-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQX2

Quant Time: Jun 14 00:12:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 09 23:33:38 2023
Response via : Initial Calibration

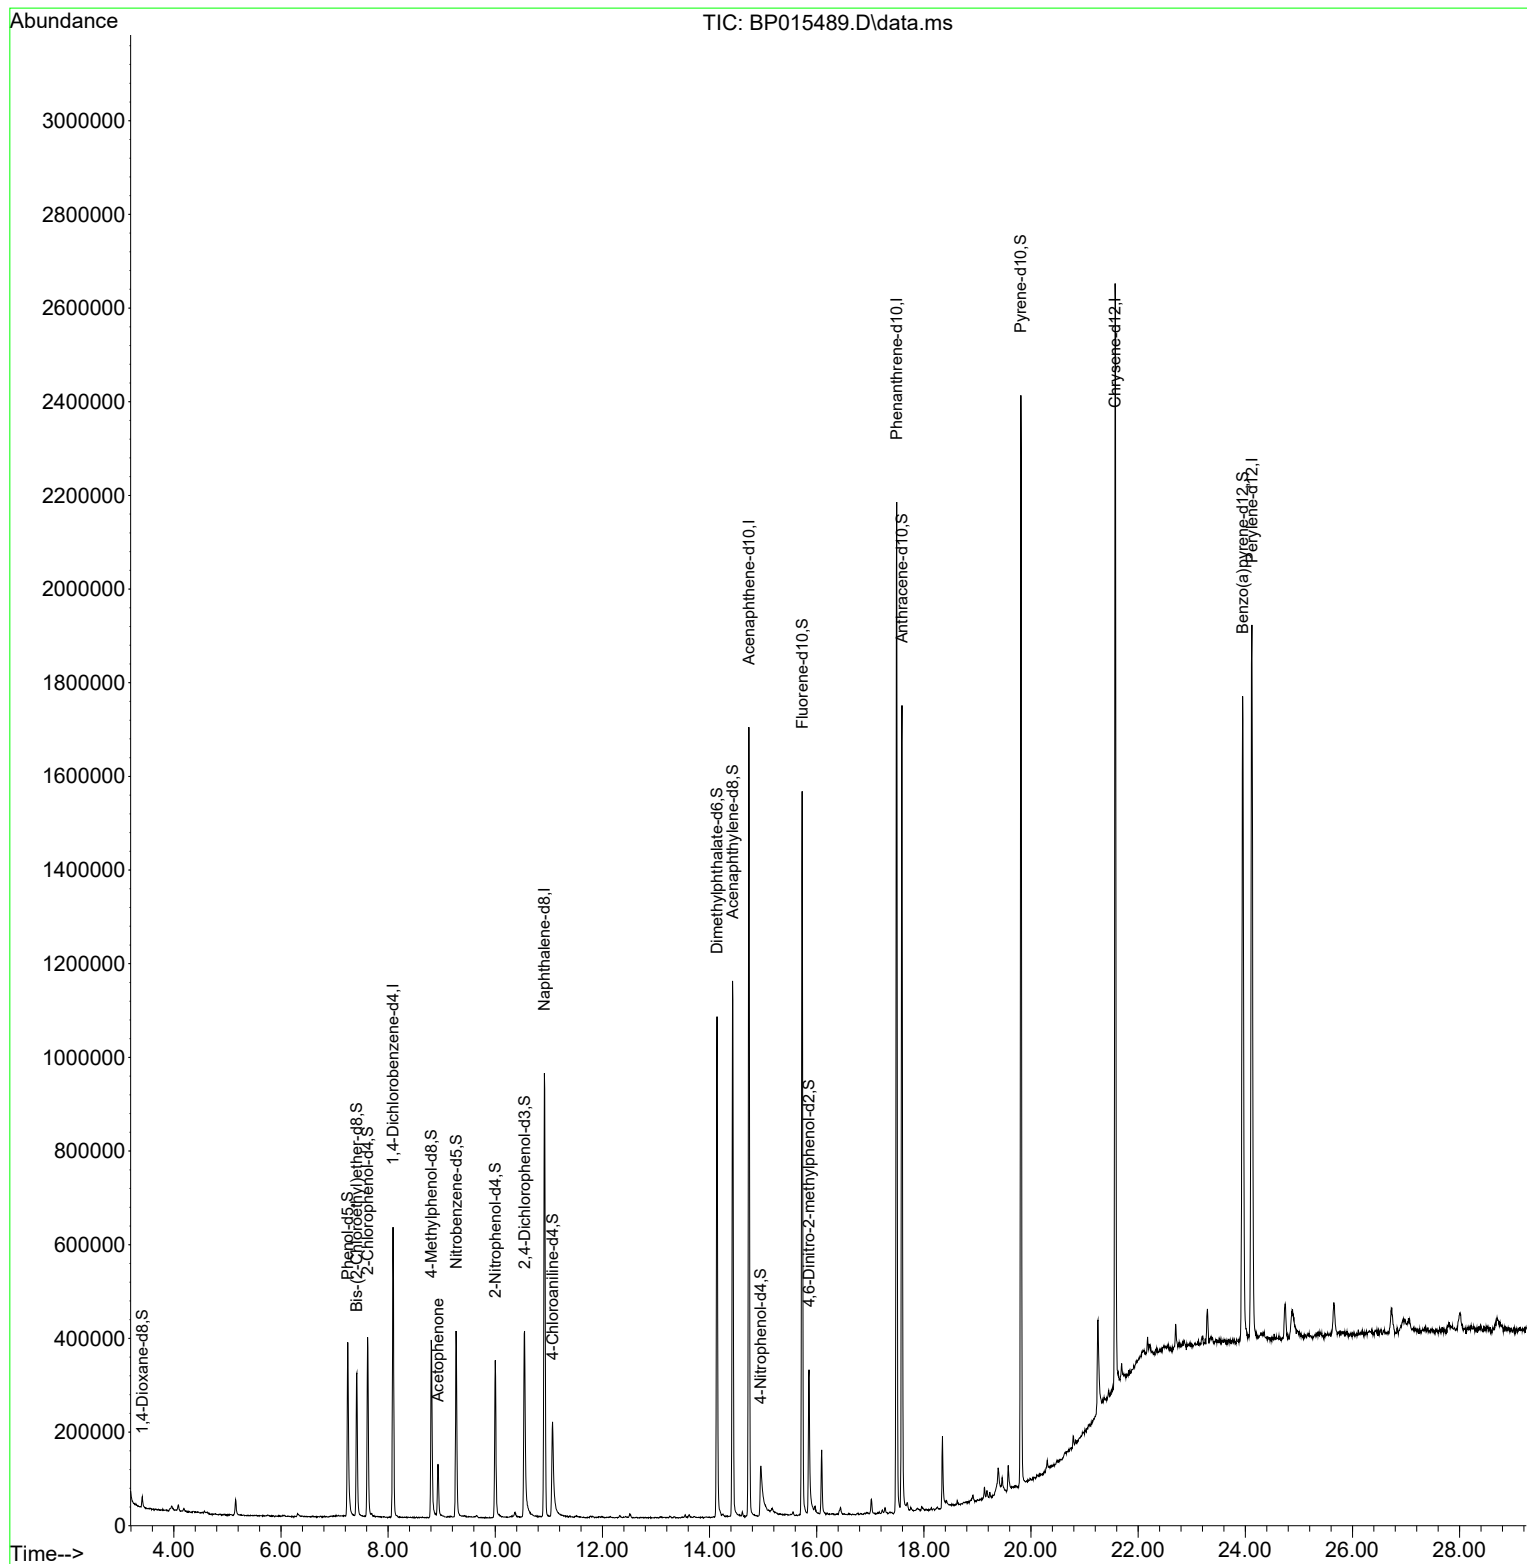

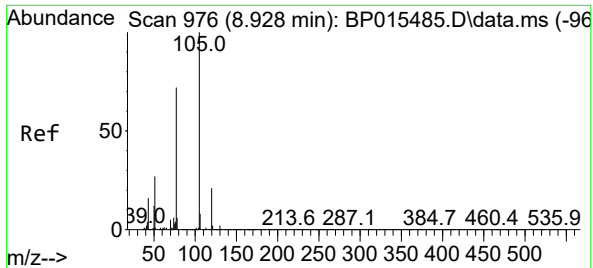

#16
 Acetophenone
 Concen: 3.199 ng/ul
 RT: 8.928 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BP015489.D
 Acq: 13 Jun 2023 11:03

Instrument :
 BNA_P
 ClientSampleId :
 ESQX2

Tgt Ion:	105	Resp:	61991
Ion Ratio	Lower	Upper	
105	100		
77	78.1	64.9	97.3
51	29.8	23.5	35.3

