

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061323\  
 Data File : BP015491.D  
 Acq On : 13 Jun 2023 12:11  
 Operator : MA/JU  
 Sample : 03078-08  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 ESQX6

Quant Time: Jun 14 00:13:11 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Jun 09 23:33:38 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.093  | 152  | 121905   | 20.000 | ng/ul | 0.00     |
| 20) Naphthalene-d8            | 10.922 | 136  | 571150   | 20.000 | ng/ul | 0.00     |
| 38) Acenaphthene-d10          | 14.734 | 164  | 407306   | 20.000 | ng/ul | 0.00     |
| 64) Phenanthrene-d10          | 17.492 | 188  | 965911   | 20.000 | ng/ul | 0.00     |
| 79) Chrysene-d12              | 21.574 | 240  | 955884   | 20.000 | ng/ul | 0.00     |
| 88) Perylene-d12              | 24.121 | 264  | 1028384  | 20.000 | ng/ul | 0.00     |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 3.405  | 96   | 9177     | 2.788  | ng/uL | 0.00     |
| 4) Pyridine-d5                | 3.858  | 84   | 448      | 0.052  | ng/ul | 0.01     |
| 7) Phenol-d5                  | 7.246  | 99   | 159652   | 14.216 | ng/ul | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.416  | 67   | 112422   | 16.761 | ng/ul | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.616  | 132  | 134214   | 16.483 | ng/ul | 0.00     |
| 15) 4-Methylphenol-d8         | 8.805  | 113  | 112014   | 12.153 | ng/ul | 0.00     |
| 21) Nitrobenzene-d5           | 9.269  | 128  | 70023    | 15.616 | ng/ul | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.999  | 143  | 79156    | 15.458 | ng/ul | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.546 | 165  | 138135   | 14.788 | ng/ul | 0.00     |
| 31) 4-Chloroaniline-d4        | 11.069 | 131  | 126374   | 9.425  | ng/ul | 0.00     |
| 46) Dimethylphthalate-d6      | 14.140 | 166  | 542890   | 16.903 | ng/ul | 0.00     |
| 49) Acenaphthylene-d8         | 14.428 | 160  | 590718   | 16.820 | ng/ul | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.957 | 143  | 37252    | 6.477  | ng/ul | 0.02     |
| 60) Fluorene-d10              | 15.728 | 176  | 473011   | 17.464 | ng/ul | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.857 | 200  | 61084    | 9.982  | ng/ul | 0.00     |
| 73) Anthracene-d10            | 17.586 | 188  | 771609   | 17.557 | ng/ul | 0.00     |
| 81) Pyrene-d10                | 19.810 | 212  | 1003640  | 19.618 | ng/ul | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.951 | 264  | 930584   | 18.035 | ng/ul | 0.00     |
| Target Compounds              |        |      |          |        |       |          |
| 16) Acetophenone              | 8.934  | 105  | 46091    | 3.133  | ng/ul | 99       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061323\  
Data File : BP015491.D  
Acq On : 13 Jun 2023 12:11  
Operator : MA/JU  
Sample : 03078-08  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
ESQX6


Quant Time: Jun 14 00:13:11 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Jun 09 23:33:38 2023  
Response via : Initial Calibration

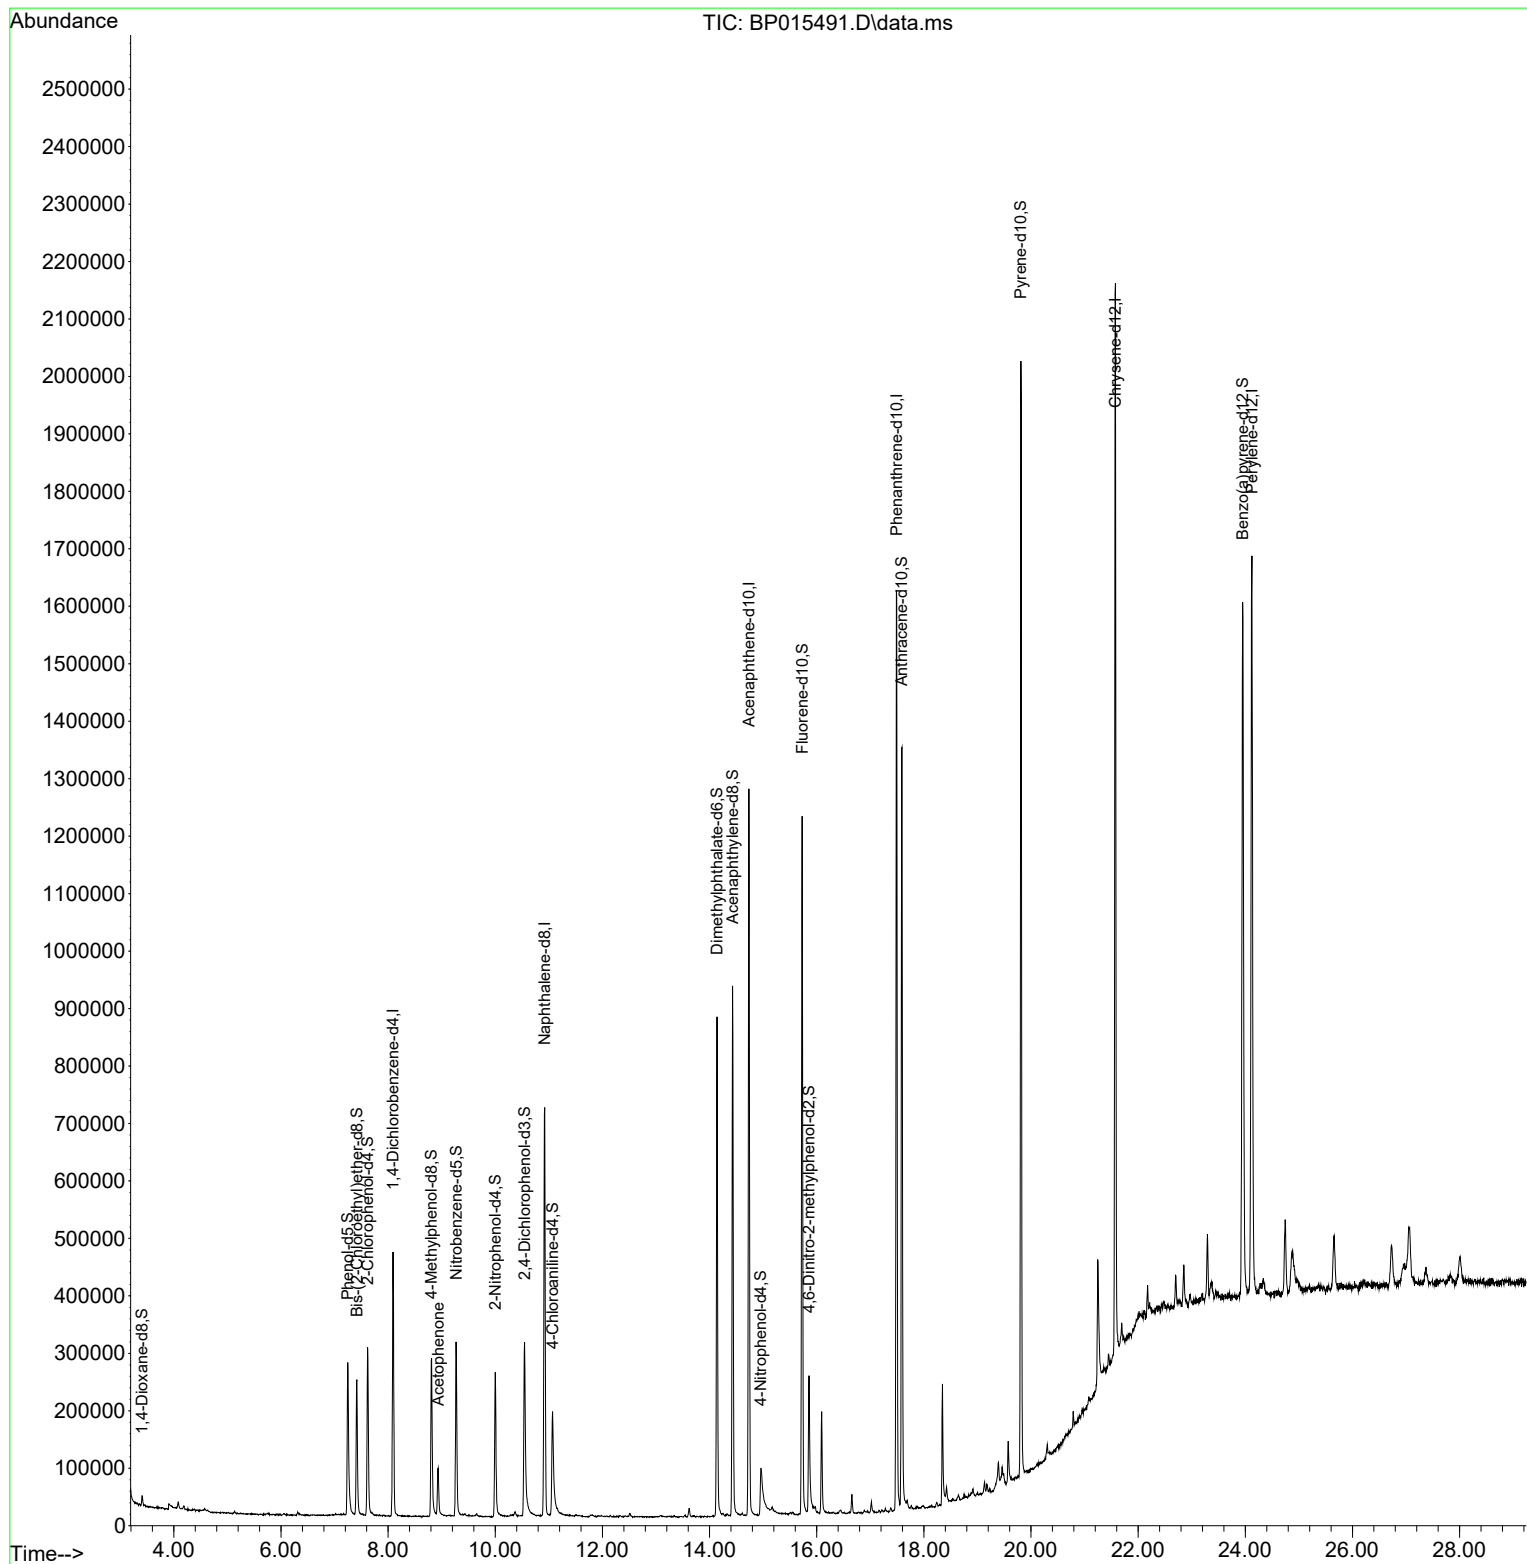

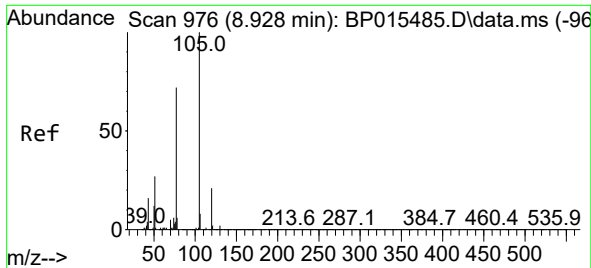

#16  
 Acetophenone  
 Concen: 3.133 ng/ul  
 RT: 8.934 min Scan# 91  
 Delta R.T. 0.006 min  
 Lab File: BP015491.D  
 Acq: 13 Jun 2023 12:11

Instrument :  
 BNA\_P  
 ClientSampleId :  
 ESQX6

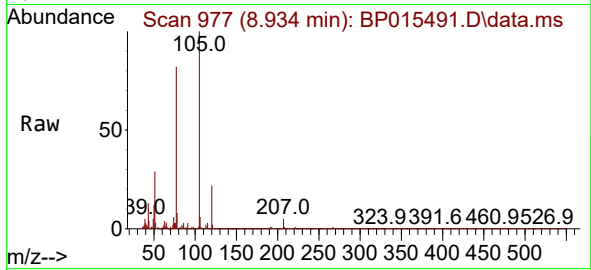

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 105   | Resp: | 46091 |
| Ion      | Ratio | Lower | Upper |
| 105      | 100   |       |       |
| 77       | 81.7  | 64.9  | 97.3  |
| 51       | 29.3  | 23.5  | 35.3  |

