

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061323\
 Data File : BP015487.D
 Acq On : 13 Jun 2023 09:55
 Operator : MA/JU
 Sample : 03078-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	35	38	42	rVB3	15892	19038	0.55%	0.064%
2	3.958	127	131	139	rVB	27956	40717	1.18%	0.138%
3	4.087	149	153	157	rVB2	15838	23983	0.70%	0.081%
4	4.187	166	170	177	rVB3	10228	17763	0.52%	0.060%
5	4.369	196	201	203	rVB5	5106	7701	0.22%	0.026%
6	4.722	257	261	262	rBV3	3600	5157	0.15%	0.017%
7	4.764	266	268	272	rVB5	4856	6445	0.19%	0.022%
8	4.999	307	308	313	rBV5	2284	3678	0.11%	0.012%
9	5.152	327	334	342	rBV2	24323	45987	1.34%	0.156%
10	5.252	348	351	355	rVB4	5673	8552	0.25%	0.029%
11	5.911	459	463	468	rBV8	1684	3444	0.10%	0.012%
12	6.052	480	487	490	rBV4	10017	17283	0.50%	0.059%
13	6.311	526	531	536	rBV5	6998	14746	0.43%	0.050%
14	6.616	580	583	586	rVB5	3290	4304	0.13%	0.015%
15	7.016	648	651	654	rVB5	2527	3862	0.11%	0.013%
16	7.246	683	690	704	rBV2	219585	492890	14.33%	1.669%
17	7.416	713	719	732	rVB	189731	314436	9.14%	1.065%
18	7.616	746	753	764	rBV	215605	385327	11.21%	1.305%
19	7.699	764	767	770	rVB4	6145	7967	0.23%	0.027%
20	7.910	799	803	807	rVB7	2605	4171	0.12%	0.014%
21	8.093	827	834	847	rBV	624952	1014627	29.51%	3.435%
22	8.575	911	916	920	rVB6	2509	4397	0.13%	0.015%
23	8.810	949	956	970	rBV	146016	292271	8.50%	0.990%
24	8.934	970	977	990	rVV	219651	403667	11.74%	1.367%
25	9.063	993	999	1010	rVV6	10167	27213	0.79%	0.092%
26	9.269	1028	1034	1048	rBV	232463	433259	12.60%	1.467%
27	9.387	1048	1054	1058	rVV5	8011	18119	0.53%	0.061%
28	9.434	1061	1062	1067	rVB5	4034	5372	0.16%	0.018%
29	9.522	1072	1077	1080	rBV7	3440	4641	0.13%	0.016%
30	9.657	1096	1100	1105	rVB8	4210	7536	0.22%	0.026%
31	10.004	1151	1159	1169	rBV	187461	361131	10.50%	1.223%
32	10.199	1186	1192	1196	rBV5	14390	35894	1.04%	0.122%
33	10.363	1215	1220	1236	rVB	32244	76218	2.22%	0.258%
34	10.481	1237	1240	1244	rBV6	3078	4147	0.12%	0.014%
35	10.551	1244	1252	1274	rBV	213894	494363	14.38%	1.674%
36	10.922	1307	1315	1324	rBV	955743	1599988	46.53%	5.417%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061323\
 Data File : BP015487.D
 Acq On : 13 Jun 2023 09:55
 Operator : MA/JU
 Sample : 03078-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	11.081	1335	1342	1352	rBV	49951	128500	3.74%	0.435%
38	11.398	1392	1396	1402	rBV8	5032	7804	0.23%	0.026%
39	11.481	1405	1410	1417	rBV8	10990	25237	0.73%	0.085%
40	11.746	1449	1455	1456	rBV3	9640	12871	0.37%	0.044%
41	11.975	1490	1494	1495	rVV4	4198	4713	0.14%	0.016%
42	11.998	1495	1498	1504	rVB8	2162	4106	0.12%	0.014%
43	12.316	1545	1552	1560	rBV7	11415	23124	0.67%	0.078%
44	12.510	1580	1585	1592	rVB7	5462	9658	0.28%	0.033%
45	13.098	1680	1685	1689	rBV8	2515	3906	0.11%	0.013%
46	13.257	1707	1712	1722	rVV8	6251	13059	0.38%	0.044%
47	13.351	1722	1728	1731	rVB8	2915	5310	0.15%	0.018%
48	13.545	1755	1761	1767	rBV6	9721	18039	0.52%	0.061%
49	13.622	1767	1774	1778	rBV2	12700	22564	0.66%	0.076%
50	14.140	1855	1862	1871	rBV	643273	969099	28.18%	3.281%
51	14.340	1890	1896	1900	rVB7	4508	7888	0.23%	0.027%
52	14.434	1904	1912	1927	rBV	705871	1071580	31.16%	3.628%
53	14.610	1938	1942	1948	rVB2	10605	13643	0.40%	0.046%
54	14.692	1951	1956	1957	rBV5	3153	4030	0.12%	0.014%
55	14.739	1957	1964	1981	rBV	1628743	2439530	70.95%	8.259%
56	14.969	1996	2003	2023	rBV2	53933	228321	6.64%	0.773%
57	15.116	2025	2028	2029	rBV3	6028	6361	0.18%	0.022%
58	15.416	2077	2079	2083	rVB5	2963	4125	0.12%	0.014%
59	15.563	2099	2104	2108	rVB3	10198	15313	0.45%	0.052%
60	15.669	2119	2122	2125	rBV5	3306	4642	0.14%	0.016%
61	15.728	2126	2132	2148	rVV	932824	1428691	41.55%	4.837%
62	15.863	2149	2155	2169	rVV	160150	324582	9.44%	1.099%
63	15.969	2170	2173	2178	rVB5	12312	20943	0.61%	0.071%
64	16.092	2188	2194	2203	rBV	79624	136152	3.96%	0.461%
65	16.310	2228	2231	2238	rVB9	3438	6054	0.18%	0.020%
66	16.445	2247	2254	2263	rBV4	20113	44302	1.29%	0.150%
67	16.951	2334	2340	2344	rVB9	3573	7932	0.23%	0.027%
68	17.022	2345	2352	2359	rBV2	32856	55509	1.61%	0.188%
69	17.228	2383	2387	2390	rBV4	8599	11123	0.32%	0.038%
70	17.275	2390	2395	2400	rVV7	11533	21004	0.61%	0.071%
71	17.363	2407	2410	2415	rBV6	4504	8728	0.25%	0.030%
72	17.492	2424	2432	2443	rBV	2157460	3165134	92.05%	10.716%
73	17.592	2443	2449	2461	rVV	1037165	1505342	43.78%	5.097%
74	17.763	2474	2478	2481	rBV5	6119	8024	0.23%	0.027%
75	17.963	2509	2512	2513	rBV3	10401	10052	0.29%	0.034%
76	18.251	2557	2561	2567	rVB2	9052	13222	0.38%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061323\
 Data File : BP015487.D
 Acq On : 13 Jun 2023 09:55
 Operator : MA/JU
 Sample : 03078-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

77	18.351	2573	2578	2585	rBV	126575	205160	5.97%	0.695%
78	18.628	2622	2625	2628	rVB4	6965	6457	0.19%	0.022%
79	18.916	2670	2674	2683	rVB2	27391	43417	1.26%	0.147%
80	19.133	2707	2711	2715	rBV	65574	80785	2.35%	0.274%
81	19.180	2716	2719	2724	rVB2	31048	43845	1.28%	0.148%
82	19.233	2724	2728	2731	rBV4	16765	23320	0.68%	0.079%
83	19.386	2748	2754	2764	rVB6	71008	209866	6.10%	0.711%
84	19.580	2783	2787	2794	rBV3	50112	82303	2.39%	0.279%
85	19.816	2820	2827	2836	rBV	1539211	2071184	60.24%	7.012%
86	21.251	3067	3071	3081	rBV4	100047	196524	5.72%	0.665%
87	21.574	3121	3126	3138	rBV	2523116	3438417	100.00%	11.641%
88	23.957	3525	3531	3545	rVB2	814421	1779660	51.76%	6.025%
89	24.121	3553	3559	3577	rVB	1459537	3334938	96.99%	11.291%




Sum of corrected areas: 29536387

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061323\
Data File : BP015487.D
Acq On : 13 Jun 2023 09:55
Operator : MA/JU
Sample : 03078-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

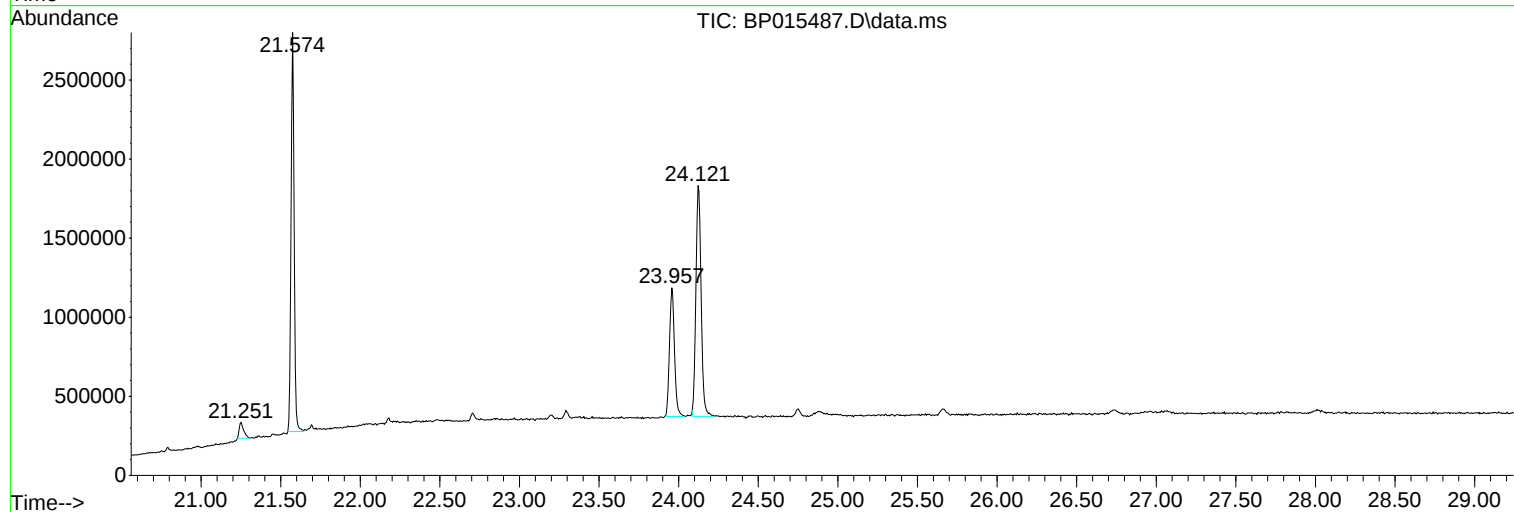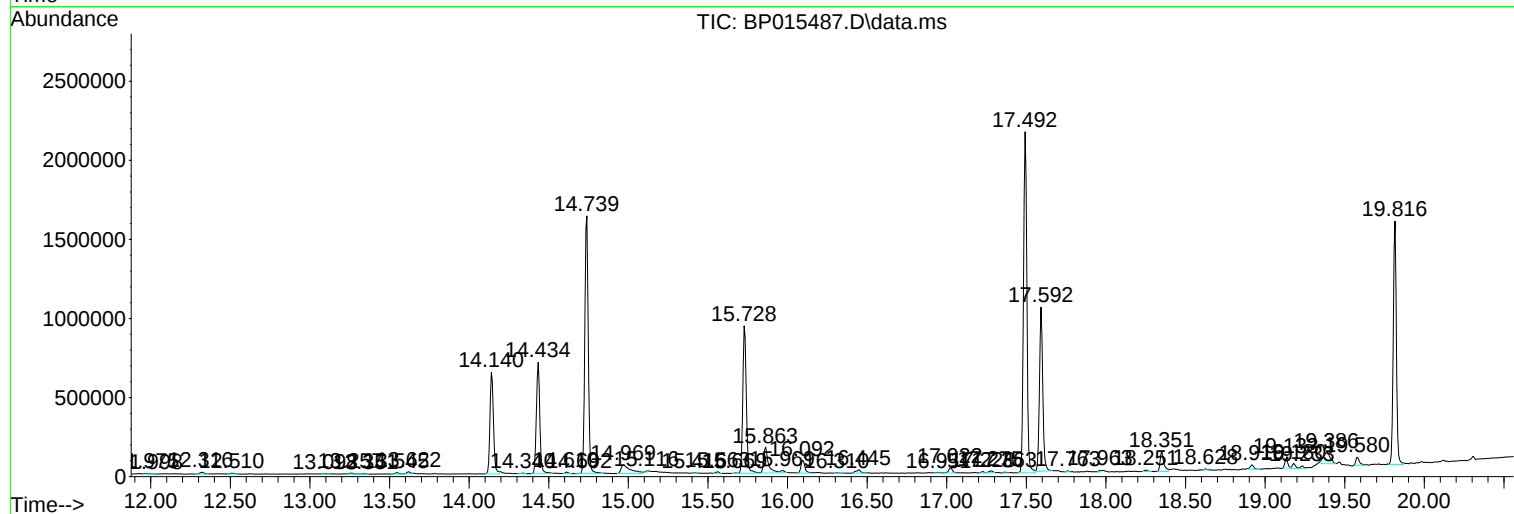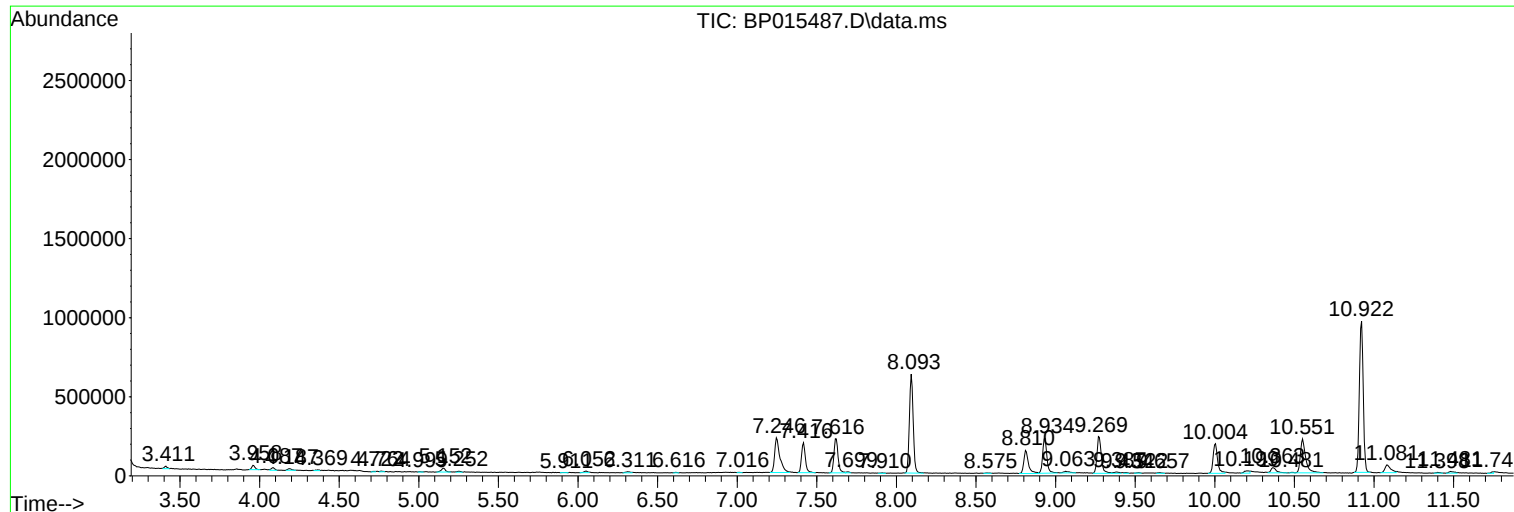

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061323\
Data File : BP015487.D
Acq On : 13 Jun 2023 09:55
Operator : MA/JU
Sample : 03078-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061323\
Data File : BP015487.D
Acq On : 13 Jun 2023 09:55
Operator : MA/JU
Sample : 03078-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------