




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015513.D
Acq On : 14 Jun 2023 12:40
Operator : MA/JU
Sample : 03098-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ7

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:08:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 09 23:33:38 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :mohammad ahmed 06/16/2023

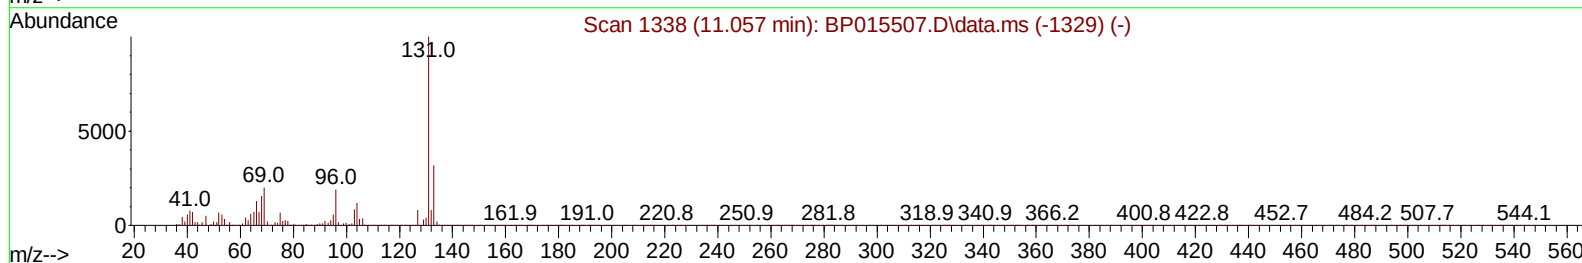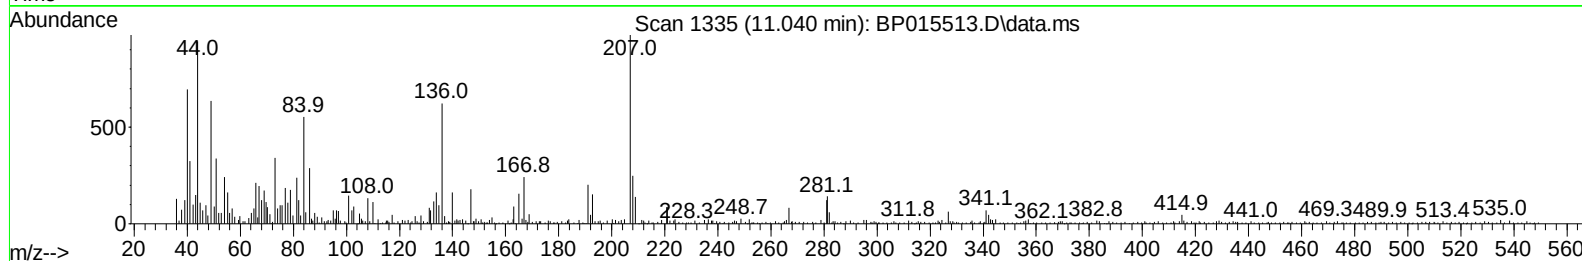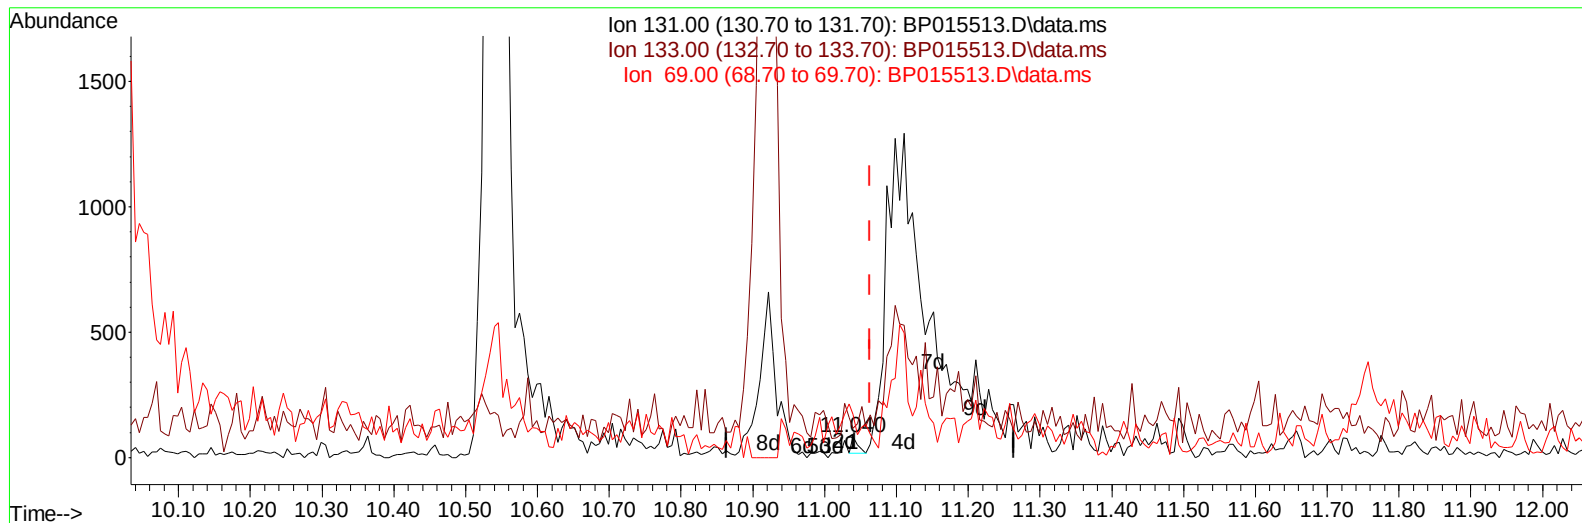

TIC: BP015513.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.040min (-0.024) 0.00 ng/u1

response 42

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	139.76#
69.00	18.30	208.43#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015513.D
 Acq On : 14 Jun 2023 12:40
 Operator : MA/JU
 Sample : 03098-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ7

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:08:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

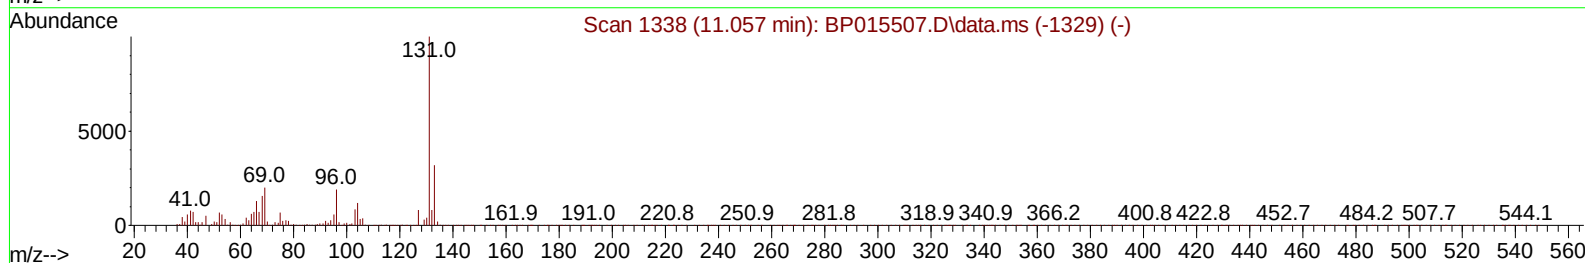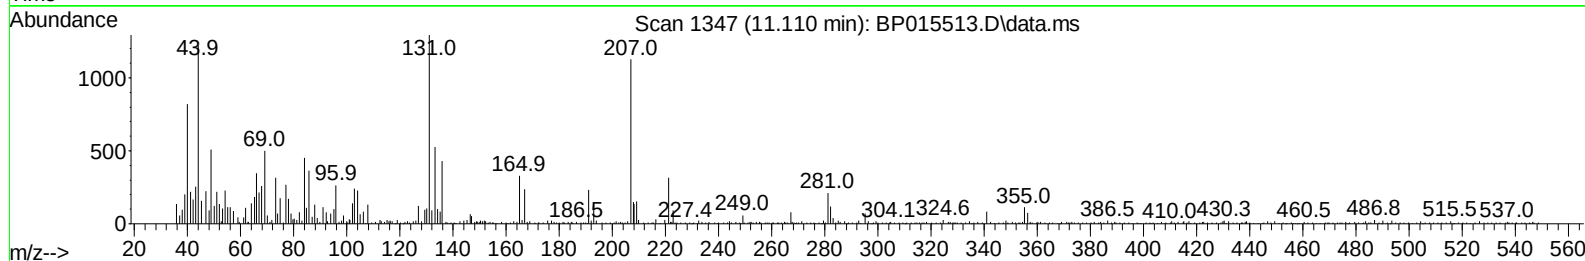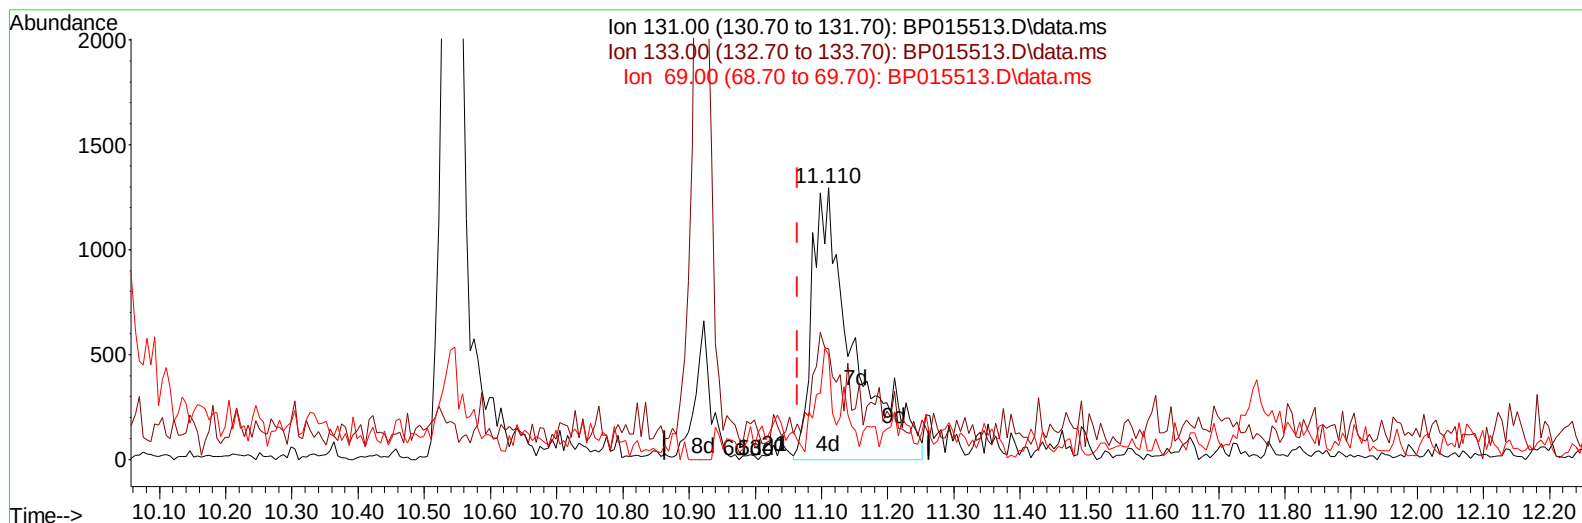

TIC: BP015513.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.110min (+ 0.047) 0.37 ng/ul m

response 5560

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	40.80#
69.00	18.30	38.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015513.D
 Acq On : 14 Jun 2023 12:40
 Operator : MA/JU
 Sample : 03098-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ7

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:08:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

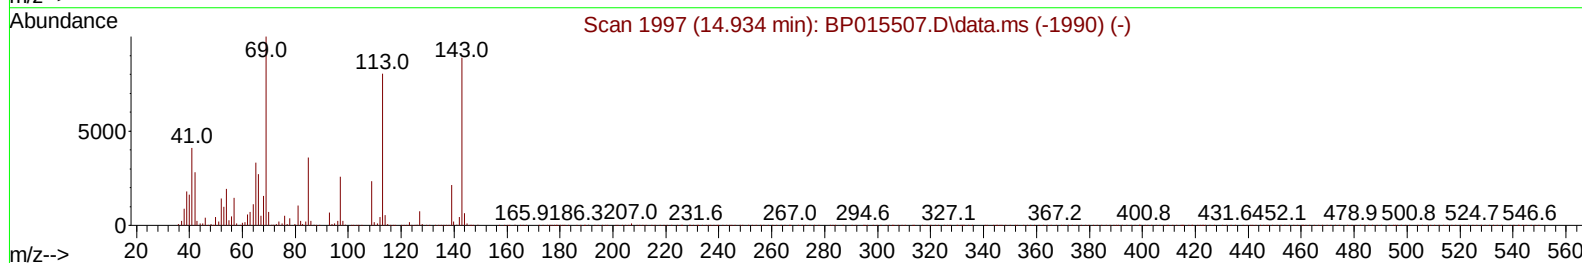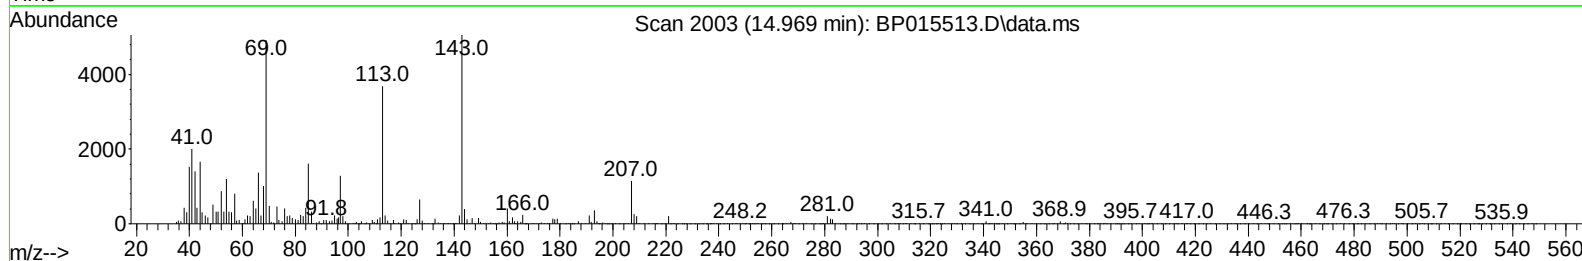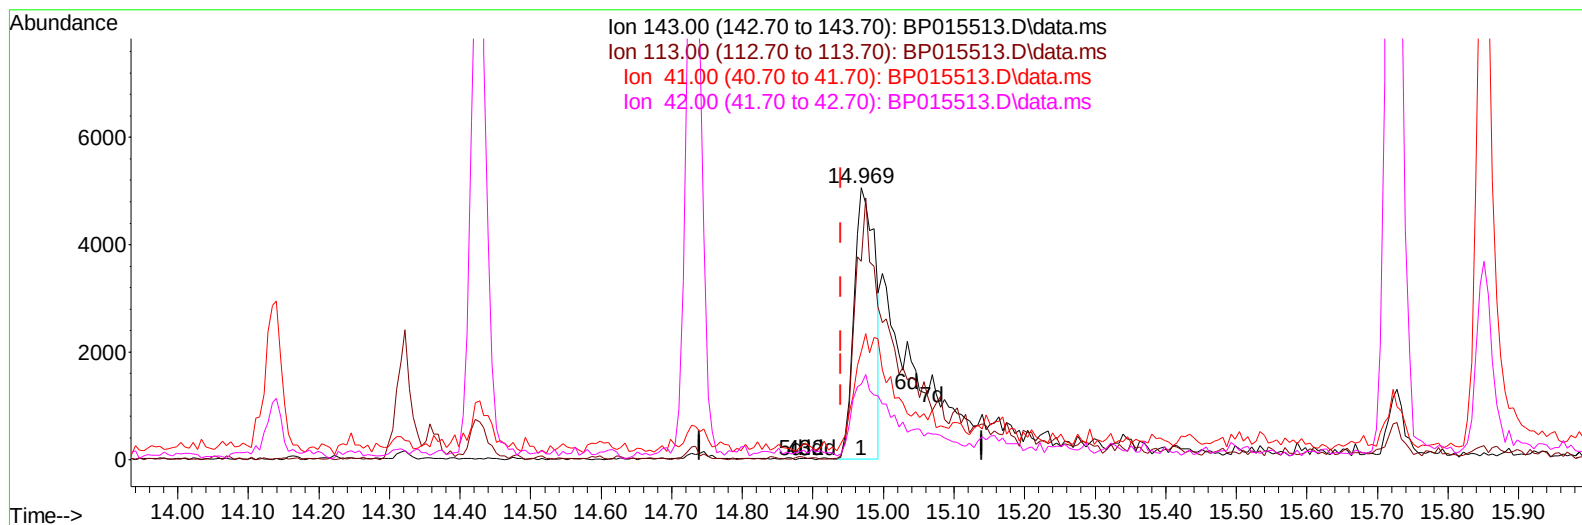

TIC: BP015513.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.969min (+ 0.029) 1.63 ng/ul

response 10498

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	72.97
41.00	42.20	39.72
42.00	29.40	27.76




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015513.D
 Acq On : 14 Jun 2023 12:40
 Operator : MA/JU
 Sample : 03098-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ7

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:25:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

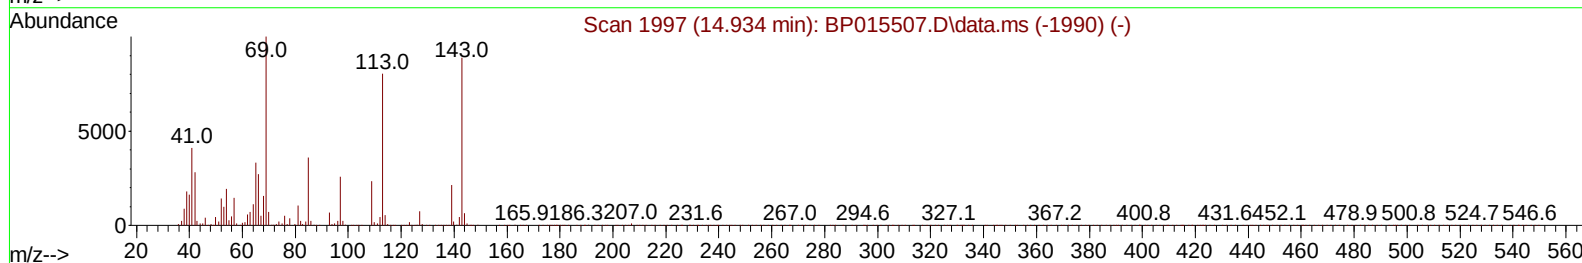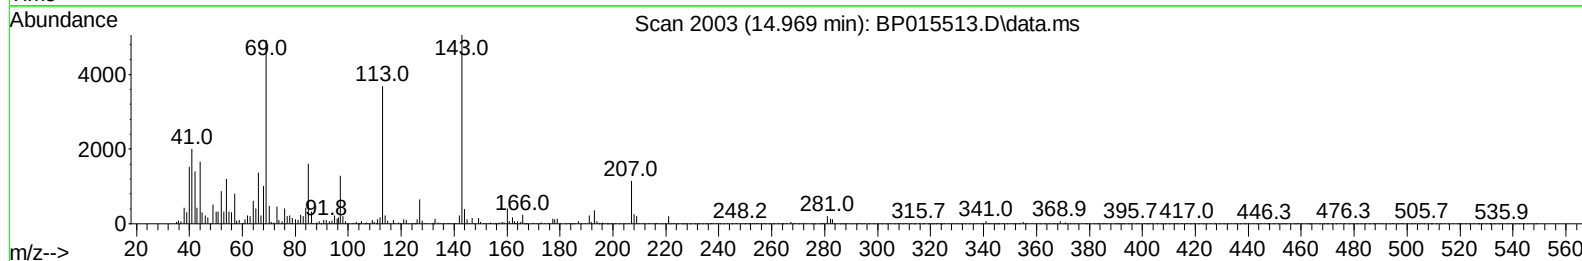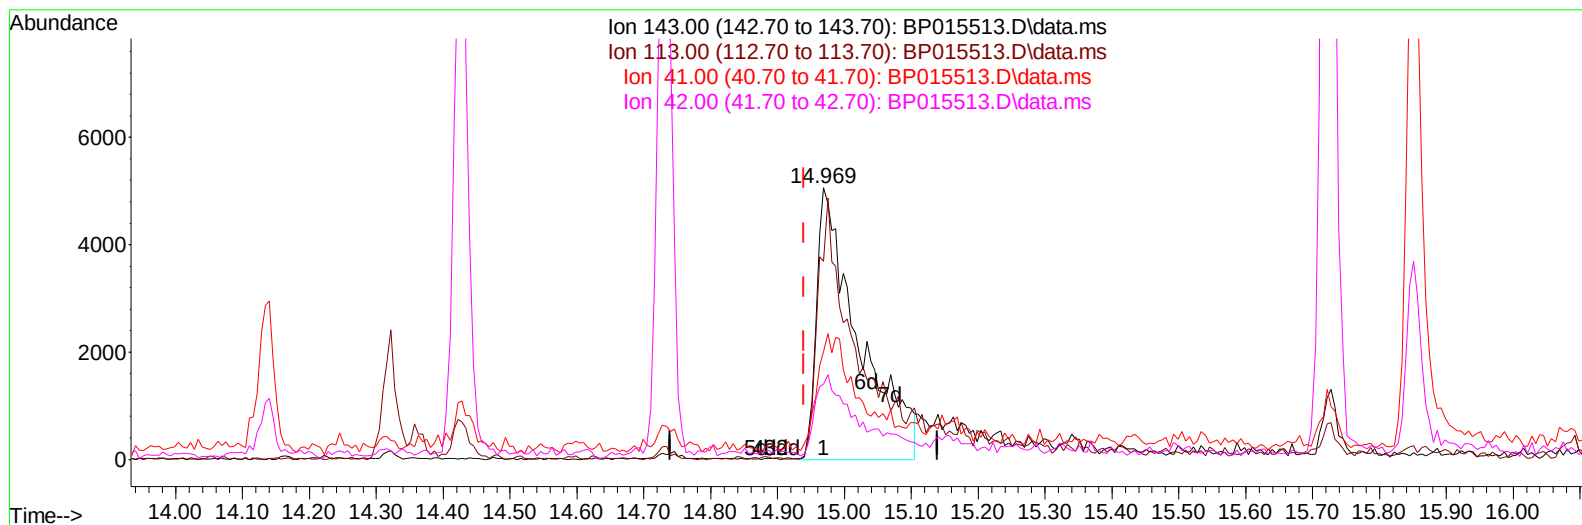

TIC: BP015513.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.969min (+ 0.029) 3.41 ng/ul m

response 21896

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	72.97
41.00	42.20	39.72
42.00	29.40	27.76

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015513.D
 Acq On : 14 Jun 2023 12:40
 Operator : MA/JU
 Sample : 03098-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 14 23:26:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	136720	20.000	ng/ul	0.00
20) Naphthalene-d8	10.916	136	645021	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.734	164	454702	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.486	188	1078476	20.000	ng/ul	0.00
79) Chrysene-d12	21.569	240	1083591	20.000	ng/ul	0.00
88) Perylene-d12	24.116	264	1186354	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	15752	4.266	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.246	99	72320	5.742	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.410	67	210479	27.981	ng/ul	0.00
11) 2-Chlorophenol-d4	7.616	132	197612	21.639	ng/ul	0.00
15) 4-Methylphenol-d8	8.805	113	138754	13.423	ng/ul	0.00
21) Nitrobenzene-d5	9.269	128	135780	26.813	ng/ul	0.00
24) 2-Nitrophenol-d4	9.993	143	148496	25.678	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.540	165	240134	22.763	ng/ul	0.00
31) 4-Chloroaniline-d4	11.110	131	5560m	0.367	ng/ul	0.05
46) Dimethylphthalate-d6	14.140	166	1075368	29.991	ng/ul	0.00
49) Acenaphthylene-d8	14.428	160	1096525	27.968	ng/ul	0.00
54) 4-Nitrophenol-d4	14.969	143	21896m	3.410	ng/ul	0.03
60) Fluorene-d10	15.722	176	904650	29.919	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.851	200	179286	26.241	ng/ul	0.00
73) Anthracene-d10	17.586	188	1545058	31.487	ng/ul	0.00
81) Pyrene-d10	19.810	212	2005094	34.573	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	1918943	32.237	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015513.D
Acq On : 14 Jun 2023 12:40
Operator : MA/JU
Sample : 03098-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 14 23:26:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 09 23:33:38 2023
Response via : Initial Calibration

