




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015517.D
Acq On : 14 Jun 2023 14:55
Operator : MA/JU
Sample : 03098-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ0

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:09:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 09 23:33:38 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :mohammad ahmed 06/16/2023

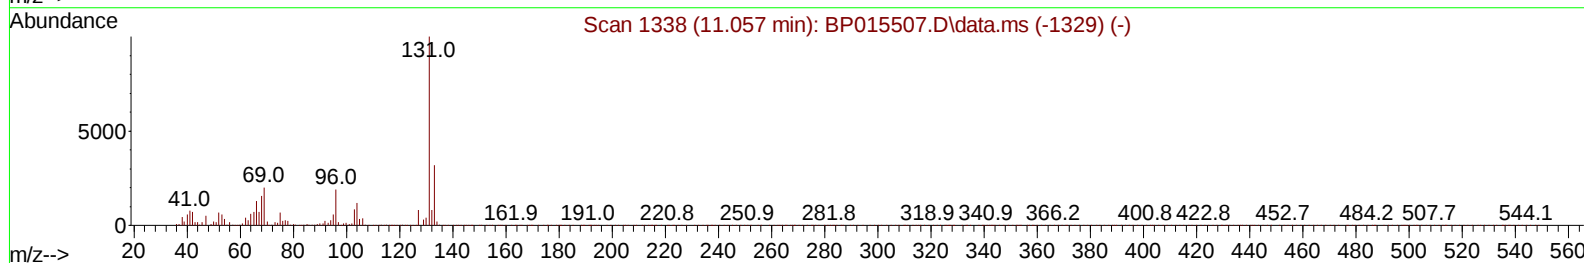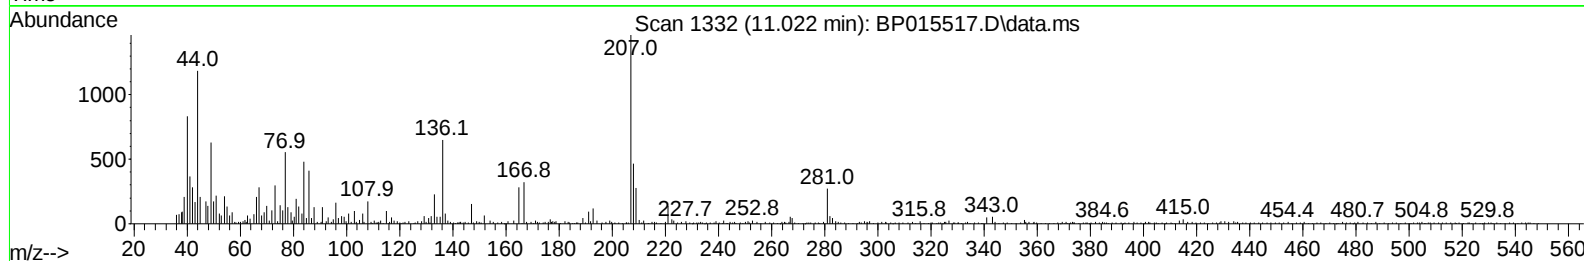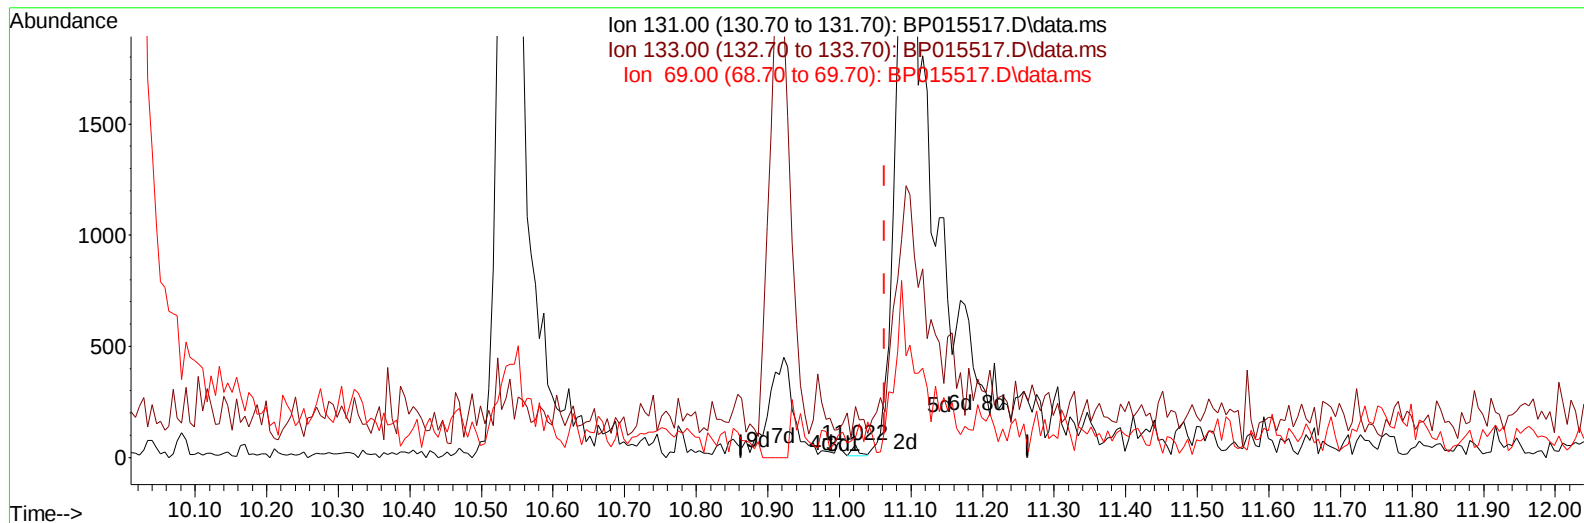

TIC: BP015517.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.022min (-0.041) 0.00 ng/u1

response 34

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	396.55#
69.00	18.30	156.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015517.D
 Acq On : 14 Jun 2023 14:55
 Operator : MA/JU
 Sample : 03098-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ0

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:09:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

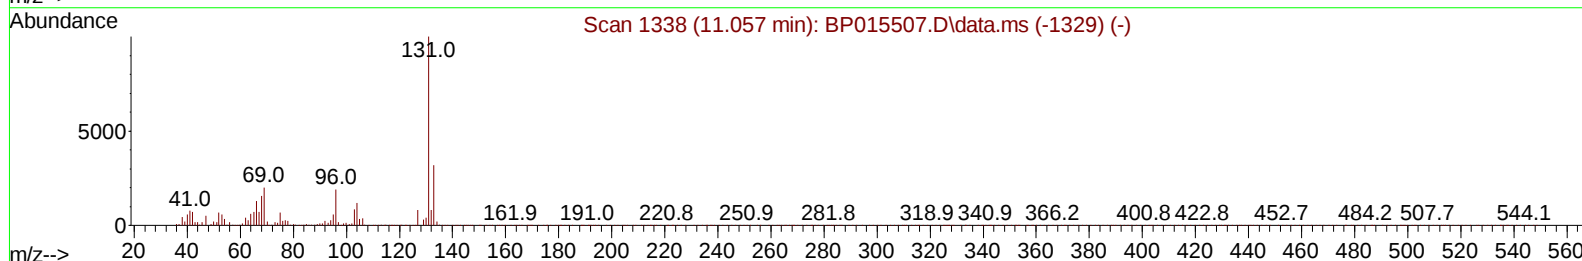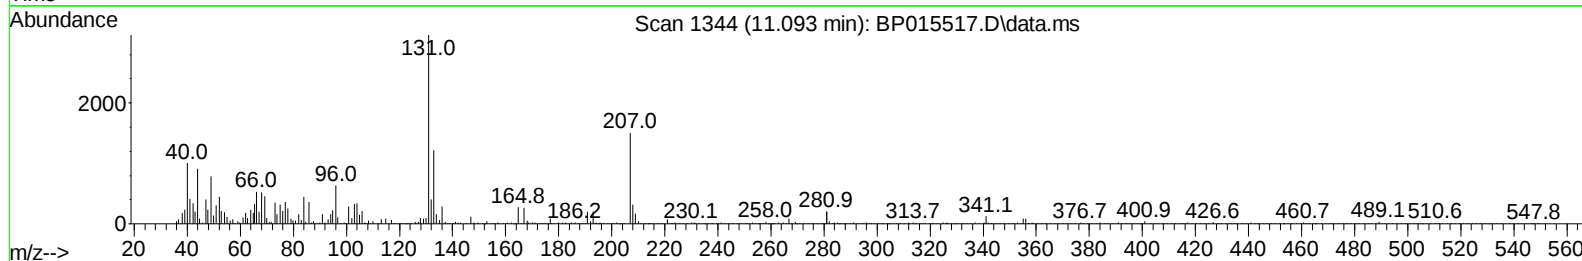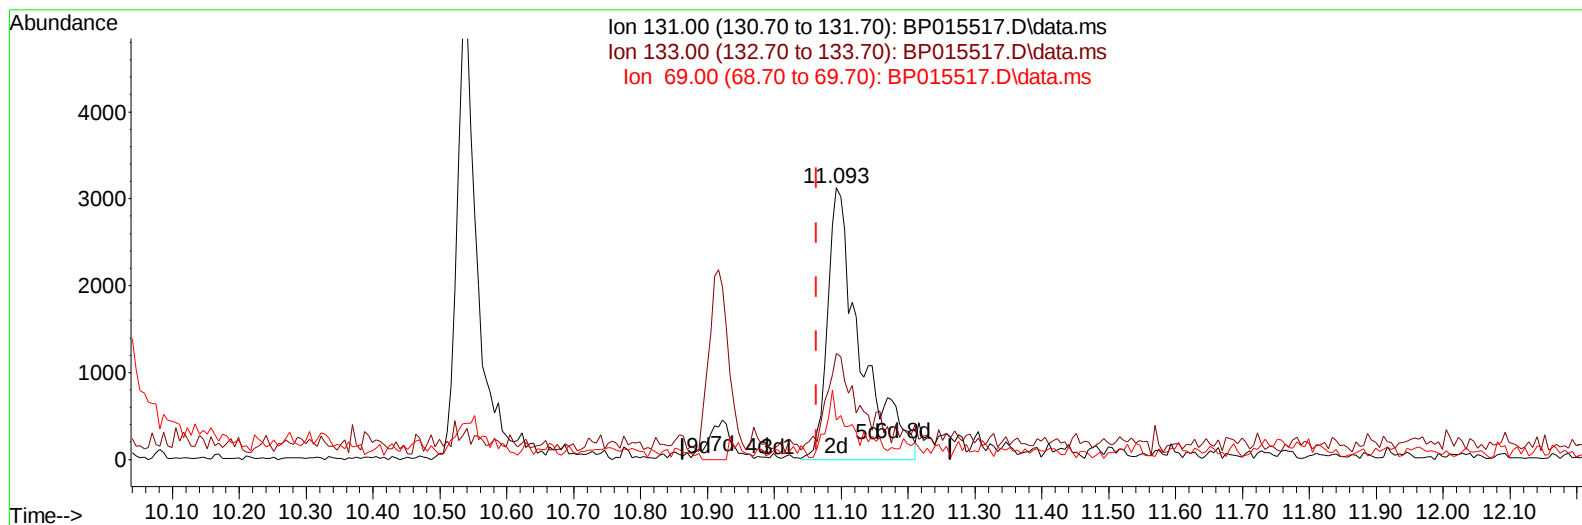

TIC: BP015517.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.093min (+ 0.029) 0.87 ng/ul m

response 10619

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	39.07#
69.00	18.30	14.62#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015517.D
 Acq On : 14 Jun 2023 14:55
 Operator : MA/JU
 Sample : 03098-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ0

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:09:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

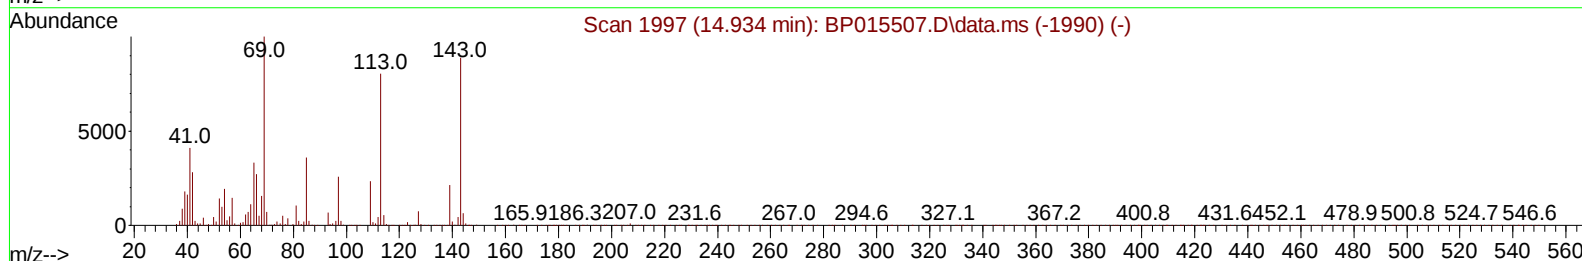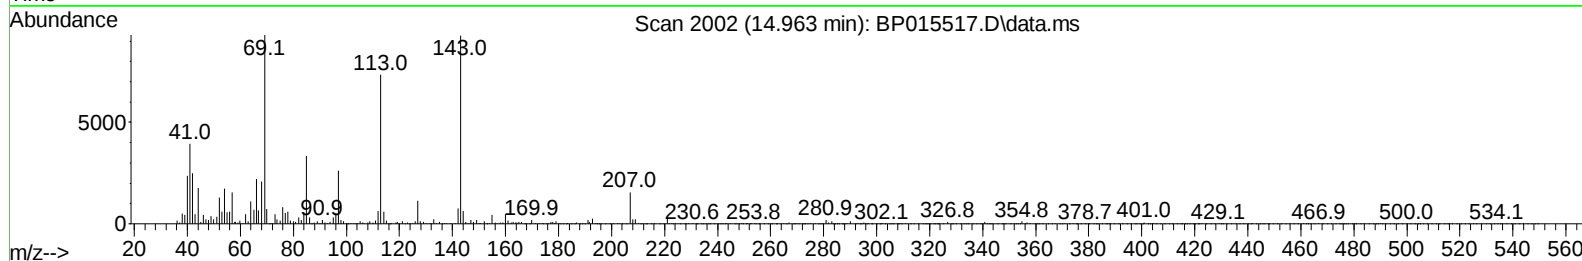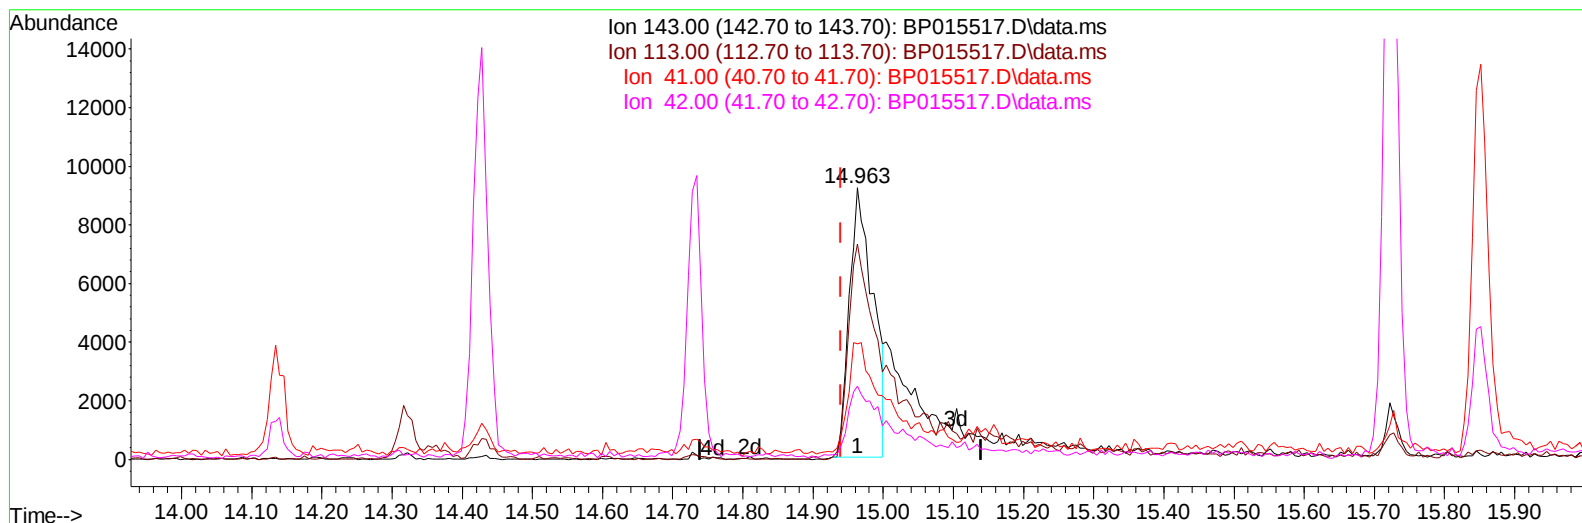

TIC: BP015517.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.963min (+ 0.024) 4.07 ng/u1

response 21564

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	79.40
41.00	42.20	42.66
42.00	29.40	26.93




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015517.D
 Acq On : 14 Jun 2023 14:55
 Operator : MA/JU
 Sample : 03098-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ0

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:09:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

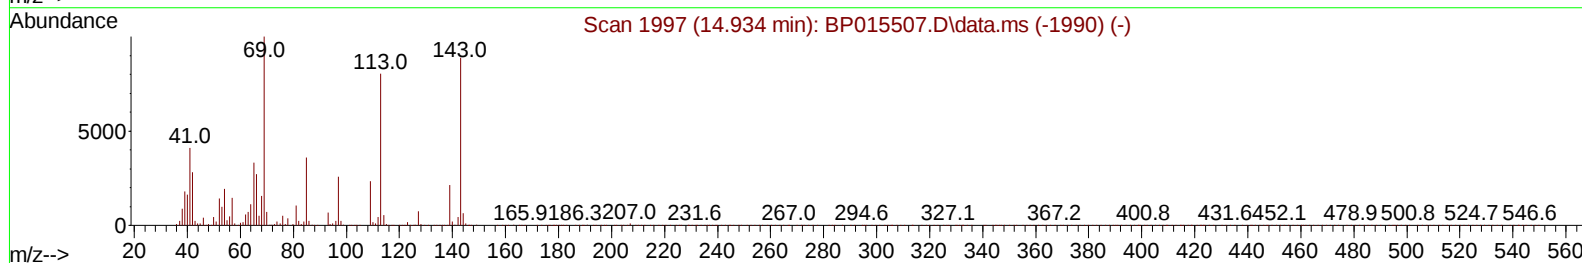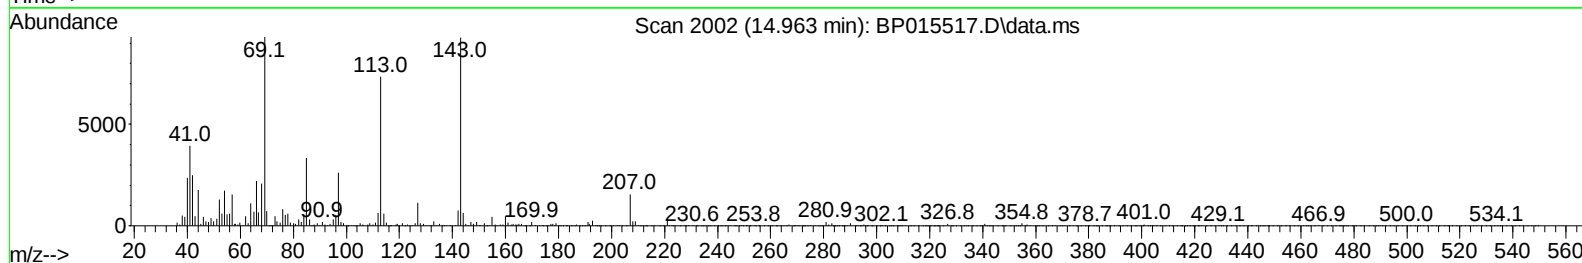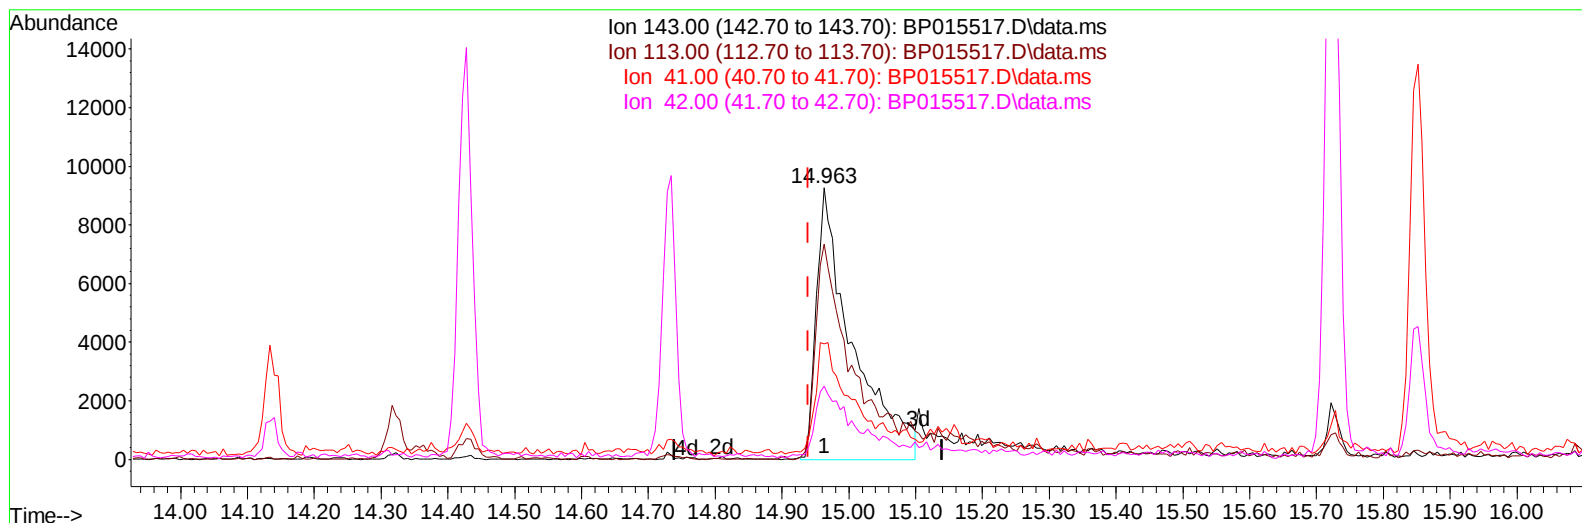

TIC: BP015517.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.963min (+ 0.024) 6.51 ng/ul m

response 34527

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	79.40
41.00	42.20	42.66
42.00	29.40	26.93

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015517.D
 Acq On : 14 Jun 2023 14:55
 Operator : MA/JU
 Sample : 03098-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 14 23:39:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.087	152	110583	20.000	ng/ul	0.00
20) Naphthalene-d8	10.916	136	522521	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.734	164	375336	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.487	188	875026	20.000	ng/ul	0.00
79) Chrysene-d12	21.569	240	866502	20.000	ng/ul	0.00
88) Perylene-d12	24.116	264	927314	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	17177	5.752	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.246	99	98485	9.667	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.411	67	258554	42.496	ng/ul	0.00
11) 2-Chlorophenol-d4	7.617	132	250548	33.921	ng/ul	0.00
15) 4-Methylphenol-d8	8.805	113	183127	21.902	ng/ul	0.00
21) Nitrobenzene-d5	9.269	128	169089	41.218	ng/ul	0.00
24) 2-Nitrophenol-d4	9.993	143	187181	39.955	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	309637	36.232	ng/ul	0.00
31) 4-Chloroaniline-d4	11.093	131	10619m	0.866	ng/ul	0.03
46) Dimethylphthalate-d6	14.140	166	1362390	46.031	ng/ul	0.00
49) Acenaphthylene-d8	14.428	160	1423563	43.986	ng/ul	0.00
54) 4-Nitrophenol-d4	14.963	143	34527m	6.514	ng/ul	0.02
60) Fluorene-d10	15.722	176	1157658	46.383	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.851	200	237542	42.852	ng/ul	0.00
73) Anthracene-d10	17.587	188	2012132	50.540	ng/ul	0.00
81) Pyrene-d10	19.810	212	2538637	54.740	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	2459465	52.859	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015517.D
Acq On : 14 Jun 2023 14:55
Operator : MA/JU
Sample : 03098-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 14 23:39:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 09 23:33:38 2023
Response via : Initial Calibration

