




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015525.D
Acq On : 14 Jun 2023 19:26
Operator : MA/JU
Sample : 03062-06RX
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEL2RX

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:11:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 09 23:33:38 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :mohammad ahmed 06/16/2023

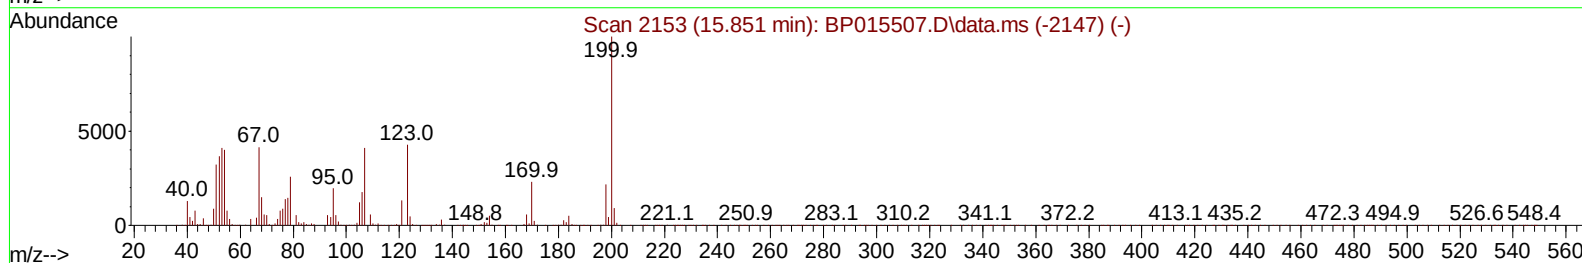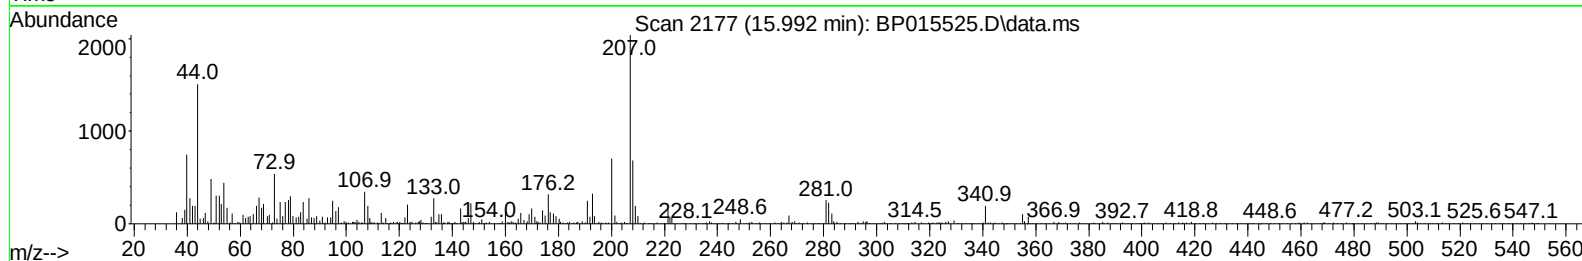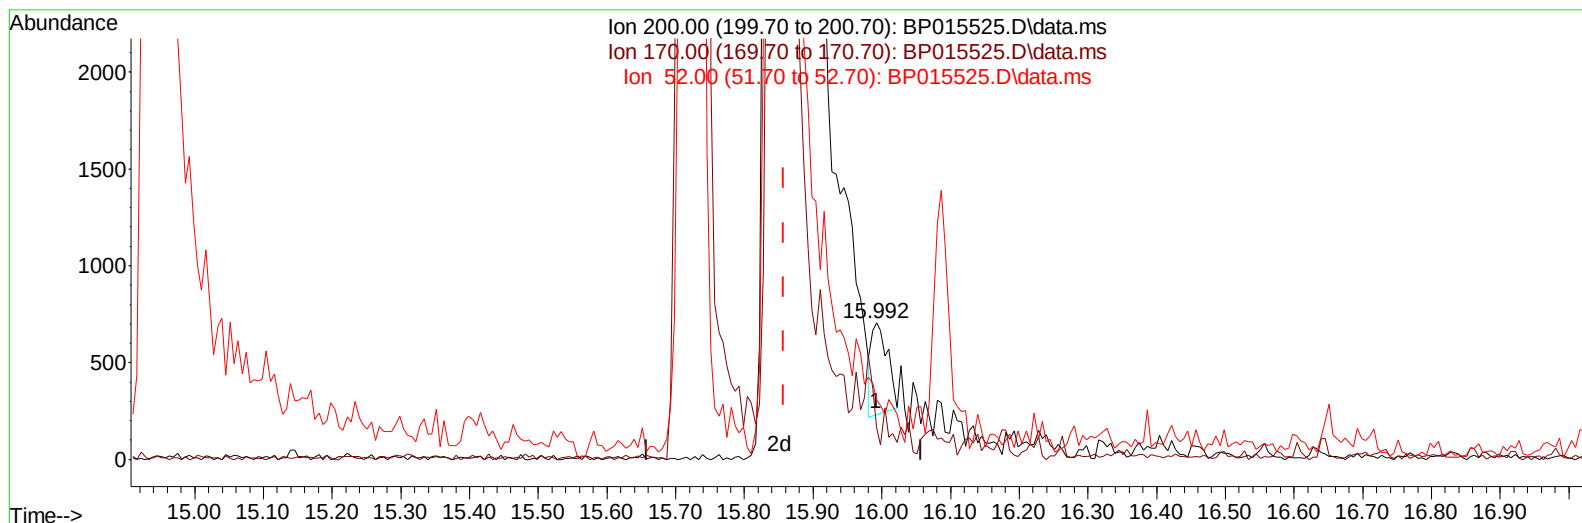

TIC: BP015525.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.992min (+ 0.135) 0.21 ng/u1

response 753

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.30	23.37
52.00	46.20	43.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015525.D
 Acq On : 14 Jun 2023 19:26
 Operator : MA/JU
 Sample : 03062-06RX
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEL2RX

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:11:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

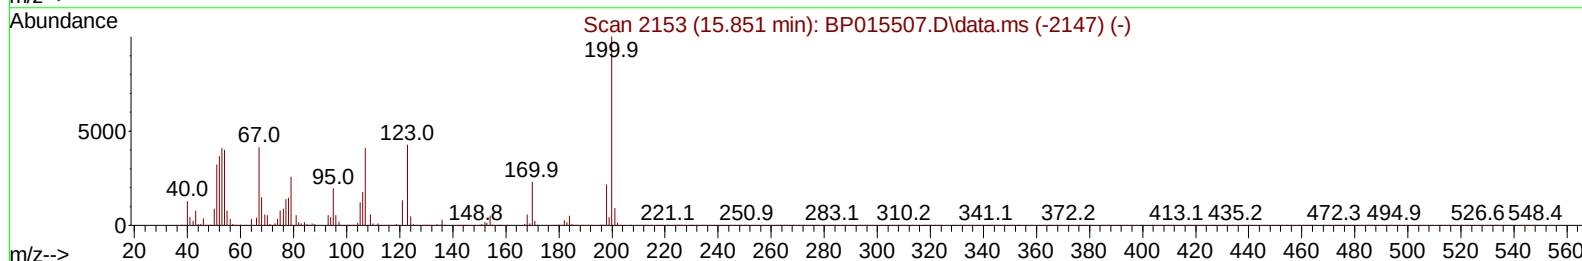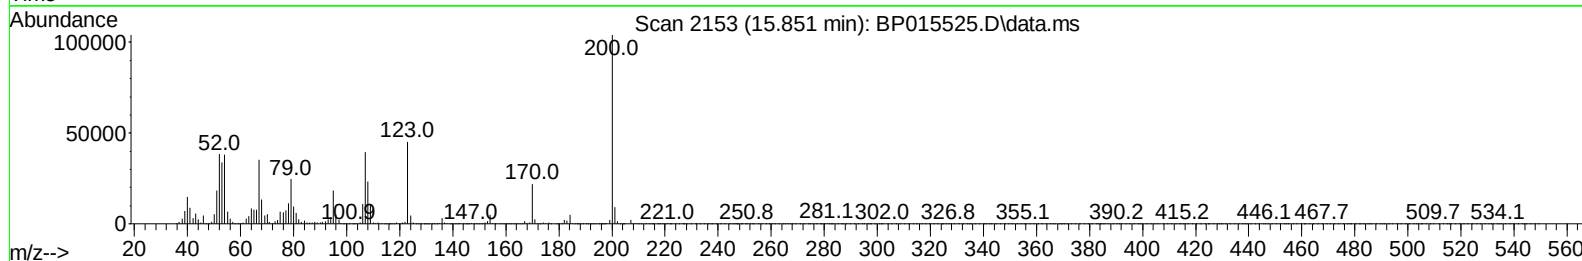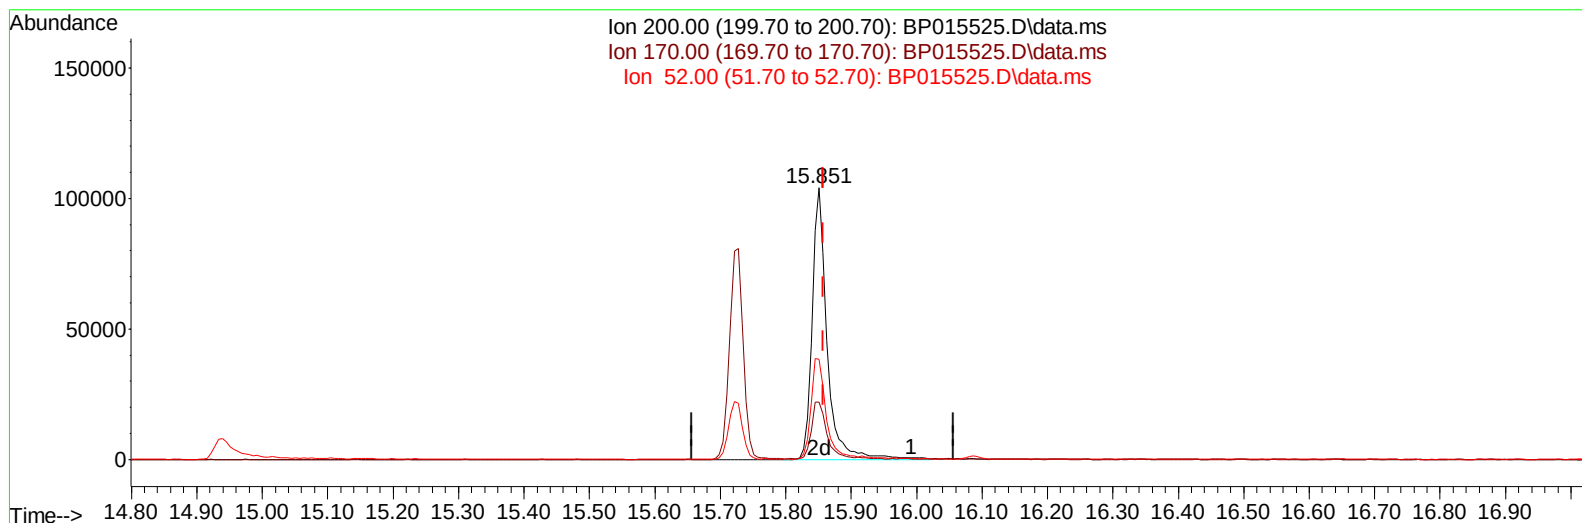

TIC: BP015525.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.851min (-0.006) 44.91 ng/ul m

response 163860

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.30	21.15
52.00	46.20	36.89#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015525.D
 Acq On : 14 Jun 2023 19:26
 Operator : MA/JU
 Sample : 03062-06RX
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEL2RX

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 14 23:55:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.087	152	73342	20.000	ng/ul	0.00
20) Naphthalene-d8	10.916	136	348657	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.734	164	242720	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.486	188	575884	20.000	ng/ul	0.00
79) Chrysene-d12	21.569	240	571729	20.000	ng/ul	0.00
88) Perylene-d12	24.115	264	623802	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	12468	6.295	ng/uL	0.00
4) Pyridine-d5	3.846	84	171789	33.392	ng/ul	0.00
7) Phenol-d5	7.240	99	259714	38.438	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.410	67	163442	40.504	ng/ul	0.00
11) 2-Chlorophenol-d4	7.616	132	194466	39.697	ng/ul	0.00
15) 4-Methylphenol-d8	8.804	113	259919	46.871	ng/ul	0.00
21) Nitrobenzene-d5	9.269	128	119888	43.798	ng/ul	0.00
24) 2-Nitrophenol-d4	9.993	143	143320	45.848	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	263344	46.182	ng/ul	0.00
31) 4-Chloroaniline-d4	11.057	131	383676	46.875	ng/ul	0.00
46) Dimethylphthalate-d6	14.140	166	1134526	59.275	ng/ul	0.00
49) Acenaphthylene-d8	14.428	160	1203619	57.510	ng/ul	0.00
54) 4-Nitrophenol-d4	14.939	143	134710	39.302	ng/ul	0.00
60) Fluorene-d10	15.728	176	958875	59.409	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.851	200	163860m	44.915	ng/ul	0.00
73) Anthracene-d10	17.586	188	1580313	60.313	ng/ul	0.00
81) Pyrene-d10	19.810	212	1966710	64.272	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	1901937	60.765	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015525.D
Acq On : 14 Jun 2023 19:26
Operator : MA/JU
Sample : 03062-06RX
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEL2RX

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:55:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 09 23:33:38 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :mohammad ahmed 06/16/2023

