




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015527.D
 Acq On : 14 Jun 2023 20:34
 Operator : MA/JU
 Sample : 03097-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEP6

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:11:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

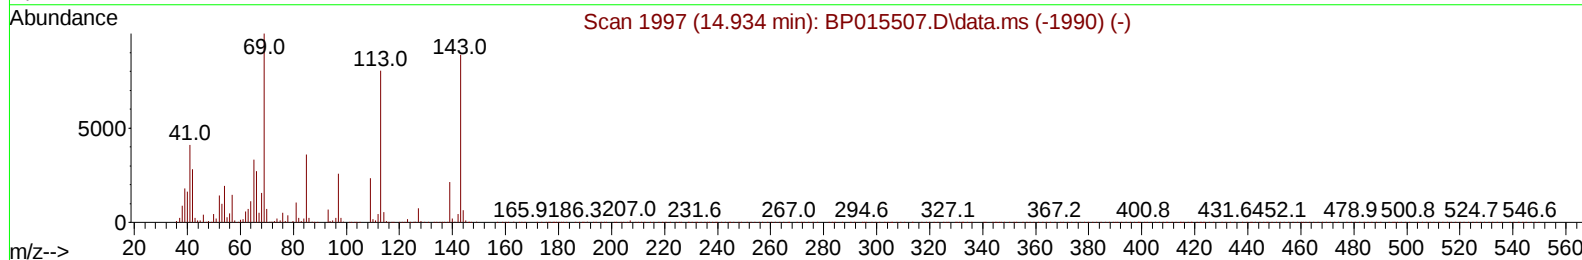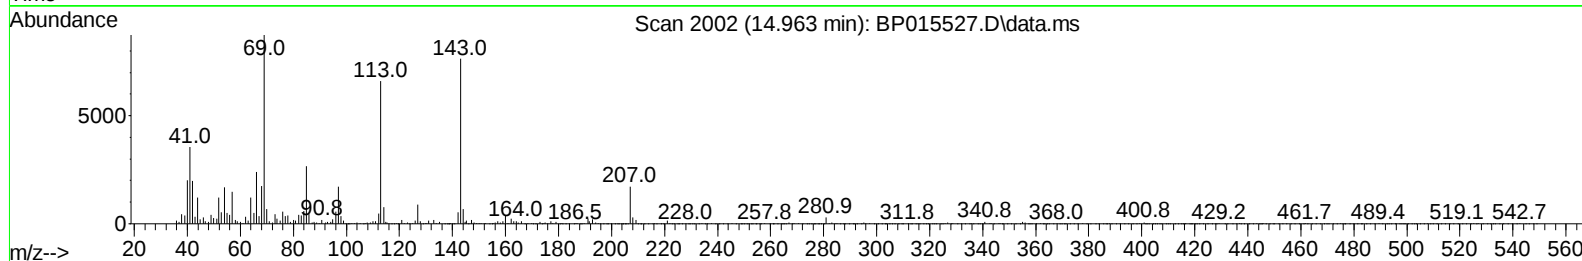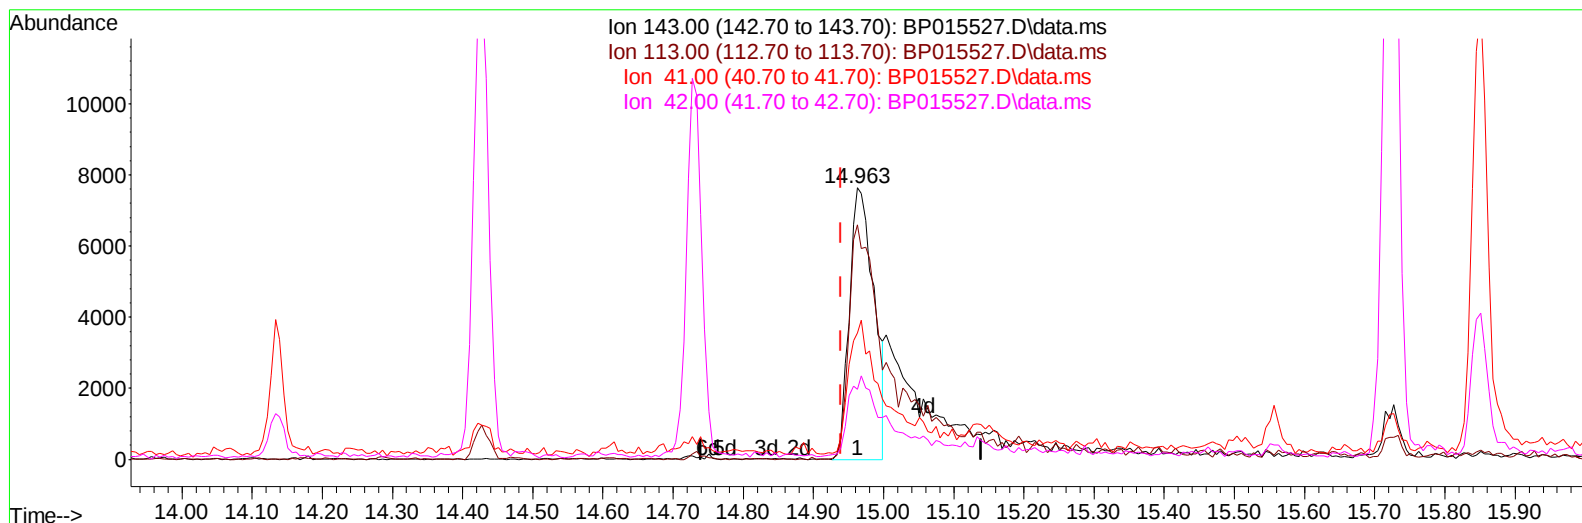

TIC: BP015527.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.963min (+ 0.023) 3.05 ng/u1

response 18604

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	86.36
41.00	42.20	46.52
42.00	29.40	25.95




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015527.D
 Acq On : 14 Jun 2023 20:34
 Operator : MA/JU
 Sample : 03097-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEP6

Manual IntegrationsAPPROVED

Quant Time: Jun 14 23:11:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

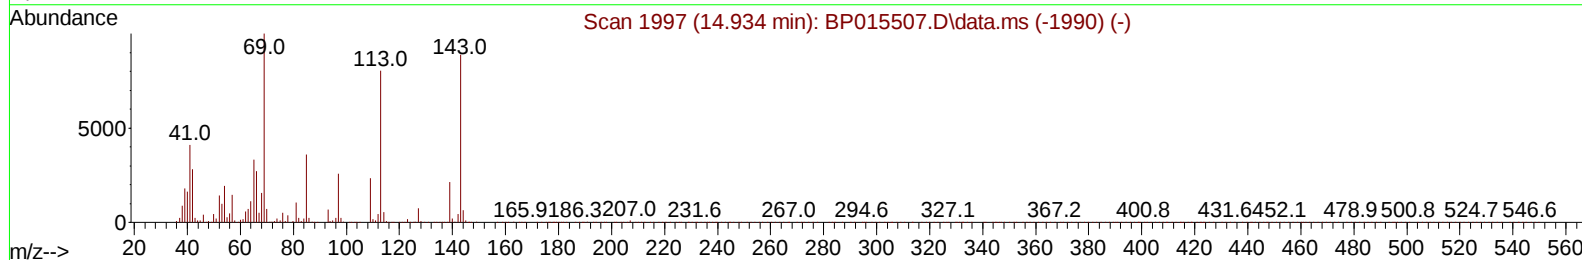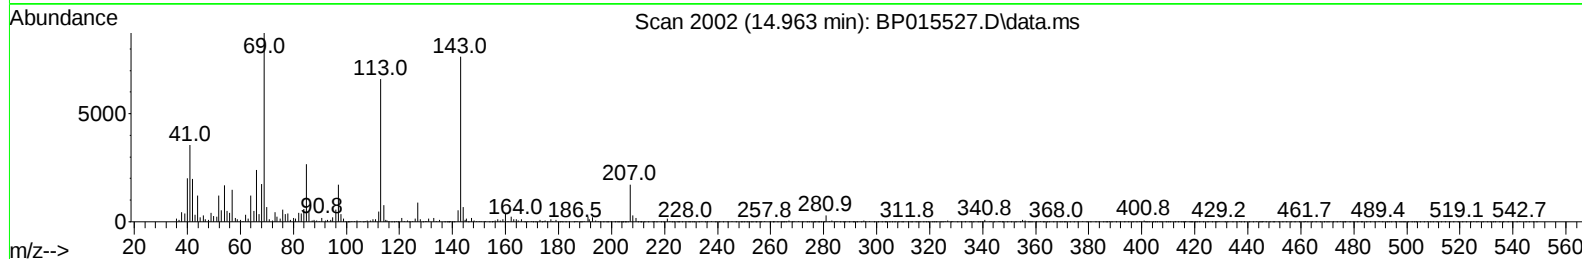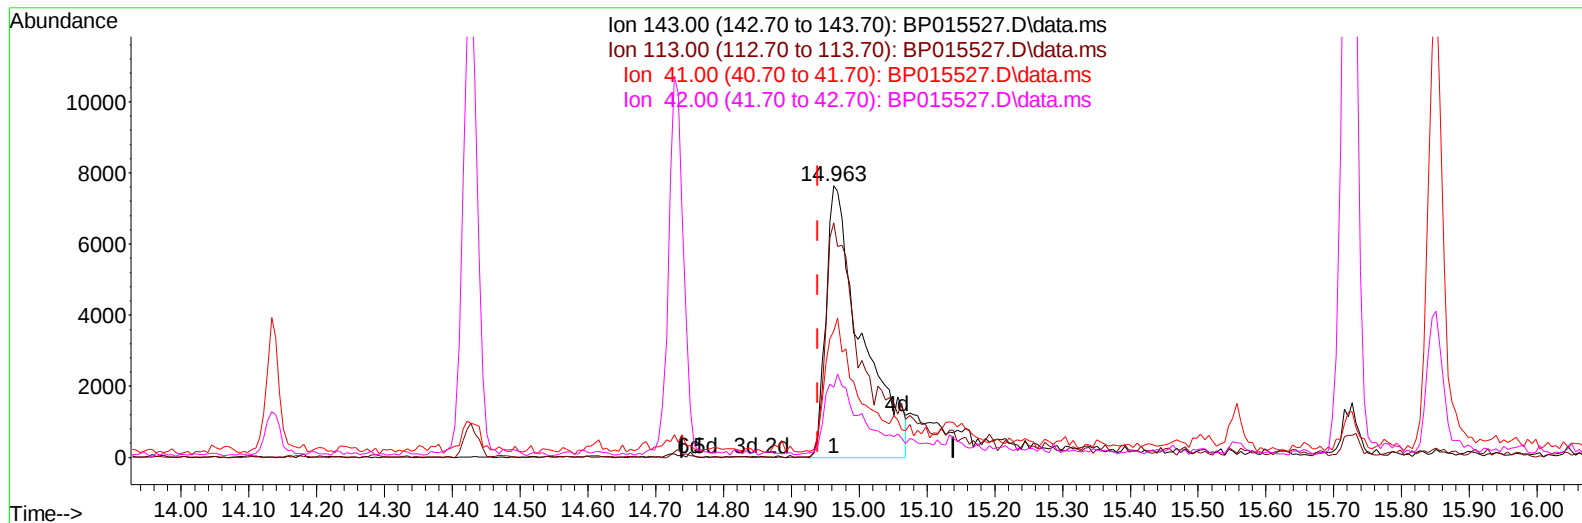

TIC: BP015527.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.963min (+ 0.023) 4.56 ng/ul m

response 27781

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	86.36
41.00	42.20	46.52
42.00	29.40	25.95

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015527.D
 Acq On : 14 Jun 2023 20:34
 Operator : MA/JU
 Sample : 03097-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEP6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 14 23:58:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.087	152	134514	20.000	ng/ul	0.00
20) Naphthalene-d8	10.916	136	624538	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.733	164	431856	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.486	188	1027743	20.000	ng/ul	0.00
79) Chrysene-d12	21.568	240	1062658	20.000	ng/ul	0.00
88) Perylene-d12	24.115	264	1131220	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.404	96	17948	4.941	ng/uL	0.00
4) Pyridine-d5	3.852	84	89881	9.526	ng/ul	0.00
7) Phenol-d5	7.245	99	96592	7.795	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.410	67	263448	35.597	ng/ul	0.00
11) 2-Chlorophenol-d4	7.616	132	260903	29.038	ng/ul	0.00
15) 4-Methylphenol-d8	8.804	113	188776	18.561	ng/ul	0.00
21) Nitrobenzene-d5	9.269	128	174758	35.641	ng/ul	0.00
24) 2-Nitrophenol-d4	9.992	143	196403	35.075	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	318232	31.155	ng/ul	0.00
31) 4-Chloroaniline-d4	11.057	131	370023	25.238	ng/ul	0.00
46) Dimethylphthalate-d6	14.139	166	1289396	37.863	ng/ul	0.00
49) Acenaphthylene-d8	14.427	160	1371623	36.835	ng/ul	0.00
54) 4-Nitrophenol-d4	14.963	143	27781m	4.555	ng/ul	0.02
60) Fluorene-d10	15.721	176	1091654	38.014	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.851	200	218900	33.621	ng/ul	0.00
73) Anthracene-d10	17.586	188	1845815	39.473	ng/ul	0.00
81) Pyrene-d10	19.809	212	2345623	41.242	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.950	264	2328634	41.026	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015527.D
Acq On : 14 Jun 2023 20:34
Operator : MA/JU
Sample : 03097-20
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZE6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 14 23:58:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 09 23:33:38 2023
Response via : Initial Calibration

