




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015547.D
Acq On : 15 Jun 2023 08:19
Operator : MA/JU
Sample : 03088-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFR2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 15 08:49:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 15 05:36:46 2023
Response via : Initial Calibration

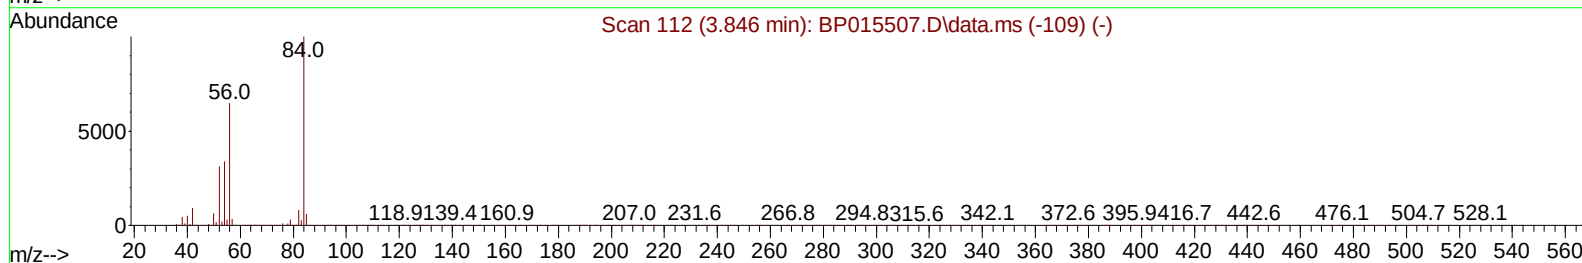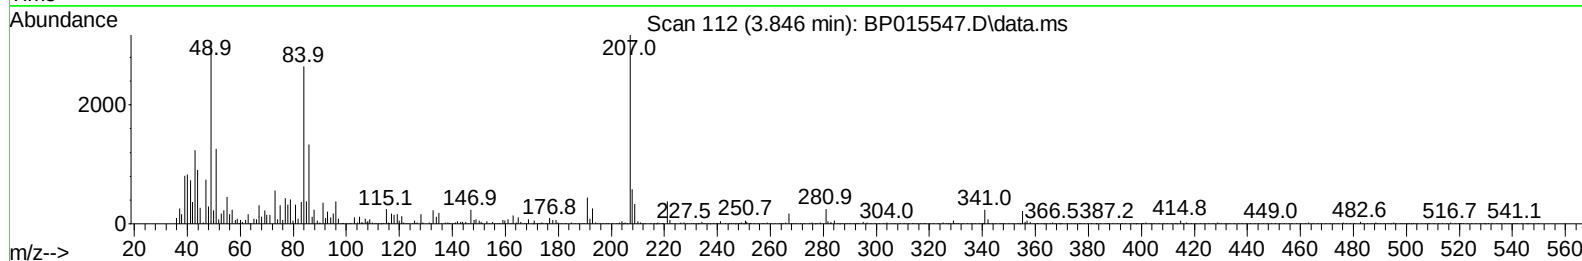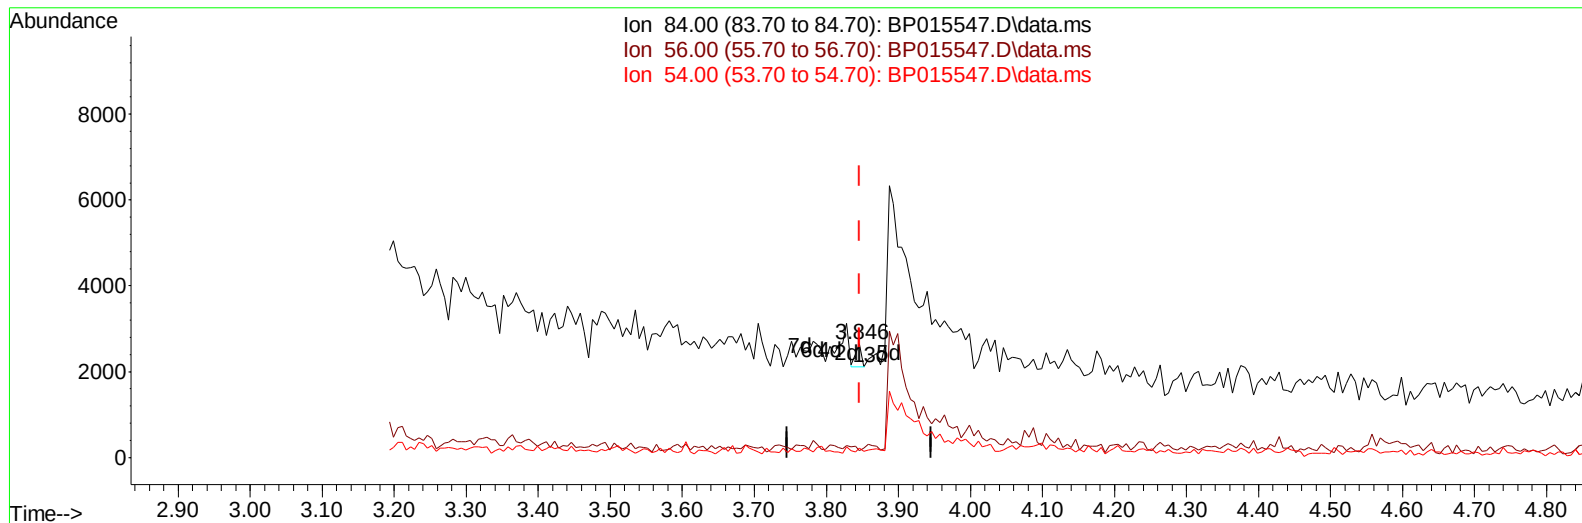

TIC: BP015547.D\data.ms

(4) Pyridine-d5 (S)

3.846min (+ 0.000) 0.03 ng/u1

response 286

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.90	6.16#
54.00	33.70	8.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015547.D
Acq On : 15 Jun 2023 08:19
Operator : MA/JU
Sample : 03088-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFR2

Manual IntegrationsAPPROVED

Quant Time: Jun 15 08:49:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 15 05:36:46 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :mohammad ahmed 06/16/2023

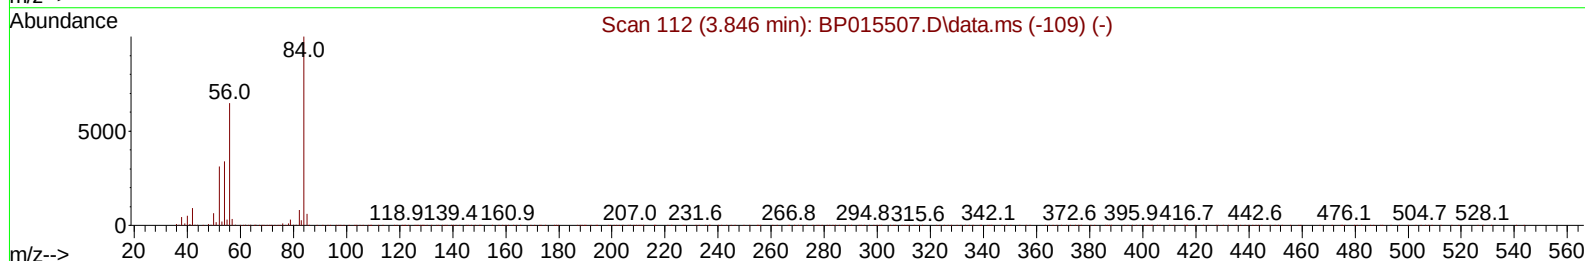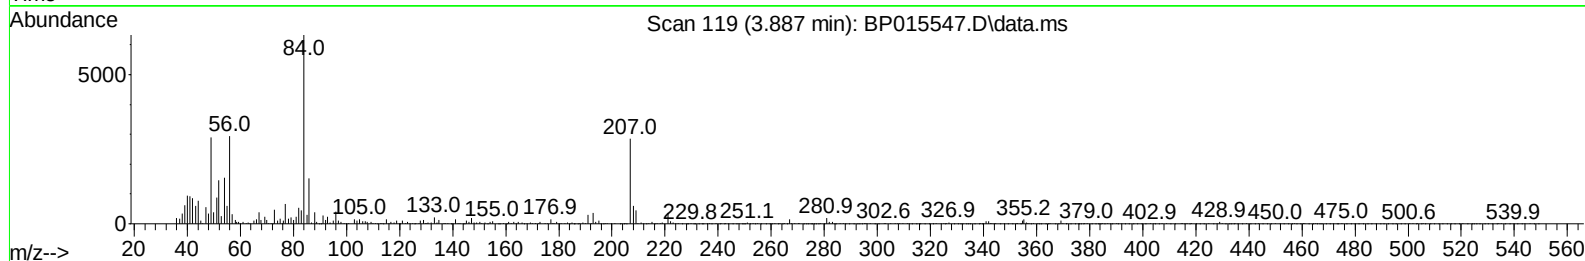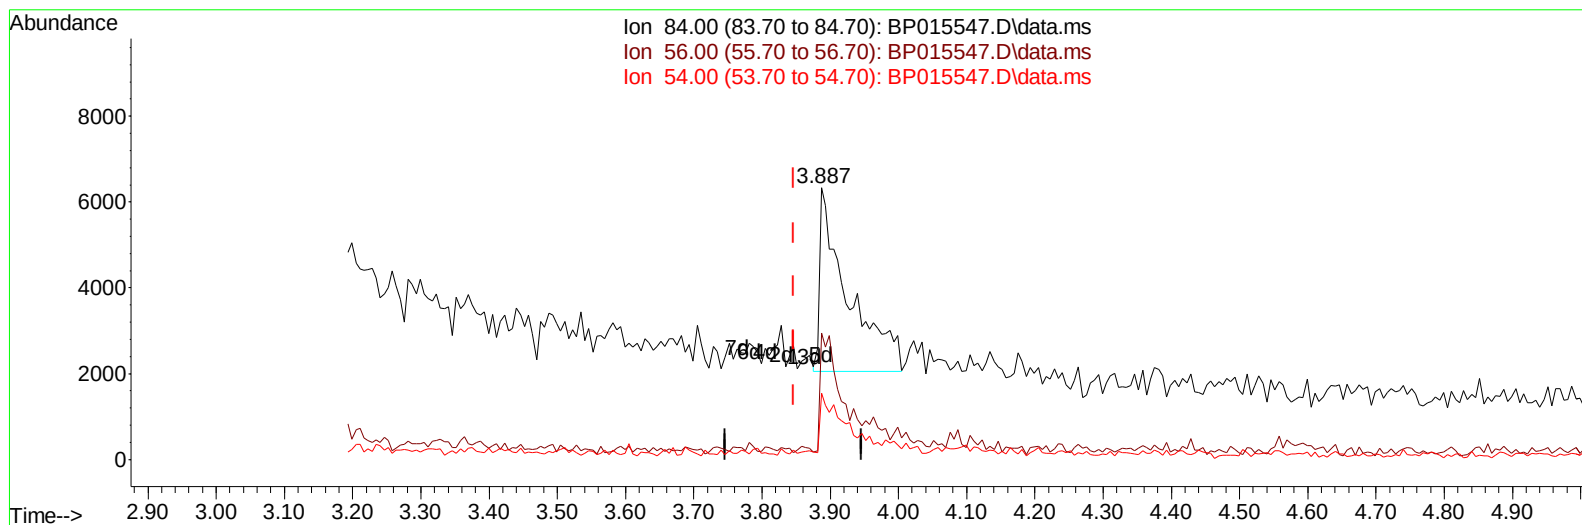

TIC: BP015547.D\data.ms

(4) Pyridine-d5 (S)

3.887min (+ 0.041) 1.31 ng/ul m

response 12376

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.90	46.60#
54.00	33.70	24.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015547.D
 Acq On : 15 Jun 2023 08:19
 Operator : MA/JU
 Sample : 03088-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFR2

Manual IntegrationsAPPROVED

Quant Time: Jun 15 08:50:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 15 05:36:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

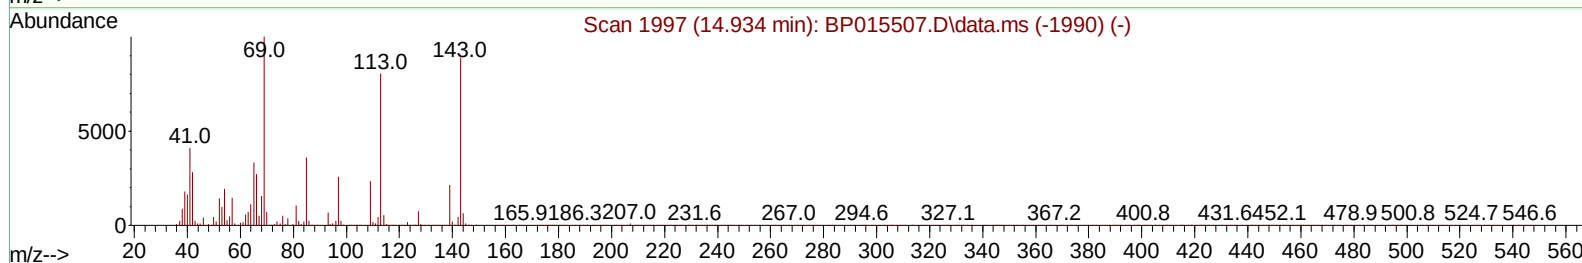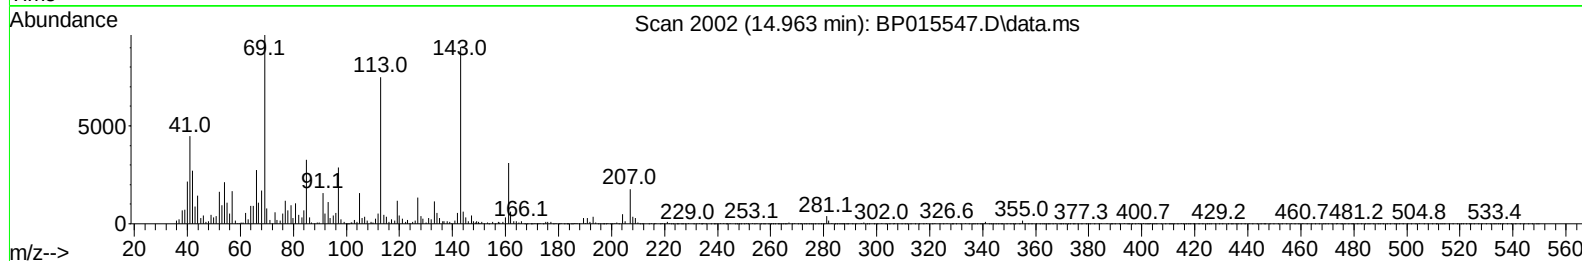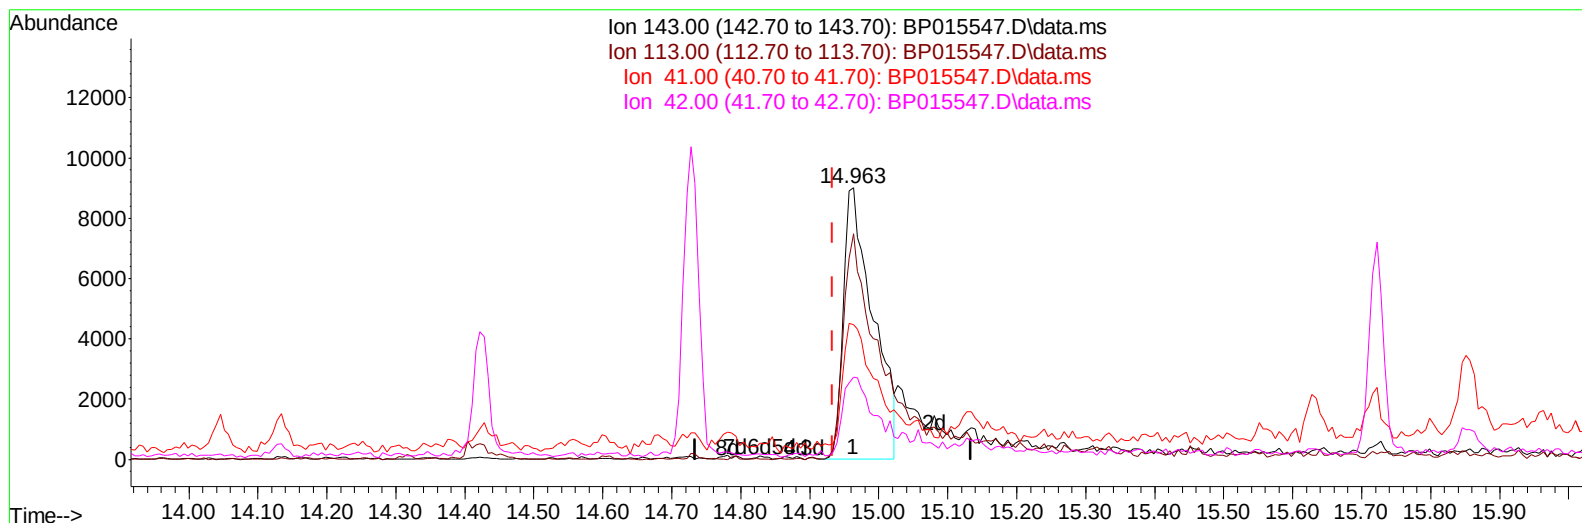

TIC: BP015547.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.963min (+ 0.029) 4.27 ng/ul

response 26780

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	83.19
41.00	42.20	49.66
42.00	29.40	30.24




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015547.D
 Acq On : 15 Jun 2023 08:19
 Operator : MA/JU
 Sample : 03088-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFR2

Manual IntegrationsAPPROVED

Quant Time: Jun 15 08:50:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 15 05:36:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

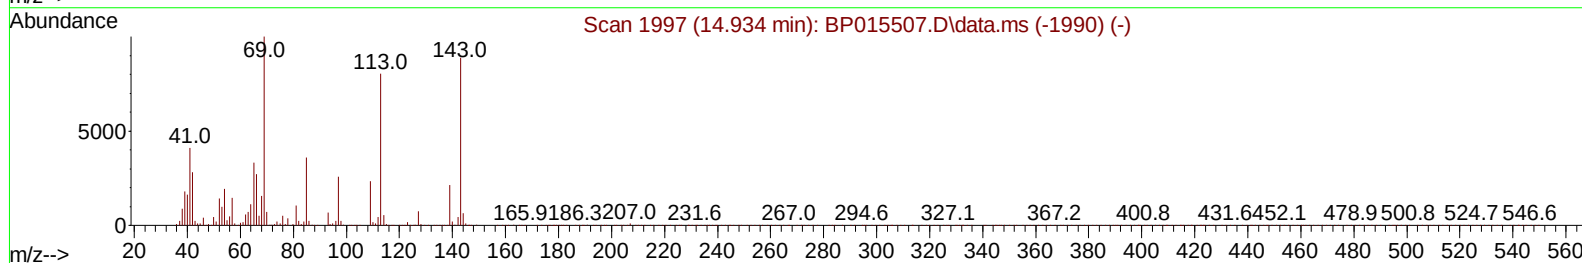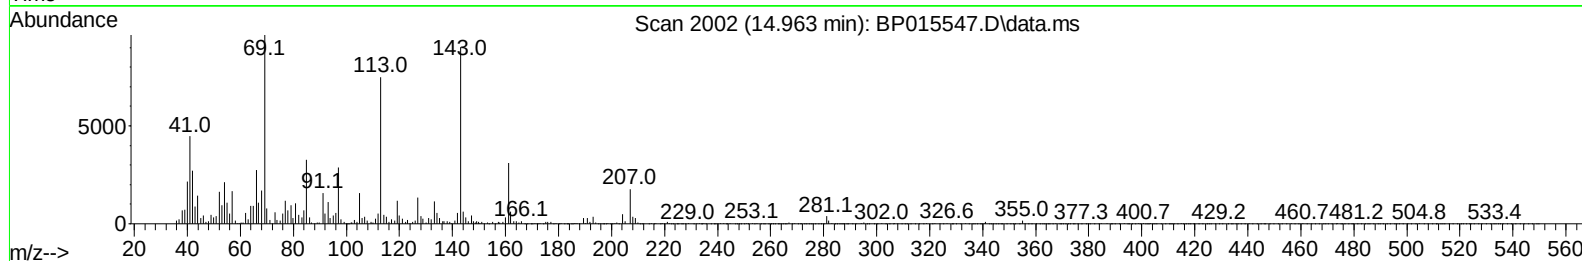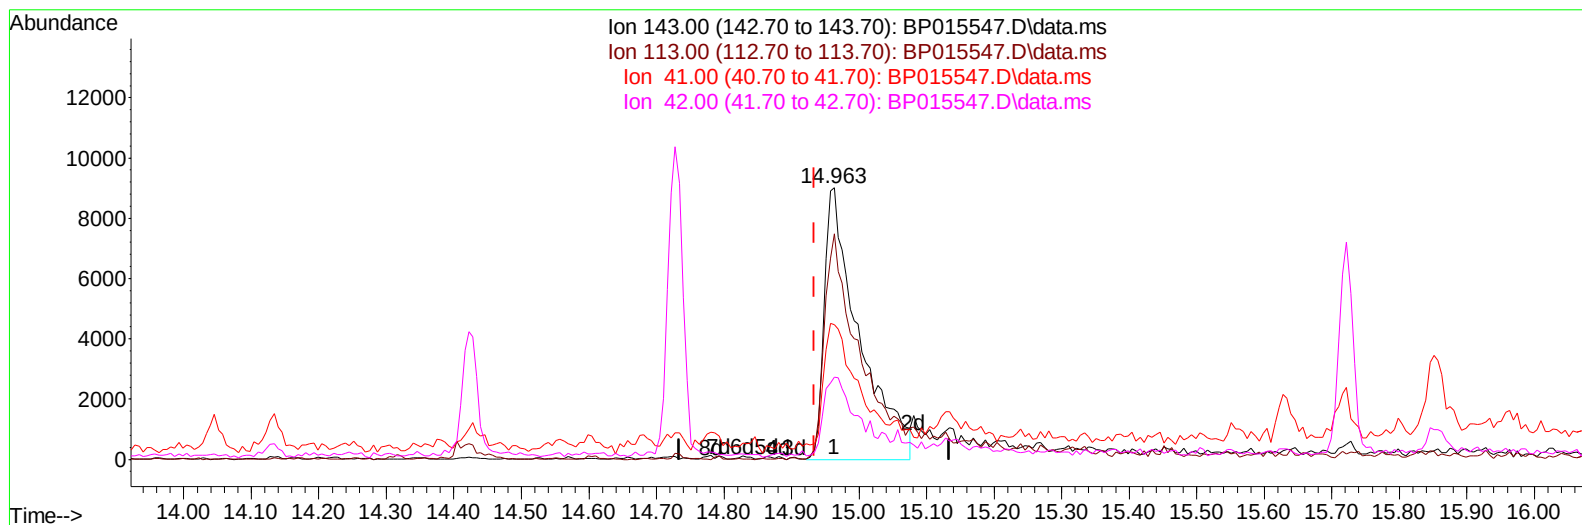

TIC: BP015547.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.963min (+ 0.029) 5.12 ng/ul m

response 32082

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	83.19
41.00	42.20	49.66
42.00	29.40	30.24

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015547.D
 Acq On : 15 Jun 2023 08:19
 Operator : MA/JU
 Sample : 03088-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFR2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 15 08:52:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 15 05:36:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.087	152	134186	20.000	ng/ul	0.00
20) Naphthalene-d8	10.910	136	640629	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.728	164	443638	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.486	188	1005118	20.000	ng/ul	0.00
79) Chrysene-d12	21.569	240	977051	20.000	ng/ul	0.00
88) Perylene-d12	24.116	264	1030236	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	5923	1.635	ng/uL	0.00
4) Pyridine-d5	3.887	84	12376m	1.315	ng/ul	0.04
7) Phenol-d5	7.240	99	120934	9.783	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.405	67	79929	10.826	ng/ul	0.00
11) 2-Chlorophenol-d4	7.611	132	100120	11.171	ng/ul	0.00
15) 4-Methylphenol-d8	8.805	113	84207	8.300	ng/ul	0.00
21) Nitrobenzene-d5	9.263	128	51222	10.184	ng/ul	0.00
24) 2-Nitrophenol-d4	9.993	143	60486	10.531	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.540	165	107816	10.290	ng/ul	0.00
31) 4-Chloroaniline-d4	11.069	131	47370	3.150	ng/ul	0.01
46) Dimethylphthalate-d6	14.134	166	408847	11.687	ng/ul	0.00
49) Acenaphthylene-d8	14.428	160	427311	11.171	ng/ul	0.00
54) 4-Nitrophenol-d4	14.963	143	32082m	5.121	ng/ul	0.03
60) Fluorene-d10	15.722	176	346018	11.729	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	45963	7.218	ng/ul	0.00
73) Anthracene-d10	17.587	188	513408	11.227	ng/ul	0.00
81) Pyrene-d10	19.810	212	445927	8.527	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.945	264	249929	4.835	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015547.D
Acq On : 15 Jun 2023 08:19
Operator : MA/JU
Sample : 03088-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFR2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 15 08:52:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 15 05:36:46 2023
Response via : Initial Calibration

