




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015562.D
 Acq On : 15 Jun 2023 18:43
 Operator : MA/JU
 Sample : 03098-05
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ1

Manual IntegrationsAPPROVED

Quant Time: Jun 15 22:07:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 15 05:36:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/16/2023
 Supervised By :mohammad ahmed 06/16/2023

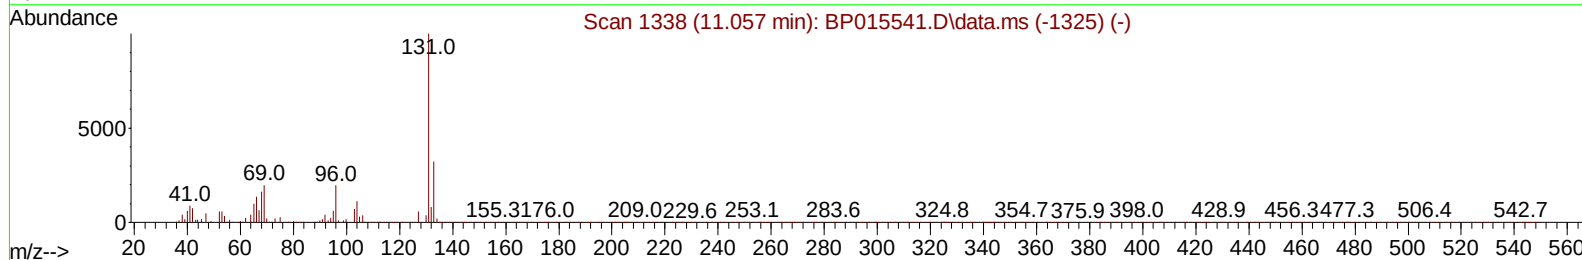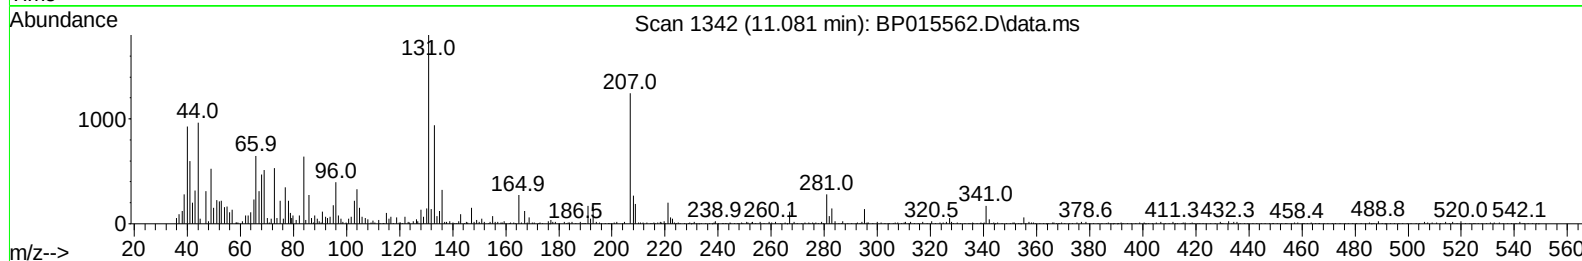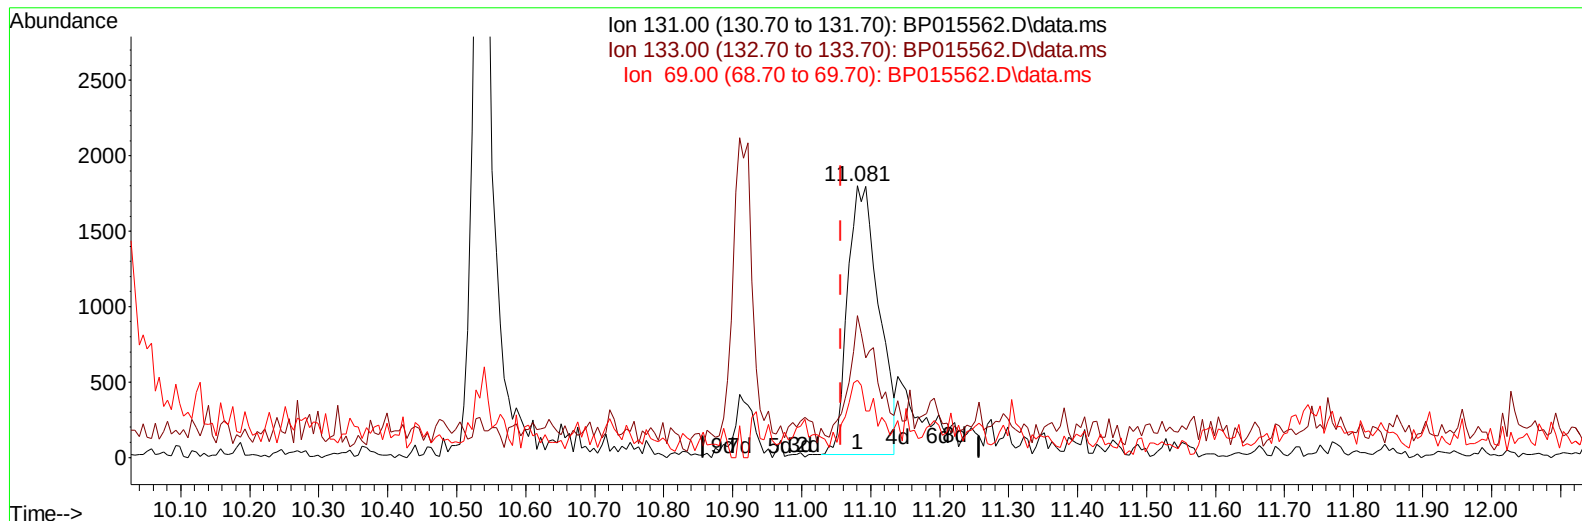

TIC: BP015562.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.081min (+ 0.023) 0.51 ng/ul

response 5584

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	52.17#
69.00	18.30	28.44#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015562.D
Acq On : 15 Jun 2023 18:43
Operator : MA/JU
Sample : 03098-05
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ1

Manual IntegrationsAPPROVED

Quant Time: Jun 15 22:07:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 15 05:36:46 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/16/2023
Supervised By :mohammad ahmed 06/16/2023

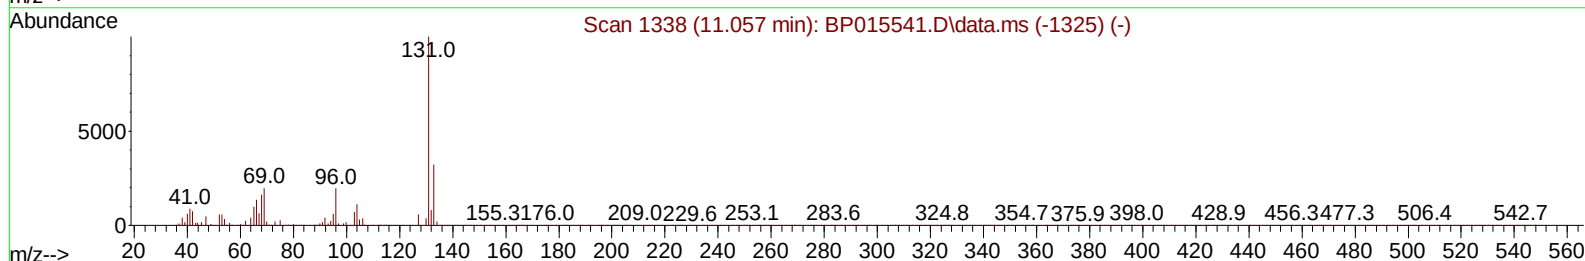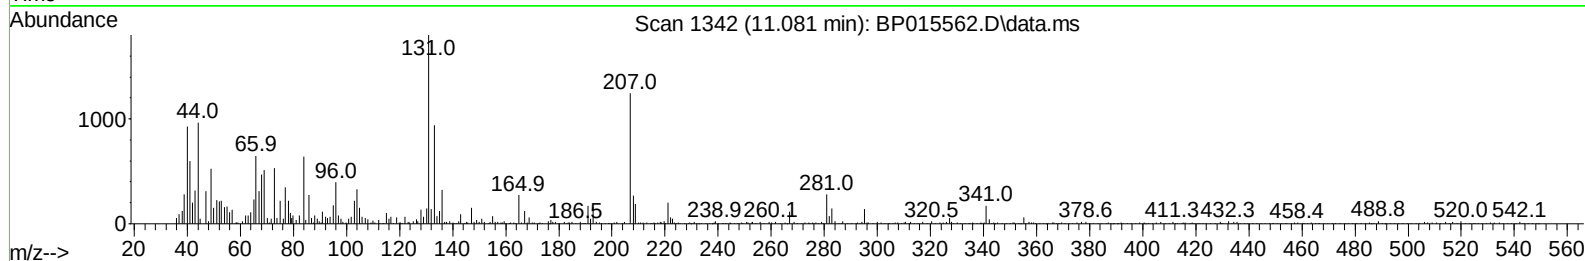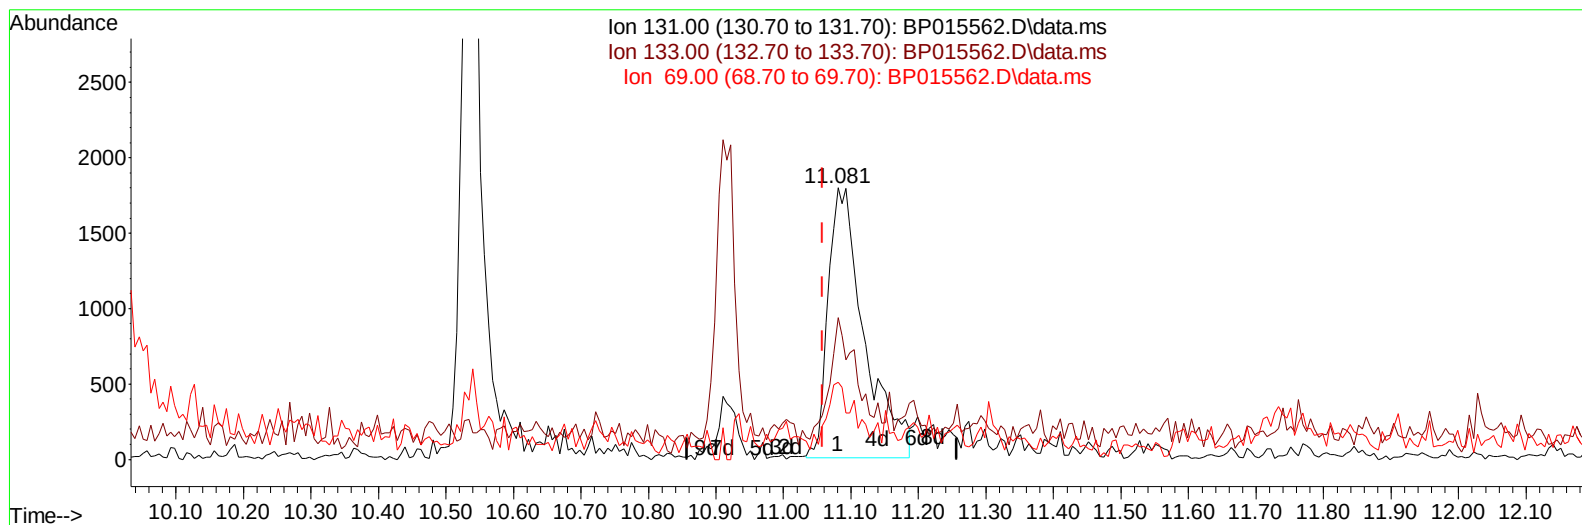

TIC: BP015562.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.081min (+ 0.023) 0.61 ng/ul m

response 6694

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	52.17#
69.00	18.30	28.44#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015562.D
Acq On : 15 Jun 2023 18:43
Operator : MA/JU
Sample : 03098-05
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ1

Manual IntegrationsAPPROVED

Quant Time: Jun 15 22:07:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 15 05:36:46 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/16/2023
Supervised By :mohammad ahmed 06/16/2023

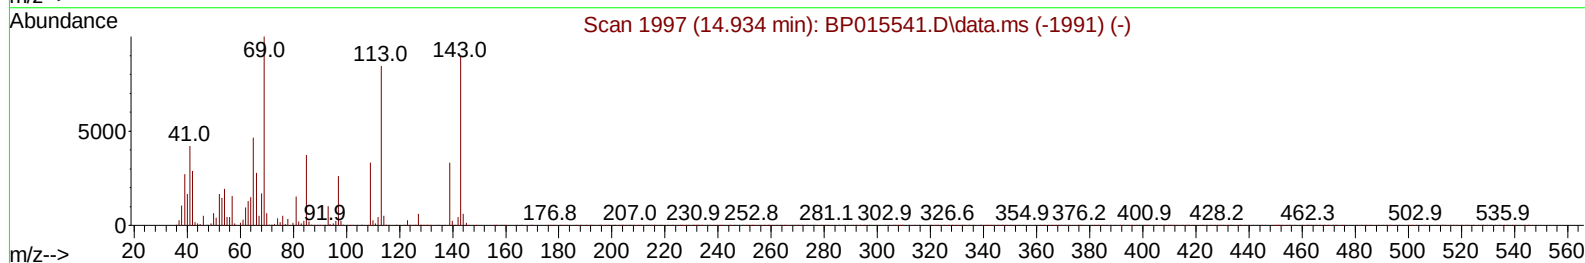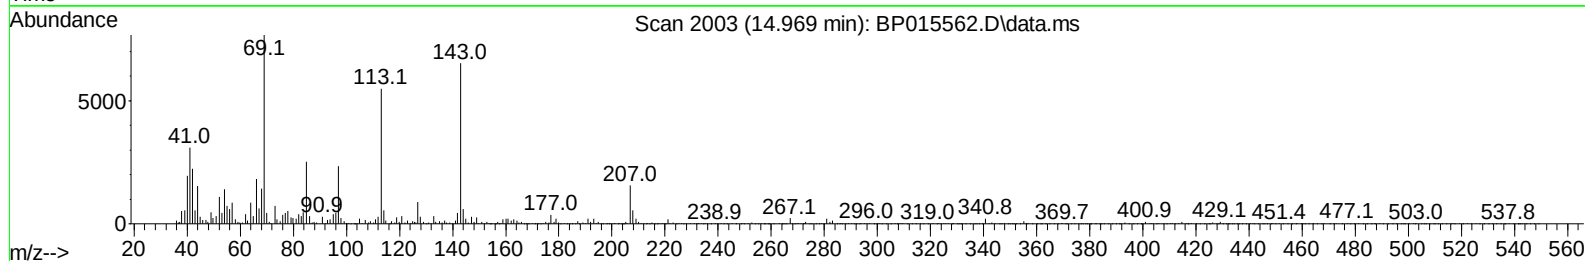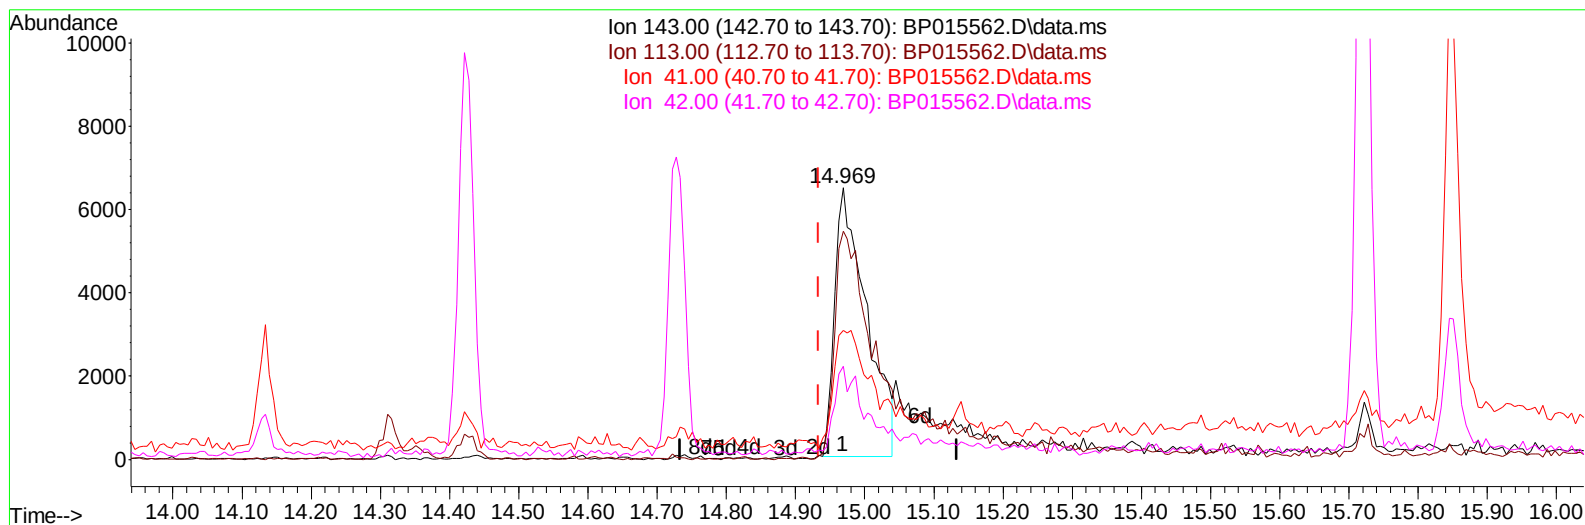

TIC: BP015562.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.969min (+ 0.035) 4.40 ng/u1

response 20498

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	84.14
41.00	42.20	47.47
42.00	29.40	34.36




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015562.D
 Acq On : 15 Jun 2023 18:43
 Operator : MA/JU
 Sample : 03098-05
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ1

Manual IntegrationsAPPROVED

Quant Time: Jun 15 23:15:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 15 05:36:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/16/2023
 Supervised By :mohammad ahmed 06/16/2023

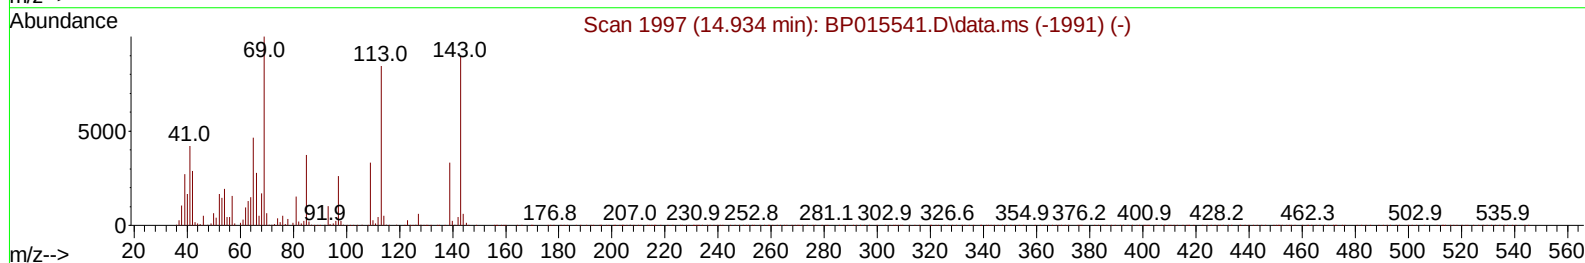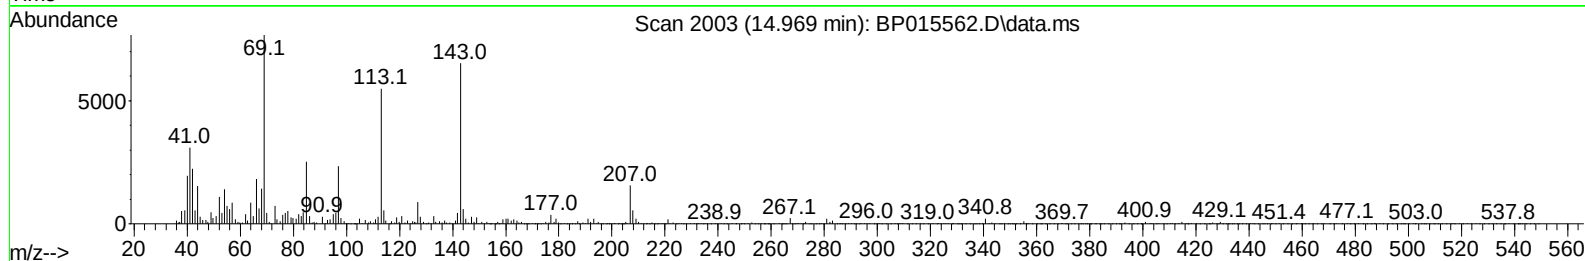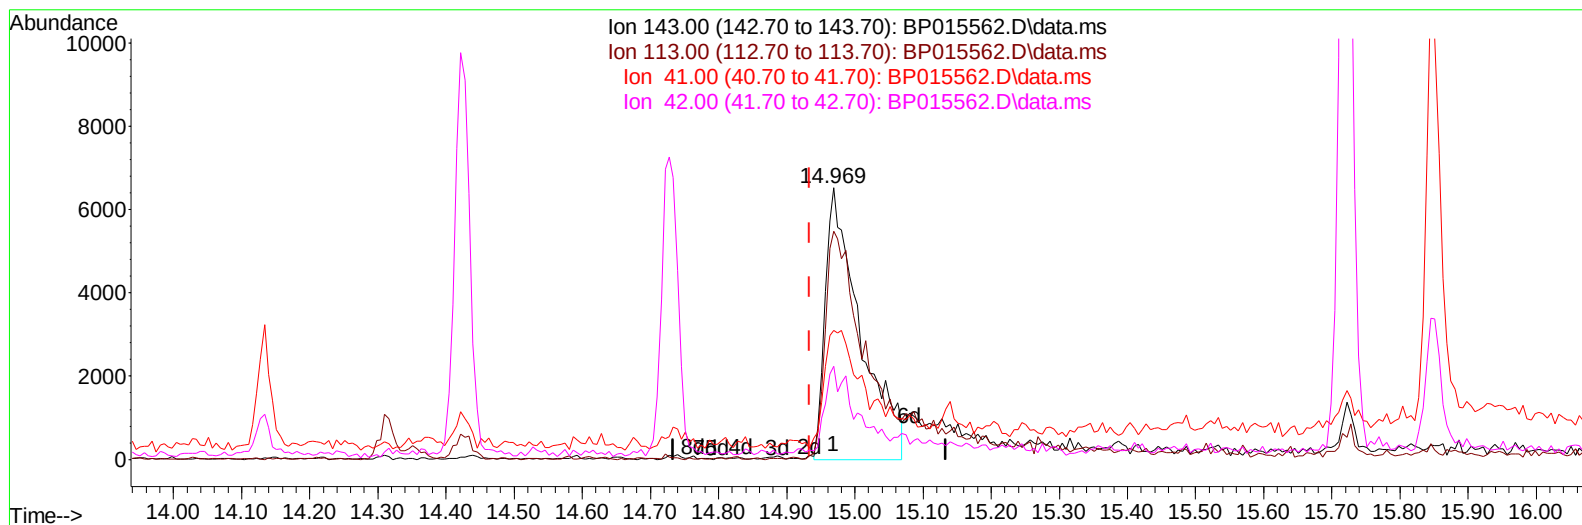

TIC: BP015562.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.969min (+ 0.035) 5.01 ng/ul m

response 23311

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	84.14
41.00	42.20	47.47
42.00	29.40	34.36

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015562.D
 Acq On : 15 Jun 2023 18:43
 Operator : MA/JU
 Sample : 03098-05
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/16/2023
 Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 15 23:16:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 15 05:36:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.087	152	99307	20.000	ng/ul	0.00
20) Naphthalene-d8	10.910	136	466896	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.728	164	329534	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.486	188	782480	20.000	ng/ul	0.00
79) Chrysene-d12	21.568	240	811700	20.000	ng/ul	0.00
88) Perylene-d12	24.115	264	876285	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	13066	4.872	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.246	99	67751	7.405	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.410	67	189762	34.731	ng/ul	0.00
11) 2-Chlorophenol-d4	7.616	132	184103	27.755	ng/ul	0.00
15) 4-Methylphenol-d8	8.804	113	130004	17.314	ng/ul	0.00
21) Nitrobenzene-d5	9.263	128	127645	34.822	ng/ul	0.00
24) 2-Nitrophenol-d4	9.993	143	146162	34.916	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	240436	31.487	ng/ul	0.00
31) 4-Chloroaniline-d4	11.081	131	6694m	0.611	ng/ul	0.02
46) Dimethylphthalate-d6	14.134	166	1027146	39.527	ng/ul	0.00
49) Acenaphthylene-d8	14.422	160	1053209	37.066	ng/ul	0.00
54) 4-Nitrophenol-d4	14.969	143	23311m	5.009	ng/ul	0.04
60) Fluorene-d10	15.722	176	855677	39.049	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.851	200	171318	34.560	ng/ul	0.00
73) Anthracene-d10	17.586	188	1455951	40.895	ng/ul	0.00
81) Pyrene-d10	19.810	212	1967131	45.280	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	1958699	44.548	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015562.D
Acq On : 15 Jun 2023 18:43
Operator : MA/JU
Sample : 03098-05
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/16/2023
Supervised By :mohammad ahmed 06/16/2023

Quant Time: Jun 15 23:16:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 15 05:36:46 2023
Response via : Initial Calibration

