

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015508.D
 Acq On : 14 Jun 2023 09:51
 Operator : MA/JU
 Sample : PB153378BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK378

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	43	rBV	41922	55281	1.05%	0.113%
2	3.852	111	113	132	rBV	195647	353539	6.71%	0.721%
3	4.181	166	169	175	rBV5	6740	10815	0.21%	0.022%
4	4.628	241	245	250	rVB7	3815	5973	0.11%	0.012%
5	7.246	683	690	708	rBV	636814	1118722	21.23%	2.280%
6	7.410	712	718	730	rVV	567570	891784	16.93%	1.818%
7	7.616	746	753	766	rBV	698769	1169362	22.19%	2.384%
8	8.093	827	834	842	rBV	516214	870581	16.52%	1.775%
9	8.804	945	955	968	rBV	877472	1532097	29.08%	3.123%
10	9.269	1026	1034	1045	rBV	724862	1252446	23.77%	2.553%
11	9.993	1150	1157	1171	rBV	624575	1101623	20.91%	2.246%
12	10.087	1171	1173	1179	rVB6	4927	7420	0.14%	0.015%
13	10.540	1242	1250	1282	rBV	774606	1649432	31.31%	3.362%
14	10.916	1307	1314	1322	rBV	856945	1433150	27.20%	2.921%
15	11.063	1331	1339	1356	rBV	290759	676517	12.84%	1.379%
16	12.522	1581	1587	1594	rBV2	11145	23919	0.45%	0.049%
17	12.804	1629	1635	1639	rBV9	2431	5610	0.11%	0.011%
18	13.551	1756	1762	1766	rBV8	4055	8263	0.16%	0.017%
19	13.616	1766	1773	1780	rVB9	8737	22947	0.44%	0.047%
20	14.139	1854	1862	1876	rBV	1860427	2710388	51.44%	5.525%
21	14.251	1879	1881	1892	rVB	4803	9034	0.17%	0.018%
22	14.428	1904	1911	1928	rBV	2097645	3108611	59.00%	6.337%
23	14.734	1956	1963	1970	rBV	1443766	2124328	40.32%	4.330%
24	14.786	1970	1972	1984	rVB7	7857	18139	0.34%	0.037%
25	14.939	1991	1998	2016	rBV	315142	925069	17.56%	1.886%
26	15.545	2097	2101	2104	rBV3	4348	6308	0.12%	0.013%
27	15.728	2124	2132	2146	rBV	2612725	3890326	73.84%	7.930%
28	15.851	2147	2153	2168	rVV	739577	1194667	22.68%	2.435%
29	15.963	2170	2172	2182	rVB4	18808	40392	0.77%	0.082%
30	16.516	2261	2266	2270	rVB8	4129	7862	0.15%	0.016%
31	16.675	2287	2293	2299	rVB10	3875	6570	0.12%	0.013%
32	17.286	2392	2397	2399	rBV5	3881	6524	0.12%	0.013%
33	17.492	2425	2432	2442	rBV	1850381	2733266	51.88%	5.572%
34	17.586	2442	2448	2468	rVB2	2883215	4417293	83.84%	9.005%
35	19.392	2750	2755	2759	rBV2	44467	59809	1.14%	0.122%
36	19.463	2763	2767	2770	rBV3	32913	47768	0.91%	0.097%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015508.D
Acq On : 14 Jun 2023 09:51
Operator : MA/JU
Sample : PB153378BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK378

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	19.816	2821	2827	2840	rBV	3759098	5268652	100.00%	10.740%
38	21.574	3120	3126	3139	rBV	1956974	2922269	55.47%	5.957%
39	23.951	3523	3530	3549	rVB2	2244200	4742906	90.02%	9.668%
40	24.121	3552	3559	3571	rVB	1168800	2626364	49.85%	5.354%




Sum of corrected areas: 49056026

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015508.D
Acq On : 14 Jun 2023 09:51
Operator : MA/JU
Sample : PB153378BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

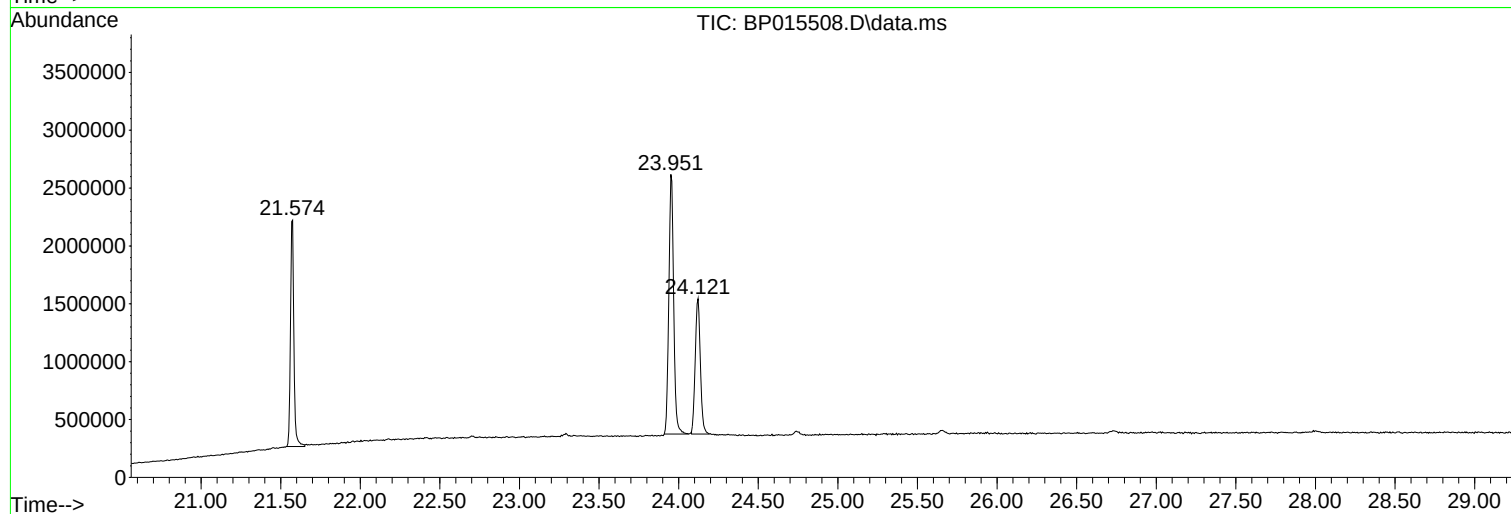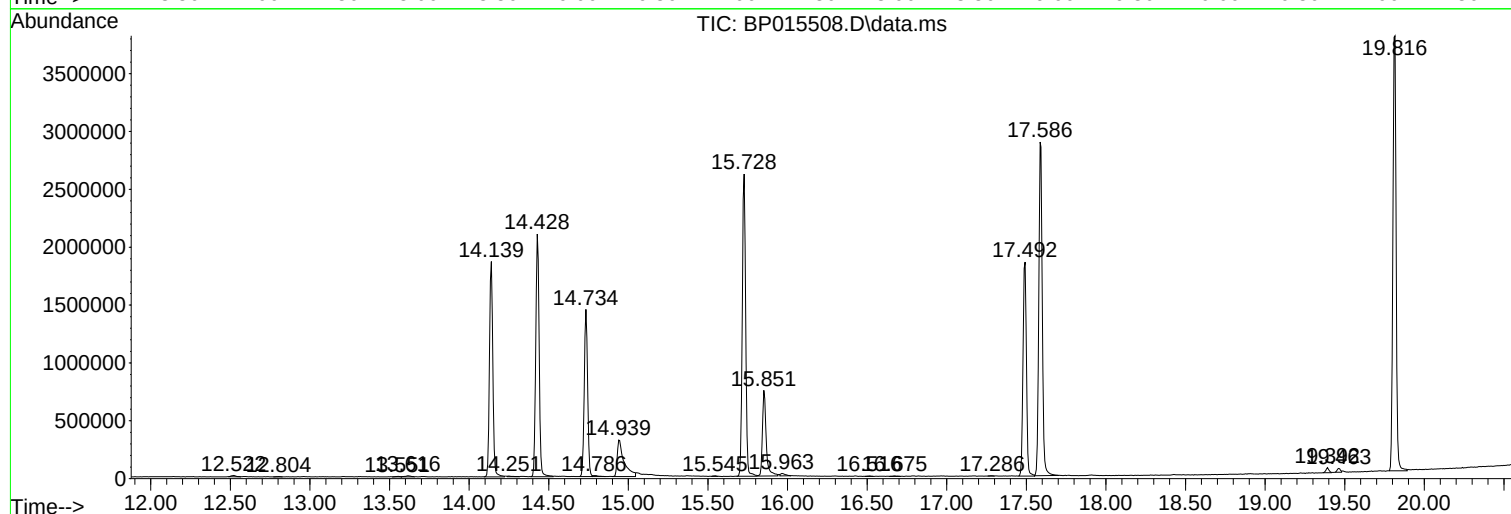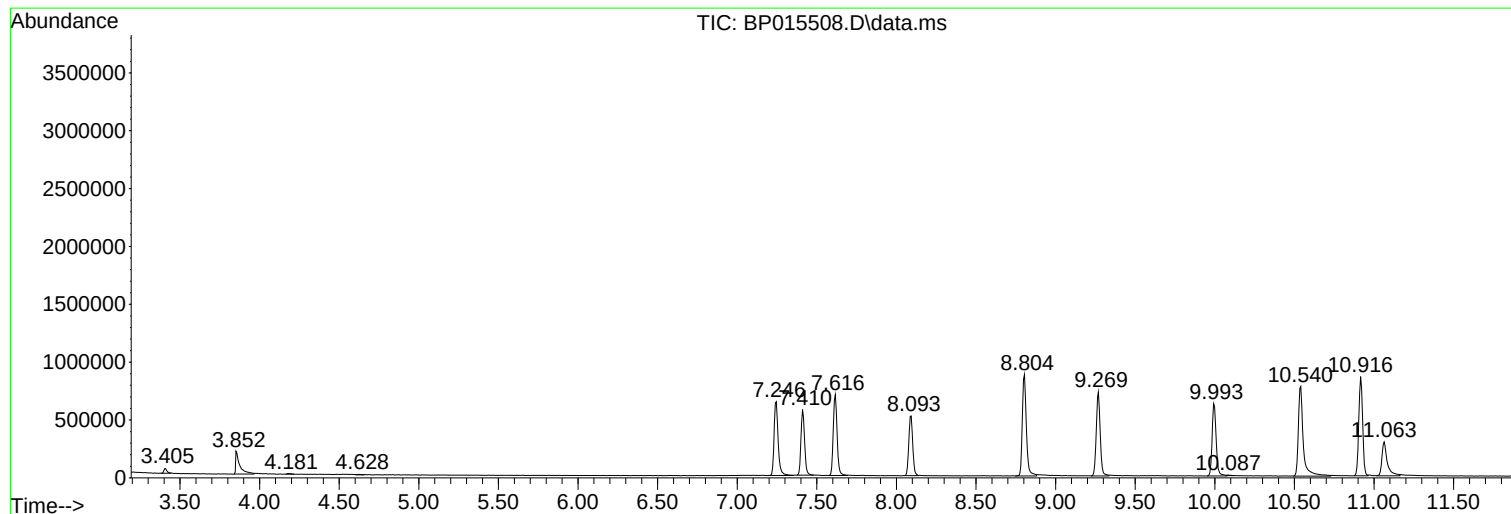

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015508.D
Acq On : 14 Jun 2023 09:51
Operator : MA/JU
Sample : PB153378BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015508.D
Acq On : 14 Jun 2023 09:51
Operator : MA/JU
Sample : PB153378BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------