

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015513.D
 Acq On : 14 Jun 2023 12:40
 Operator : MA/JU
 Sample : 03098-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	34	37	47	rVB	29077	44451	0.85%	0.099%
2	4.081	149	152	159	rVB4	8390	14327	0.27%	0.032%
3	4.181	165	169	174	rBV3	7717	14273	0.27%	0.032%
4	7.246	685	690	702	rBV	116889	217896	4.15%	0.485%
5	7.411	712	718	731	rBV	456227	745305	14.19%	1.659%
6	7.616	746	753	772	rVB	442874	758893	14.45%	1.689%
7	8.087	824	833	843	rBV	501233	853888	16.26%	1.901%
8	8.805	948	955	966	rBV	359811	633789	12.07%	1.411%
9	9.269	1026	1034	1047	rBV	597516	1047295	19.94%	2.331%
10	9.422	1053	1060	1062	rBV8	4255	5857	0.11%	0.013%
11	9.652	1094	1099	1108	rVB8	4216	9397	0.18%	0.021%
12	9.993	1149	1157	1173	rBV	494414	894047	17.02%	1.990%
13	10.540	1243	1250	1283	rBV	566866	1268603	24.15%	2.824%
14	10.916	1307	1314	1328	rBV	825631	1391920	26.50%	3.099%
15	11.110	1341	1347	1353	rBV9	4760	9013	0.17%	0.020%
16	11.757	1448	1457	1469	rBV4	19007	56974	1.08%	0.127%
17	12.510	1579	1585	1593	rBV3	9107	19343	0.37%	0.043%
18	13.063	1673	1679	1683	rBV9	2519	6212	0.12%	0.014%
19	13.616	1767	1773	1782	rVB	24578	41267	0.79%	0.092%
20	14.140	1855	1862	1873	rBV	1700164	2435121	46.36%	5.421%
21	14.245	1879	1880	1885	rVB5	6555	6709	0.13%	0.015%
22	14.322	1889	1893	1899	rVB2	8795	11894	0.23%	0.026%
23	14.428	1903	1911	1926	rBV	1723823	2614893	49.78%	5.821%
24	14.734	1954	1963	1973	rBV	1448185	2090453	39.80%	4.654%
25	14.975	1997	2004	2015	rBV3	37617	127122	2.42%	0.283%
26	15.140	2029	2032	2038	rVB7	6726	11766	0.22%	0.026%
27	15.545	2097	2101	2106	rVB3	6040	8162	0.16%	0.018%
28	15.722	2125	2131	2147	rBV	2295777	3484582	66.33%	7.757%
29	15.851	2147	2153	2169	rVV	836969	1309581	24.93%	2.915%
30	15.963	2169	2172	2179	rVB5	13242	27067	0.52%	0.060%
31	16.087	2187	2193	2207	rBV	427836	622996	11.86%	1.387%
32	16.510	2262	2265	2271	rVB8	4960	6667	0.13%	0.015%
33	16.651	2284	2289	2299	rBV	106309	157750	3.00%	0.351%
34	16.881	2325	2328	2335	rBV8	4456	7248	0.14%	0.016%
35	17.075	2357	2361	2367	rVB8	6310	11106	0.21%	0.025%
36	17.163	2372	2376	2382	rBV8	7987	16015	0.30%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015513.D
 Acq On : 14 Jun 2023 12:40
 Operator : MA/JU
 Sample : 03098-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	17.281	2393	2396	2399	rVB5	4548	5901	0.11%	0.013%
38	17.363	2406	2410	2411	rBV4	4037	5427	0.10%	0.012%
39	17.486	2424	2431	2442	rBV	1925827	2723407	51.84%	6.063%
40	17.586	2442	2448	2468	rVB2	2815220	4069000	77.46%	9.058%
41	17.757	2474	2477	2482	rVB4	6460	9920	0.19%	0.022%
42	18.128	2538	2540	2545	rVV6	5293	6383	0.12%	0.014%
43	18.186	2546	2550	2553	rVB5	4768	6657	0.13%	0.015%
44	18.345	2572	2577	2585	rBV	127548	189136	3.60%	0.421%
45	18.422	2587	2590	2597	rVB	25690	39123	0.74%	0.087%
46	19.386	2750	2754	2759	rBV	42356	59227	1.13%	0.132%
47	19.457	2762	2766	2774	rVB2	51118	76959	1.47%	0.171%
48	19.569	2781	2785	2794	rBV3	59537	96964	1.85%	0.216%
49	19.810	2820	2826	2837	rBV	4091232	5253022	100.00%	11.694%
50	21.245	3067	3070	3079	rBV6	90743	181703	3.46%	0.404%
51	21.569	3120	3125	3134	rBV	2156100	3016516	57.42%	6.715%
52	23.951	3522	3530	3542	rBV2	2469241	5125506	97.57%	11.410%
53	24.116	3551	3558	3571	rVB	1413313	3074463	58.53%	6.844%




Sum of corrected areas: 44921196

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015513.D
Acq On : 14 Jun 2023 12:40
Operator : MA/JU
Sample : 03098-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

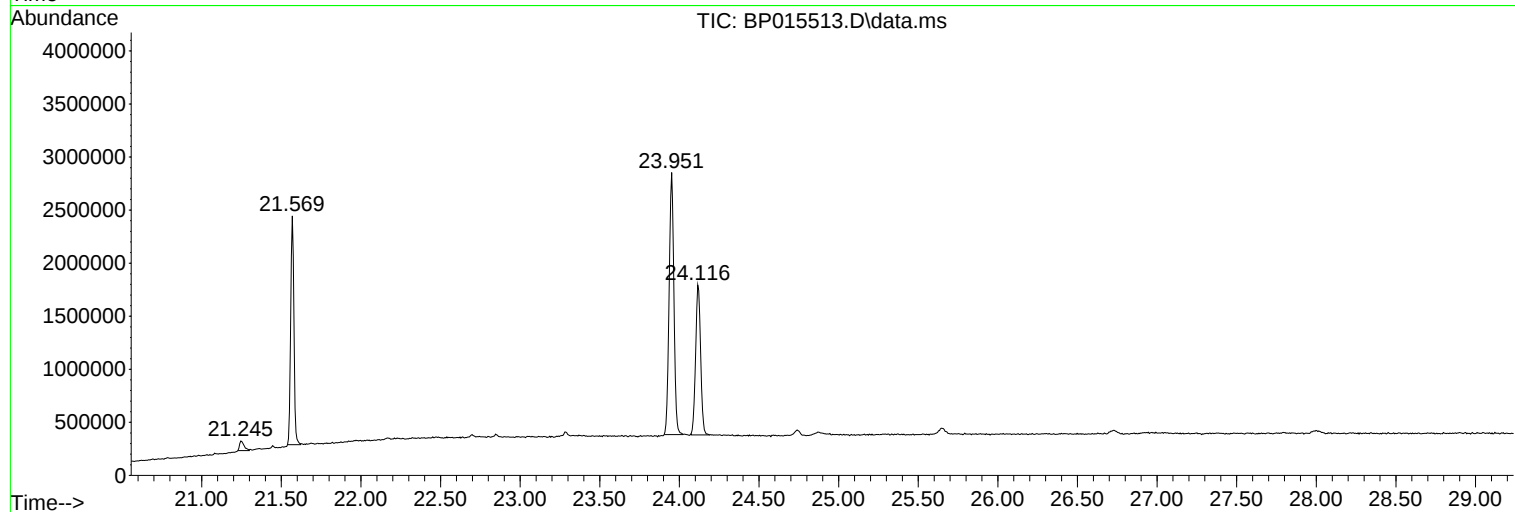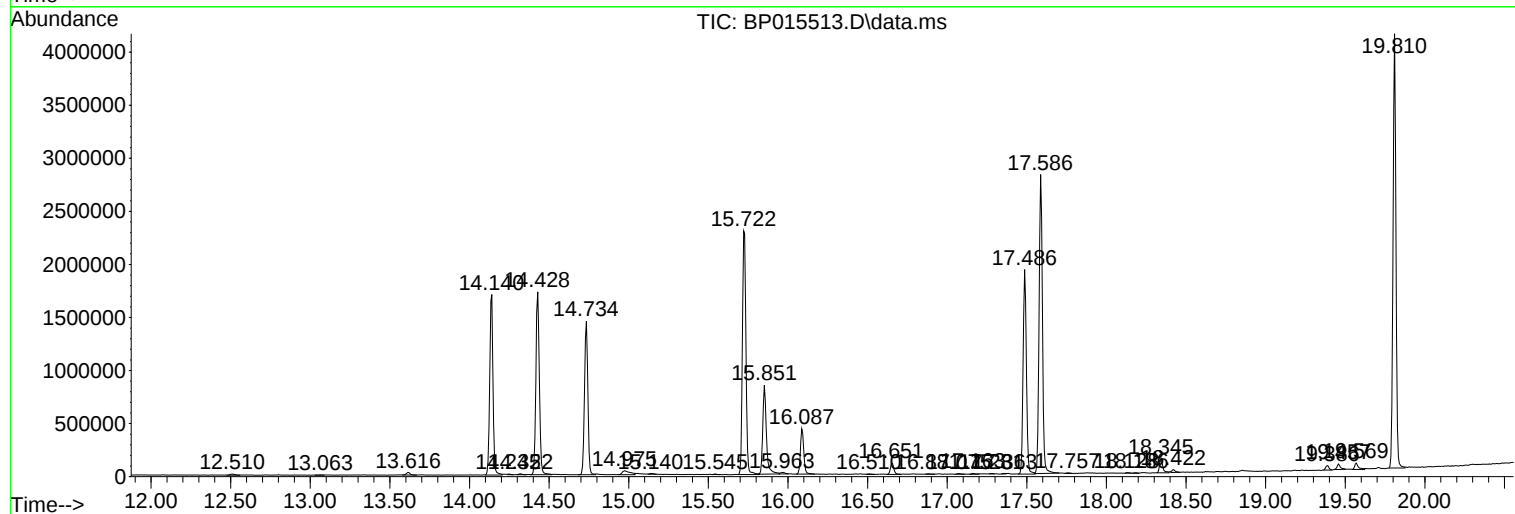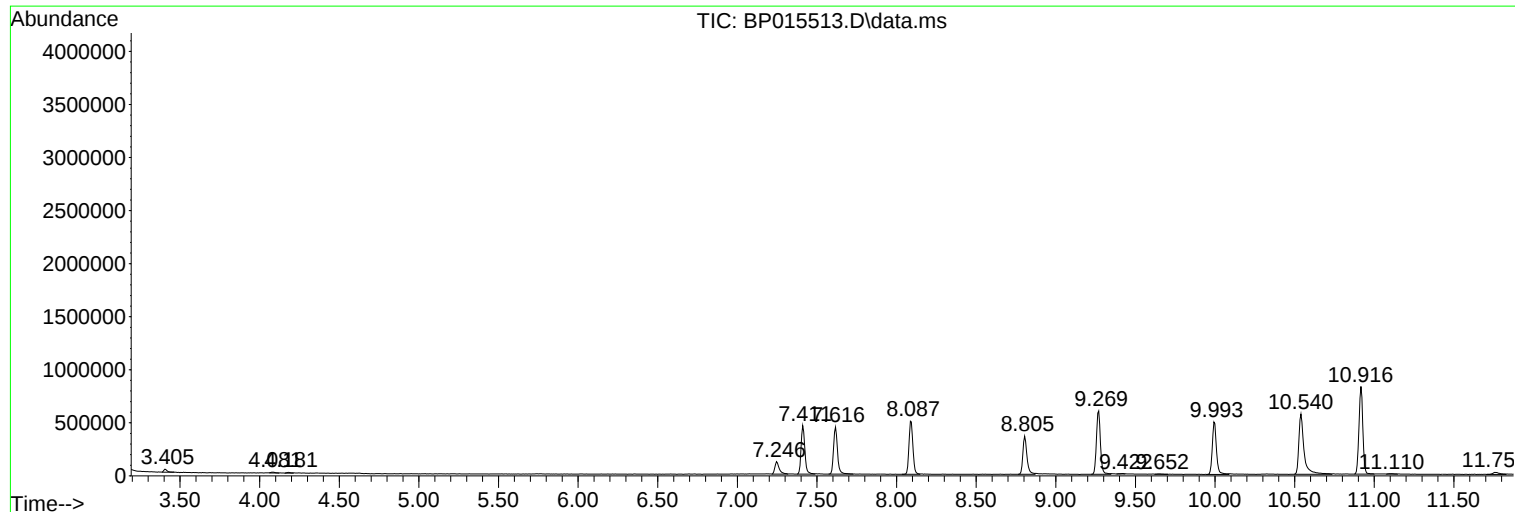

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015513.D
Acq On : 14 Jun 2023 12:40
Operator : MA/JU
Sample : 03098-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.087	5.96 ng/ul	622996	Acenaphthene-d10	14.734

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	91
5			1,2,4,5-Tetroxane, 3,3,6,6-tetra...	396	C26H20O4	016204-36-7	64

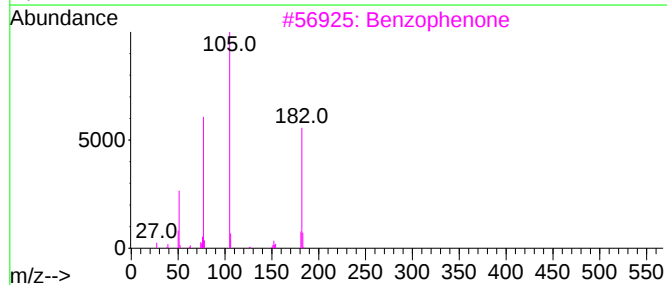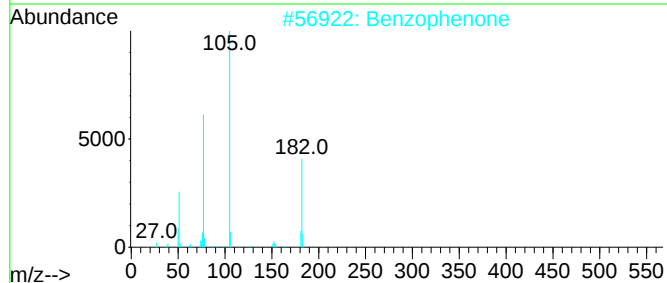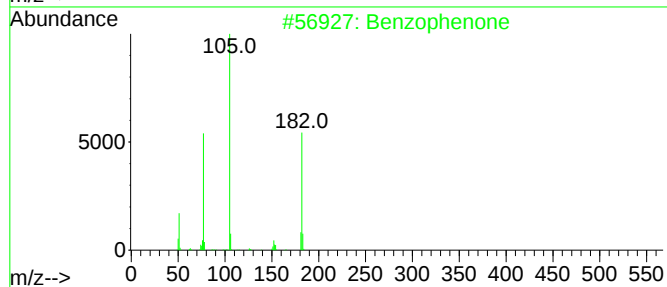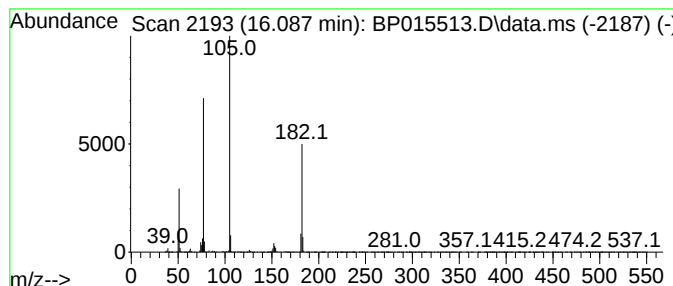

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015513.D
Acq On : 14 Jun 2023 12:40
Operator : MA/JU
Sample : 03098-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	16.087	6.0	ng/u1	622996	3	14.734	2090450	20.0