

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015515.D
 Acq On : 14 Jun 2023 13:48
 Operator : MA/JU
 Sample : 03098-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	34	37	43	rBV	32267	46412	0.81%	0.099%
2	4.081	148	152	157	rVB3	9713	14503	0.25%	0.031%
3	4.181	166	169	174	rBV2	7779	9757	0.17%	0.021%
4	7.246	684	690	704	rBV	120555	227099	3.96%	0.485%
5	7.410	711	718	730	rBV	475639	769573	13.41%	1.644%
6	7.616	745	753	763	rBV	462031	784347	13.67%	1.675%
7	7.693	764	766	773	rVB7	5306	6866	0.12%	0.015%
8	8.087	826	833	846	rBV	532035	893383	15.57%	1.908%
9	8.804	948	955	968	rBV	369798	665612	11.60%	1.422%
10	9.269	1024	1034	1045	rBV	619137	1093496	19.06%	2.335%
11	9.993	1148	1157	1171	rBV	504965	904235	15.76%	1.931%
12	10.540	1242	1250	1274	rBV	580937	1266312	22.07%	2.704%
13	10.916	1306	1314	1326	rBV	861656	1422310	24.79%	3.038%
14	11.763	1450	1458	1469	rBV10	11133	35885	0.63%	0.077%
15	12.510	1579	1585	1592	rBV2	11793	23151	0.40%	0.049%
16	13.616	1765	1773	1778	rBV	38612	62814	1.09%	0.134%
17	14.139	1854	1862	1875	rBV	1707142	2401052	41.85%	5.128%
18	14.239	1877	1879	1886	rVV7	7613	14166	0.25%	0.030%
19	14.316	1889	1892	1898	rVB	7461	12086	0.21%	0.026%
20	14.428	1903	1911	1922	rBV	1793357	2627432	45.80%	5.611%
21	14.734	1956	1963	1972	rBV	1445874	2086179	36.36%	4.455%
22	14.969	1997	2003	2016	rBV4	36633	131124	2.29%	0.280%
23	15.545	2097	2101	2106	rVB7	3470	6061	0.11%	0.013%
24	15.728	2125	2132	2147	rBV	2340685	3413650	59.50%	7.290%
25	15.851	2147	2153	2169	rVV	808134	1272417	22.18%	2.717%
26	15.969	2170	2173	2180	rVB4	15726	25402	0.44%	0.054%
27	16.086	2188	2193	2209	rVB	514052	743847	12.97%	1.589%
28	16.657	2284	2290	2297	rBV	98042	142482	2.48%	0.304%
29	17.075	2357	2361	2366	rVB7	6362	9001	0.16%	0.019%
30	17.163	2373	2376	2380	rVB5	4576	5879	0.10%	0.013%
31	17.216	2383	2385	2389	rBV5	5614	8063	0.14%	0.017%
32	17.363	2407	2410	2414	rBV6	5318	9599	0.17%	0.021%
33	17.486	2425	2431	2442	rBV	1832515	2714574	47.32%	5.797%
34	17.592	2442	2449	2469	rVB	2667926	4035871	70.35%	8.619%
35	17.957	2508	2511	2518	rVB9	6603	8779	0.15%	0.019%
36	18.133	2537	2541	2546	rBV5	11243	15879	0.28%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015515.D
 Acq On : 14 Jun 2023 13:48
 Operator : MA/JU
 Sample : 03098-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	18.345	2572	2577	2584	rBV	143579	199723	3.48%	0.427%
38	18.422	2586	2590	2597	rVB	20414	38627	0.67%	0.082%
39	18.622	2622	2624	2626	rBV3	8601	7412	0.13%	0.016%
40	19.386	2750	2754	2759	rBV	47258	65039	1.13%	0.139%
41	19.457	2763	2766	2772	rVV	52536	79023	1.38%	0.169%
42	19.510	2772	2775	2779	rVV2	34664	40285	0.70%	0.086%
43	19.569	2781	2785	2792	rBV4	59813	94164	1.64%	0.201%
44	19.810	2820	2826	2836	rBV	4087214	5513985	96.11%	11.776%
45	21.251	3067	3071	3081	rBV3	142116	288798	5.03%	0.617%
46	21.568	3120	3125	3137	rBV	2480207	3424481	59.69%	7.314%
47	23.951	3523	3530	3542	rVB2	2720478	5737187	100.00%	12.253%
48	24.115	3551	3558	3570	rVB	1525141	3425257	59.70%	7.315%




Sum of corrected areas: 46823279

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015515.D
Acq On : 14 Jun 2023 13:48
Operator : MA/JU
Sample : 03098-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEP7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

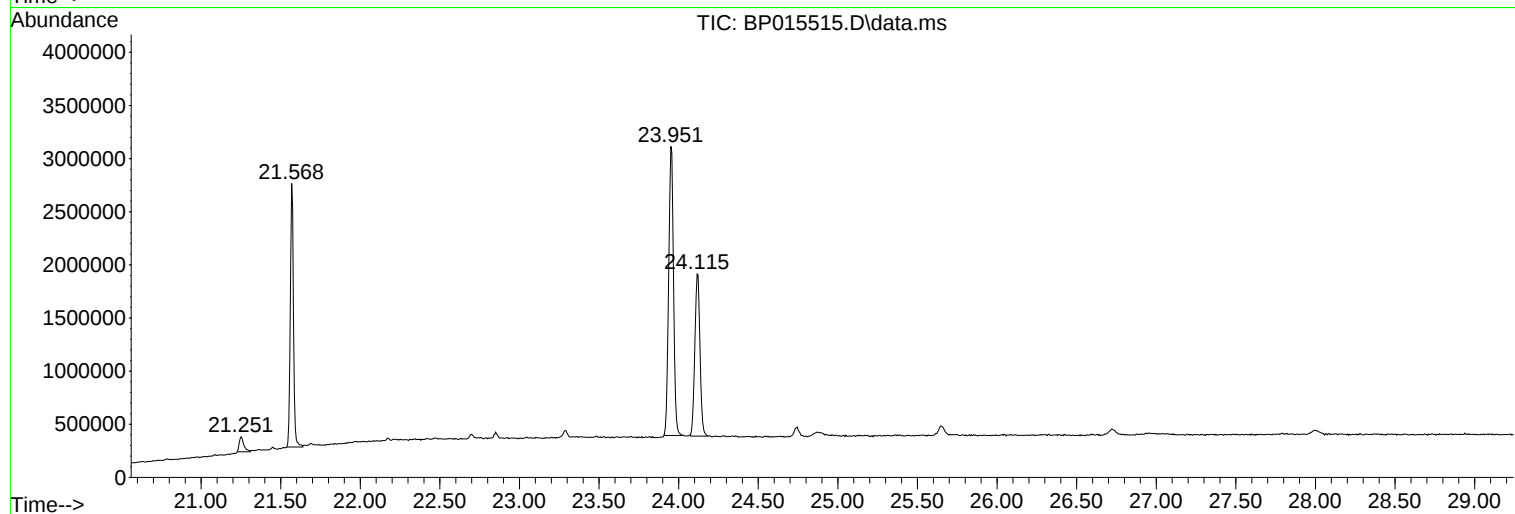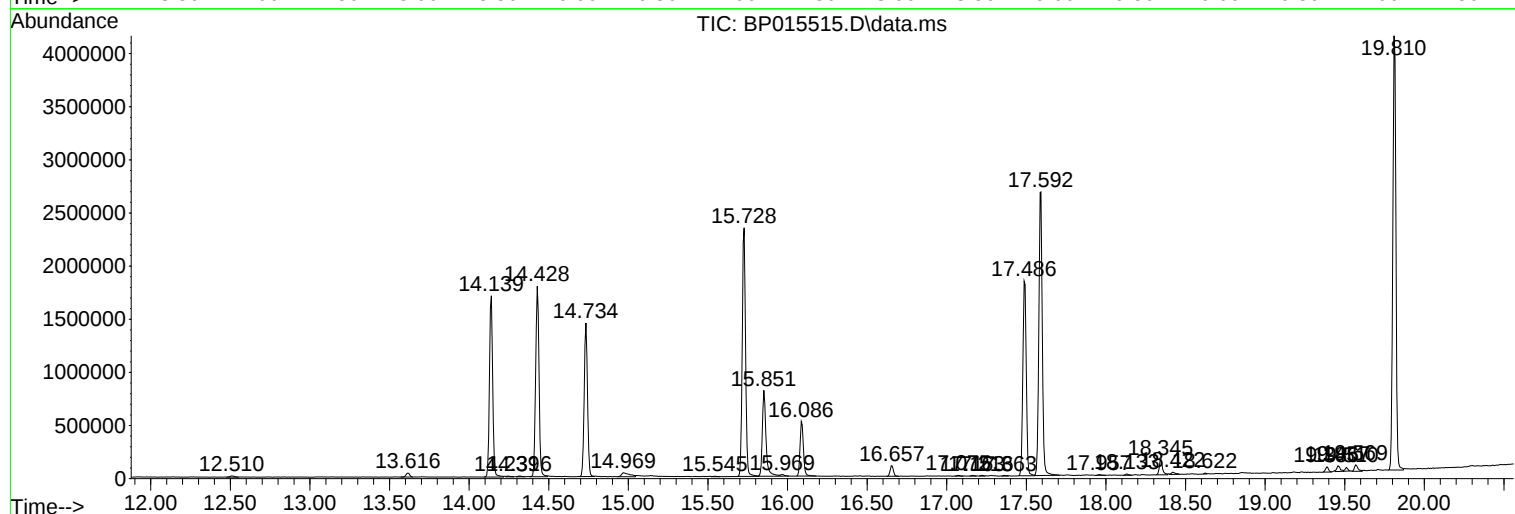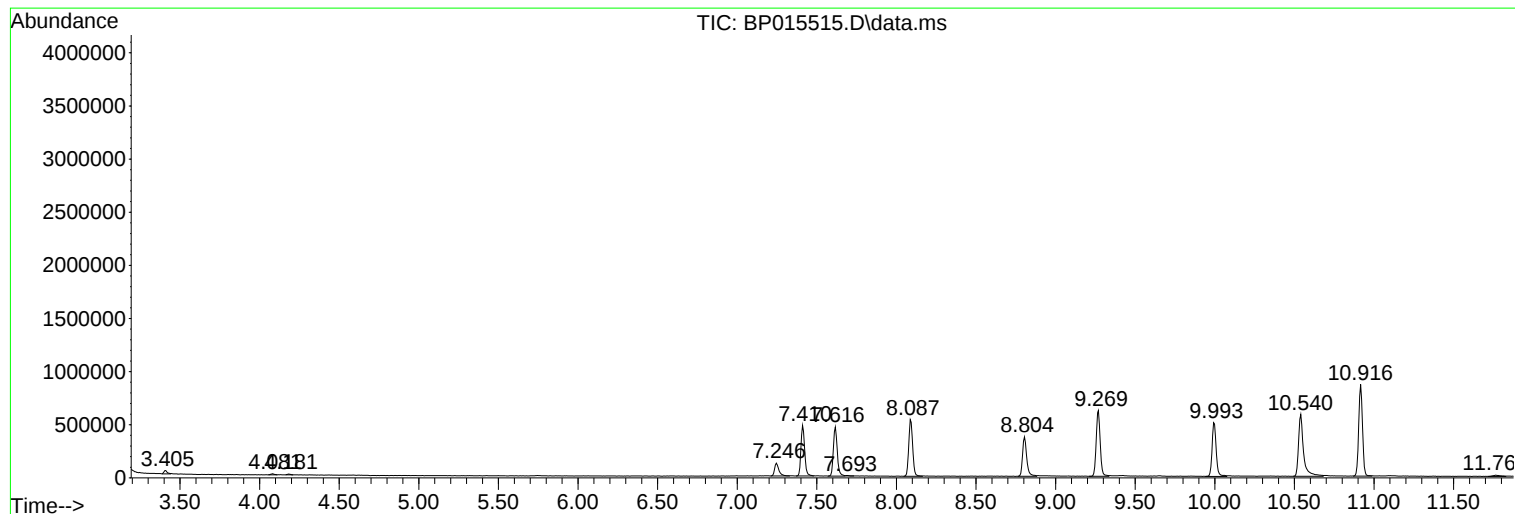

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015515.D
Acq On : 14 Jun 2023 13:48
Operator : MA/JU
Sample : 03098-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEP7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.086	7.13 ng/ul	743847	Acenaphthene-d10	14.733

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	95
5			Benzophenone	182	C13H10O	000119-61-9	91

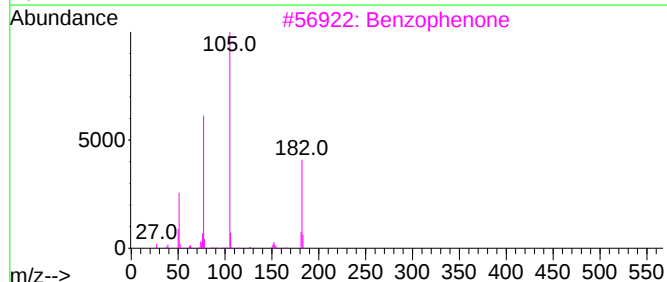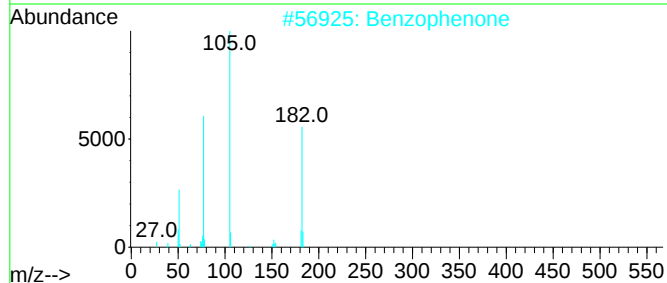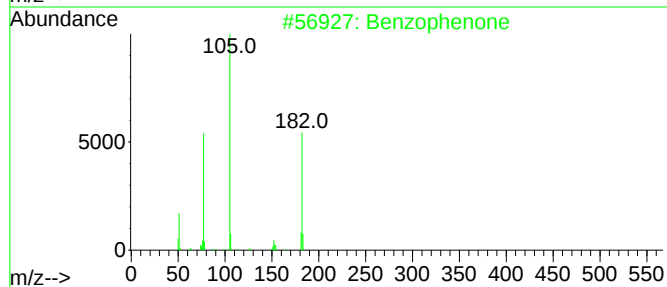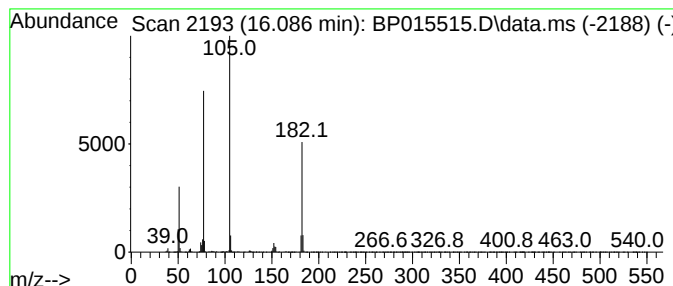

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015515.D
Acq On : 14 Jun 2023 13:48
Operator : MA/JU
Sample : 03098-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	16.086	7.1	ng/ul	743847	3	14.733	2086180	20.0