

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015519.D
 Acq On : 14 Jun 2023 16:03
 Operator : MA/JU
 Sample : 03104-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	34	37	42	rVB	27432	37620	0.62%	0.077%
2	3.869	114	116	125	rBV	45625	91829	1.51%	0.187%
3	4.081	148	152	158	rVB4	8630	14632	0.24%	0.030%
4	4.187	166	170	175	rVB6	7164	11886	0.20%	0.024%
5	4.728	258	262	269	rVB9	7392	12073	0.20%	0.025%
6	5.152	329	334	346	rVB	18566	32318	0.53%	0.066%
7	6.110	493	497	504	rVB6	6186	9823	0.16%	0.020%
8	7.246	684	690	705	rVB	118491	219279	3.61%	0.447%
9	7.410	712	718	730	rBV	590372	936541	15.42%	1.908%
10	7.616	745	753	763	rBV	541477	925505	15.24%	1.886%
11	8.093	826	834	845	rBV	425642	726392	11.96%	1.480%
12	8.804	948	955	973	rBV	438271	770767	12.69%	1.570%
13	9.269	1024	1034	1047	rBV	777767	1343635	22.12%	2.737%
14	9.428	1058	1061	1068	rVB9	3092	6171	0.10%	0.013%
15	9.993	1148	1157	1174	rBV	655144	1163408	19.15%	2.370%
16	10.534	1240	1249	1273	rBV	776710	1569074	25.83%	3.197%
17	10.916	1306	1314	1325	rVB	704756	1195629	19.68%	2.436%
18	11.057	1331	1338	1361	rBV	478049	1056332	17.39%	2.152%
19	12.522	1579	1587	1594	rBV4	13330	34531	0.57%	0.070%
20	13.610	1767	1772	1780	rBV3	16827	33955	0.56%	0.069%
21	14.139	1853	1862	1877	rBV	2038480	2922175	48.11%	5.953%
22	14.428	1903	1911	1930	rBV2	2319176	3373073	55.53%	6.872%
23	14.734	1956	1963	1973	rBV	1223223	1786543	29.41%	3.640%
24	14.981	1998	2005	2016	rBV5	28742	109446	1.80%	0.223%
25	15.728	2125	2132	2147	rBV	2813683	4216334	69.42%	8.590%
26	15.851	2147	2153	2169	rVV	941247	1495642	24.62%	3.047%
27	15.969	2170	2173	2178	rVB4	17269	26071	0.43%	0.053%
28	16.428	2247	2251	2255	rBV7	3197	6375	0.10%	0.013%
29	17.280	2390	2396	2398	rBV6	4200	8352	0.14%	0.017%
30	17.486	2424	2431	2441	rBV	1617011	2348483	38.66%	4.785%
31	17.592	2442	2449	2466	rVB	3173714	4967654	81.79%	10.121%
32	18.351	2573	2578	2584	rBV3	41602	66351	1.09%	0.135%
33	18.427	2588	2591	2594	rVB2	6487	8822	0.15%	0.018%
34	19.392	2750	2755	2760	rBV2	50040	74795	1.23%	0.152%
35	19.463	2761	2767	2770	rBV	50423	82330	1.36%	0.168%
36	19.574	2783	2786	2792	rBV5	26911	39297	0.65%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015519.D
Acq On : 14 Jun 2023 16:03
Operator : MA/JU
Sample : 03104-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	19.816	2820	2827	2841	rBV	4309429	6056671	99.72%	12.340%
38	21.568	3120	3125	3138	rBV	1834429	2675762	44.05%	5.451%
39	23.951	3523	3530	3543	rVB2	2857205	6073953	100.00%	12.375%
40	24.121	3552	3559	3572	rVB	1109980	2553932	42.05%	5.203%




Sum of corrected areas: 49083461

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015519.D
Acq On : 14 Jun 2023 16:03
Operator : MA/JU
Sample : 03104-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

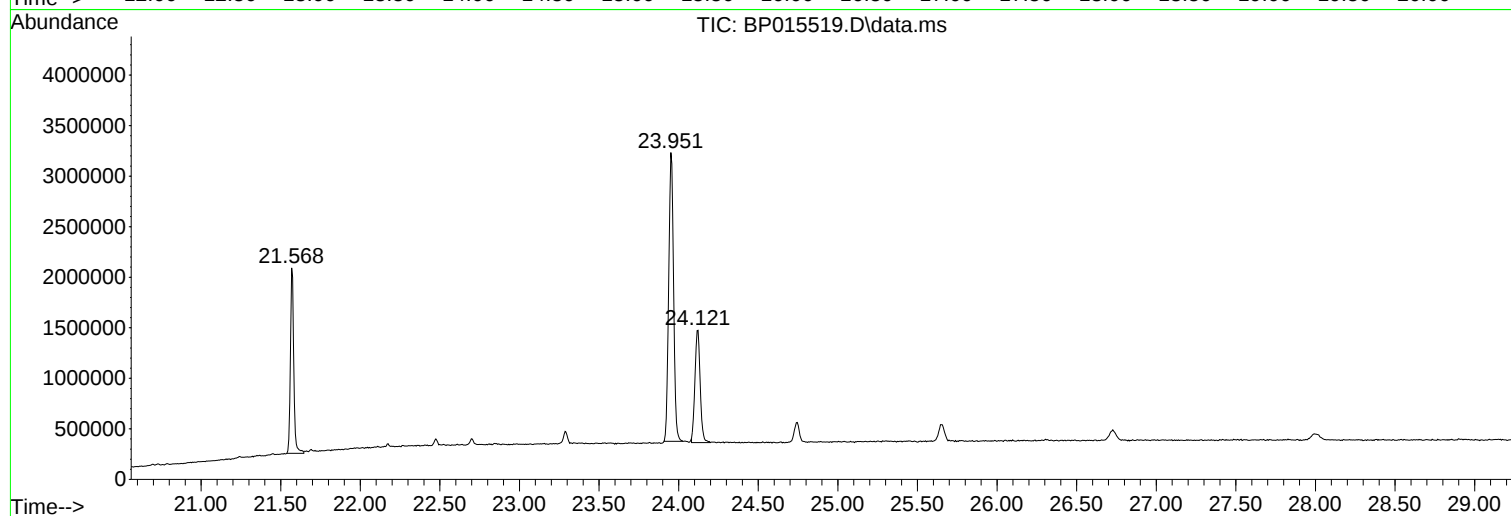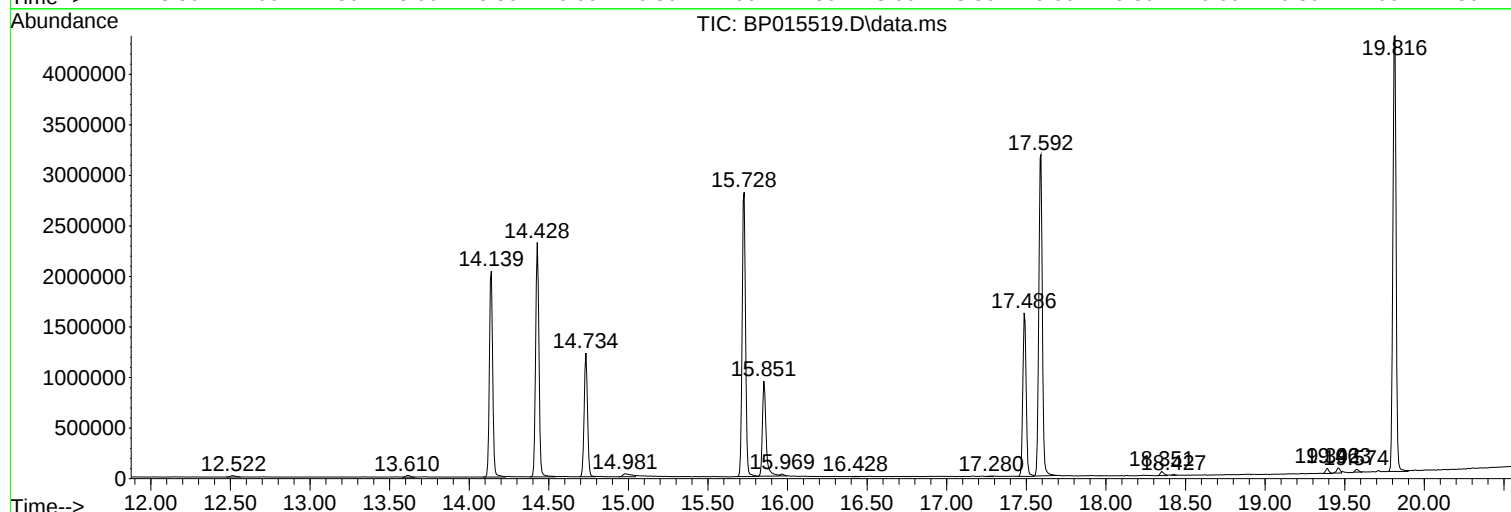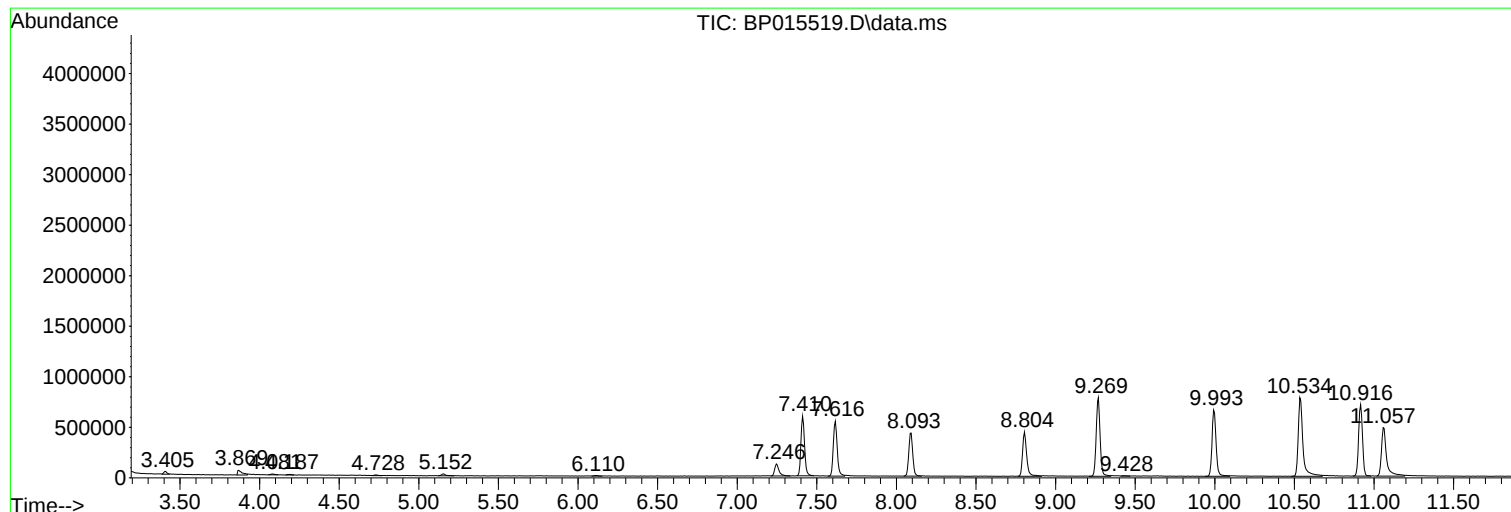

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015519.D
Acq On : 14 Jun 2023 16:03
Operator : MA/JU
Sample : 03104-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015519.D
Acq On : 14 Jun 2023 16:03
Operator : MA/JU
Sample : 03104-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0NR1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc