

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015521.D
 Acq On : 14 Jun 2023 17:11
 Operator : MA/JU
 Sample : 03104-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	27	31	34	rBV2	25550	33557	0.58%	0.076%
2	3.405	34	37	42	rVB	24055	31280	0.54%	0.071%
3	3.864	112	115	134	rBV	76176	170615	2.95%	0.388%
4	4.081	148	152	160	rVB	11425	18338	0.32%	0.042%
5	4.181	166	169	174	rBV4	10913	15432	0.27%	0.035%
6	7.246	683	690	702	rBV	118024	217840	3.76%	0.495%
7	7.411	712	718	730	rBV	531384	841768	14.54%	1.914%
8	7.616	745	753	763	rBV	503345	849716	14.68%	1.932%
9	8.087	824	833	846	rBV	360004	615318	10.63%	1.399%
10	8.805	947	955	975	rBV	402895	727798	12.57%	1.655%
11	9.263	1026	1033	1044	rBV	675699	1196025	20.66%	2.720%
12	9.993	1149	1157	1170	rBV	578210	1004956	17.36%	2.286%
13	10.534	1242	1249	1267	rBV	679526	1374917	23.75%	3.127%
14	10.916	1307	1314	1321	rBV	581813	986008	17.03%	2.242%
15	11.063	1329	1339	1356	rBV	335354	758743	13.11%	1.726%
16	12.516	1578	1586	1595	rBV5	11180	24416	0.42%	0.056%
17	13.546	1756	1761	1763	rBV6	4021	6134	0.11%	0.014%
18	13.616	1768	1773	1778	rVB4	11946	20983	0.36%	0.048%
19	14.140	1855	1862	1875	rBV	1863892	2690056	46.47%	6.118%
20	14.428	1904	1911	1929	rBV	2065523	2984536	51.55%	6.788%
21	14.598	1937	1940	1945	rVB7	3229	5864	0.10%	0.013%
22	14.734	1956	1963	1973	rBV	962356	1461485	25.24%	3.324%
23	14.981	1997	2005	2019	rBV4	30579	126315	2.18%	0.287%
24	15.145	2029	2033	2042	rVB4	5361	13867	0.24%	0.032%
25	15.728	2125	2132	2147	rBV	2567870	3880087	67.02%	8.824%
26	15.851	2147	2153	2169	rVV	885708	1403074	24.24%	3.191%
27	15.969	2170	2173	2179	rVB5	15920	27465	0.47%	0.062%
28	16.092	2188	2194	2202	rBV	83177	123946	2.14%	0.282%
29	16.516	2262	2266	2271	rVB8	3875	6653	0.11%	0.015%
30	17.169	2372	2377	2381	rBV7	4394	7969	0.14%	0.018%
31	17.281	2392	2396	2401	rBV8	4365	6846	0.12%	0.016%
32	17.486	2425	2431	2441	rBV	1341598	1888482	32.62%	4.295%
33	17.586	2442	2448	2473	rVV	3113382	4788110	82.71%	10.889%
34	17.763	2476	2478	2482	rVB5	5643	6238	0.11%	0.014%
35	18.134	2539	2541	2545	rVB5	5785	6011	0.10%	0.014%
36	18.345	2573	2577	2587	rBV4	60866	100756	1.74%	0.229%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015521.D
Acq On : 14 Jun 2023 17:11
Operator : MA/JU
Sample : 03104-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONQ6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	19.386	2750	2754	2759	rBV2	46437	69083	1.19%	0.157%
38	19.457	2762	2766	2774	rVB	42049	69895	1.21%	0.159%
39	19.569	2782	2785	2793	rBV5	42892	67837	1.17%	0.154%
40	19.810	2820	2826	2835	rBV	4258562	5789240	100.00%	13.166%
41	21.569	3120	3125	3136	rBV	1410490	2127218	36.74%	4.838%
42	23.957	3523	3531	3545	rVB2	2536576	5436296	93.90%	12.364%
43	24.121	3552	3559	3571	rVB	867991	1989111	34.36%	4.524%




Sum of corrected areas: 43970284

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015521.D
Acq On : 14 Jun 2023 17:11
Operator : MA/JU
Sample : 03104-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONQ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

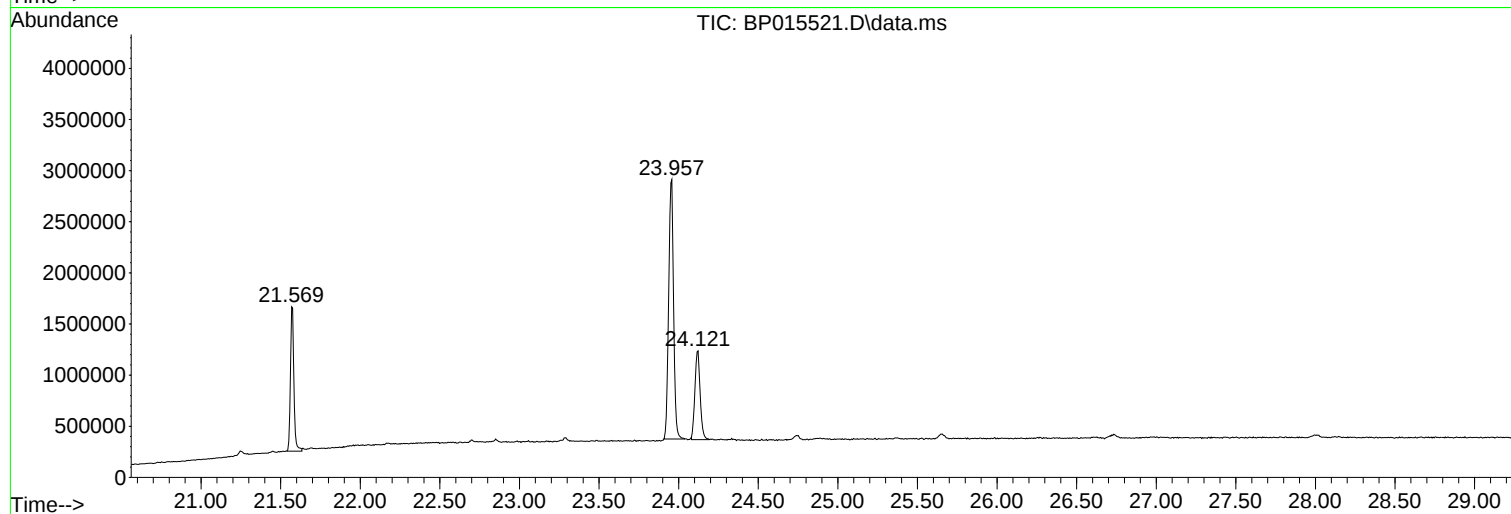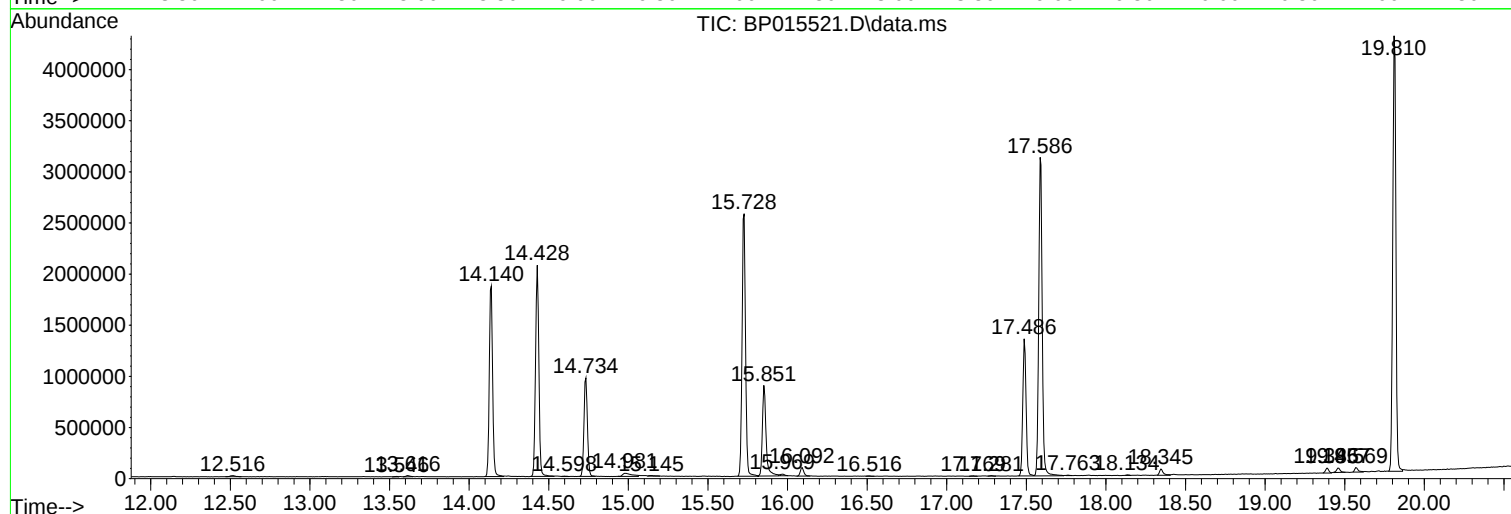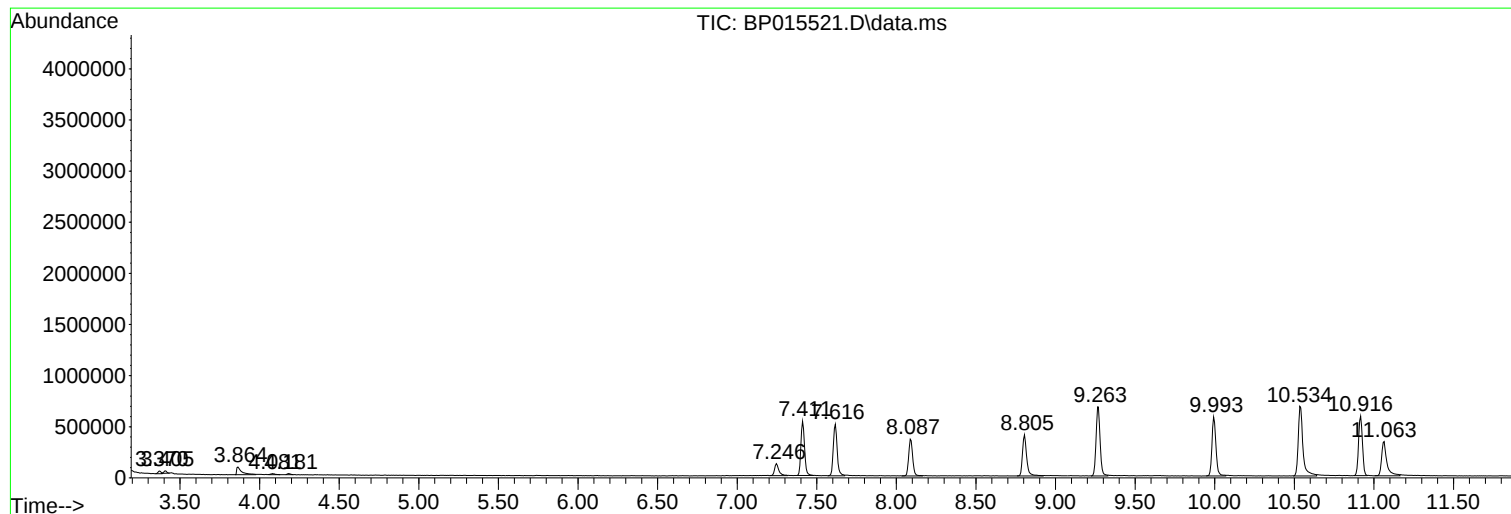

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015521.D
Acq On : 14 Jun 2023 17:11
Operator : MA/JU
Sample : 03104-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONQ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015521.D
Acq On : 14 Jun 2023 17:11
Operator : MA/JU
Sample : 03104-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONQ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------