

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015523.D
 Acq On : 14 Jun 2023 18:18
 Operator : MA/JU
 Sample : PB153379BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK379

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	49	rVB	47630	75221	1.43%	0.153%
2	3.852	110	113	132	rBV	209222	406595	7.71%	0.827%
3	4.175	167	168	175	rVB6	7417	9244	0.18%	0.019%
4	7.240	681	689	705	rBV	628450	1083374	20.54%	2.203%
5	7.411	711	718	728	rBV	523990	819291	15.53%	1.666%
6	7.616	745	753	765	rBV	640460	1102381	20.90%	2.242%
7	8.087	824	833	843	rBV	494183	820882	15.56%	1.669%
8	8.799	946	954	970	rBV	812547	1459260	27.67%	2.967%
9	9.263	1025	1033	1045	rBV	674642	1196067	22.68%	2.432%
10	9.993	1149	1157	1169	rBV	614737	1064737	20.19%	2.165%
11	10.075	1169	1171	1179	rVB9	5915	13816	0.26%	0.028%
12	10.534	1241	1249	1272	rBV	763918	1538058	29.16%	3.128%
13	10.916	1305	1314	1327	rBV	783590	1346032	25.52%	2.737%
14	11.063	1331	1339	1360	rBV	332131	776188	14.72%	1.578%
15	11.234	1366	1368	1375	rVB8	4064	6939	0.13%	0.014%
16	12.510	1579	1585	1594	rBV5	11635	25893	0.49%	0.053%
17	12.804	1627	1635	1641	rBV7	4544	10053	0.19%	0.020%
18	12.957	1654	1661	1664	rBV8	4460	8932	0.17%	0.018%
19	13.210	1696	1704	1709	rBV8	2577	6752	0.13%	0.014%
20	13.328	1716	1724	1727	rBV10	3216	5981	0.11%	0.012%
21	13.545	1757	1761	1765	rBV7	4849	7881	0.15%	0.016%
22	13.616	1768	1773	1780	rVB5	15531	32573	0.62%	0.066%
23	14.134	1854	1861	1876	rBV	1750770	2606664	49.42%	5.301%
24	14.428	1903	1911	1927	rBV	1996742	2963527	56.19%	6.026%
25	14.734	1956	1963	1971	rBV	1356053	1980703	37.55%	4.028%
26	14.798	1971	1974	1979	rVB2	9675	13485	0.26%	0.027%
27	14.940	1991	1998	2016	rBV	416085	1095476	20.77%	2.228%
28	15.369	2067	2071	2076	rVV6	6097	8272	0.16%	0.017%
29	15.545	2096	2101	2105	rVB	7954	11020	0.21%	0.022%
30	15.728	2125	2132	2138	rBV	2488519	3663082	69.45%	7.449%
31	15.851	2147	2153	2168	rBV	843154	1314535	24.92%	2.673%
32	15.963	2169	2172	2182	rVB8	17245	42882	0.81%	0.087%
33	16.516	2261	2266	2269	rVB7	3701	5514	0.10%	0.011%
34	16.675	2288	2293	2298	rVB9	6357	10869	0.21%	0.022%
35	16.786	2307	2312	2317	rBV7	9447	14499	0.27%	0.029%
36	16.969	2336	2343	2346	rVB8	3628	5625	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015523.D
 Acq On : 14 Jun 2023 18:18
 Operator : MA/JU
 Sample : PB153379BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK379

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	17.163	2373	2376	2382	rVB8	4555	6384	0.12%	0.013%
38	17.281	2392	2396	2402	rVB5	4769	9560	0.18%	0.019%
39	17.486	2425	2431	2442	rBV	1818304	2630771	49.88%	5.350%
40	17.586	2442	2448	2468	rVB	2917932	4283572	81.21%	8.711%
41	17.916	2498	2504	2506	rBV6	4549	7072	0.13%	0.014%
42	18.422	2587	2590	2595	rVB2	6752	9329	0.18%	0.019%
43	19.392	2751	2755	2760	rVB2	42256	56599	1.07%	0.115%
44	19.463	2762	2767	2770	rBV	36987	57268	1.09%	0.116%
45	19.810	2820	2826	2840	rBV	3944285	5274427	100.00%	10.726%
46	21.569	3120	3125	3139	rBV	2063060	3065401	58.12%	6.234%
47	23.951	3523	3530	3544	rVB2	2439637	5249389	99.53%	10.675%
48	24.121	3551	3559	3575	rVB	1311716	2972866	56.36%	6.045%




Sum of corrected areas: 49174941

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015523.D
Acq On : 14 Jun 2023 18:18
Operator : MA/JU
Sample : PB153379BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

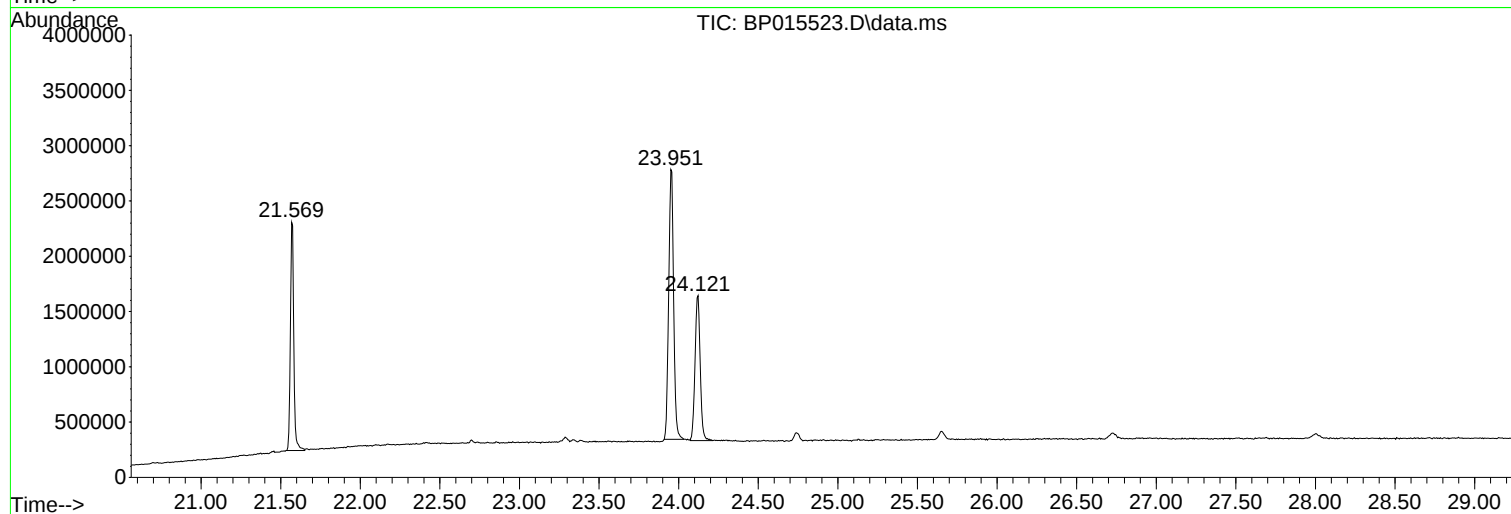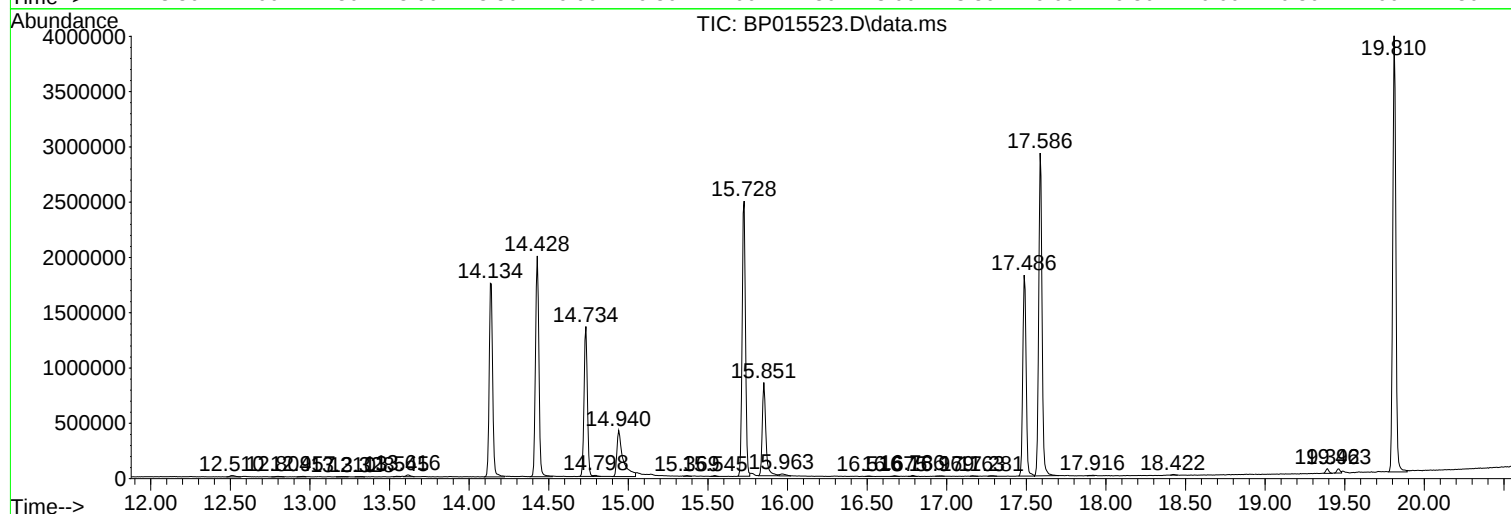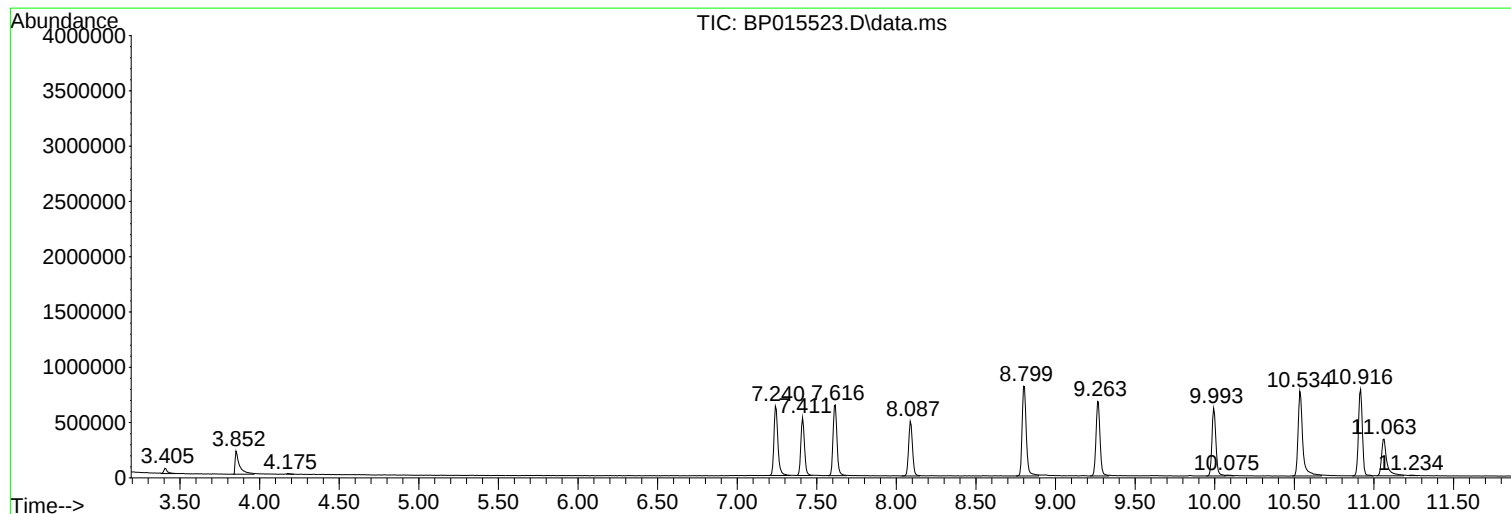

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015523.D
Acq On : 14 Jun 2023 18:18
Operator : MA/JU
Sample : PB153379BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015523.D
Acq On : 14 Jun 2023 18:18
Operator : MA/JU
Sample : PB153379BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------