

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015531.D
 Acq On : 14 Jun 2023 22:49
 Operator : MA/JU
 Sample : 03104-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	26	31	35	rBV	236172	344192	5.01%	0.624%
2	3.864	113	115	128	rBV	80267	163165	2.38%	0.296%
3	4.075	148	151	158	rVB2	11498	18932	0.28%	0.034%
4	4.181	167	169	177	rVB5	9430	12877	0.19%	0.023%
5	7.246	683	690	703	rBV	167648	304332	4.43%	0.552%
6	7.410	711	718	729	rBV	598260	940747	13.70%	1.705%
7	7.610	746	752	764	rBV	594231	1010596	14.72%	1.832%
8	8.087	825	833	843	rBV	549094	889597	12.96%	1.613%
9	8.799	948	954	971	rBV	512632	903273	13.16%	1.637%
10	9.263	1024	1033	1046	rBV	824271	1394403	20.31%	2.528%
11	9.646	1091	1098	1102	rVB7	5263	11292	0.16%	0.020%
12	9.993	1148	1157	1171	rBV	702298	1204661	17.55%	2.184%
13	10.534	1240	1249	1273	rBV	865817	1662909	24.22%	3.014%
14	10.916	1304	1314	1321	rBV	830119	1425973	20.77%	2.585%
15	11.057	1330	1338	1362	rBV	611822	1276969	18.60%	2.315%
16	12.145	1520	1523	1527	rVB5	5180	7316	0.11%	0.013%
17	12.510	1577	1585	1595	rBV2	12670	31899	0.46%	0.058%
18	13.610	1765	1772	1780	rBV4	10012	18493	0.27%	0.034%
19	14.134	1855	1861	1877	rBV	2053459	3019958	43.99%	5.474%
20	14.428	1903	1911	1922	rBV	2251070	3359185	48.93%	6.089%
21	14.734	1955	1963	1978	rBV	1392101	2106849	30.69%	3.819%
22	14.963	1996	2002	2024	rBV2	56832	229869	3.35%	0.417%
23	15.475	2083	2089	2093	rBV5	5251	8746	0.13%	0.016%
24	15.722	2125	2131	2146	rBV	2956942	4348186	63.34%	7.882%
25	15.851	2147	2153	2168	rVV	1090950	1708644	24.89%	3.097%
26	15.969	2169	2173	2180	rVB4	18939	33074	0.48%	0.060%
27	16.086	2188	2193	2203	rVB	67288	102053	1.49%	0.185%
28	16.510	2260	2265	2269	rBV8	4736	7144	0.10%	0.013%
29	17.163	2372	2376	2382	rBV9	5065	7258	0.11%	0.013%
30	17.275	2391	2395	2402	rBV5	5195	8972	0.13%	0.016%
31	17.486	2424	2431	2441	rBV	1963582	2733949	39.83%	4.956%
32	17.586	2441	2448	2465	rVV2	3652874	5298510	77.18%	9.605%
33	17.886	2495	2499	2502	rBV6	5266	7836	0.11%	0.014%
34	18.345	2572	2577	2586	rBV2	107395	164373	2.39%	0.298%
35	19.386	2750	2754	2758	rBV3	54050	70257	1.02%	0.127%
36	19.457	2762	2766	2772	rVV	60310	82738	1.21%	0.150%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015531.D
 Acq On : 14 Jun 2023 22:49
 Operator : MA/JU
 Sample : 03104-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	19.510	2772	2775	2780	rVB5	22000	28128	0.41%	0.051%
38	19.569	2781	2785	2793	rBV	135235	193850	2.82%	0.351%
39	19.810	2820	2826	2836	rBV	4906607	6559887	95.56%	11.891%
40	20.004	2857	2859	2862	rBV4	12071	12298	0.18%	0.022%
41	20.686	2972	2975	2979	rVB3	33375	38301	0.56%	0.069%
42	21.239	3067	3069	3076	rBV5	43805	77245	1.13%	0.140%
43	21.569	3120	3125	3137	rBV	2327755	3288333	47.90%	5.961%
44	23.951	3522	3530	3548	rVB2	3199895	6864894	100.00%	12.444%
45	24.115	3551	3558	3569	rVB	1466383	3184672	46.39%	5.773%




Sum of corrected areas: 55166835

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015531.D
Acq On : 14 Jun 2023 22:49
Operator : MA/JU
Sample : 03104-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONL9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

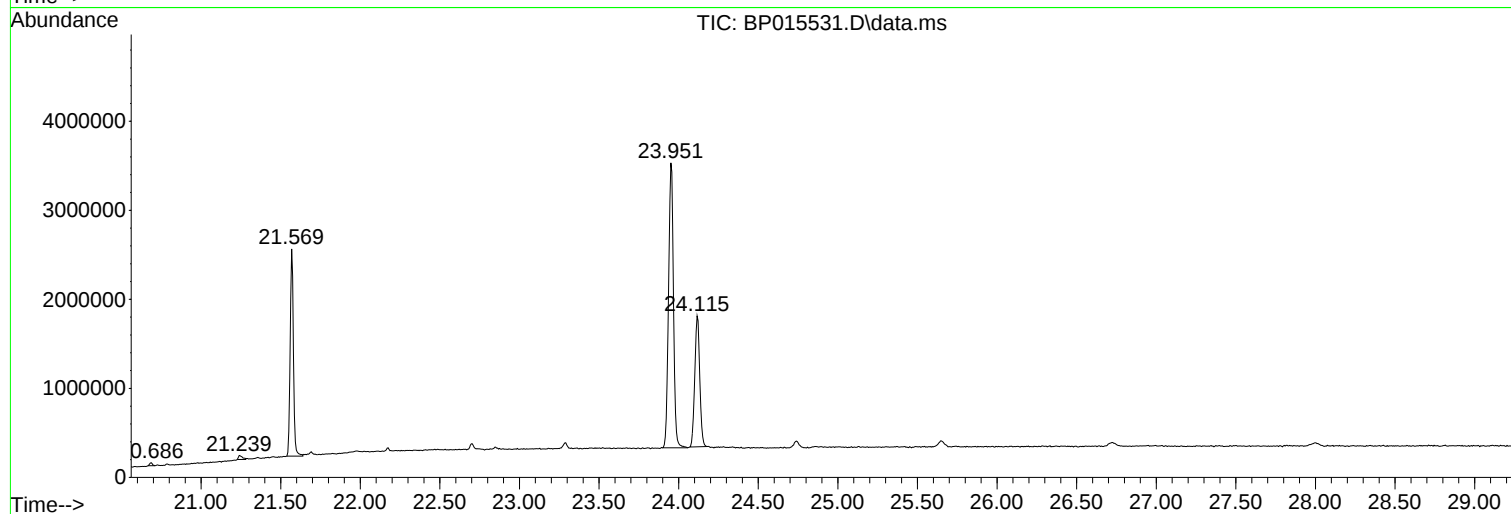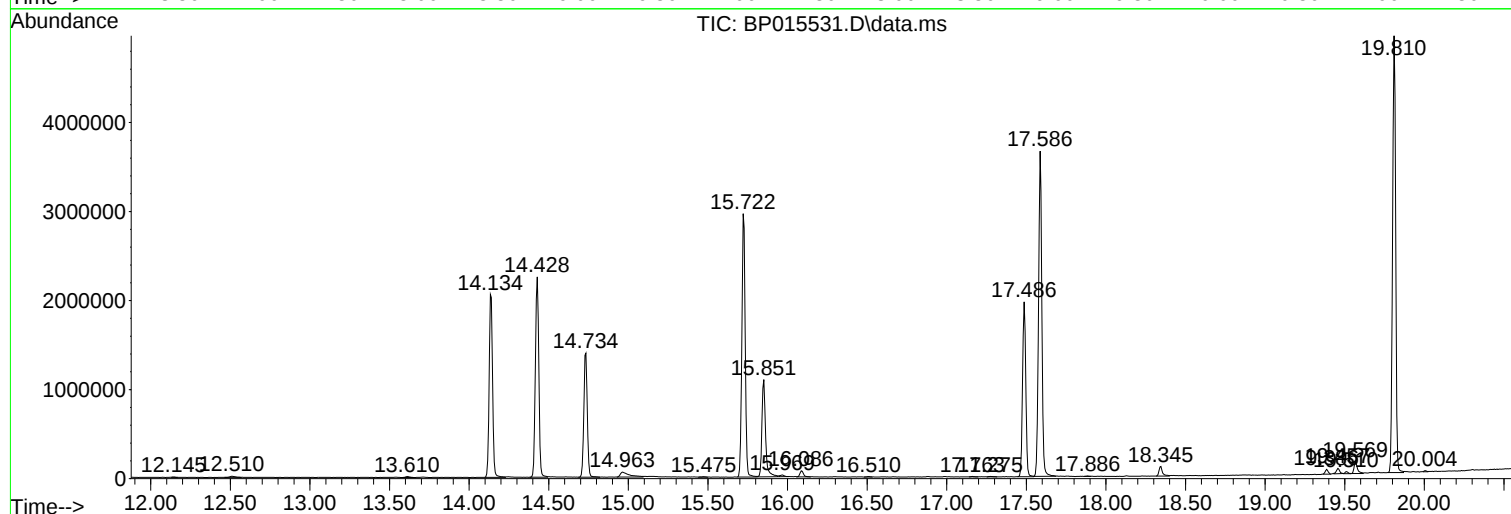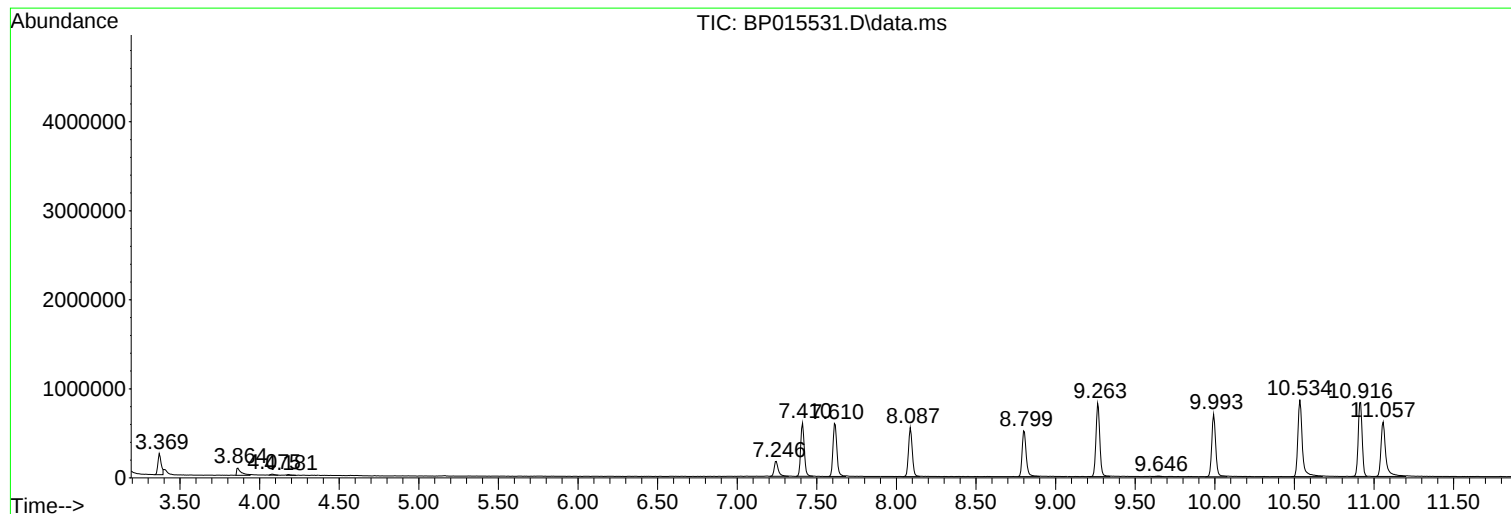

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015531.D
Acq On : 14 Jun 2023 22:49
Operator : MA/JU
Sample : 03104-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONL9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015531.D
Acq On : 14 Jun 2023 22:49
Operator : MA/JU
Sample : 03104-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONL9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc