

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015537.D
 Acq On : 15 Jun 2023 02:10
 Operator : MA/JU
 Sample : 03104-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	34	37	48	rVB	28284	44561	0.73%	0.093%
2	3.863	112	115	130	rBV	69227	150264	2.45%	0.314%
3	4.081	148	152	158	rVB3	9359	15890	0.26%	0.033%
4	4.181	165	169	174	rBV	7075	9543	0.16%	0.020%
5	5.152	330	334	339	rBV2	18307	26454	0.43%	0.055%
6	7.246	684	690	703	rBV	115056	219084	3.57%	0.458%
7	7.410	711	718	738	rVB	501548	824912	13.44%	1.726%
8	7.610	745	752	771	rBV	503256	858388	13.99%	1.796%
9	8.087	825	833	846	rBV	445422	744572	12.14%	1.557%
10	8.799	947	954	967	rBV	401792	713977	11.64%	1.493%
11	9.263	1025	1033	1050	rBV	707324	1206684	19.67%	2.524%
12	9.422	1057	1060	1070	rVB	3499	7184	0.12%	0.015%
13	9.993	1149	1157	1168	rBV	602831	1022348	16.66%	2.138%
14	10.534	1241	1249	1276	rBV	702850	1409484	22.97%	2.948%
15	10.910	1306	1313	1329	rVB	703350	1205523	19.65%	2.522%
16	11.057	1329	1338	1361	rBV	442091	971566	15.84%	2.032%
17	12.510	1581	1585	1599	rVB2	11250	27415	0.45%	0.057%
18	13.610	1767	1772	1778	rBV2	17027	28609	0.47%	0.060%
19	14.134	1854	1861	1876	rBV	1961163	2693164	43.89%	5.633%
20	14.245	1878	1880	1887	rVB7	5132	9162	0.15%	0.019%
21	14.428	1903	1911	1930	rBV	1992845	2980873	48.58%	6.235%
22	14.728	1955	1962	1978	rBV	1173016	1788329	29.15%	3.741%
23	14.975	1997	2004	2017	rBV2	36555	140296	2.29%	0.293%
24	15.722	2124	2131	2139	rBV	2694418	3958532	64.52%	8.280%
25	15.775	2139	2140	2147	rVV5	27569	43465	0.71%	0.091%
26	15.851	2147	2153	2169	rVV	982006	1535745	25.03%	3.212%
27	15.963	2169	2172	2178	rVB5	16012	26363	0.43%	0.055%
28	16.086	2188	2193	2205	rVB	124467	185621	3.03%	0.388%
29	16.651	2284	2289	2295	rVB4	11119	18493	0.30%	0.039%
30	17.163	2371	2376	2380	rBV8	5923	8798	0.14%	0.018%
31	17.486	2423	2431	2441	rBV	1641281	2331886	38.01%	4.878%
32	17.586	2441	2448	2463	rVV	3357085	4798513	78.21%	10.037%
33	18.345	2572	2577	2585	rBV	54633	85652	1.40%	0.179%
34	19.386	2750	2754	2760	rVB2	44747	60891	0.99%	0.127%
35	19.457	2762	2766	2772	rVV	63651	90338	1.47%	0.189%
36	19.569	2782	2785	2791	rBV3	33626	48892	0.80%	0.102%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015537.D
Acq On : 15 Jun 2023 02:10
Operator : MA/JU
Sample : 03104-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONL7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	19.710	2807	2809	2813	rVB4	10464	10990	0.18%	0.023%
38	19.810	2820	2826	2841	rBV	4502651	5955230	97.06%	12.457%
39	21.568	3120	3125	3135	rBV2	1869142	2734411	44.57%	5.720%
40	23.951	3522	3530	3544	rBV2	2870686	6135554	100.00%	12.834%
41	24.115	3551	3558	3570	rVB	1221247	2679457	43.67%	5.605%




Sum of corrected areas: 47807113

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015537.D
Acq On : 15 Jun 2023 02:10
Operator : MA/JU
Sample : 03104-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONL7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

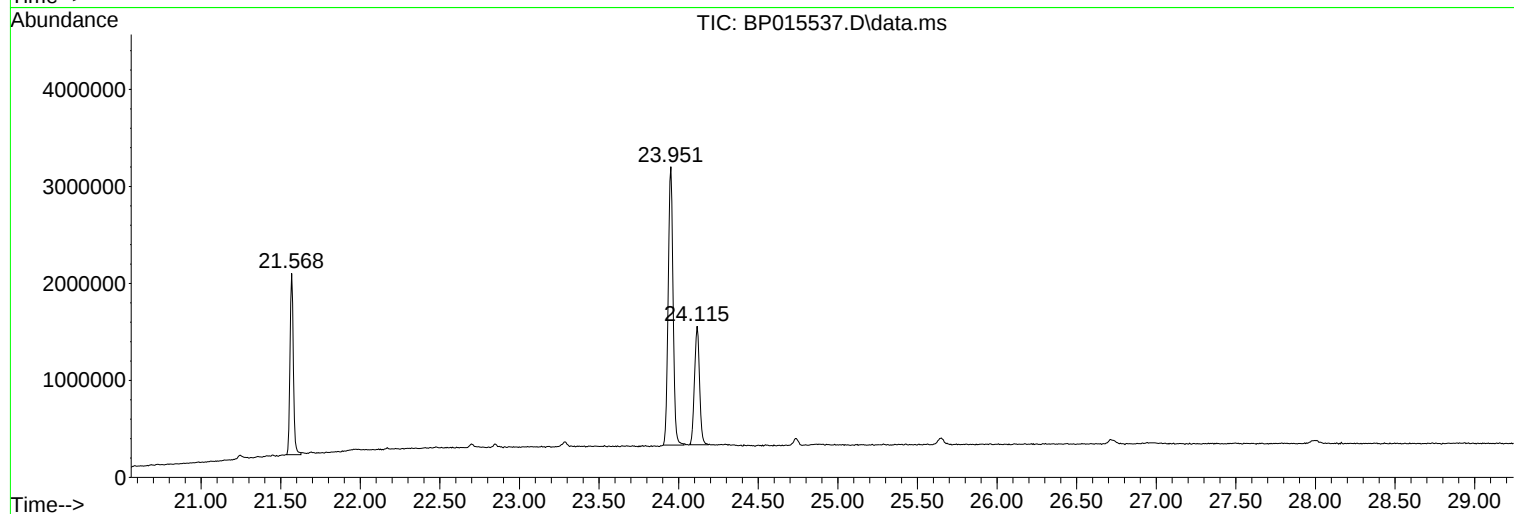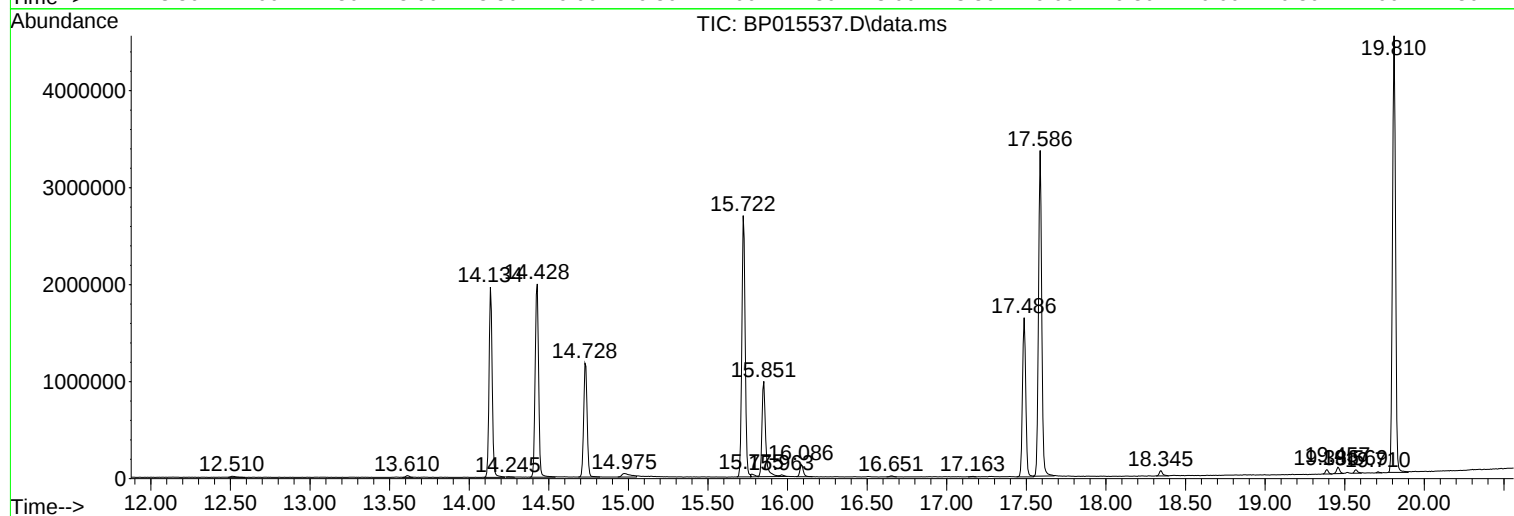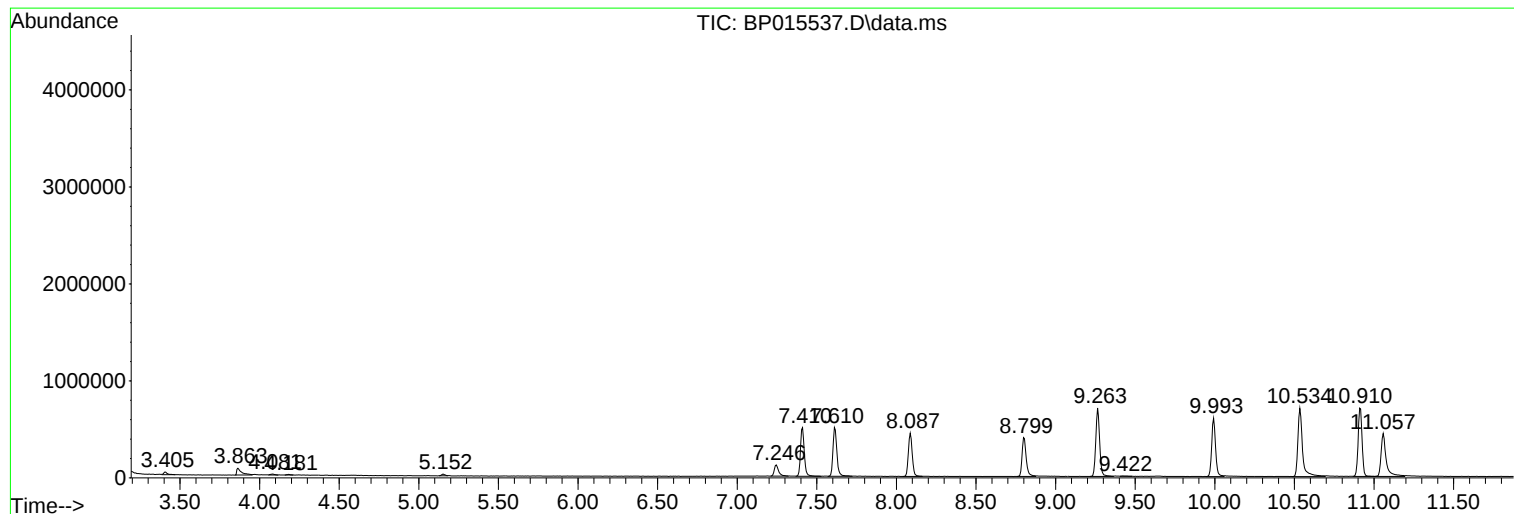

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015537.D
Acq On : 15 Jun 2023 02:10
Operator : MA/JU
Sample : 03104-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONL7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.086	2.08 ng/ul	185621	Acenaphthene-d10	14.728

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	95
3			Benzophenone	182	C13H10O	000119-61-9	94
4			Benzophenone	182	C13H10O	000119-61-9	94
5			Benzophenone	182	C13H10O	000119-61-9	91

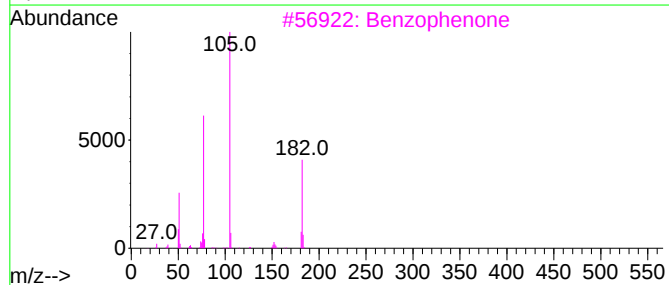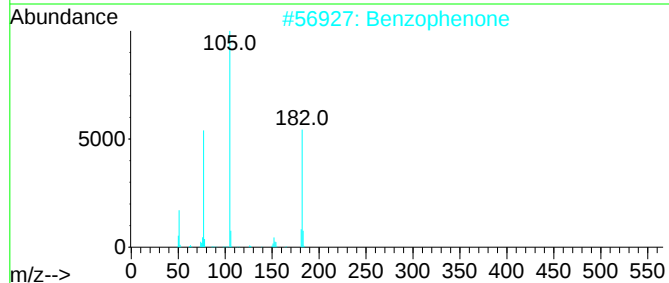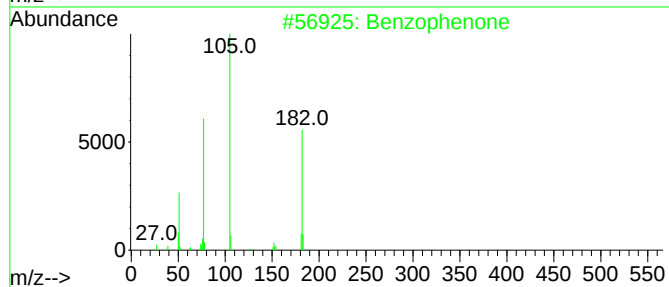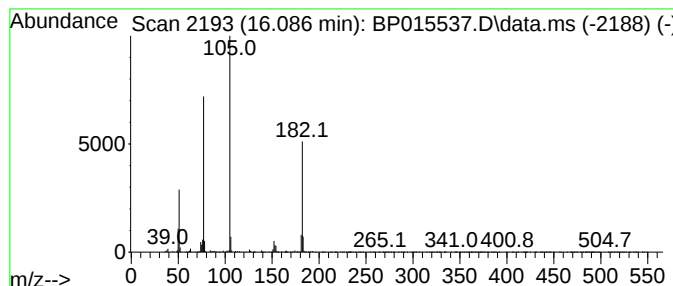

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015537.D
Acq On : 15 Jun 2023 02:10
Operator : MA/JU
Sample : 03104-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONL7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	16.086	2.1	ng/u1	185621	3	14.728	1788330	20.0