

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015542.D
 Acq On : 15 Jun 2023 05:31
 Operator : MA/JU
 Sample : PB153338BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK338

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	46	rBV	38634	56668	1.10%	0.116%
2	3.846	109	112	133	rBV	417722	758717	14.77%	1.556%
3	4.181	167	169	172	rVB3	8189	7194	0.14%	0.015%
4	7.240	682	689	701	rBV	667879	1121871	21.84%	2.301%
5	7.410	711	718	734	rVB	517387	858238	16.71%	1.761%
6	7.610	745	752	767	rBV	691995	1148199	22.35%	2.355%
7	8.087	826	833	845	rBV	483131	803929	15.65%	1.649%
8	8.799	947	954	972	rBV	878047	1526141	29.71%	3.131%
9	9.263	1025	1033	1044	rBV	721019	1231517	23.97%	2.526%
10	9.993	1147	1157	1173	rBV	654824	1126917	21.94%	2.312%
11	10.534	1242	1249	1273	rBV	805183	1607235	31.28%	3.297%
12	10.910	1305	1313	1323	rBV	770334	1306562	25.43%	2.680%
13	11.057	1329	1338	1360	rBV	654946	1406790	27.38%	2.886%
14	12.516	1581	1586	1595	rBV3	11335	26210	0.51%	0.054%
15	13.610	1767	1772	1778	rBV3	16258	28264	0.55%	0.058%
16	14.134	1851	1861	1875	rBV	1892013	2701658	52.59%	5.542%
17	14.422	1901	1910	1931	rBV	1951935	3073711	59.83%	6.305%
18	14.728	1955	1962	1976	rBV	1317976	1973766	38.42%	4.049%
19	14.940	1991	1998	2027	rBV	364316	1113922	21.68%	2.285%
20	15.722	2124	2131	2146	rBV	2594777	3782488	73.63%	7.759%
21	15.851	2147	2153	2168	rVV	761438	1310201	25.50%	2.688%
22	15.963	2170	2172	2185	rVB8	20431	37437	0.73%	0.077%
23	17.157	2371	2375	2380	rBV8	4632	7521	0.15%	0.015%
24	17.486	2424	2431	2441	rBV	1761378	2497937	48.62%	5.124%
25	17.586	2441	2448	2467	rVV	2878351	4281323	83.34%	8.783%
26	19.386	2750	2754	2761	rBV2	39103	53030	1.03%	0.109%
27	19.457	2762	2766	2773	rVV	37956	53838	1.05%	0.110%
28	19.810	2820	2826	2837	rBV	3827430	5137428	100.00%	10.539%
29	21.569	3120	3125	3140	rBV	1829224	2679448	52.16%	5.497%
30	23.951	3522	3530	3548	rVB2	2122776	4587187	89.29%	9.410%
31	24.115	3551	3558	3575	rVB	1093607	2442729	47.55%	5.011%




Sum of corrected areas: 48748076

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015542.D
Acq On : 15 Jun 2023 05:31
Operator : MA/JU
Sample : PB153338BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK338

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

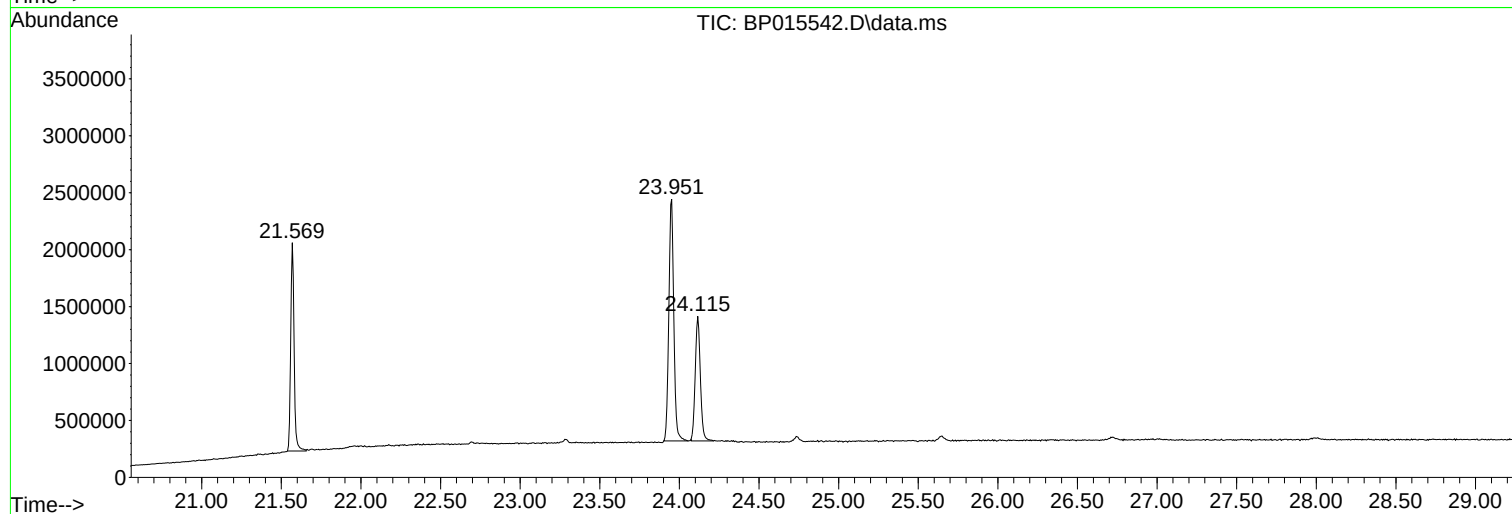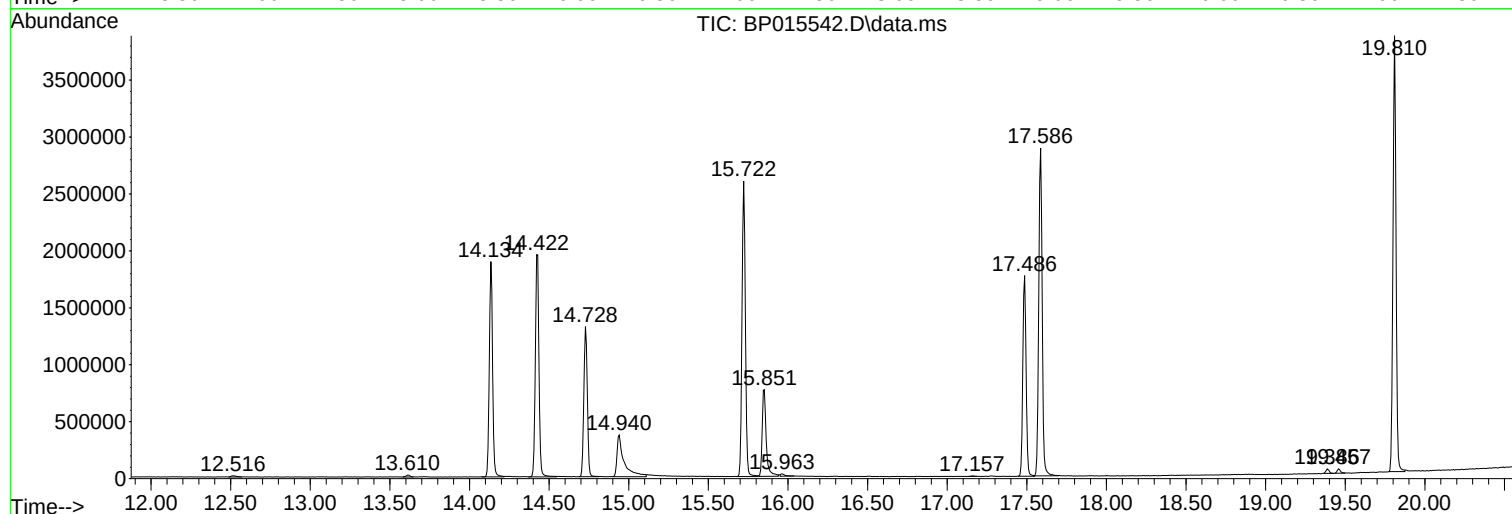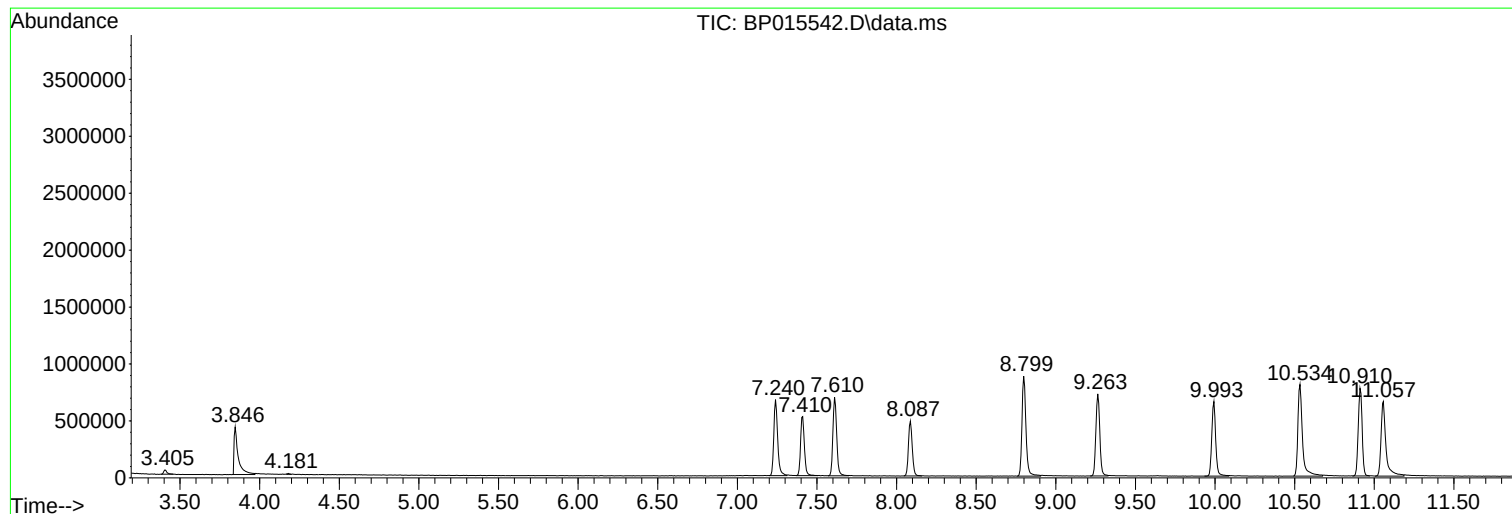

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015542.D
Acq On : 15 Jun 2023 05:31
Operator : MA/JU
Sample : PB153338BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK338

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015542.D
Acq On : 15 Jun 2023 05:31
Operator : MA/JU
Sample : PB153338BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK338

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------