

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
 Data File : BP015558.D
 Acq On : 15 Jun 2023 16:27
 Operator : MA/JU
 Sample : PB153338BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK338

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	44	rBV	32999	44399	0.99%	0.100%
2	3.846	110	112	129	rBV	440670	764131	16.99%	1.717%
3	4.181	166	169	172	rVB3	5873	6817	0.15%	0.015%
4	7.246	683	690	708	rBV	558869	981790	21.83%	2.206%
5	7.411	711	718	728	rBV	446883	711211	15.81%	1.598%
6	7.611	746	752	763	rBV	597821	983946	21.88%	2.211%
7	8.087	826	833	843	rBV	474670	762673	16.96%	1.714%
8	8.805	946	955	968	rBV	765203	1353945	30.11%	3.042%
9	9.263	1024	1033	1044	rBV	630515	1067388	23.73%	2.399%
10	9.993	1149	1157	1168	rBV	556148	974737	21.67%	2.190%
11	10.534	1241	1249	1273	rBV	751700	1448184	32.20%	3.254%
12	10.910	1304	1313	1323	rBV	732463	1246449	27.72%	2.801%
13	11.057	1329	1338	1365	rBV	875668	1732760	38.53%	3.894%
14	12.499	1578	1583	1590	rBV2	12852	26331	0.59%	0.059%
15	13.610	1766	1772	1780	rVB4	11761	21950	0.49%	0.049%
16	14.134	1854	1861	1875	rBV	1678772	2337564	51.98%	5.253%
17	14.428	1903	1911	1925	rBV	1709180	2654905	59.04%	5.966%
18	14.728	1956	1962	1973	rBV	1253106	1832327	40.74%	4.117%
19	14.946	1992	1999	2028	rBV	349936	1014855	22.57%	2.280%
20	15.722	2124	2131	2143	rBV	2262994	3245227	72.16%	7.292%
21	15.851	2146	2153	2169	rVV	652675	1062157	23.62%	2.387%
22	15.963	2169	2172	2178	rVB5	13956	22477	0.50%	0.051%
23	17.163	2371	2376	2381	rBV9	4825	9311	0.21%	0.021%
24	17.487	2424	2431	2441	rBV	1647632	2341443	52.06%	5.261%
25	17.587	2441	2448	2463	rVV2	2581085	3709088	82.48%	8.335%
26	18.351	2576	2578	2582	rBV5	4003	5280	0.12%	0.012%
27	19.386	2750	2754	2758	rBV2	35334	45782	1.02%	0.103%
28	19.457	2763	2766	2773	rVB	32486	44405	0.99%	0.100%
29	19.810	2820	2826	2839	rBV	3405724	4495226	99.96%	10.101%
30	21.569	3120	3125	3135	rBV2	1805043	2605820	57.94%	5.856%
31	23.951	3523	3530	3545	rVB2	2089179	4497154	100.00%	10.106%
32	24.116	3552	3558	3571	rVB	1128457	2451971	54.52%	5.510%




Sum of corrected areas: 44501703

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015558.D
Acq On : 15 Jun 2023 16:27
Operator : MA/JU
Sample : PB153338BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK338

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

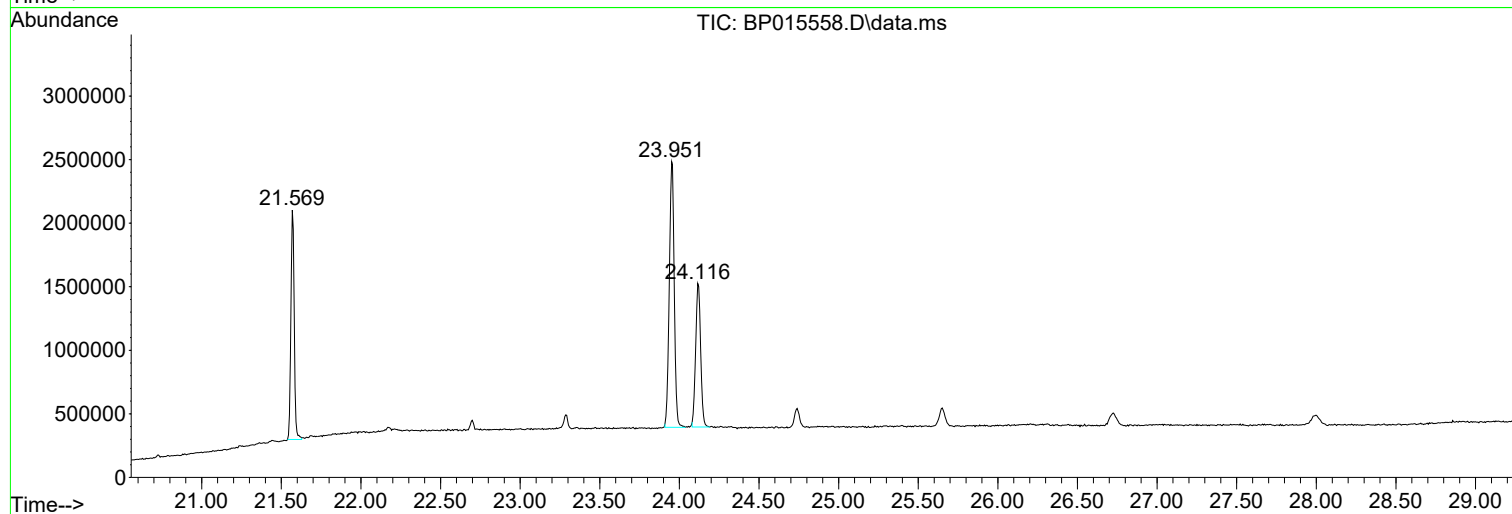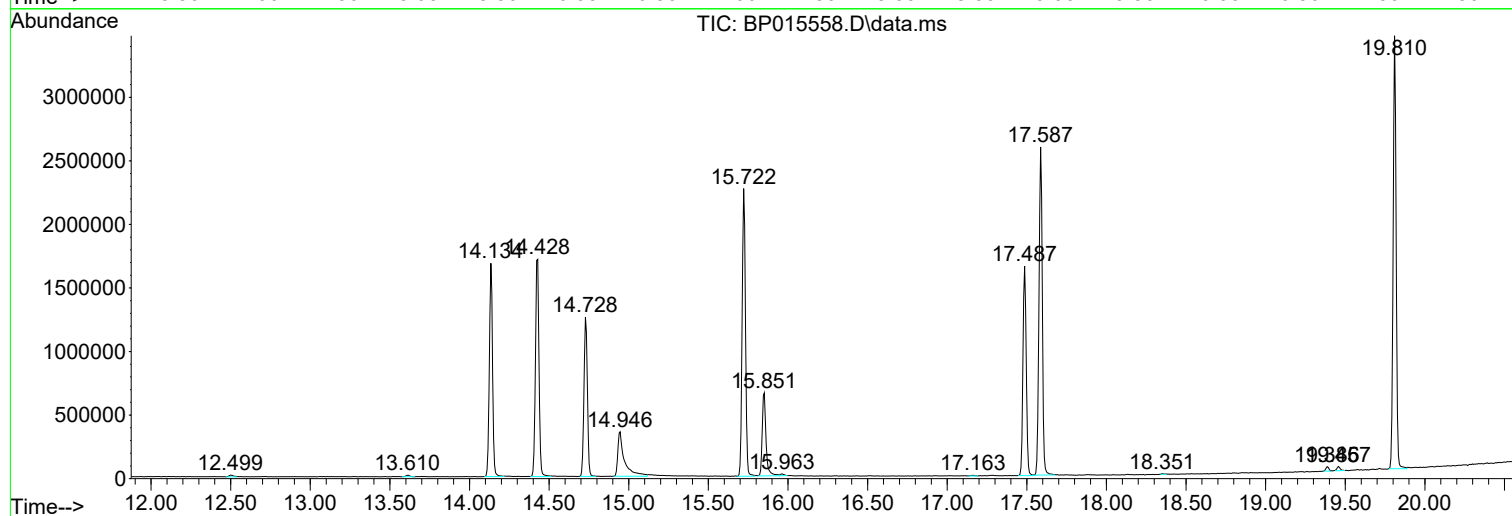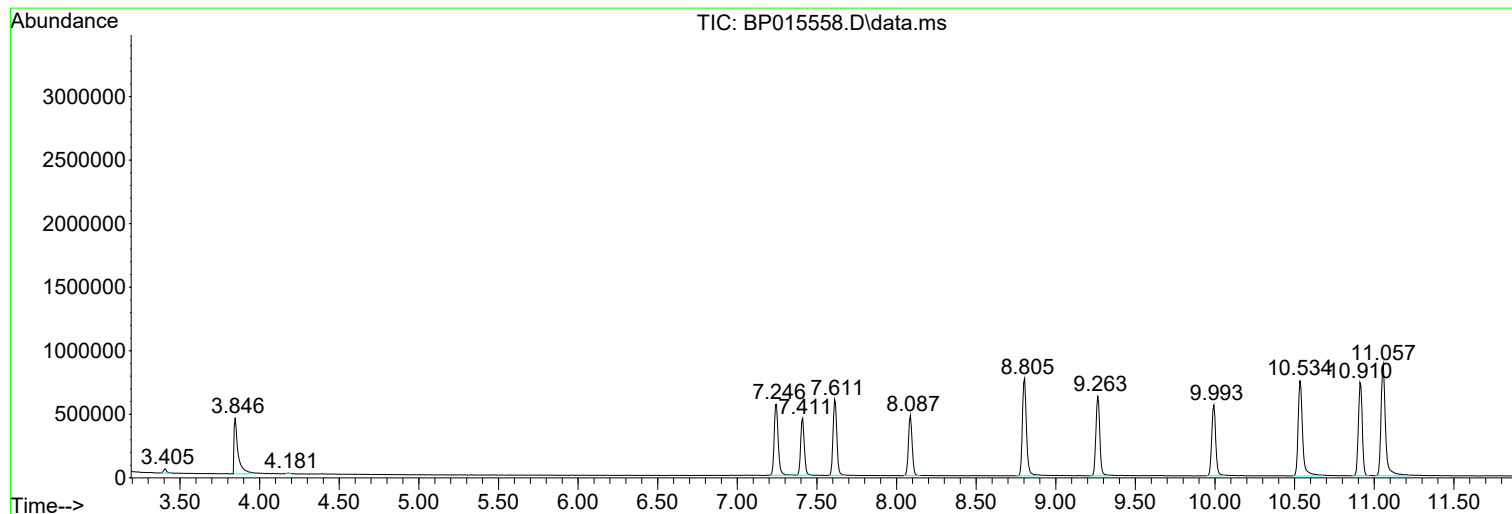

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015558.D
Acq On : 15 Jun 2023 16:27
Operator : MA/JU
Sample : PB153338BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK338

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061423\
Data File : BP015558.D
Acq On : 15 Jun 2023 16:27
Operator : MA/JU
Sample : PB153338BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK338

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------