
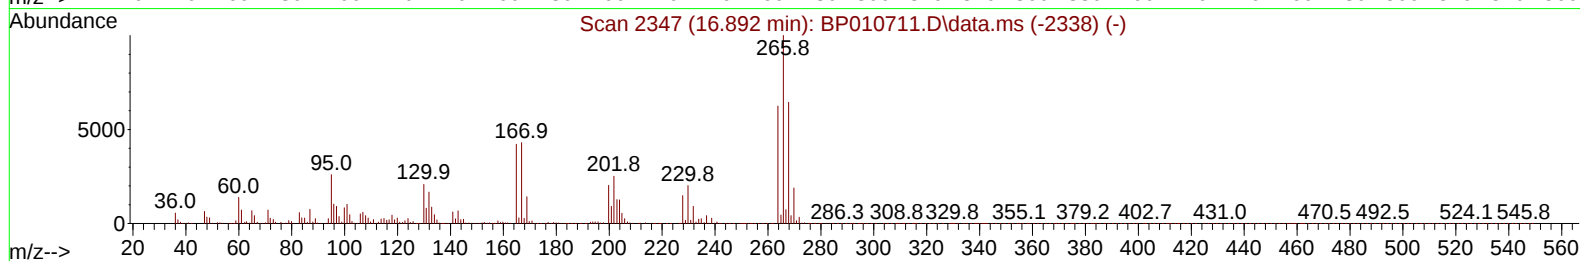
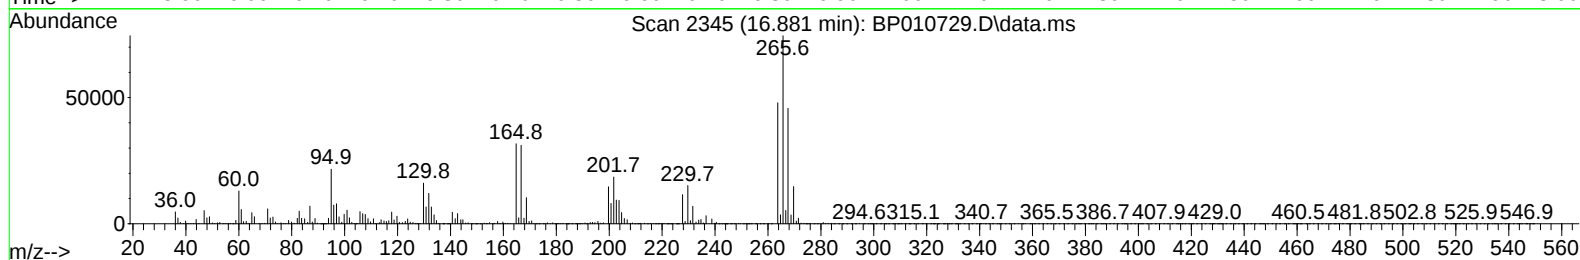


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061522\
 Data File : BP010729.D
 Acq On : 15 Jun 2022 14:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 00:22:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 16 00:00:39 2022
 Response via : Initial Calibration

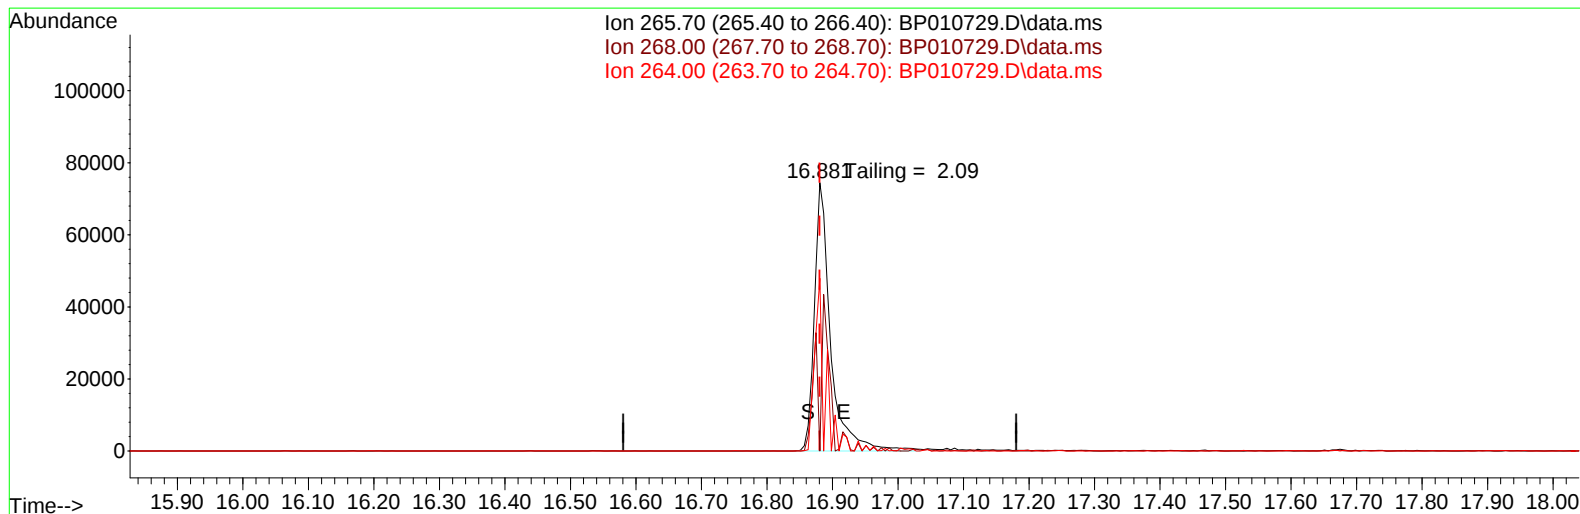

TIC: BP010729.D\data.ms

(70) Pentachlorophenol (C)




16.881min (+ 0.000) 850698.77 ng

response 128385

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	4.69#
264.00	63.00	69.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061522\
Data File : BP010729.D
Acq On : 15 Jun 2022 14:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 00:22:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 16 00:00:39 2022
Response via : Initial Calibration

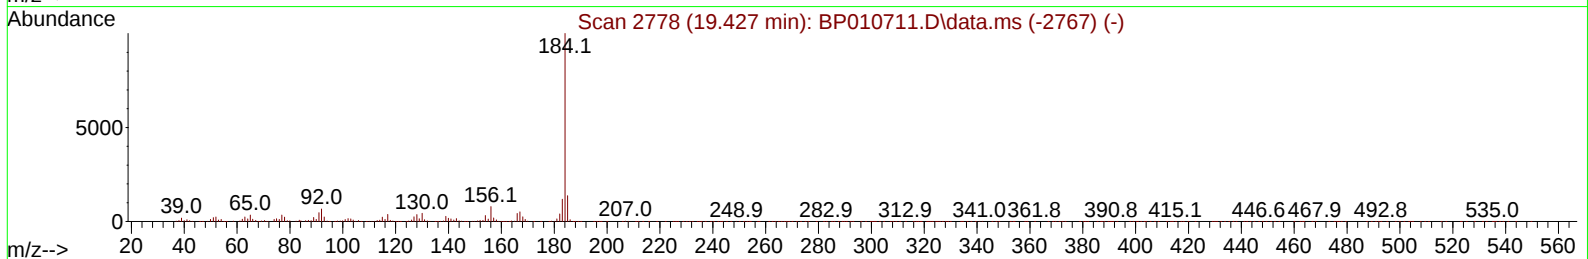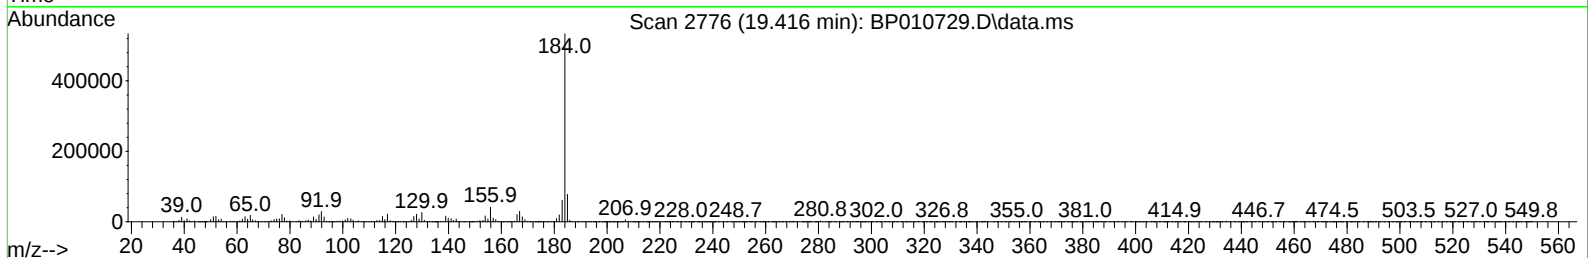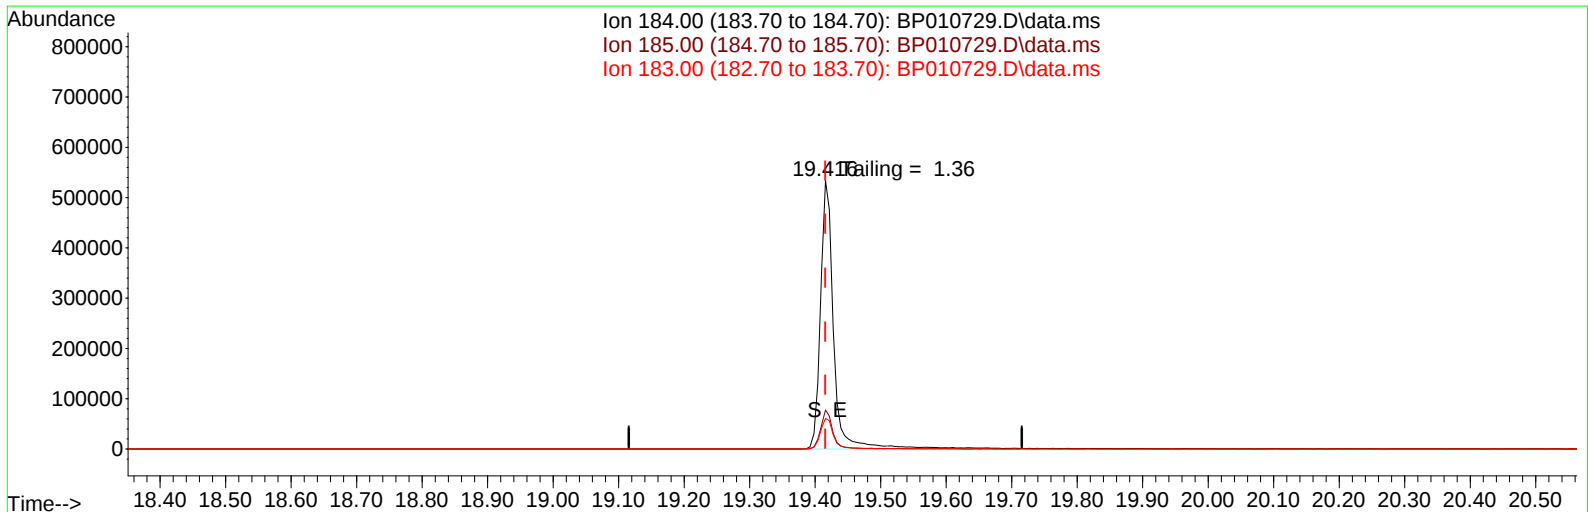

TIC: BP010729.D\data.ms

(77) Benzidine**19.416min (+ 0.000) 1019855.03 ng****response 737390**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.57
183.00	11.30	11.42
0.00	0.00	0.00