

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061522\
 Data File : BP010745.D
 Acq On : 16 Jun 2022 00:03
 Operator : CG/JU
 Sample : N3354-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MW-60

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010745.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	390	396	413	rBV	620953	991092	11.04%	3.457%
2	7.011	658	667	683	rBV	395751	719961	8.02%	2.511%
3	7.828	797	806	816	rBV	254478	433215	4.83%	1.511%
4	8.993	996	1004	1023	rBV	1102965	1987719	22.15%	6.934%
5	10.628	1273	1282	1296	rBV	372629	675305	7.52%	2.356%
6	13.093	1691	1701	1717	rBV	3150483	4698091	52.34%	16.388%
7	14.469	1927	1935	1942	rBV	645793	1005362	11.20%	3.507%
8	15.963	2182	2189	2202	rBV	3028979	4268744	47.56%	14.891%
9	17.222	2396	2403	2413	rBV	894324	1318199	14.69%	4.598%
10	19.786	2833	2839	2848	rBV	7676714	8975516	100.00%	31.309%
11	21.022	3045	3049	3057	rBV3	123202	176314	1.96%	0.615%
12	21.310	3094	3098	3109	rBV	1309544	1714825	19.11%	5.982%
13	23.704	3499	3505	3513	rVB2	842464	1702764	18.97%	5.940%




Sum of corrected areas: 28667107

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061522\
Data File : BP010745.D
Acq On : 16 Jun 2022 00:03
Operator : CG/JU
Sample : N3354-16
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

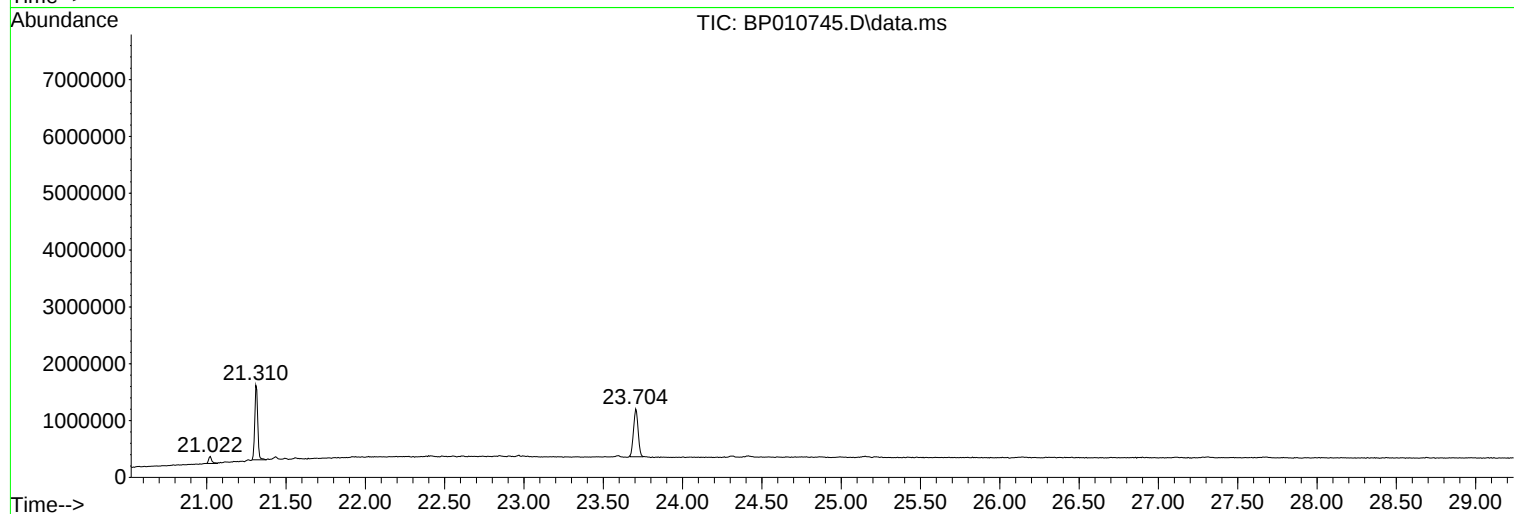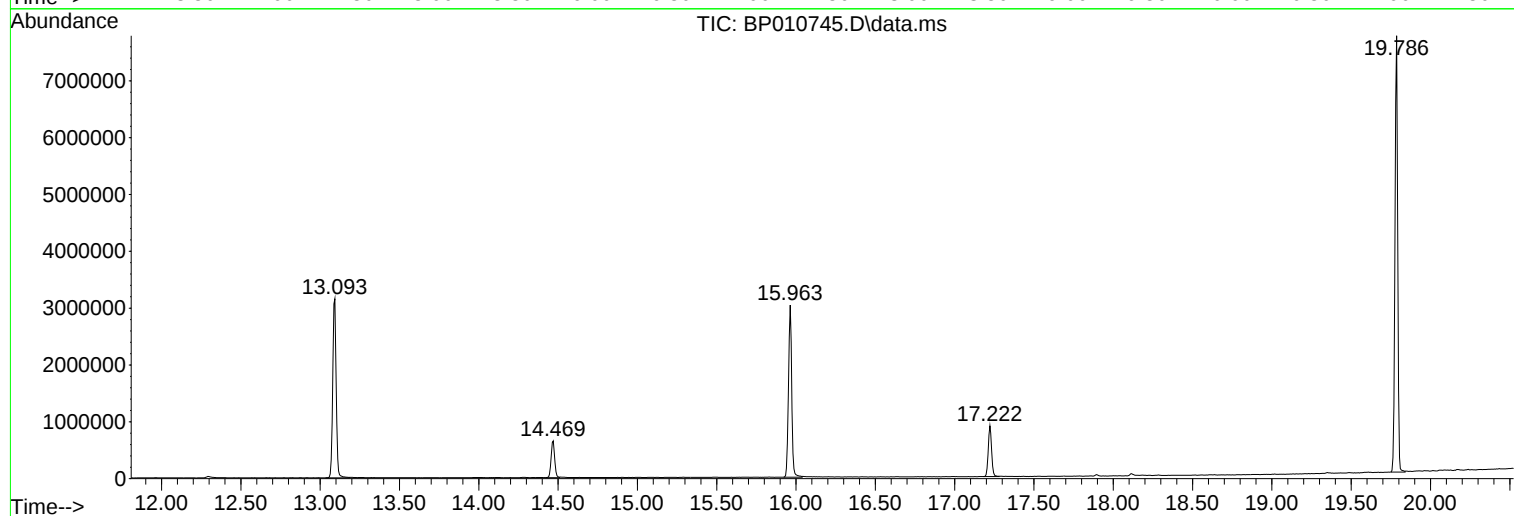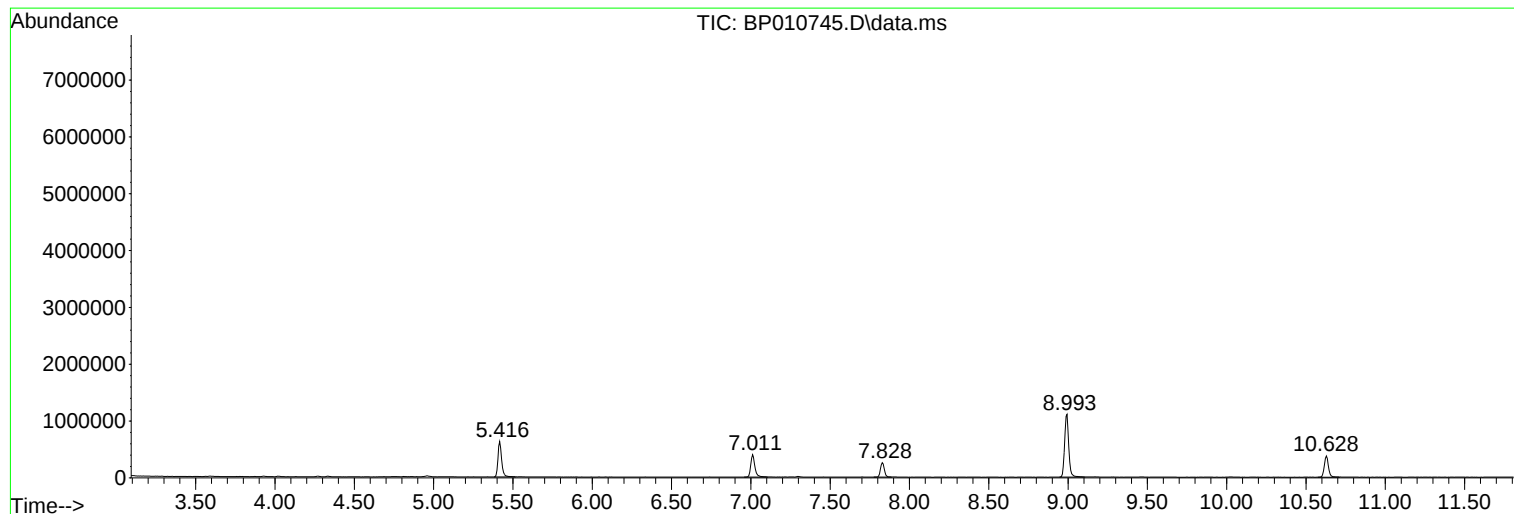

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061522\
Data File : BP010745.D
Acq On : 16 Jun 2022 00:03
Operator : CG/JU
Sample : N3354-16
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-60










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Docosene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.022	2.06 ng	176314	Chrysene-d12	21.310

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Docosene			308	C22H44	001599-67-3	99
2	Heptacosyl acetate			438	C29H58O2	1000351-78-2	99
3	Triacontyl acetate			480	C32H64O2	041755-58-2	98
4	Ethyl triacontyl ether			467	C32H66O	1000406-37-1	97
5	1-Hexacosene			364	C26H52	018835-33-1	97

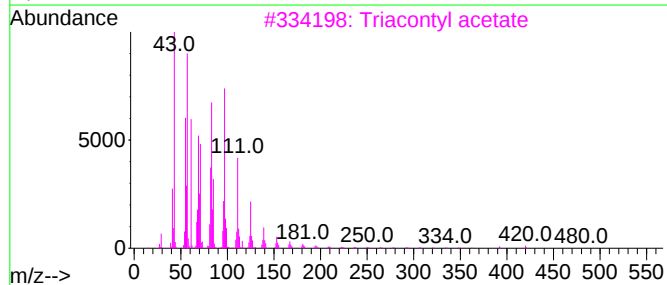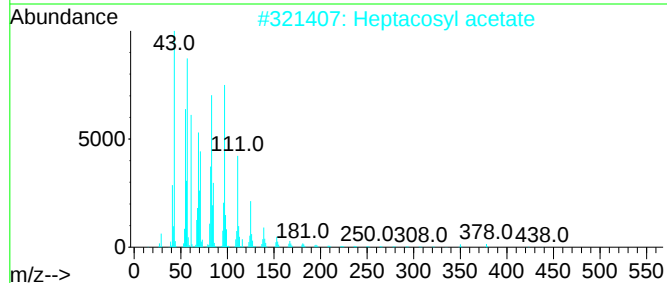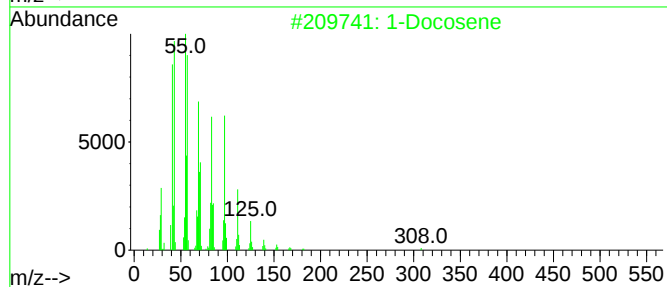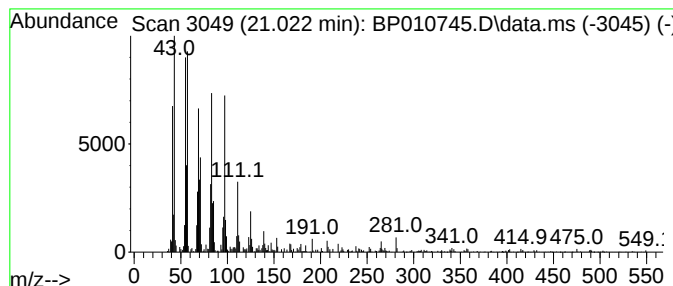

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061522\
Data File : BP010745.D
Acq On : 16 Jun 2022 00:03
Operator : CG/JU
Sample : N3354-16
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Docosene	21.022	2.1	ng	176314	5	21.310	1714830	20.0