
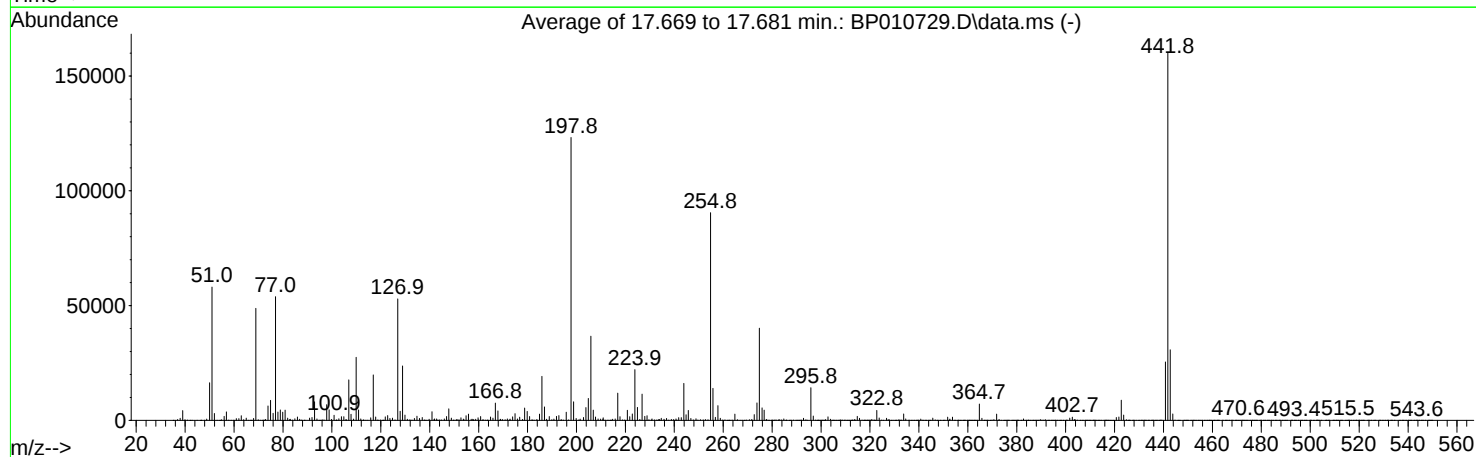


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061522\  
 Data File : BP010729.D  
 Acq On : 15 Jun 2022 14:12  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060722.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jun 16 00:00:39 2022

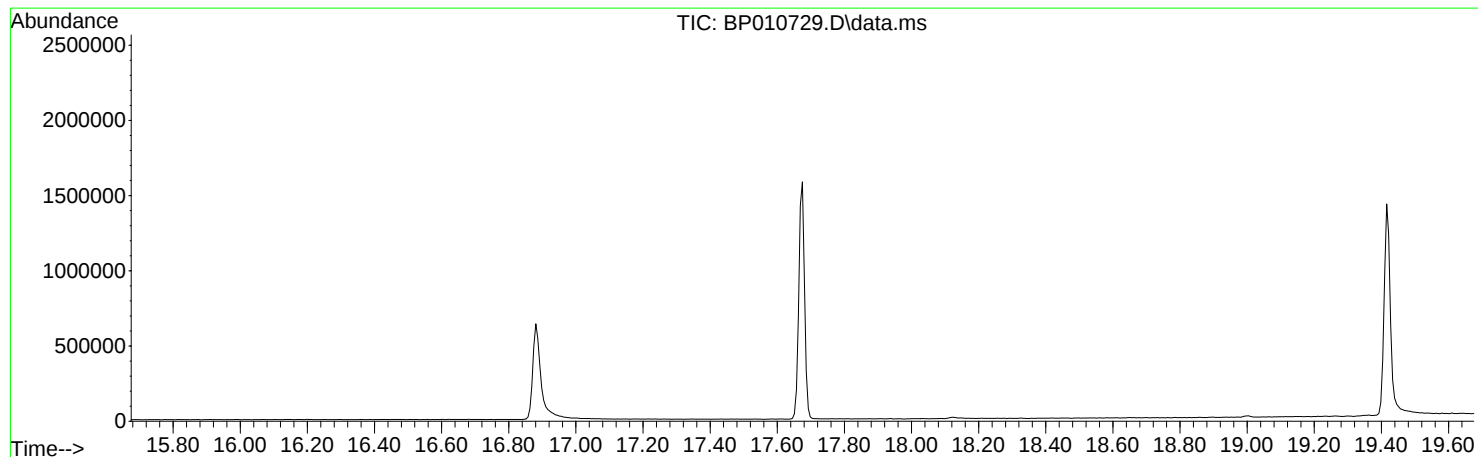

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2468

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 47.1         | 58052      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 809        | PASS                |
| 69             | 198             | 0.00            | 100             | 39.6         | 48806      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 284        | PASS                |
| 127            | 198             | 10              | 80              | 42.9         | 52925      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 195        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 123256     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 8127       | PASS                |
| 275            | 198             | 10              | 60              | 32.6         | 40165      | PASS                |
| 365            | 198             | 1               | 100             | 5.8          | 7098       | PASS                |
| 441            | 198             | 0.01            | 100             | 20.6         | 25423      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 160256     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 30739      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/15/2022     | BNA_P            | <u>BP010729.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 487618           | 20.616             |
| DDD           | 4193             | 20.239             |
| DDE           | 344              | 19.71              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 4537          | 492155           | 0.92               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061522\  
 Data File : BP010729.D  
 Acq On : 15 Jun 2022 14:12  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 16 00:22:32 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060722.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 16 00:00:39 2022  
 Response via : Initial Calibration

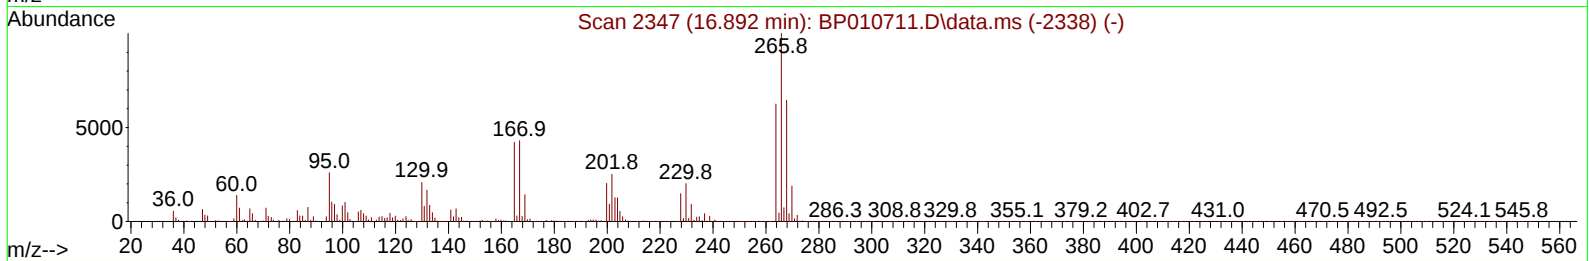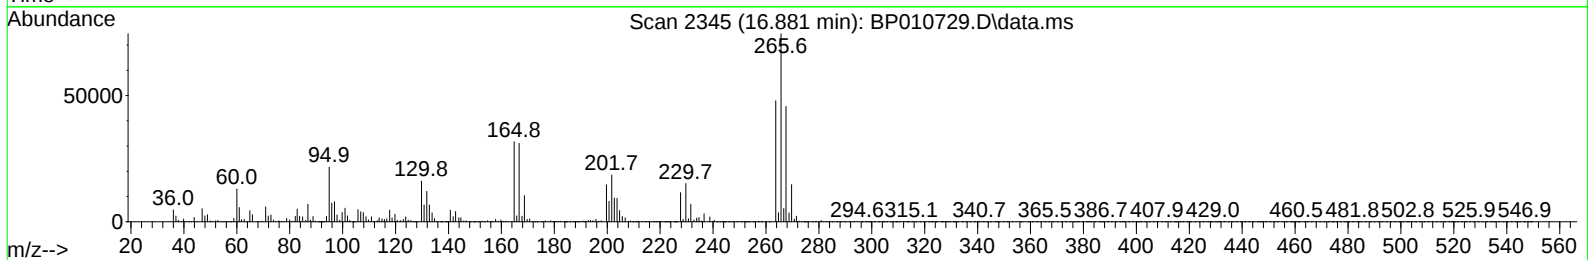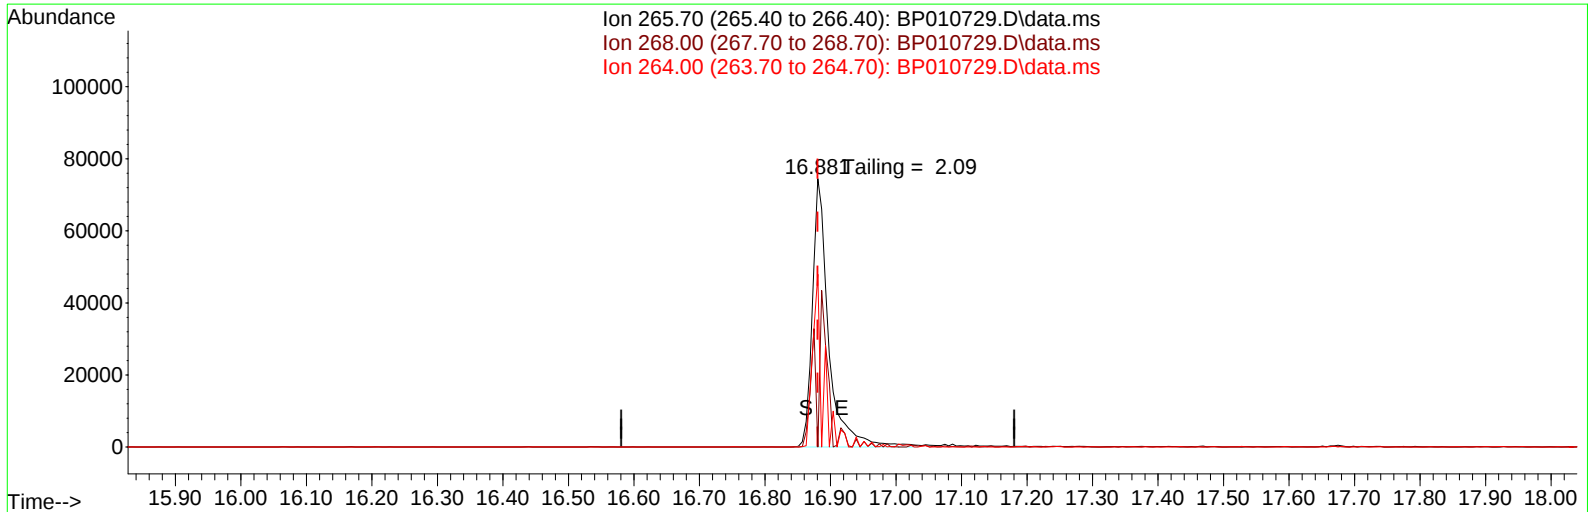

TIC: BP010729.D\data.ms

**(70) Pentachlorophenol (C)**

16.881min (+ 0.000) 850698.77 ng




response 128385

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.10  | 4.69#  |
| 264.00 | 63.00  | 69.09  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061522\  
Data File : BP010729.D  
Acq On : 15 Jun 2022 14:12  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Jun 16 00:22:32 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 16 00:00:39 2022  
Response via : Initial Calibration

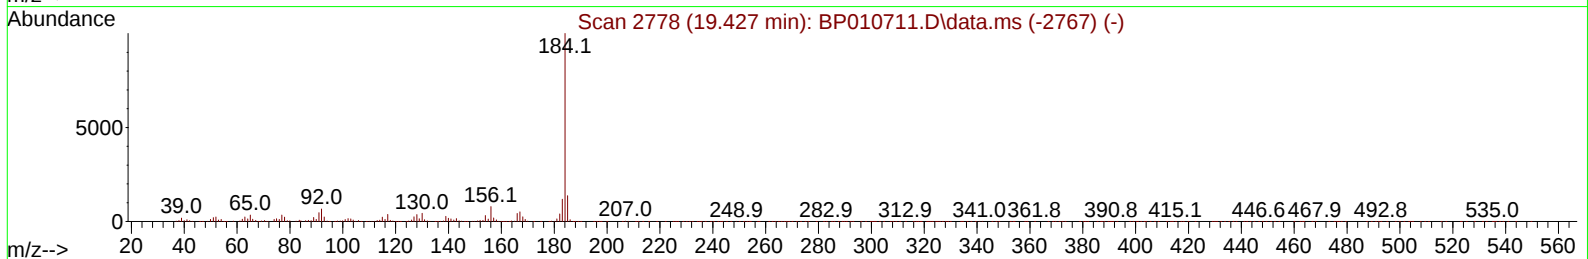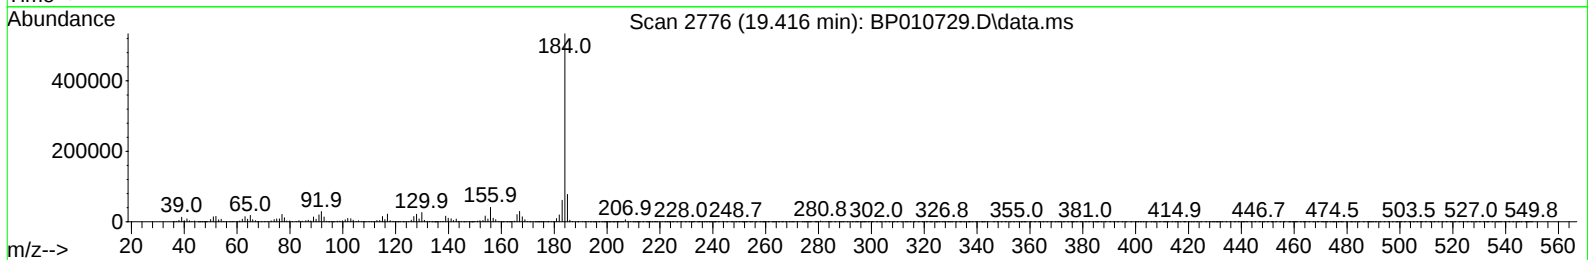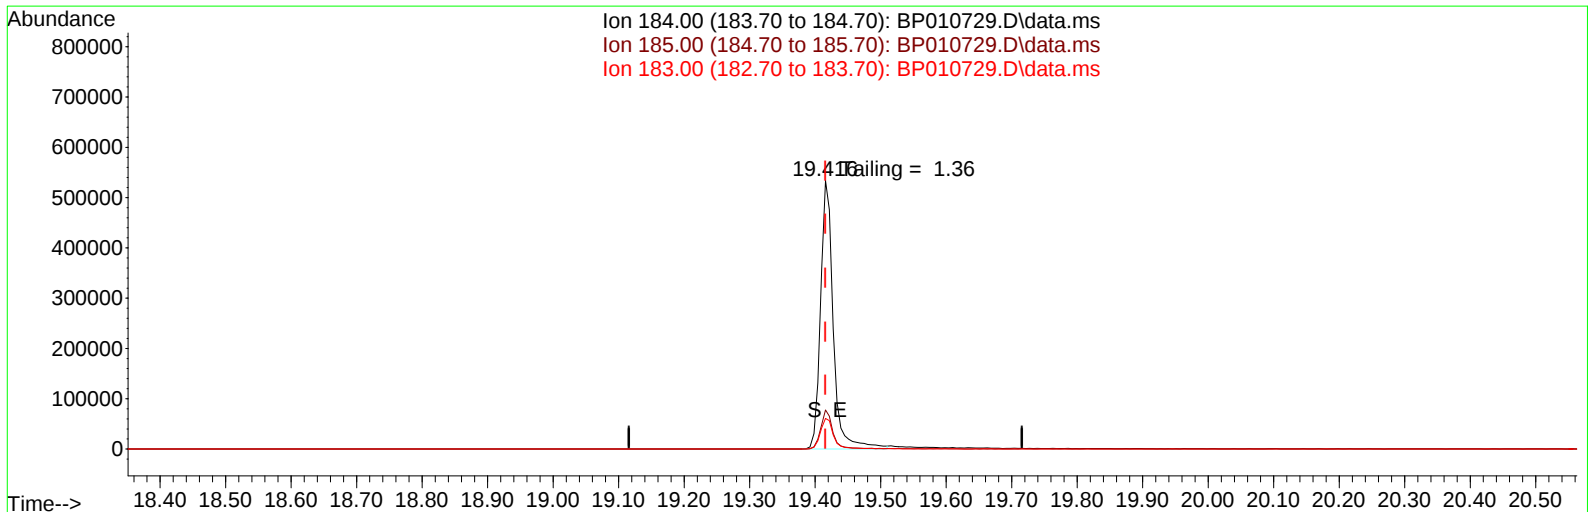

TIC: BP010729.D\data.ms

**(77) Benzidine**

**19.416min (+ 0.000) 1019855.03 ng**

**response 737390**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.40  | 14.57  |
| 183.00 | 11.30  | 11.42  |
| 0.00   | 0.00   | 0.00   |