




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015577.D
Acq On : 16 Jun 2023 12:58
Operator : MA/JU
Sample : 03220-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/19/2023
Supervised By :mohammad ahmed 06/20/2023

Quant Time: Jun 16 22:06:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 15 05:36:46 2023
Response via : Initial Calibration

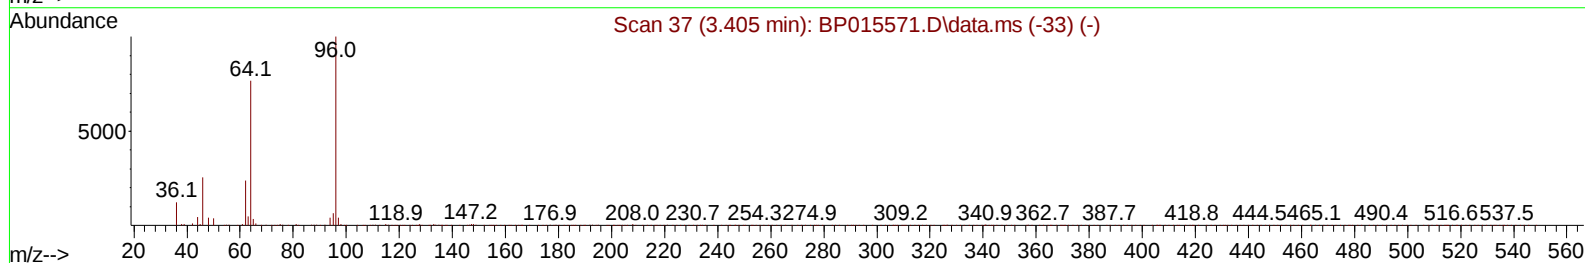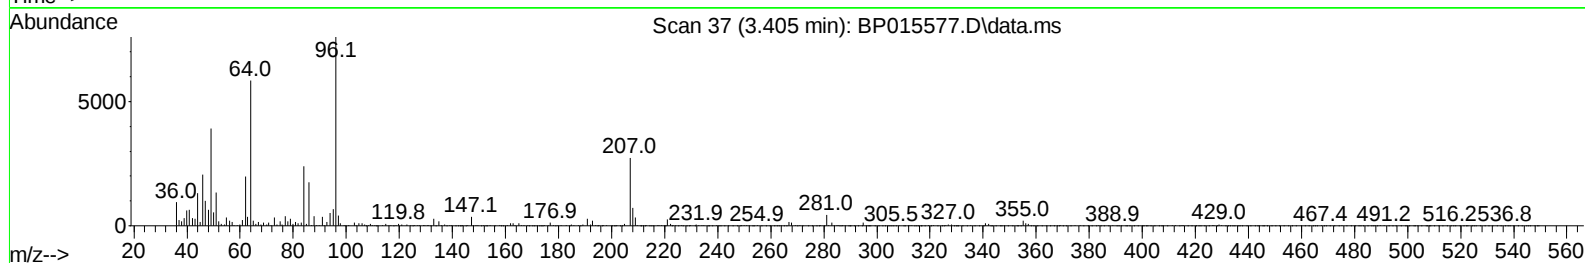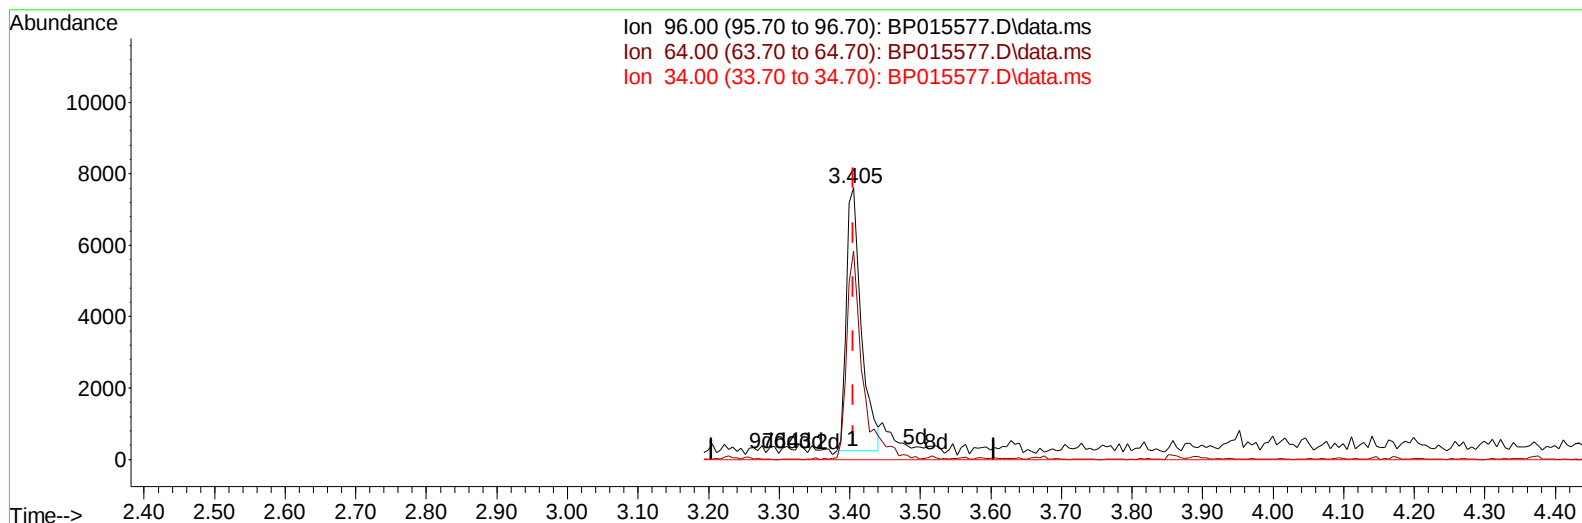

TIC: BP015577.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.405min (+ 0.000) 4.70 ng/uL

response 11019

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	75.60	76.82
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015577.D
 Acq On : 16 Jun 2023 12:58
 Operator : MA/JU
 Sample : 03220-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONR4

Manual IntegrationsAPPROVED

Quant Time: Jun 16 22:06:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 15 05:36:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/19/2023
 Supervised By :mohammad ahmed 06/20/2023

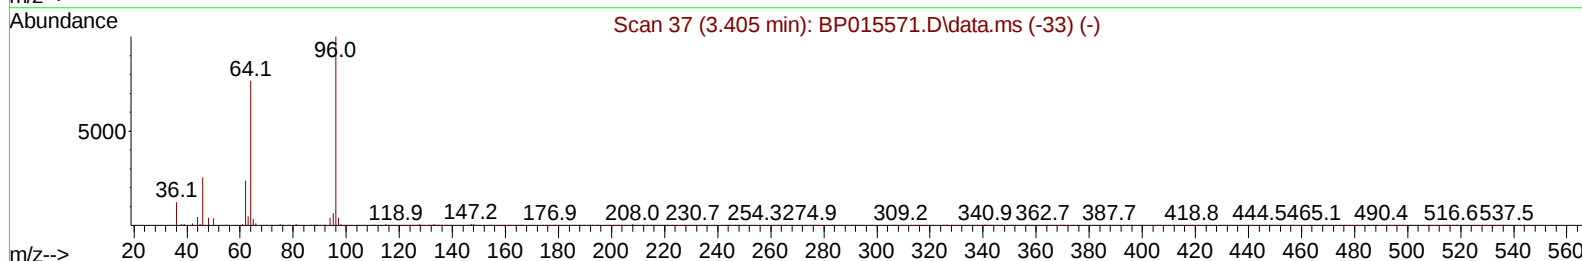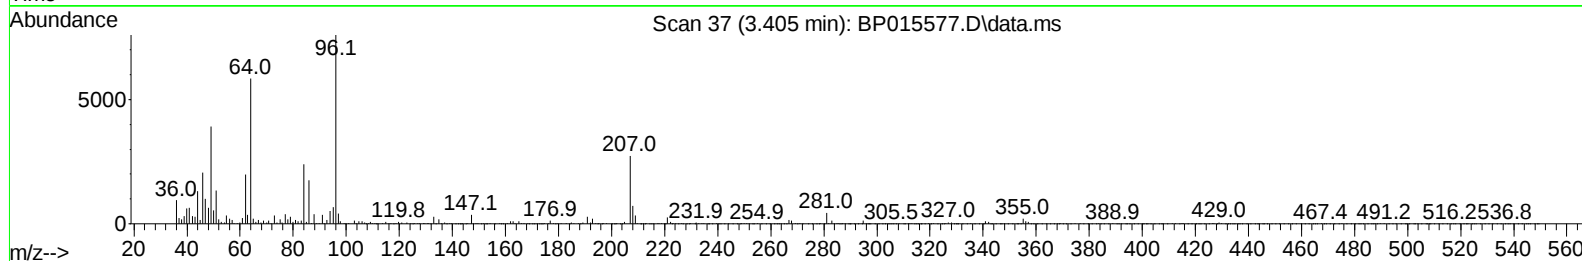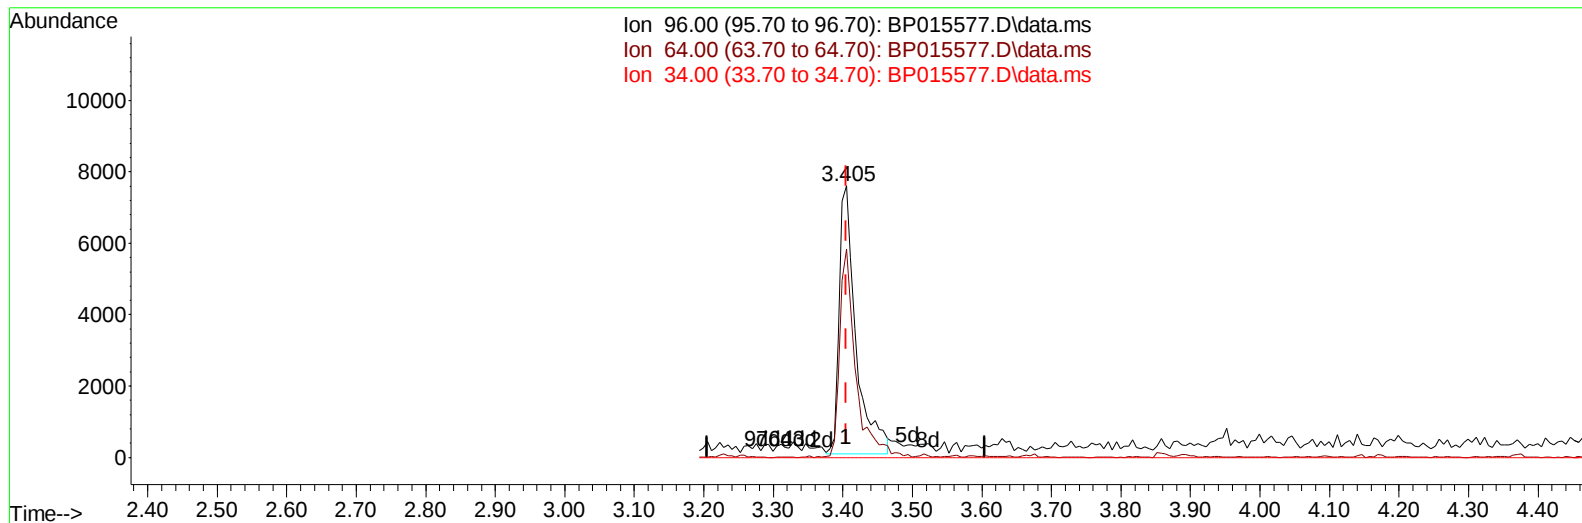

TIC: BP015577.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.405min (+ 0.000) 5.31 ng/uL m

response 12459

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	75.60	76.82
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015577.D
 Acq On : 16 Jun 2023 12:58
 Operator : MA/JU
 Sample : 03220-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONR4

Manual IntegrationsAPPROVED

Quant Time: Jun 16 22:25:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 15 05:36:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/19/2023
 Supervised By :mohammad ahmed 06/20/2023

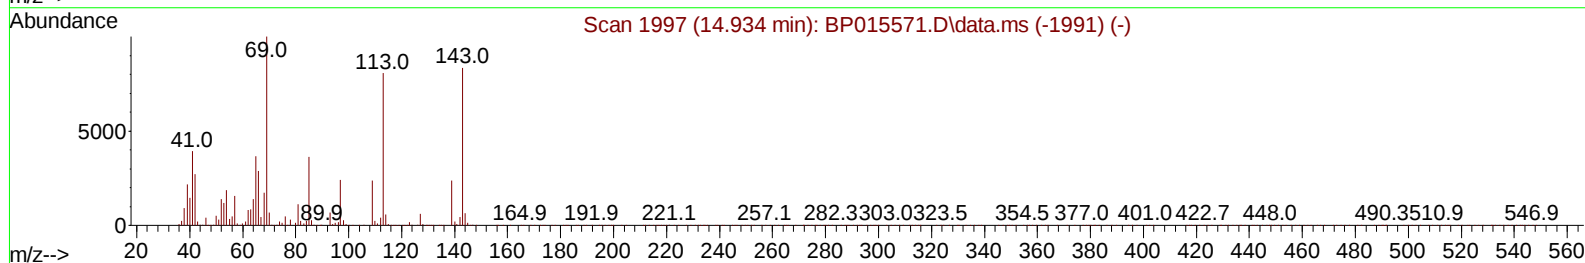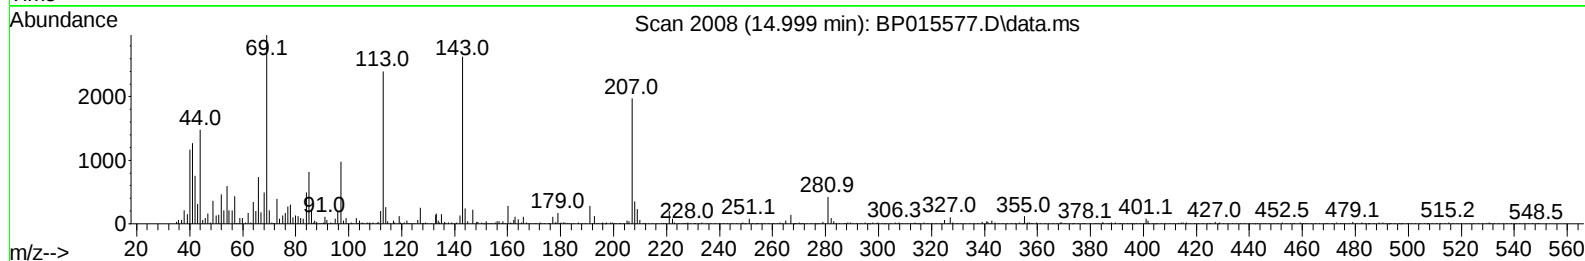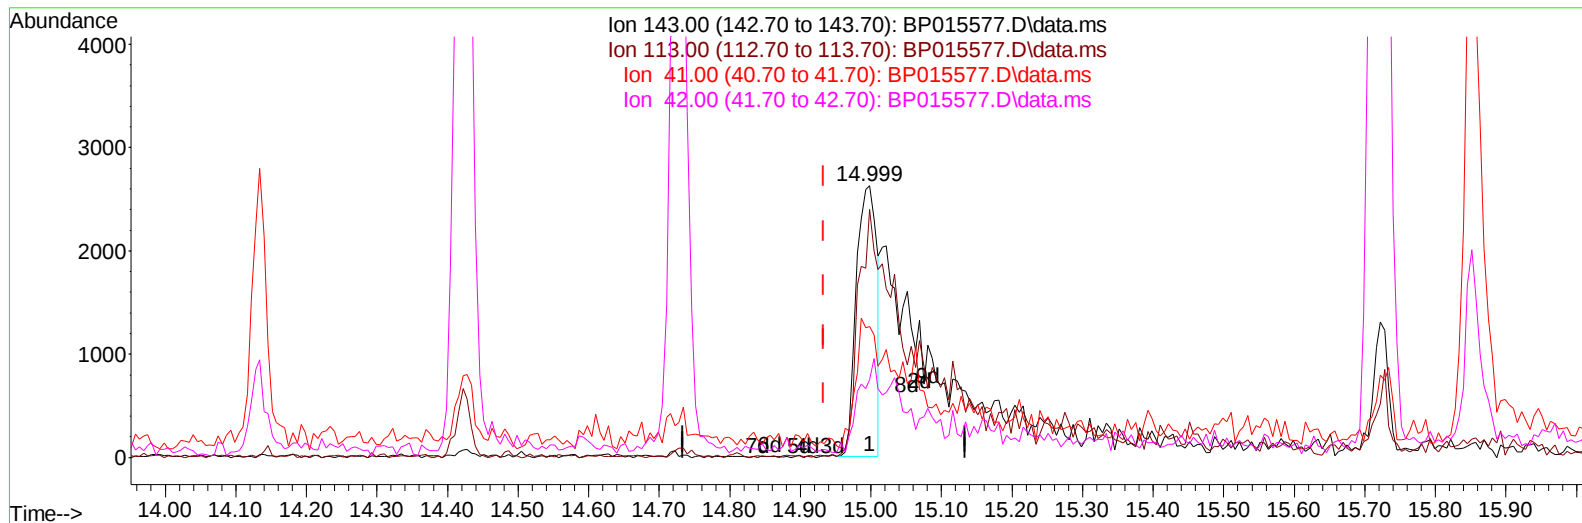

TIC: BP015577.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.999min (+ 0.065) 1.30 ng/u1

response 5292

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	91.33
41.00	42.20	48.27
42.00	29.40	28.72




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015577.D
Acq On : 16 Jun 2023 12:58
Operator : MA/JU
Sample : 03220-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR4

Manual IntegrationsAPPROVED

Quant Time: Jun 16 22:25:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 15 05:36:46 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/19/2023
Supervised By :mohammad ahmed 06/20/2023

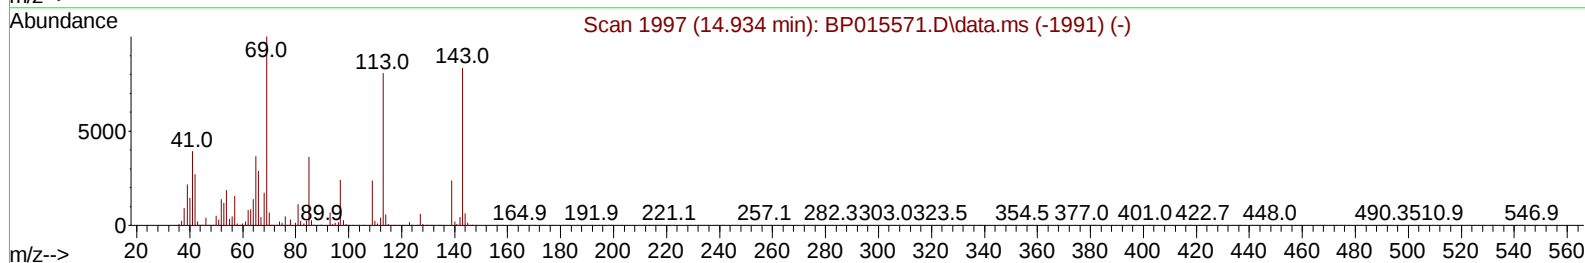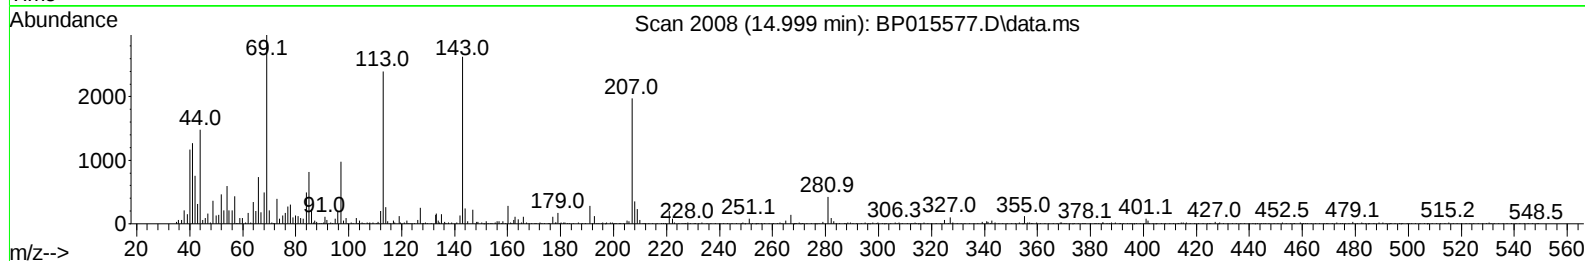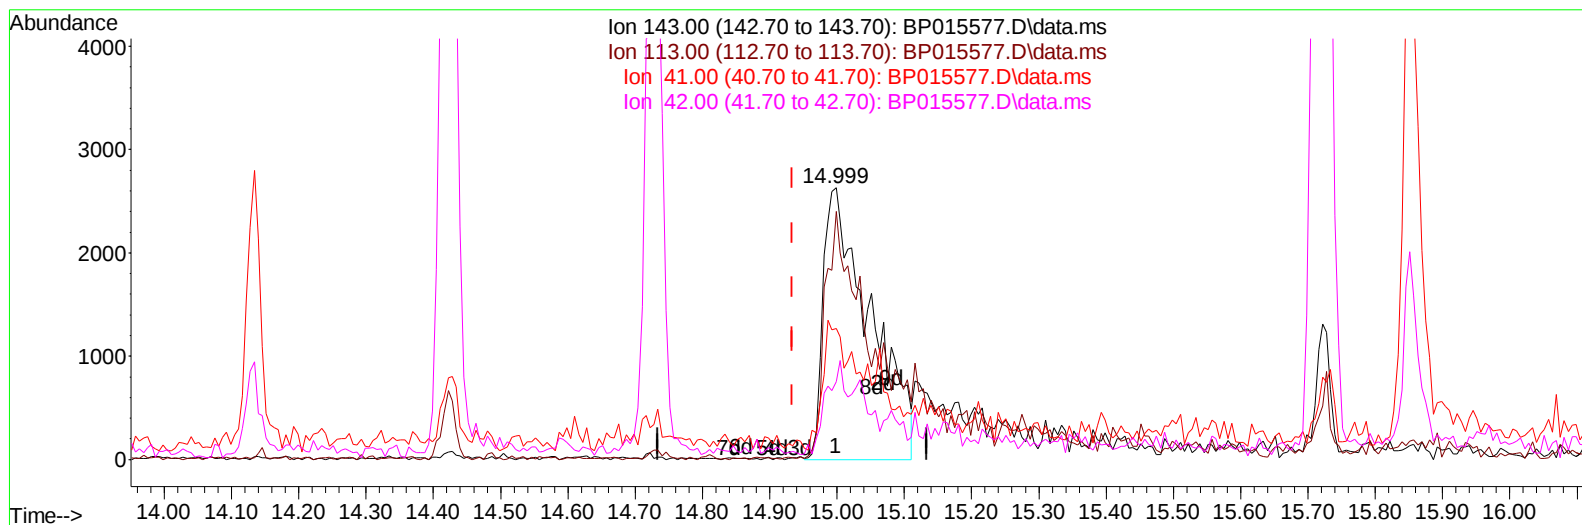

TIC: BP015577.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.999min (+ 0.065) 3.12 ng/ul m

response 12635

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	91.33
41.00	42.20	48.27
42.00	29.40	28.72

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015577.D
 Acq On : 16 Jun 2023 12:58
 Operator : MA/JU
 Sample : 03220-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONR4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/19/2023
 Supervised By :mohammad ahmed 06/20/2023

Quant Time: Jun 16 22:26:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 15 05:36:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.087	152	86835	20.000	ng/ul	0.00
20) Naphthalene-d8	10.910	136	402279	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.728	164	287210	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.487	188	693491	20.000	ng/ul	0.00
79) Chrysene-d12	21.569	240	717375	20.000	ng/ul	0.00
88) Perylene-d12	24.110	264	781580	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	12459m	5.313	ng/uL	0.00
4) Pyridine-d5	3.858	84	67534	11.087	ng/ul	0.01
7) Phenol-d5	7.246	99	53387	6.674	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.405	67	183576	38.424	ng/ul	0.00
11) 2-Chlorophenol-d4	7.611	132	172531	29.746	ng/ul	0.00
15) 4-Methylphenol-d8	8.805	113	108549	16.533	ng/ul	0.00
21) Nitrobenzene-d5	9.264	128	119565	37.858	ng/ul	0.00
24) 2-Nitrophenol-d4	9.993	143	131381	36.426	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	211366	32.126	ng/ul	0.00
31) 4-Chloroaniline-d4	11.058	131	250395	26.514	ng/ul	0.00
46) Dimethylphthalate-d6	14.134	166	987991	43.623	ng/ul	0.00
49) Acenaphthylene-d8	14.422	160	996811	40.251	ng/ul	0.00
54) 4-Nitrophenol-d4	14.999	143	12635m	3.115	ng/ul	0.06
60) Fluorene-d10	15.722	176	850695	44.542	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.851	200	103735	23.612	ng/ul	0.00
73) Anthracene-d10	17.587	188	1530921	48.519	ng/ul	0.00
81) Pyrene-d10	19.810	212	1960225	51.054	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.945	264	1956201	49.882	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015577.D
Acq On : 16 Jun 2023 12:58
Operator : MA/JU
Sample : 03220-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/19/2023
Supervised By :mohammad ahmed 06/20/2023

Quant Time: Jun 16 22:26:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 15 05:36:46 2023
Response via : Initial Calibration

