

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015572.D
 Acq On : 16 Jun 2023 10:08
 Operator : MA/JU
 Sample : PB153448BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK448

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	46	rVB	35192	51008	1.14%	0.120%
2	3.846	109	112	140	rBV	429471	779648	17.44%	1.838%
3	4.175	165	168	171	rBV4	7627	9084	0.20%	0.021%
4	7.240	681	689	703	rBV	555699	978360	21.89%	2.306%
5	7.410	711	718	729	rVB	451367	726849	16.26%	1.713%
6	7.610	745	752	764	rBV	600279	986810	22.07%	2.326%
7	8.087	824	833	843	rBV	460072	754509	16.88%	1.778%
8	8.805	948	955	970	rBV	715380	1303710	29.16%	3.073%
9	9.263	1025	1033	1046	rBV	611922	1048925	23.46%	2.472%
10	9.993	1149	1157	1171	rBV	544973	928862	20.78%	2.189%
11	10.534	1241	1249	1272	rBV	687481	1381636	30.91%	3.256%
12	10.728	1281	1282	1291	rVB9	2949	4598	0.10%	0.011%
13	10.916	1305	1314	1327	rBV	702474	1199802	26.84%	2.828%
14	11.057	1330	1338	1364	rBV	692962	1416319	31.68%	3.338%
15	12.510	1577	1585	1592	rBV2	11843	25189	0.56%	0.059%
16	12.722	1615	1621	1624	rVB8	2766	5684	0.13%	0.013%
17	13.616	1766	1773	1780	rVB4	15555	28178	0.63%	0.066%
18	14.140	1852	1862	1876	rBV	1625003	2317403	51.84%	5.462%
19	14.428	1902	1911	1929	rBV	1725953	2593549	58.02%	6.113%
20	14.734	1954	1963	1980	rBV	1201939	1760603	39.38%	4.149%
21	14.951	1993	2000	2024	rBV	261049	850434	19.02%	2.004%
22	15.669	2118	2122	2125	rBV4	3572	5053	0.11%	0.012%
23	15.728	2125	2132	2145	rVV	2255905	3233005	72.32%	7.620%
24	15.857	2148	2154	2169	rVV	593399	997733	22.32%	2.352%
25	15.969	2169	2173	2187	rVB8	16626	41788	0.93%	0.098%
26	16.510	2262	2265	2269	rBV6	3731	5465	0.12%	0.013%
27	16.928	2332	2336	2339	rBV6	3578	4890	0.11%	0.012%
28	17.169	2371	2377	2382	rBV9	4729	9201	0.21%	0.022%
29	17.281	2393	2396	2400	rVB5	4243	6019	0.13%	0.014%
30	17.492	2425	2432	2442	rBV	1567992	2238149	50.07%	5.275%
31	17.592	2442	2449	2471	rVB	2602401	3711087	83.01%	8.747%
32	19.392	2752	2755	2760	rVB2	36033	43834	0.98%	0.103%
33	19.463	2763	2767	2772	rBV	31298	44666	1.00%	0.105%
34	19.816	2821	2827	2840	rBV	3436354	4470447	100.00%	10.536%
35	21.574	3121	3126	3137	rBV	1664910	2398151	53.64%	5.652%
36	23.957	3524	3531	3546	rVB2	1822655	3885752	86.92%	9.158%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015572.D
Acq On : 16 Jun 2023 10:08
Operator : MA/JU
Sample : PB153448BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	24.127	3553	3560	3573	rVB	968154	2182936	48.83%	5.145%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 42429336

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015572.D
Acq On : 16 Jun 2023 10:08
Operator : MA/JU
Sample : PB153448BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

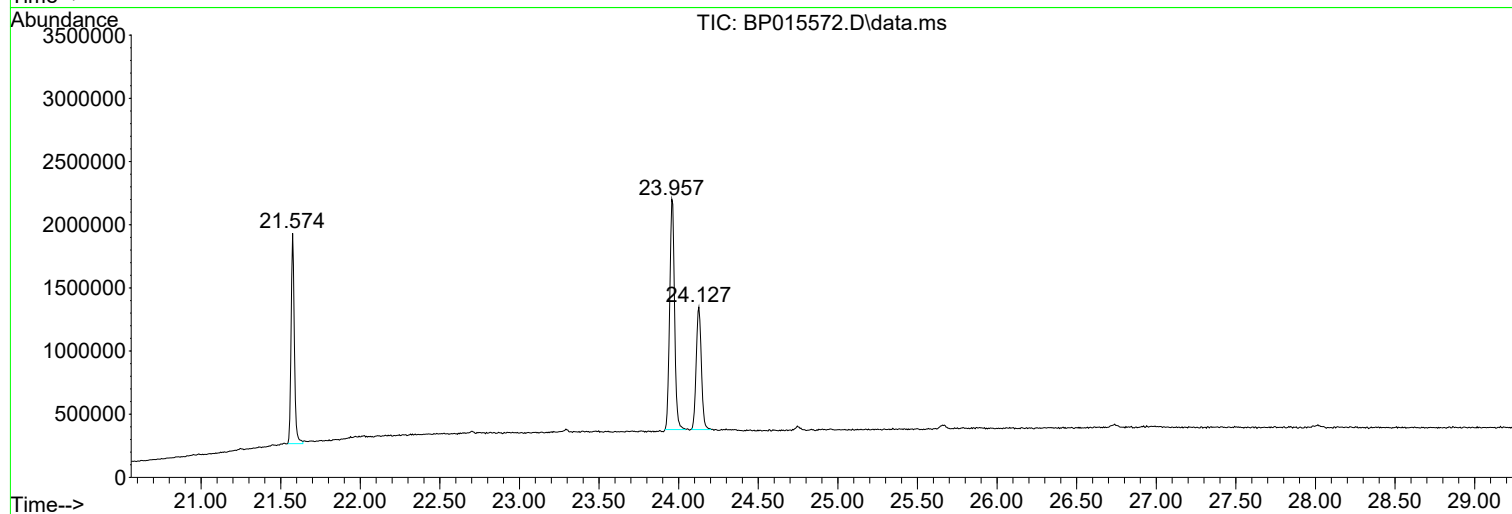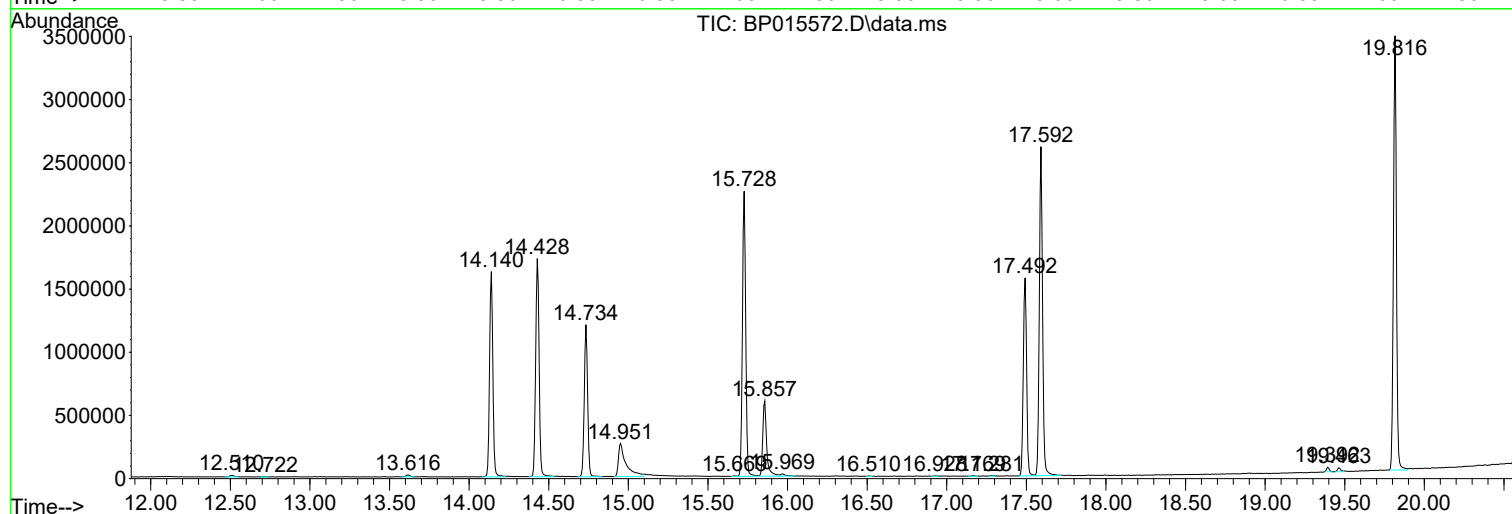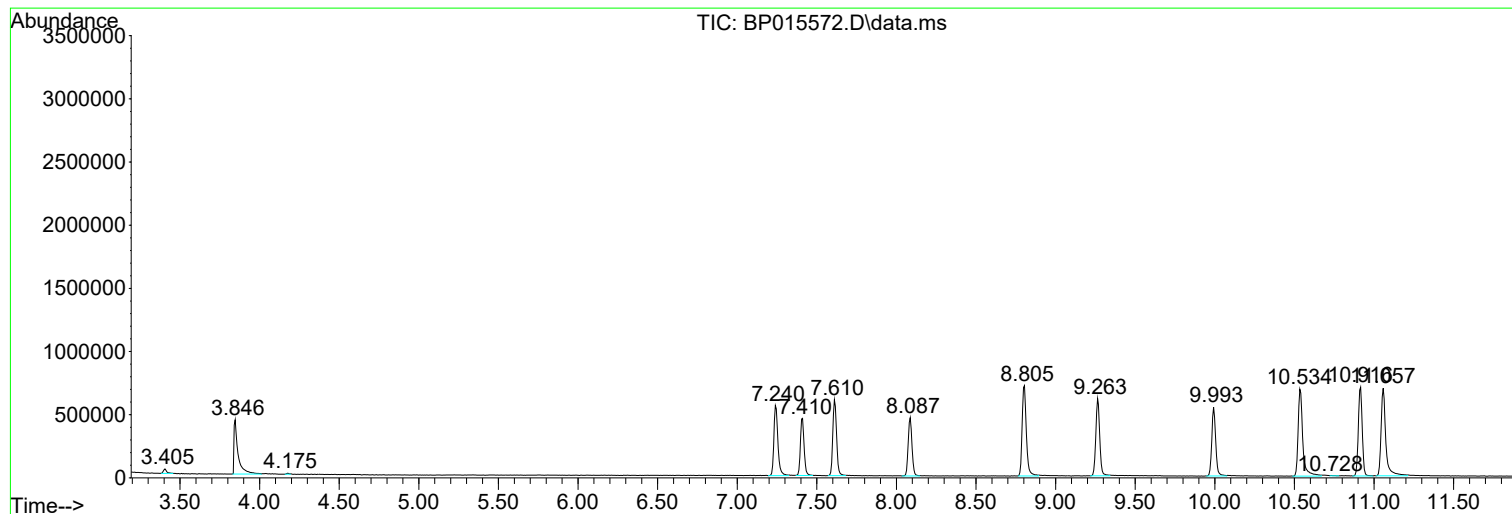

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015572.D
Acq On : 16 Jun 2023 10:08
Operator : MA/JU
Sample : PB153448BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015572.D
Acq On : 16 Jun 2023 10:08
Operator : MA/JU
Sample : PB153448BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------