

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015574.D
 Acq On : 16 Jun 2023 11:17
 Operator : MA/JU
 Sample : 03220-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	34	37	47	rVB	29252	45318	0.80%	0.097%
2	3.852	112	113	133	rBV	148454	269445	4.74%	0.575%
3	4.081	147	152	159	rVB3	9003	14808	0.26%	0.032%
4	4.181	164	169	173	rBV6	9053	13681	0.24%	0.029%
5	7.246	684	690	702	rVB	101147	185622	3.27%	0.396%
6	7.405	711	717	730	rBV	505720	827484	14.56%	1.765%
7	7.611	745	752	766	rBV	470547	804256	14.15%	1.716%
8	8.087	825	833	842	rBV	527923	874392	15.38%	1.865%
9	8.805	948	955	971	rBV	349769	644044	11.33%	1.374%
10	9.263	1026	1033	1044	rBV	701466	1180678	20.77%	2.519%
11	9.640	1092	1097	1102	rVB7	5639	9694	0.17%	0.021%
12	9.993	1149	1157	1170	rBV	550233	991993	17.45%	2.116%
13	10.534	1241	1249	1272	rBV	688615	1359163	23.91%	2.900%
14	10.910	1306	1313	1323	rBV	837027	1377796	24.24%	2.939%
15	11.058	1327	1338	1361	rBV	655182	1352988	23.80%	2.886%
16	12.505	1578	1584	1591	rBV3	12754	24392	0.43%	0.052%
17	12.722	1614	1621	1628	rVB3	2205	6223	0.11%	0.013%
18	13.334	1720	1725	1729	rBV8	4994	7244	0.13%	0.015%
19	13.534	1755	1759	1765	rVB9	3491	6954	0.12%	0.015%
20	13.610	1769	1772	1778	rVB8	5693	9106	0.16%	0.019%
21	14.134	1850	1861	1877	rBV	1938206	2770688	48.74%	5.911%
22	14.240	1877	1879	1885	rVB7	3636	6420	0.11%	0.014%
23	14.422	1903	1910	1923	rBV	1909084	2930992	51.57%	6.253%
24	14.728	1956	1962	1972	rBV	1394965	2028435	35.69%	4.327%
25	14.987	1999	2006	2020	rBV5	23719	95338	1.68%	0.203%
26	15.722	2124	2131	2147	rBV	2744198	3893594	68.50%	8.306%
27	15.851	2147	2153	2166	rVV	800183	1296281	22.81%	2.765%
28	15.969	2169	2173	2180	rVB4	17024	33094	0.58%	0.071%
29	16.087	2188	2193	2205	rVB	105930	161946	2.85%	0.345%
30	17.163	2373	2376	2381	rVB7	5057	7749	0.14%	0.017%
31	17.216	2381	2385	2388	rBV6	4646	6457	0.11%	0.014%
32	17.275	2392	2395	2399	rVB5	4097	6647	0.12%	0.014%
33	17.487	2424	2431	2441	rBV	1824251	2601857	45.77%	5.551%
34	17.587	2441	2448	2470	rVV	3206116	4720288	83.04%	10.070%
35	17.757	2474	2477	2483	rVB5	6072	9379	0.17%	0.020%
36	18.134	2537	2541	2543	rBV5	5250	7178	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015574.D
Acq On : 16 Jun 2023 11:17
Operator : MA/JU
Sample : 03220-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	18.345	2573	2577	2586	rBV	67509	102997	1.81%	0.220%
38	18.422	2587	2590	2598	rVB	12852	20061	0.35%	0.043%
39	19.386	2750	2754	2760	rBV	47524	65384	1.15%	0.139%
40	19.457	2762	2766	2775	rVB	47391	73629	1.30%	0.157%
41	19.575	2782	2786	2793	rBV5	32430	52201	0.92%	0.111%
42	19.810	2820	2826	2836	rBV	4346628	5684046	100.00%	12.126%
43	21.251	3068	3071	3082	rVB7	72878	145703	2.56%	0.311%
44	21.569	3120	3125	3139	rBV	1928833	2747828	48.34%	5.862%
45	23.951	3522	3530	3542	rBV2	2380025	4931482	86.76%	10.520%
46	24.116	3551	3558	3569	rVB	1110900	2470569	43.46%	5.270%




Sum of corrected areas: 46875524

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015574.D
Acq On : 16 Jun 2023 11:17
Operator : MA/JU
Sample : 03220-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

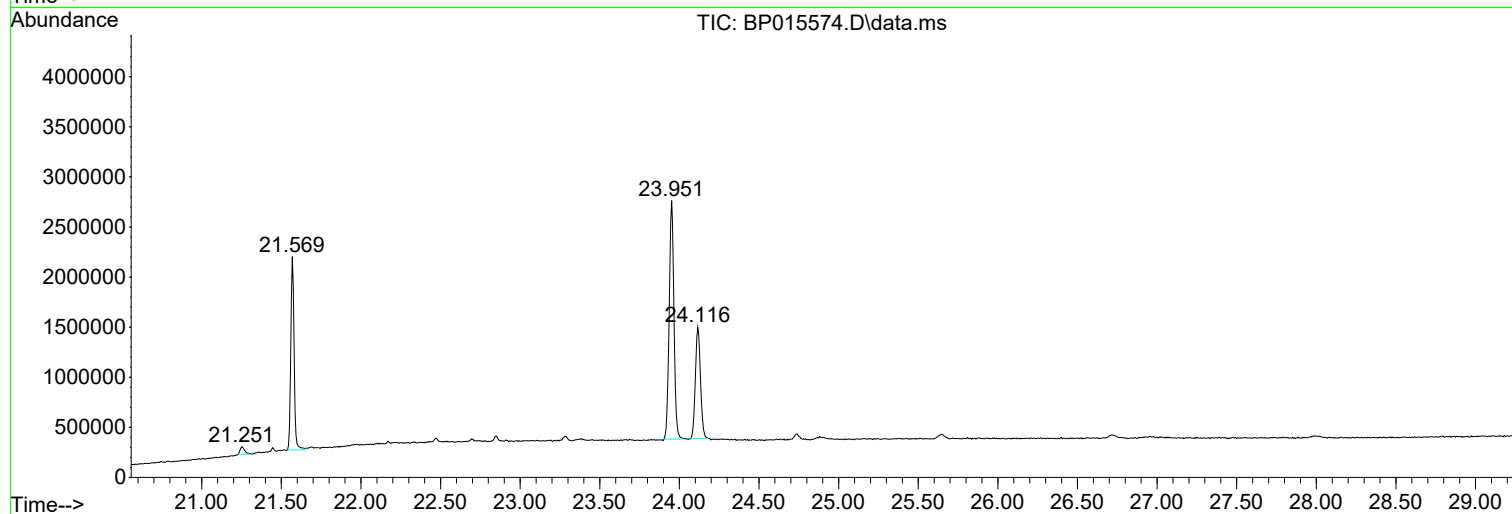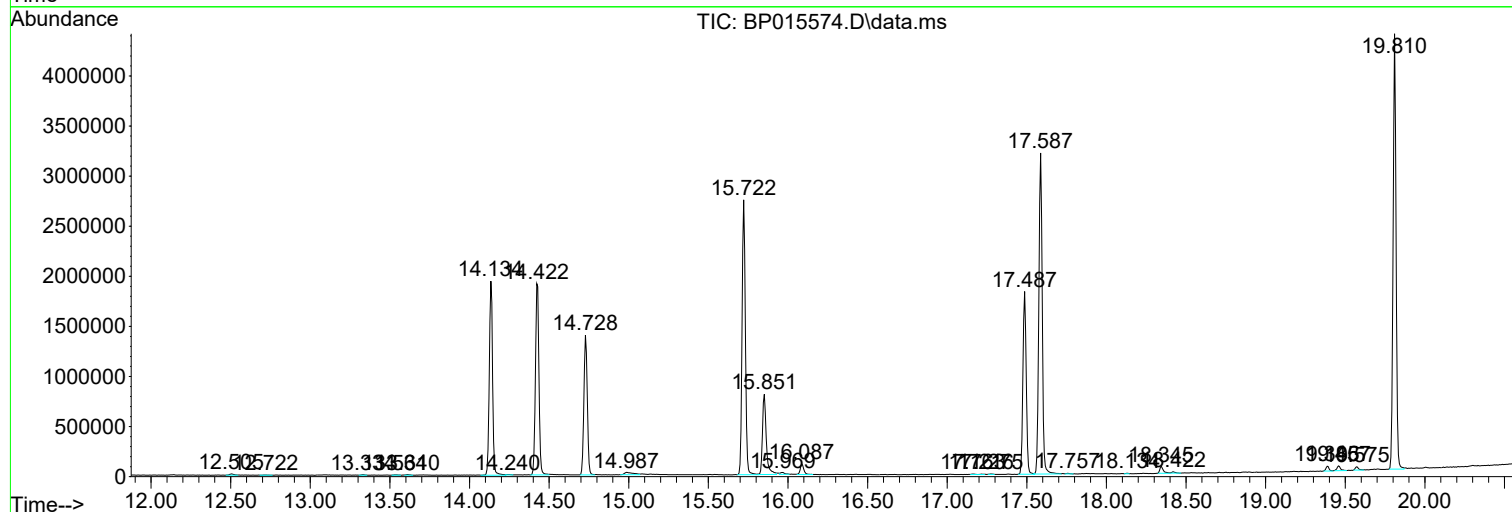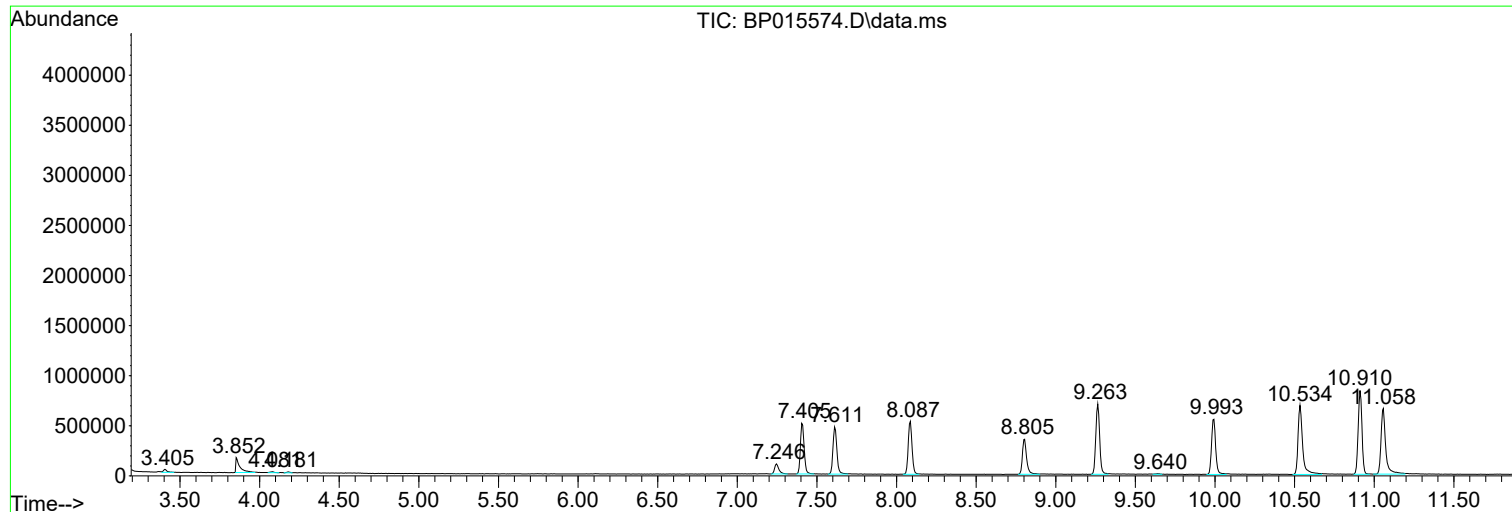

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015574.D
Acq On : 16 Jun 2023 11:17
Operator : MA/JU
Sample : 03220-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015574.D
Acq On : 16 Jun 2023 11:17
Operator : MA/JU
Sample : 03220-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc