

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015578.D
 Acq On : 16 Jun 2023 13:32
 Operator : MA/JU
 Sample : 03220-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	34	37	42	rBV	16914	22558	1.15%	0.125%
2	3.858	112	114	135	rBV	74160	162982	8.34%	0.901%
3	4.887	287	289	292	rBV4	2734	2913	0.15%	0.016%
4	5.393	372	375	377	rBV4	1499	2095	0.11%	0.012%
5	6.175	504	508	511	rVB6	2161	2796	0.14%	0.015%
6	6.211	511	514	518	rVB6	1398	2025	0.10%	0.011%
7	6.587	577	578	581	rBV3	2319	2089	0.11%	0.012%
8	7.169	673	677	683	rVB9	3021	7389	0.38%	0.041%
9	7.246	683	690	704	rBV	94553	194993	9.98%	1.078%
10	7.346	705	707	710	rVB4	2296	2193	0.11%	0.012%
11	7.410	712	718	729	rVV	126168	219213	11.22%	1.212%
12	7.616	746	753	766	rBV	130487	242724	12.43%	1.342%
13	7.757	774	777	780	rBV5	1979	2089	0.11%	0.012%
14	7.981	811	815	819	rBV7	1616	2560	0.13%	0.014%
15	8.087	825	833	846	rBV	318716	537632	27.52%	2.972%
16	8.805	949	955	970	rBV	135535	285086	14.59%	1.576%
17	9.269	1025	1034	1045	rBV	154274	299395	15.33%	1.655%
18	9.340	1045	1046	1051	rVB5	2941	4007	0.21%	0.022%
19	9.640	1094	1097	1100	rVB5	2094	2241	0.11%	0.012%
20	9.993	1150	1157	1167	rBV	111743	223467	11.44%	1.235%
21	10.075	1169	1171	1175	rVB5	2042	2895	0.15%	0.016%
22	10.546	1243	1251	1266	rBV	116229	311599	15.95%	1.722%
23	10.699	1275	1277	1281	rVB5	2465	3014	0.15%	0.017%
24	10.910	1303	1313	1323	rBV	485713	836663	42.83%	4.625%
25	11.063	1331	1339	1356	rBV	144562	372880	19.09%	2.061%
26	11.328	1382	1384	1389	rVB6	3411	4044	0.21%	0.022%
27	11.416	1396	1399	1401	rBV3	1695	2022	0.10%	0.011%
28	12.134	1519	1521	1524	rVB3	2228	2025	0.10%	0.011%
29	12.263	1537	1543	1546	rBV8	1604	3535	0.18%	0.020%
30	12.334	1551	1555	1556	rBV4	1442	2302	0.12%	0.013%
31	12.516	1581	1586	1595	rBV4	2810	6353	0.33%	0.035%
32	12.640	1604	1607	1611	rVB5	1631	2702	0.14%	0.015%
33	12.769	1627	1629	1634	rVB5	2182	3095	0.16%	0.017%
34	12.851	1640	1643	1647	rBV5	1215	1994	0.10%	0.011%
35	13.610	1767	1772	1776	rBV3	8855	13974	0.72%	0.077%
36	13.716	1788	1790	1794	rVB4	2102	2339	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015578.D
 Acq On : 16 Jun 2023 13:32
 Operator : MA/JU
 Sample : 03220-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	13.792	1800	1803	1804	rBV3	2117	2261	0.12%	0.012%
38	14.134	1852	1861	1879	rBV	500134	791923	40.54%	4.378%
39	14.422	1903	1910	1924	rBV	510307	813812	41.66%	4.499%
40	14.728	1955	1962	1974	rBV	883950	1299765	66.54%	7.185%
41	15.010	2004	2010	2013	rBV5	16619	37940	1.94%	0.210%
42	15.439	2080	2083	2084	rBV3	2398	2105	0.11%	0.012%
43	15.722	2125	2131	2144	rBV	701873	1098882	56.26%	6.074%
44	15.863	2150	2155	2168	rBV	55200	118140	6.05%	0.653%
45	16.098	2191	2195	2202	rVB2	10271	17246	0.88%	0.095%
46	16.657	2287	2290	2294	rBV6	3032	4259	0.22%	0.024%
47	16.751	2301	2306	2308	rBV5	1570	2216	0.11%	0.012%
48	16.910	2328	2333	2335	rBV6	1617	3367	0.17%	0.019%
49	17.269	2390	2394	2400	rVV8	3360	6270	0.32%	0.035%
50	17.486	2423	2431	2441	rBV	1132137	1715439	87.82%	9.483%
51	17.586	2442	2448	2466	rVB	806008	1288835	65.98%	7.124%
52	17.992	2515	2517	2519	rBV3	2336	2258	0.12%	0.012%
53	18.357	2575	2579	2581	rBV4	9752	12562	0.64%	0.069%
54	19.386	2751	2754	2758	rBV5	12684	16837	0.86%	0.093%
55	19.810	2820	2826	2836	rBV	1167410	1641271	84.02%	9.073%
56	21.569	3120	3125	3138	rBV	1340162	1953351	100.00%	10.798%
57	23.945	3523	3529	3542	rVB2	723910	1551399	79.42%	8.576%
58	24.110	3551	3557	3569	rVB	847449	1918422	98.21%	10.605%




Sum of corrected areas: 18090443

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015578.D
Acq On : 16 Jun 2023 13:32
Operator : MA/JU
Sample : 03220-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

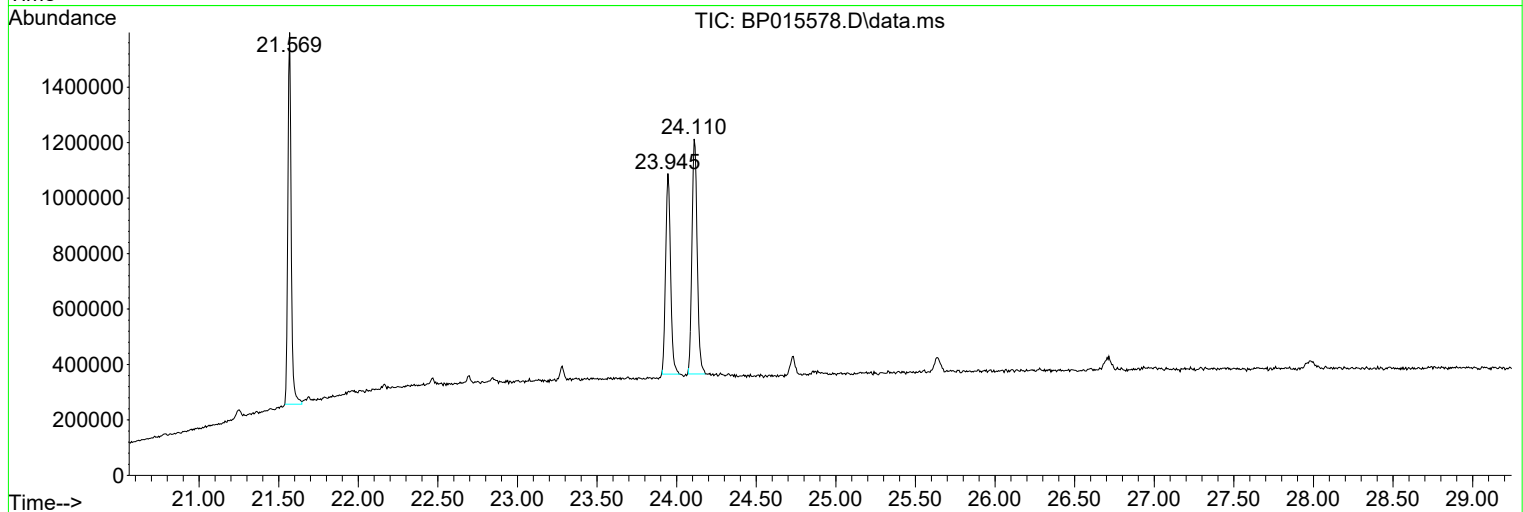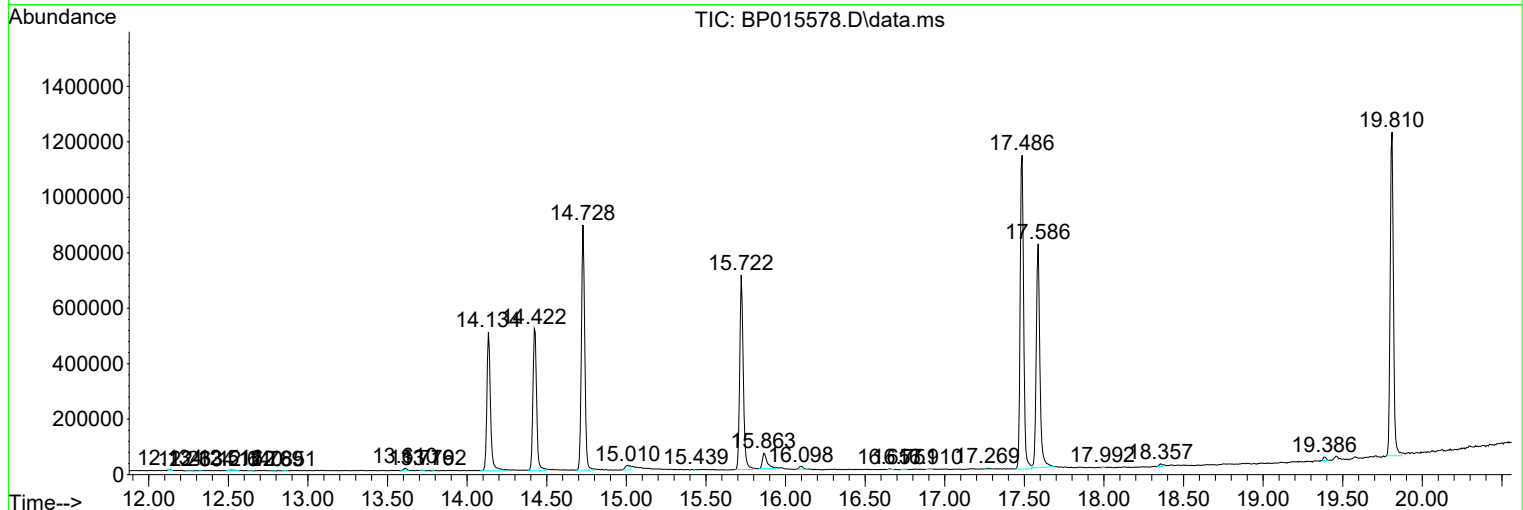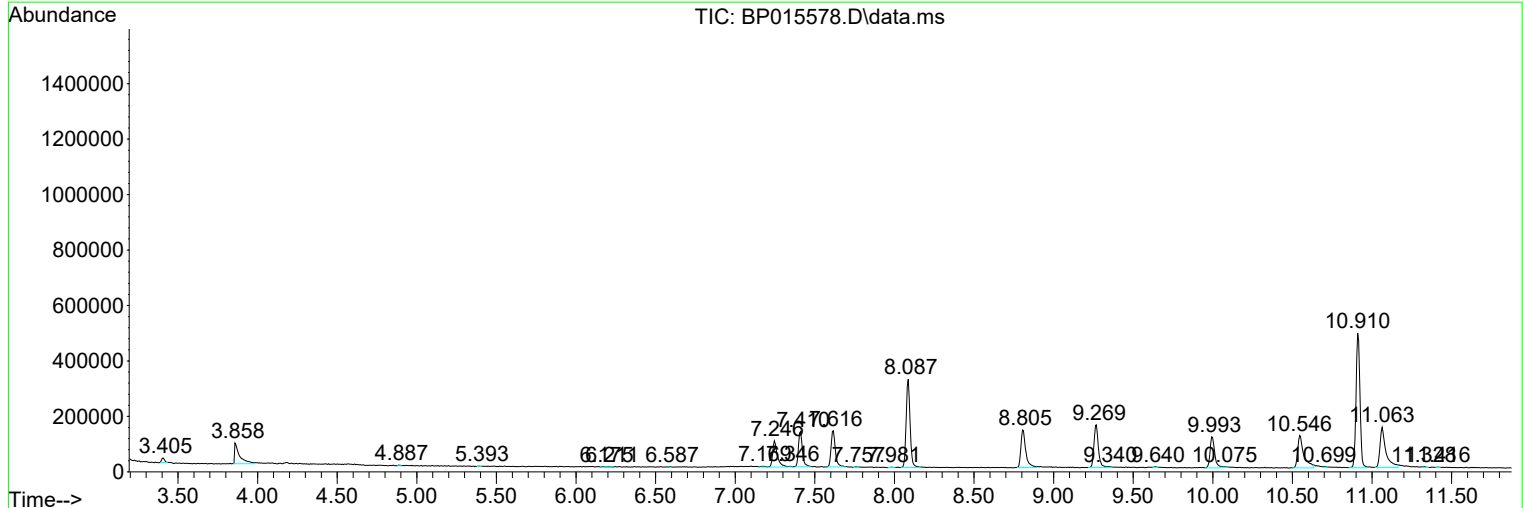

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015578.D
Acq On : 16 Jun 2023 13:32
Operator : MA/JU
Sample : 03220-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015578.D
Acq On : 16 Jun 2023 13:32
Operator : MA/JU
Sample : 03220-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0NR5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc