

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015582.D
 Acq On : 16 Jun 2023 15:48
 Operator : MA/JU
 Sample : 03104-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	34	rBV2	18378	26958	0.56%	0.072%
2	3.405	34	37	41	rVB	18337	23993	0.50%	0.064%
3	3.858	112	114	126	rBV	85737	158047	3.29%	0.422%
4	4.075	149	151	159	rVB4	9937	15472	0.32%	0.041%
5	4.181	165	169	177	rVB2	14072	21702	0.45%	0.058%
6	7.246	684	690	703	rBV	68173	137267	2.86%	0.366%
7	7.405	711	717	729	rBV	356384	594430	12.36%	1.587%
8	7.610	745	752	764	rBV	331086	568035	11.82%	1.516%
9	8.087	826	833	847	rBV	357681	613072	12.75%	1.636%
10	8.804	947	955	971	rBV	240221	463423	9.64%	1.237%
11	9.263	1026	1033	1047	rBV	479009	839811	17.47%	2.241%
12	9.799	1120	1124	1130	rVB9	2654	5154	0.11%	0.014%
13	9.993	1149	1157	1170	rBV	377962	686689	14.28%	1.833%
14	10.534	1240	1249	1269	rBV	440949	905862	18.84%	2.418%
15	10.910	1305	1313	1327	rVB	569879	946450	19.69%	2.526%
16	11.057	1330	1338	1363	rBV	418346	920542	19.15%	2.457%
17	12.510	1579	1585	1592	rBV4	8400	19261	0.40%	0.051%
18	13.610	1767	1772	1778	rVV	20670	33814	0.70%	0.090%
19	14.134	1852	1861	1876	rBV	1477398	2092793	43.53%	5.586%
20	14.422	1903	1910	1924	rBV	1493051	2229493	46.37%	5.951%
21	14.592	1934	1939	1945	rVB10	3497	8606	0.18%	0.023%
22	14.728	1955	1962	1973	rBV	986951	1454511	30.25%	3.882%
23	14.998	2001	2008	2014	rBV7	16188	51735	1.08%	0.138%
24	15.469	2085	2088	2094	rVV6	4558	6903	0.14%	0.018%
25	15.722	2124	2131	2141	rBV	2040393	3066395	63.78%	8.184%
26	15.851	2146	2153	2168	rVV	627598	1099791	22.88%	2.935%
27	15.963	2168	2172	2185	rVV5	17453	41168	0.86%	0.110%
28	16.086	2188	2193	2203	rVB	77299	122556	2.55%	0.327%
29	16.504	2260	2264	2267	rVB6	3242	4809	0.10%	0.013%
30	17.157	2372	2375	2380	rVB6	2947	5220	0.11%	0.014%
31	17.280	2393	2396	2404	rVB10	4329	6706	0.14%	0.018%
32	17.480	2424	2430	2441	rBV	1342215	1967245	40.92%	5.251%
33	17.586	2441	2448	2464	rVV	2536365	3819794	79.45%	10.195%
34	17.751	2474	2476	2484	rVB9	5944	10339	0.22%	0.028%
35	18.339	2572	2576	2584	rBV2	98964	142866	2.97%	0.381%
36	19.386	2750	2754	2758	rBV	37446	45663	0.95%	0.122%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015582.D
Acq On : 16 Jun 2023 15:48
Operator : MA/JU
Sample : 03104-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	19.457	2762	2766	2773	rVB	36618	59164	1.23%	0.158%
38	19.569	2780	2785	2791	rBV3	62727	101654	2.11%	0.271%
39	19.810	2819	2826	2838	rBV	3407614	4765204	99.12%	12.718%
40	21.569	3119	3125	3137	rBV	1506165	2281281	47.45%	6.089%
41	23.945	3521	3529	3544	rBV2	2229069	4807536	100.00%	12.831%
42	24.110	3550	3557	3569	rVB	1056126	2295445	47.75%	6.127%




Sum of corrected areas: 37466859

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015582.D
Acq On : 16 Jun 2023 15:48
Operator : MA/JU
Sample : 03104-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

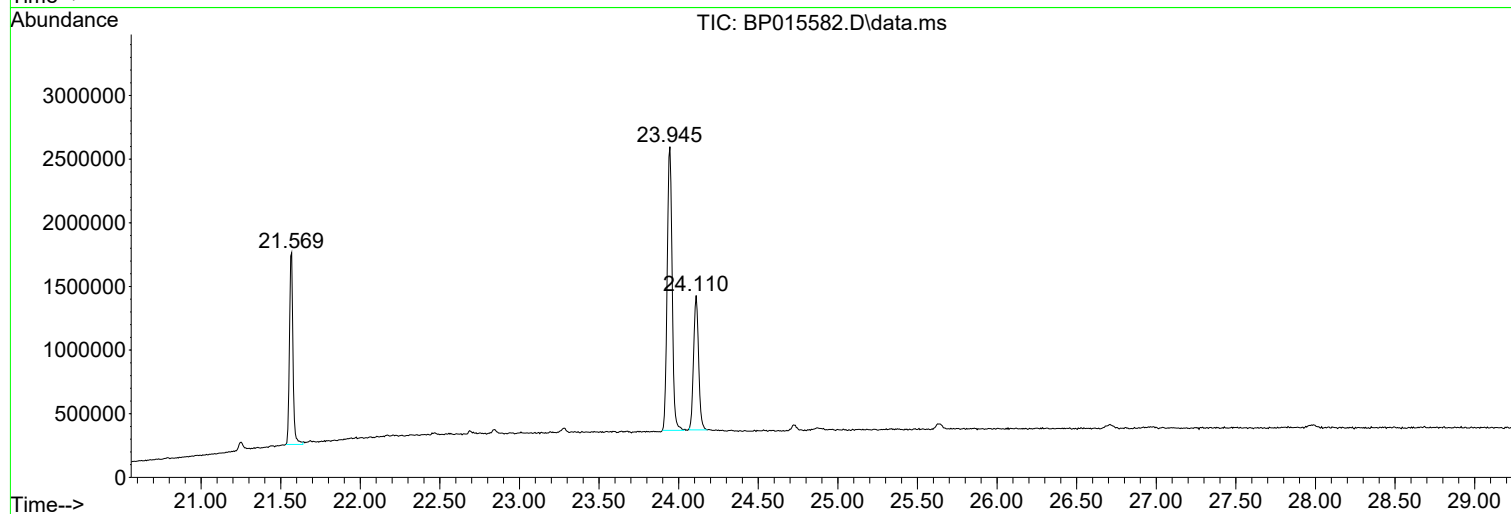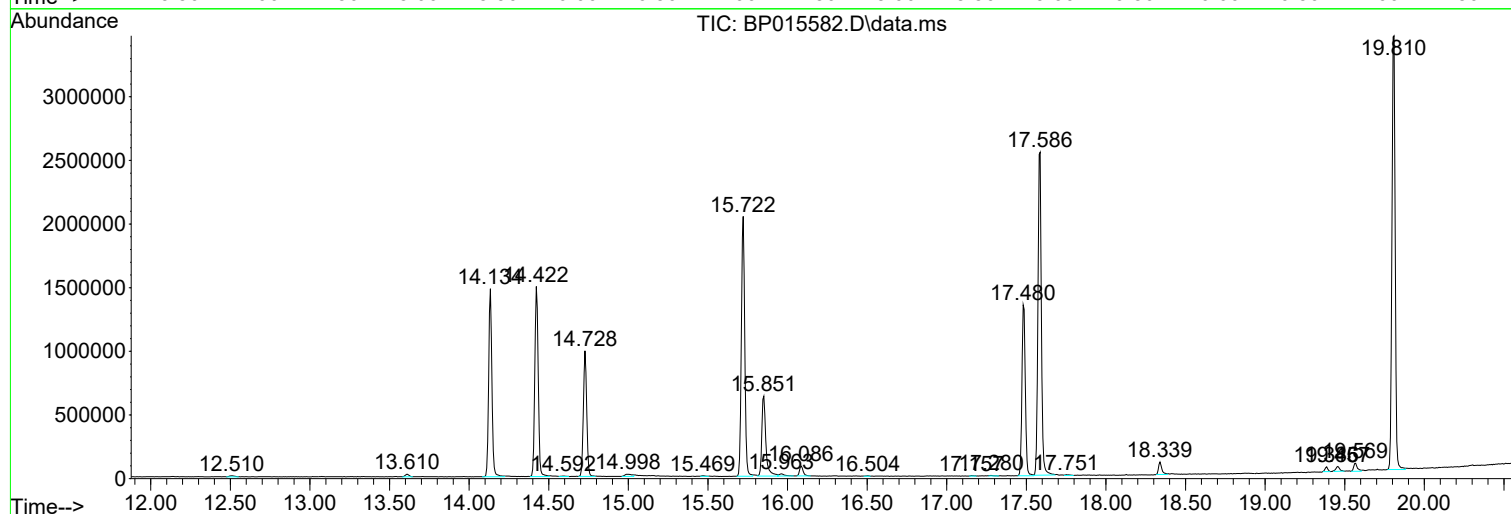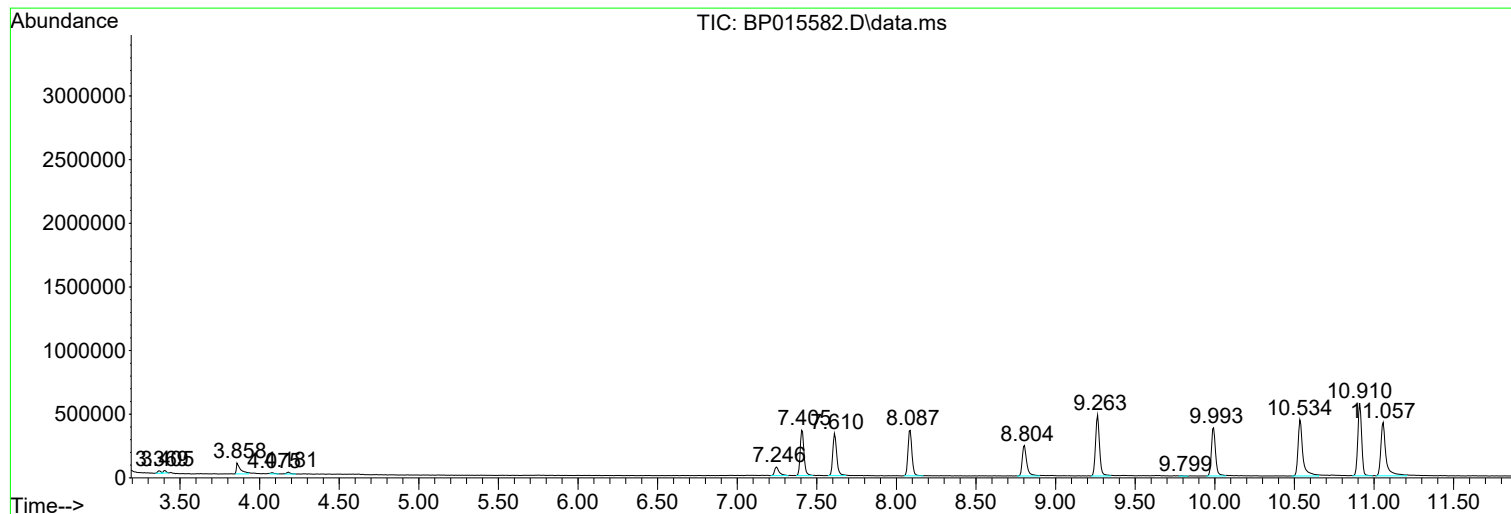

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015582.D
Acq On : 16 Jun 2023 15:48
Operator : MA/JU
Sample : 03104-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONR2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015582.D
Acq On : 16 Jun 2023 15:48
Operator : MA/JU
Sample : 03104-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0NR2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc