

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015583.D
 Acq On : 16 Jun 2023 16:21
 Operator : MA/JU
 Sample : 03220-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	34	rBV2	19386	26751	0.46%	0.056%
2	3.405	34	37	44	rVB	36792	49671	0.86%	0.103%
3	3.852	111	113	127	rBV	143188	261243	4.50%	0.542%
4	4.081	147	152	156	rVB4	12754	19980	0.34%	0.041%
5	4.181	165	169	173	rBV3	6560	9709	0.17%	0.020%
6	6.110	491	497	503	rBV5	6784	11828	0.20%	0.025%
7	7.240	682	689	702	rBV	110937	212192	3.66%	0.440%
8	7.405	709	717	731	rBV	533972	856153	14.75%	1.777%
9	7.610	745	752	763	rBV	504911	833059	14.35%	1.729%
10	7.681	763	764	773	rVB9	6399	7976	0.14%	0.017%
11	8.081	826	832	842	rBV	474285	798101	13.75%	1.656%
12	8.799	947	954	968	rBV	381742	687182	11.84%	1.426%
13	9.263	1024	1033	1048	rBV	694050	1205397	20.76%	2.502%
14	9.640	1094	1097	1102	rVB6	5100	8108	0.14%	0.017%
15	9.987	1148	1156	1175	rBV	580003	1019091	17.55%	2.115%
16	10.534	1242	1249	1269	rBV	665019	1333253	22.97%	2.767%
17	10.910	1304	1313	1329	rVB	735473	1219150	21.00%	2.530%
18	11.051	1329	1337	1356	rBV	629353	1297774	22.36%	2.693%
19	12.510	1578	1585	1593	rBV3	12337	27628	0.48%	0.057%
20	12.722	1613	1621	1628	rBV	13265	24405	0.42%	0.051%
21	13.057	1670	1678	1680	rBV9	3453	7519	0.13%	0.016%
22	13.328	1720	1724	1730	rBV8	5385	7763	0.13%	0.016%
23	13.610	1765	1772	1778	rBV2	28897	47529	0.82%	0.099%
24	14.134	1853	1861	1876	rBV	2073674	2956688	50.93%	6.136%
25	14.228	1876	1877	1884	rVB6	5380	9470	0.16%	0.020%
26	14.422	1903	1910	1921	rBV	2111542	3076942	53.00%	6.385%
27	14.728	1951	1962	1971	rBV	1259509	1864899	32.12%	3.870%
28	14.981	1998	2005	2014	rBV4	27591	94258	1.62%	0.196%
29	15.539	2097	2100	2108	rVB5	6551	11987	0.21%	0.025%
30	15.722	2124	2131	2146	rVV	2832434	4127597	71.10%	8.566%
31	15.845	2146	2152	2168	rVV	929842	1467845	25.29%	3.046%
32	15.963	2168	2172	2177	rVB3	15652	29153	0.50%	0.060%
33	16.086	2187	2193	2206	rVB	101366	171546	2.96%	0.356%
34	16.498	2262	2263	2269	rVB6	4331	6566	0.11%	0.014%
35	16.651	2284	2289	2295	rVB	21627	29116	0.50%	0.060%
36	17.157	2372	2375	2379	rVB6	5332	7457	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015583.D
 Acq On : 16 Jun 2023 16:21
 Operator : MA/JU
 Sample : 03220-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	17.275	2391	2395	2398	rBV6	4260	6617	0.11%	0.014%
38	17.375	2407	2412	2416	rBV8	5778	9174	0.16%	0.019%
39	17.486	2421	2431	2440	rBV	1682900	2470960	42.57%	5.128%
40	17.586	2441	2448	2463	rVV	3260251	4794969	82.60%	9.951%
41	17.757	2472	2477	2485	rVB3	10668	23095	0.40%	0.048%
42	18.339	2572	2576	2583	rBV2	107232	152983	2.64%	0.317%
43	18.422	2586	2590	2592	rVV	13977	21075	0.36%	0.044%
44	18.445	2592	2594	2598	rVB4	11053	13838	0.24%	0.029%
45	18.857	2662	2664	2666	rBV2	5840	6744	0.12%	0.014%
46	19.386	2749	2754	2759	rBV2	51151	76056	1.31%	0.158%
47	19.457	2762	2766	2770	rVB	46580	64669	1.11%	0.134%
48	19.569	2781	2785	2793	rBV3	62028	91934	1.58%	0.191%
49	19.810	2819	2826	2836	rBV	4296054	5805144	100.00%	12.047%
50	21.251	3066	3071	3080	rBV5	102904	239288	4.12%	0.497%
51	21.568	3119	3125	3134	rBV	1802272	2598645	44.76%	5.393%
52	23.945	3521	3529	3540	rBV2	2489294	5465029	94.14%	11.341%
53	24.110	3550	3557	3569	rBV	1132158	2521723	43.44%	5.233%




Sum of corrected areas: 48186929

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015583.D
Acq On : 16 Jun 2023 16:21
Operator : MA/JU
Sample : 03220-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONK8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

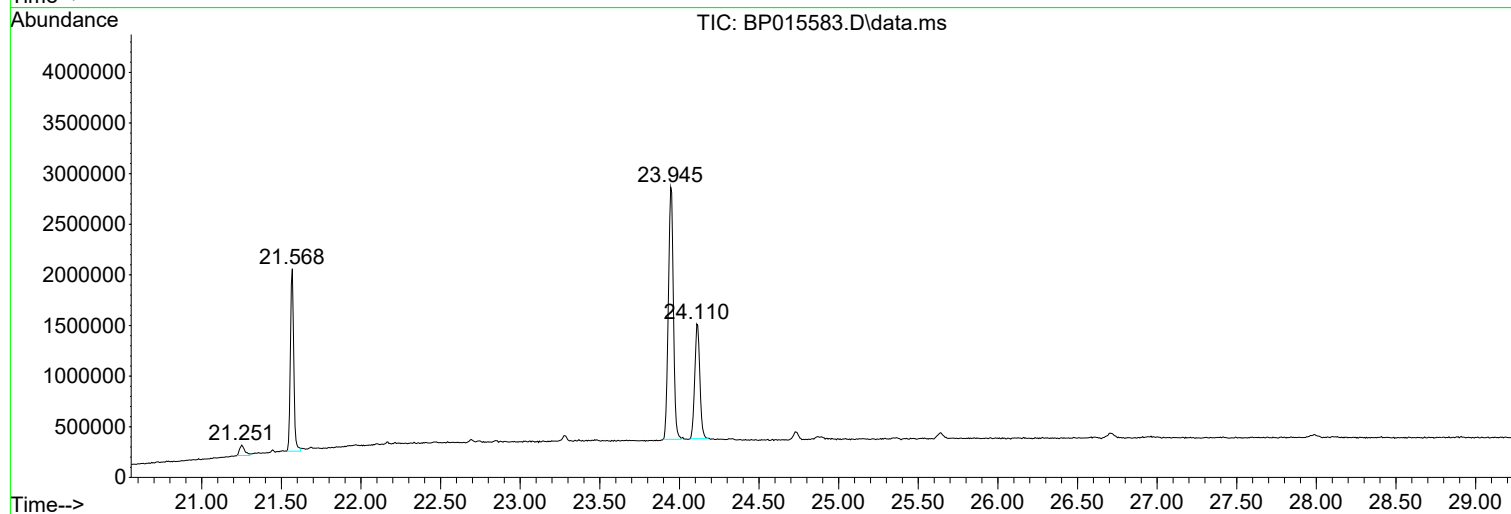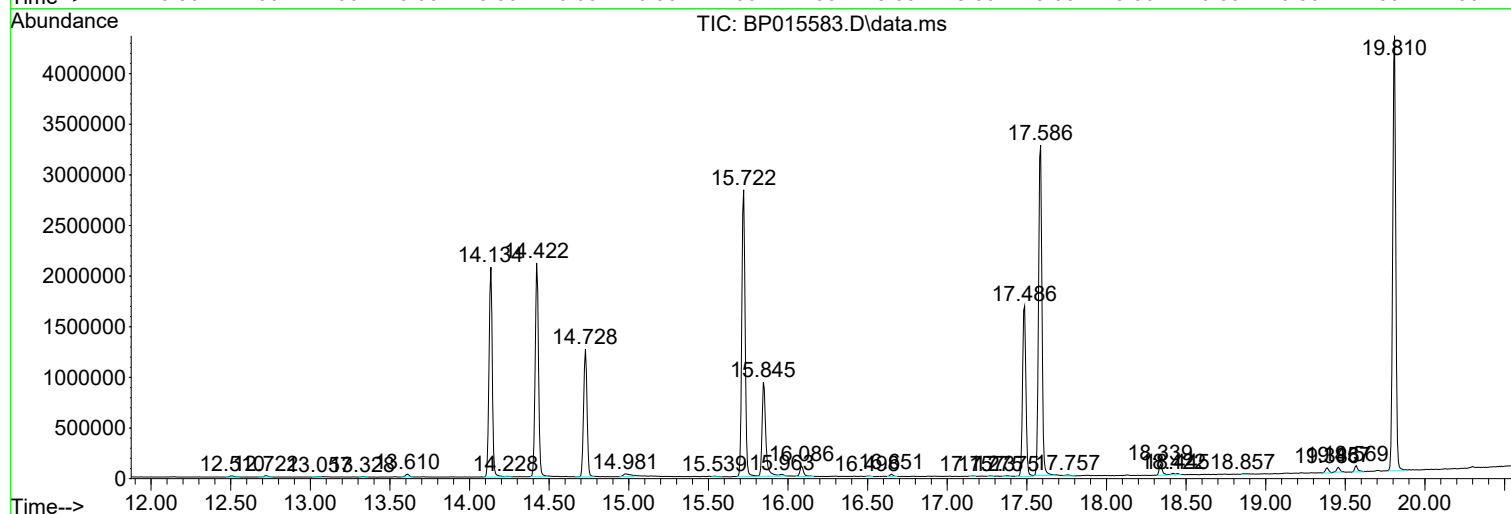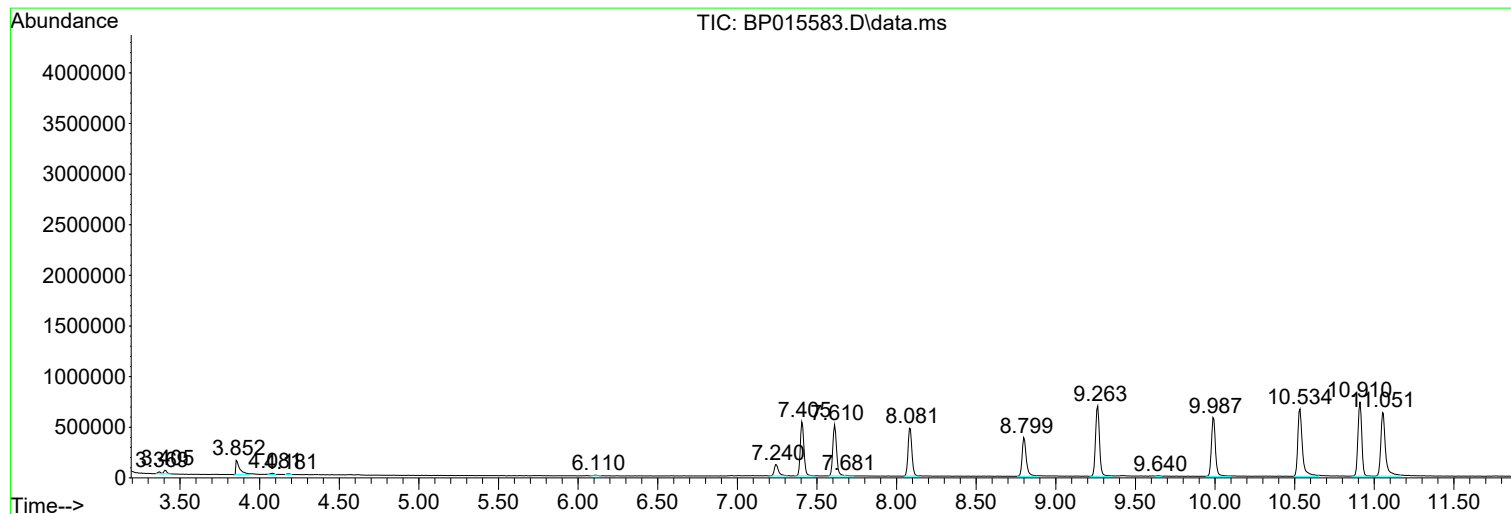

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015583.D
Acq On : 16 Jun 2023 16:21
Operator : MA/JU
Sample : 03220-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONK8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015583.D
Acq On : 16 Jun 2023 16:21
Operator : MA/JU
Sample : 03220-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONK8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------