

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015585.D
 Acq On : 16 Jun 2023 17:29
 Operator : MA/JU
 Sample : 03220-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015585.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	44	rBV	23128	31214	0.66%	0.084%
2	3.858	112	114	133	rBV	90229	198638	4.18%	0.535%
3	4.075	149	151	157	rVB3	10168	13856	0.29%	0.037%
4	4.175	165	168	173	rBV3	6540	9990	0.21%	0.027%
5	6.111	493	497	504	rVB8	3917	6854	0.14%	0.018%
6	7.246	683	690	702	rBV	82266	159049	3.34%	0.429%
7	7.405	710	717	732	rBV	388265	626060	13.16%	1.688%
8	7.610	744	752	762	rBV	353514	610323	12.83%	1.645%
9	8.087	825	833	843	rBV	363830	619936	13.03%	1.671%
10	8.805	947	955	968	rBV	268753	514600	10.82%	1.387%
11	9.263	1025	1033	1048	rBV	500238	874375	18.38%	2.357%
12	9.993	1150	1157	1178	rBV	399502	732336	15.39%	1.974%
13	10.534	1242	1249	1273	rBV	461855	970946	20.41%	2.618%
14	10.910	1305	1313	1323	rBV	565331	942852	19.82%	2.542%
15	11.057	1331	1338	1358	rBV	433786	938786	19.73%	2.531%
16	12.510	1578	1585	1590	rBV2	8540	17687	0.37%	0.048%
17	12.728	1613	1622	1629	rBV	10049	19978	0.42%	0.054%
18	13.334	1720	1725	1729	rVB8	4138	6768	0.14%	0.018%
19	13.610	1767	1772	1777	rVB2	12857	18685	0.39%	0.050%
20	14.134	1854	1861	1877	rBV	1546023	2200970	46.26%	5.933%
21	14.422	1903	1910	1923	rVV	1526143	2255590	47.41%	6.081%
22	14.728	1954	1962	1971	rBV	978205	1425297	29.96%	3.842%
23	14.992	2001	2007	2009	rBV4	18680	33940	0.71%	0.091%
24	15.134	2030	2031	2040	rVB9	3855	6766	0.14%	0.018%
25	15.539	2097	2100	2106	rVB3	5711	8353	0.18%	0.023%
26	15.722	2124	2131	2146	rVV	2070065	3120022	65.58%	8.411%
27	15.851	2147	2153	2168	rVV	380546	687942	14.46%	1.855%
28	15.957	2168	2171	2179	rVB4	13329	26806	0.56%	0.072%
29	16.086	2188	2193	2202	rBV	74186	114129	2.40%	0.308%
30	16.510	2260	2265	2269	rBV8	3423	5871	0.12%	0.016%
31	16.604	2277	2281	2285	rBV7	3287	5648	0.12%	0.015%
32	16.657	2285	2290	2295	rVB3	13497	22803	0.48%	0.061%
33	17.157	2372	2375	2378	rBV5	4204	5861	0.12%	0.016%
34	17.375	2410	2412	2418	rVB6	4703	6028	0.13%	0.016%
35	17.486	2424	2431	2441	rBV	1301080	1889619	39.72%	5.094%
36	17.586	2441	2448	2465	rVV	2519202	3809818	80.08%	10.271%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015585.D
 Acq On : 16 Jun 2023 17:29
 Operator : MA/JU
 Sample : 03220-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	17.757	2474	2477	2483	rVB4	6987	10008	0.21%	0.027%
38	17.951	2508	2510	2515	rBV6	3128	5216	0.11%	0.014%
39	18.339	2572	2576	2585	rBV2	37987	62705	1.32%	0.169%
40	18.416	2587	2589	2596	rVB2	14871	19705	0.41%	0.053%
41	18.545	2608	2611	2616	rBV6	8559	11561	0.24%	0.031%
42	19.386	2750	2754	2759	rVB2	38940	53631	1.13%	0.145%
43	19.457	2762	2766	2776	rVB	38934	61365	1.29%	0.165%
44	19.569	2782	2785	2789	rBV6	17016	26736	0.56%	0.072%
45	19.810	2819	2826	2837	rBV	3477072	4757369	100.00%	12.825%
46	21.245	3067	3070	3078	rBV5	67709	137227	2.88%	0.370%
47	21.569	3120	3125	3137	rBV	1430042	2092814	43.99%	5.642%
48	23.945	3522	3529	3545	rVB2	2290550	4753257	99.91%	12.814%
49	24.110	3551	3557	3570	rVB	939605	2164123	45.49%	5.834%




Sum of corrected areas: 37094113

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015585.D
Acq On : 16 Jun 2023 17:29
Operator : MA/JU
Sample : 03220-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONQ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

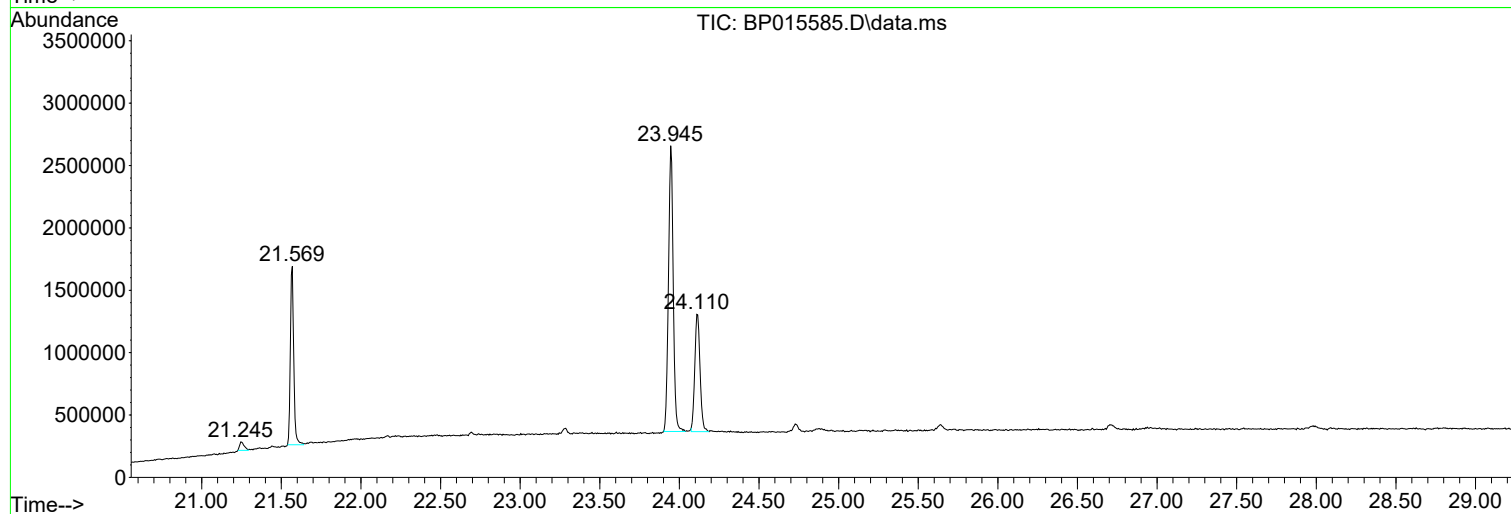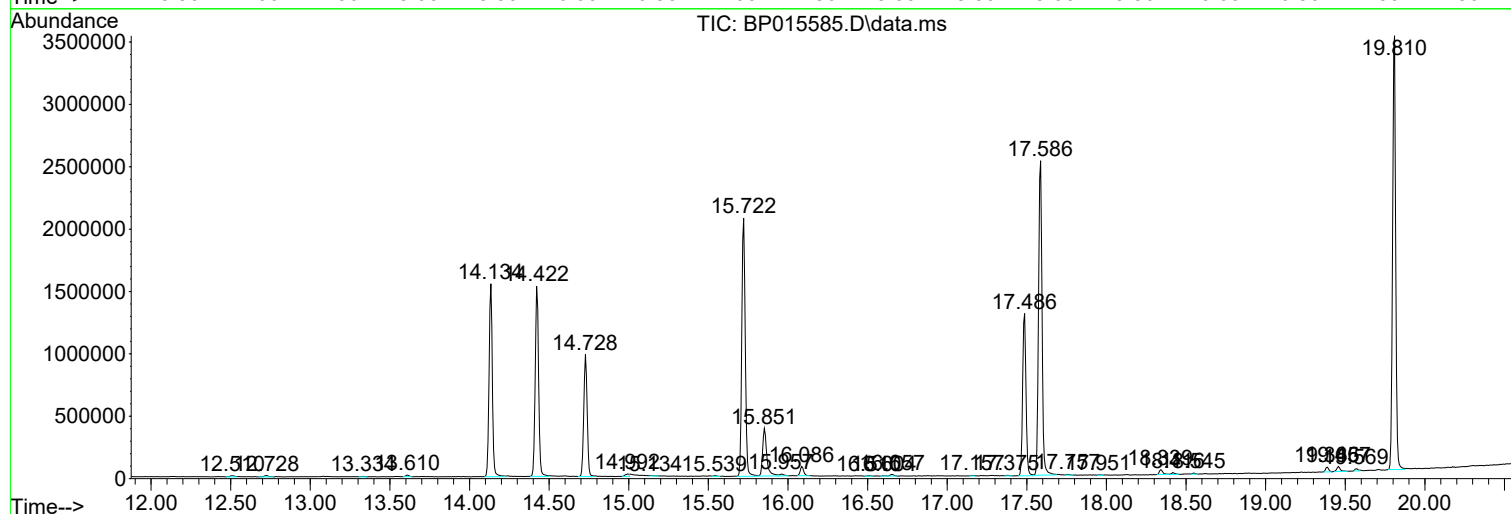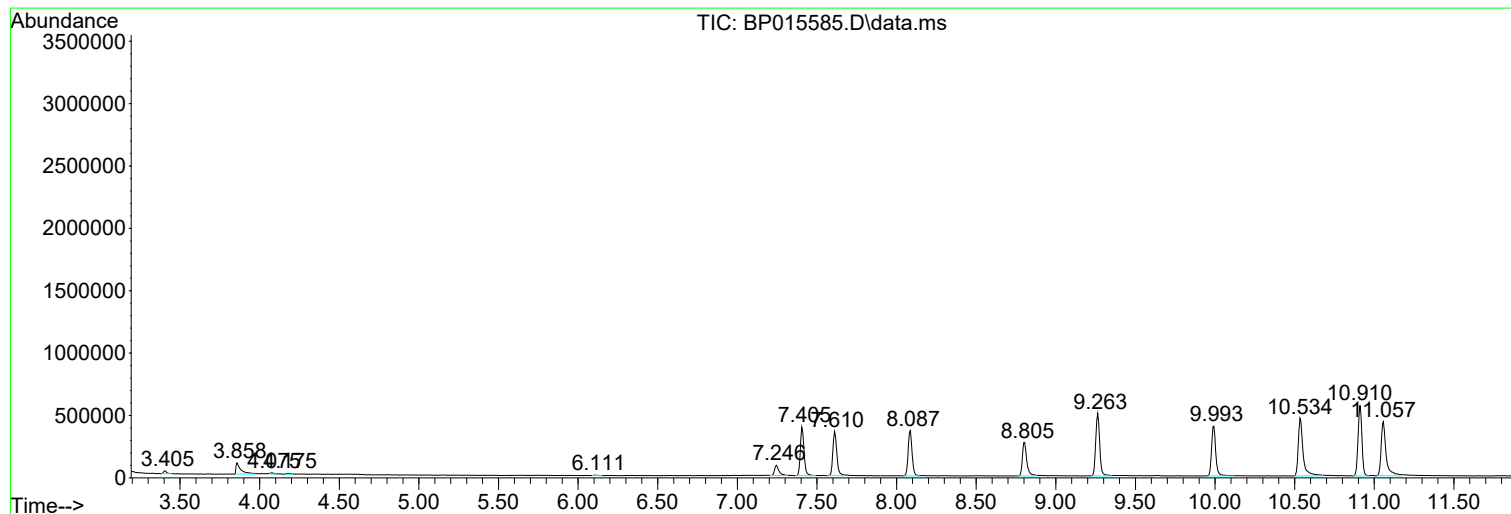

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015585.D
Acq On : 16 Jun 2023 17:29
Operator : MA/JU
Sample : 03220-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONQ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015585.D
Acq On : 16 Jun 2023 17:29
Operator : MA/JU
Sample : 03220-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONQ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------