

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
 Data File : BP015587.D
 Acq On : 16 Jun 2023 18:37
 Operator : MA/JU
 Sample : PB153428BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK428

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.404	33	37	44	rVB	33877	45726	1.00%	0.111%
2	3.846	109	112	133	rBV	393506	727118	15.91%	1.767%
3	4.175	166	168	174	rVB6	6945	8662	0.19%	0.021%
4	7.240	682	689	702	rBV	505055	876683	19.19%	2.130%
5	7.404	711	717	732	rVB	436835	711242	15.57%	1.728%
6	7.610	744	752	766	rBV	545827	915952	20.05%	2.226%
7	8.081	826	832	844	rBV	373704	635263	13.90%	1.544%
8	8.798	947	954	969	rBV	663796	1171731	25.64%	2.847%
9	9.263	1026	1033	1043	rBV	558999	972302	21.28%	2.363%
10	9.986	1149	1156	1174	rBV	472087	864773	18.93%	2.101%
11	10.533	1240	1249	1273	rBV	570096	1206652	26.41%	2.932%
12	10.910	1305	1313	1323	rBV	591408	977920	21.40%	2.376%
13	11.051	1330	1337	1357	rBV	613053	1301455	28.48%	3.162%
14	12.116	1514	1518	1526	rBV	1765	4598	0.10%	0.011%
15	12.510	1580	1585	1591	rBV3	8332	16612	0.36%	0.040%
16	13.610	1768	1772	1779	rVB8	7930	12704	0.28%	0.031%
17	14.133	1852	1861	1876	rBV	1604262	2340803	51.23%	5.688%
18	14.422	1903	1910	1927	rBV2	1668388	2505625	54.84%	6.088%
19	14.727	1954	1962	1977	rBV	1025390	1521361	33.30%	3.697%
20	14.945	1993	1999	2028	rBV	264650	897861	19.65%	2.182%
21	15.721	2124	2131	2146	rBV	2186169	3203370	70.11%	7.784%
22	15.845	2146	2152	2168	rVV	674155	1110379	24.30%	2.698%
23	15.963	2169	2172	2181	rVB5	14366	27008	0.59%	0.066%
24	17.157	2369	2375	2379	rBV9	4772	9093	0.20%	0.022%
25	17.268	2392	2394	2399	rBV5	3722	4817	0.11%	0.012%
26	17.486	2423	2431	2440	rBV	1373639	2037565	44.59%	4.951%
27	17.580	2441	2447	2469	rVB2	2342141	3692425	80.81%	8.972%
28	17.992	2514	2517	2519	rBV4	3540	4736	0.10%	0.012%
29	19.386	2750	2754	2760	rVB2	36020	46425	1.02%	0.113%
30	19.457	2762	2766	2772	rVV2	33158	51568	1.13%	0.125%
31	19.804	2819	2825	2839	rBV	3246645	4569132	100.00%	11.103%
32	21.568	3120	3125	3136	rBV	1557201	2217112	48.52%	5.387%
33	23.945	3521	3529	3548	rBV	1956569	4335442	94.89%	10.535%
34	24.109	3551	3557	3568	rVB	944473	2129783	46.61%	5.175%

Sum of corrected areas: 41153898




Instrument :
BNA_P
ClientSampleId :
SBLK428

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015587.D
Acq On : 16 Jun 2023 18:37
Operator : MA/JU
Sample : PB153428BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK428

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

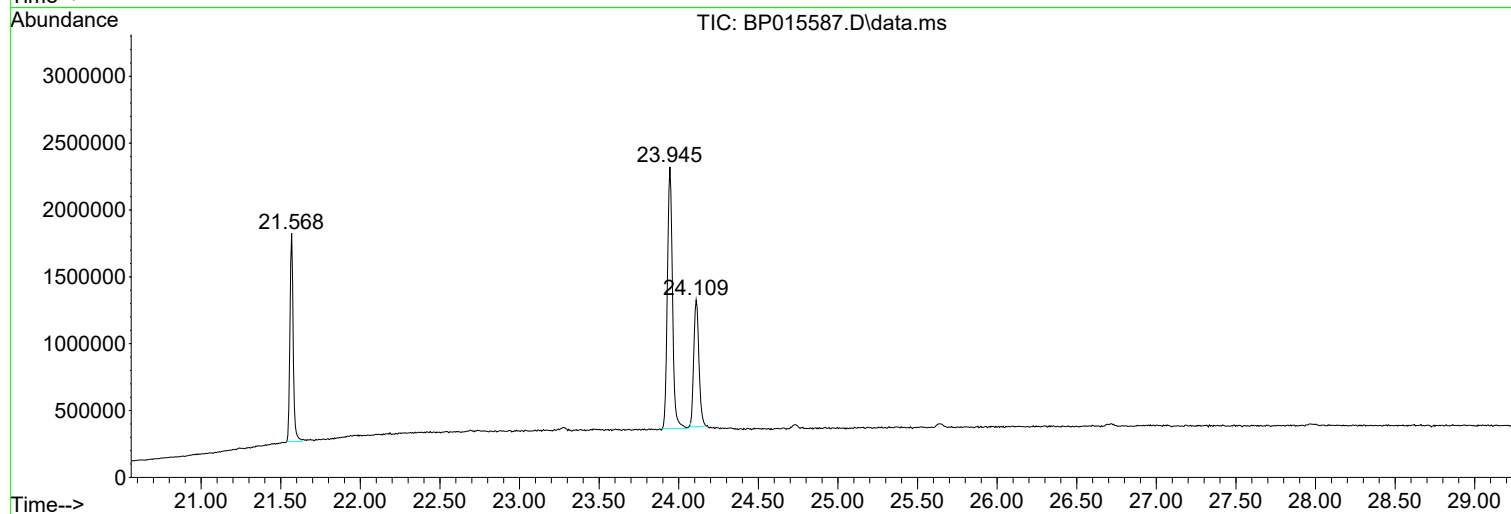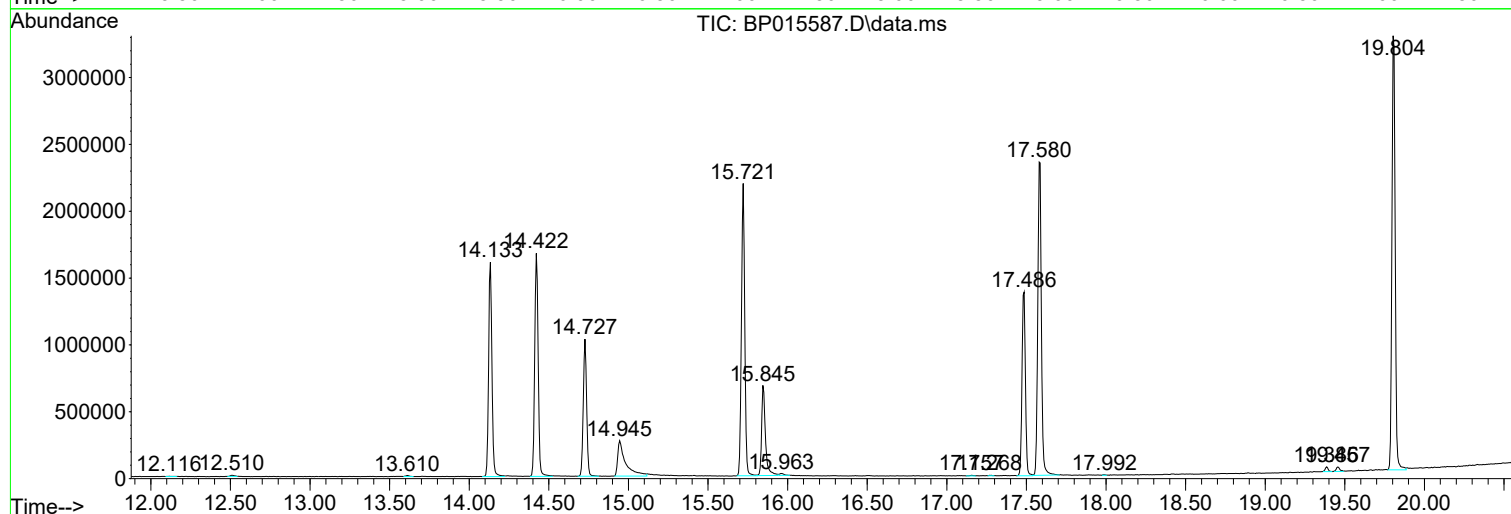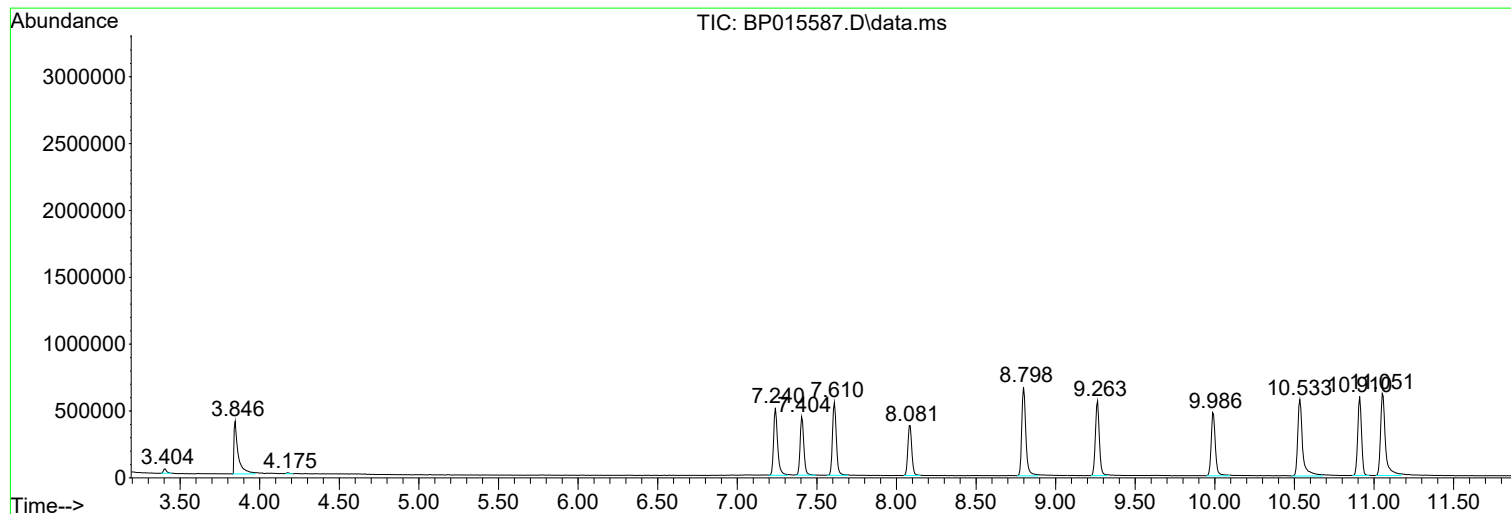

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015587.D
Acq On : 16 Jun 2023 18:37
Operator : MA/JU
Sample : PB153428BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK428

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061623\
Data File : BP015587.D
Acq On : 16 Jun 2023 18:37
Operator : MA/JU
Sample : PB153428BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK428

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc