
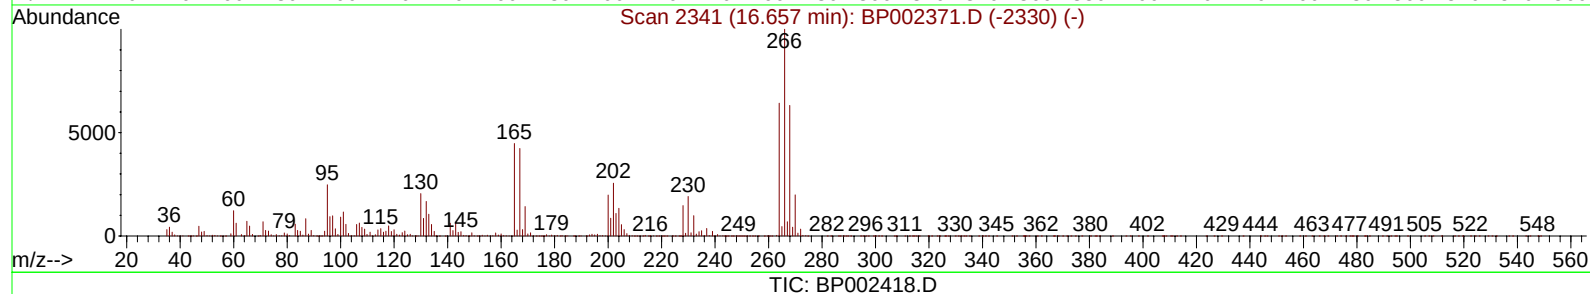
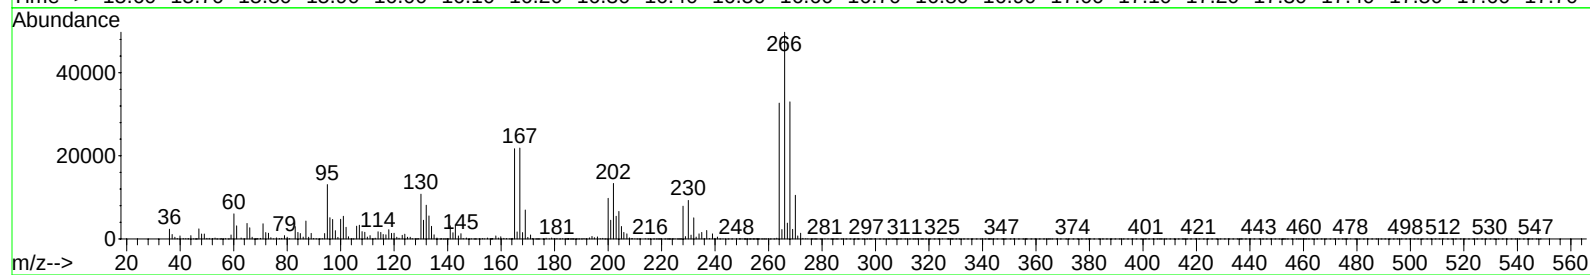


```
Data Path   : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061720\  
Data File   : BP002418.D  
Acq On      : 17 Jun 2020   14:36  
Operator    : CG/JU  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jun 17 18:32:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

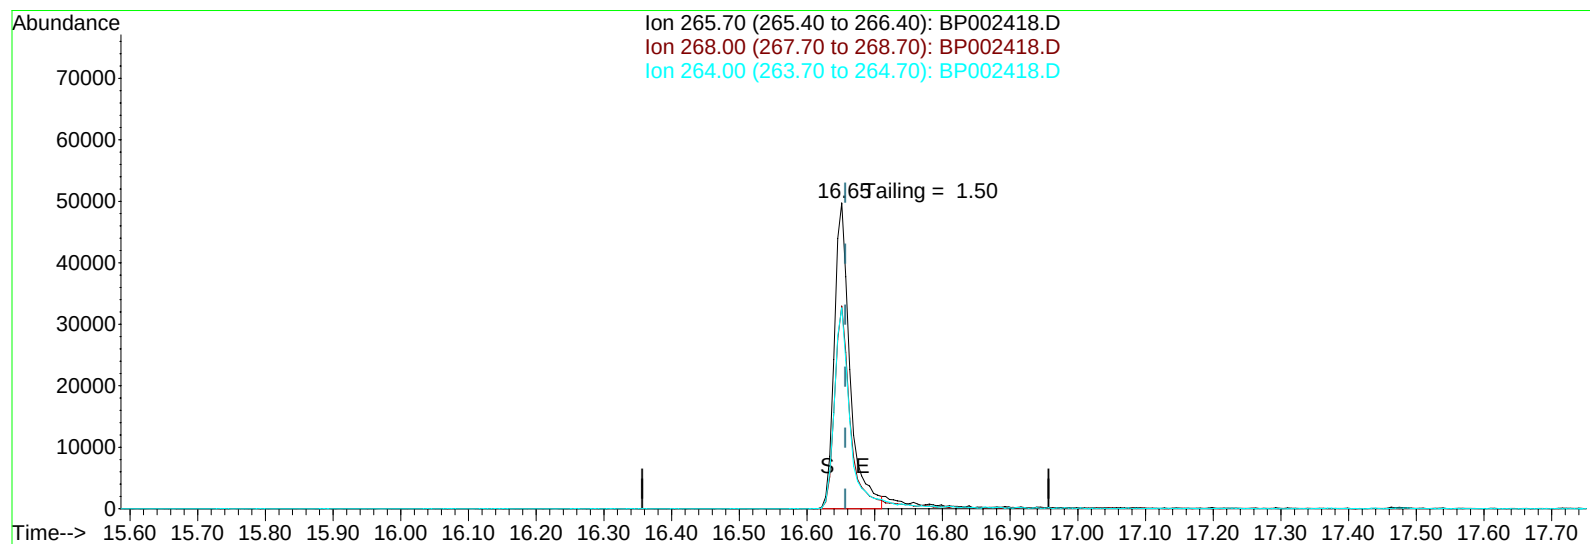

(70) Pentachlorophenol (C)




16.651min (-0.005) 1072151.10ng

response 83824

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	66.30
264.00	64.20	65.69
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061720\
 Data File : BP002418.D
 Acq On : 17 Jun 2020 14:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 18:32:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

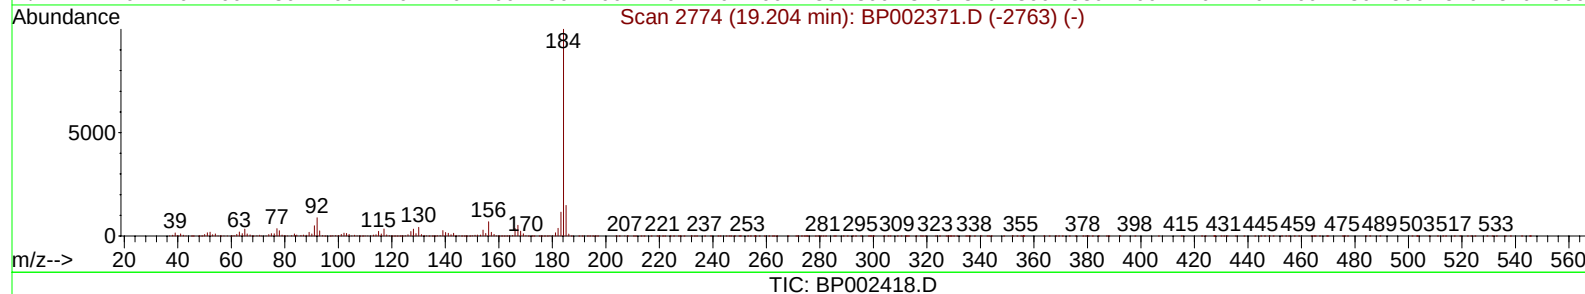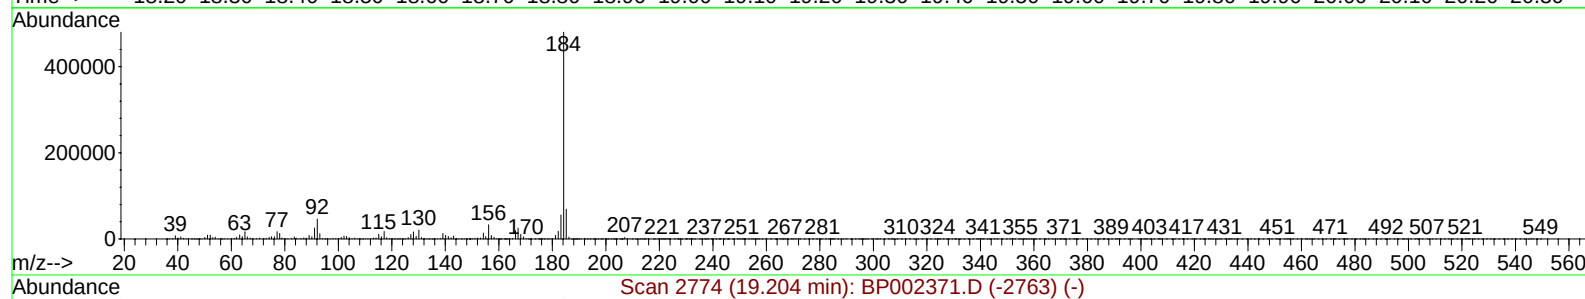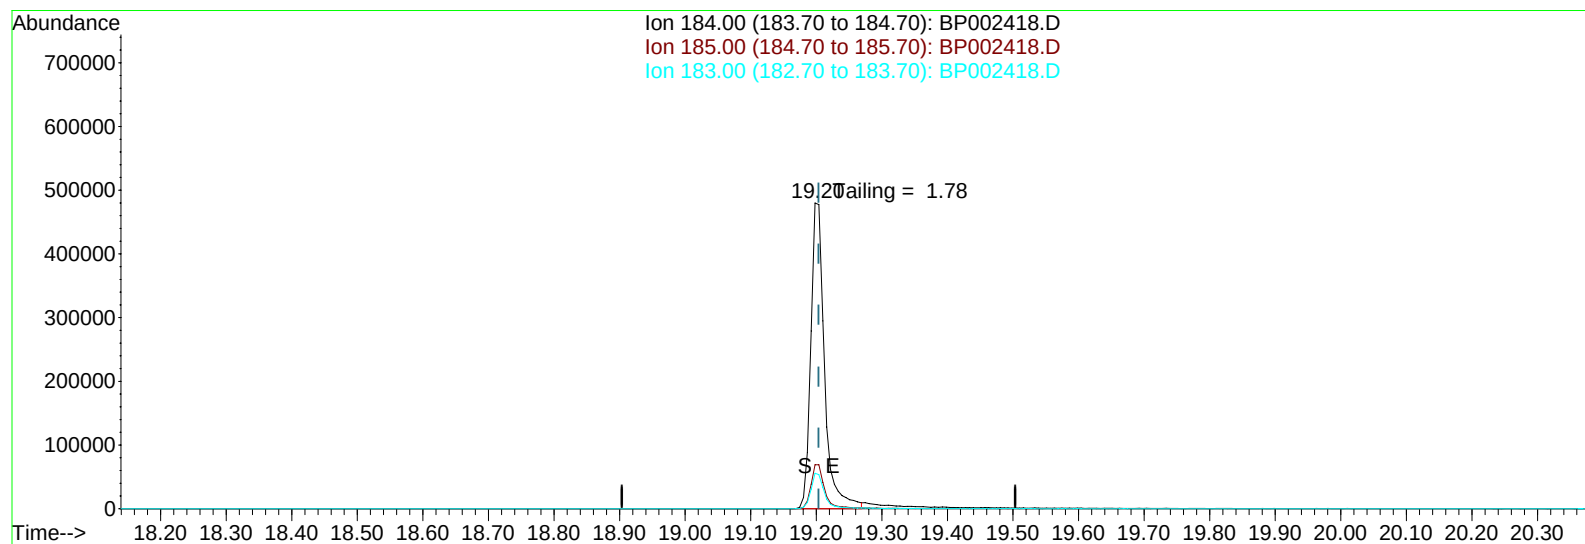

(77) Benzidine

19.198min (-0.005) 1256089.19ng

response 729751

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.40
183.00	11.50	11.64
0.00	0.00	0.00