

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061720\
 Data File : BP002420.D
 Acq On : 17 Jun 2020 15:44
 Operator : CG/JU
 Sample : PB129590BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129590BL

Quant Time: Jun 17 16:43:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	134952	20.00	ng	0.00
21) Naphthalene-d8	10.36	136	546505	20.00	ng	0.00
39) Acenaphthene-d10	14.23	164	341647	20.00	ng	0.00
64) Phenanthrene-d10	16.99	188	776432	20.00	ng	0.00
76) Chrysene-d12	21.09	240	804286	20.00	ng	-0.02
86) Perylene-d12	23.29	264	844770	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.20	112	1085396	148.83	ng	0.00
7) Phenol-d6	6.78	99	1442580	148.57	ng	0.00
23) Nitrobenzene-d5	8.73	82	983429	107.46	ng	-0.01
42) 2,4,6-Tribromophenol	15.73	330	536742	164.09	ng	0.00
45) 2-Fluorobiphenyl	12.85	172	2102925	103.50	ng	0.00
79) Terphenyl-d14	19.58	244	3449108	122.46	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061720\
Data File : BP002420.D
Acq On : 17 Jun 2020 15:44
Operator : CG/JU
Sample : PB129590BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129590BL

Quant Time: Jun 17 16:43:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

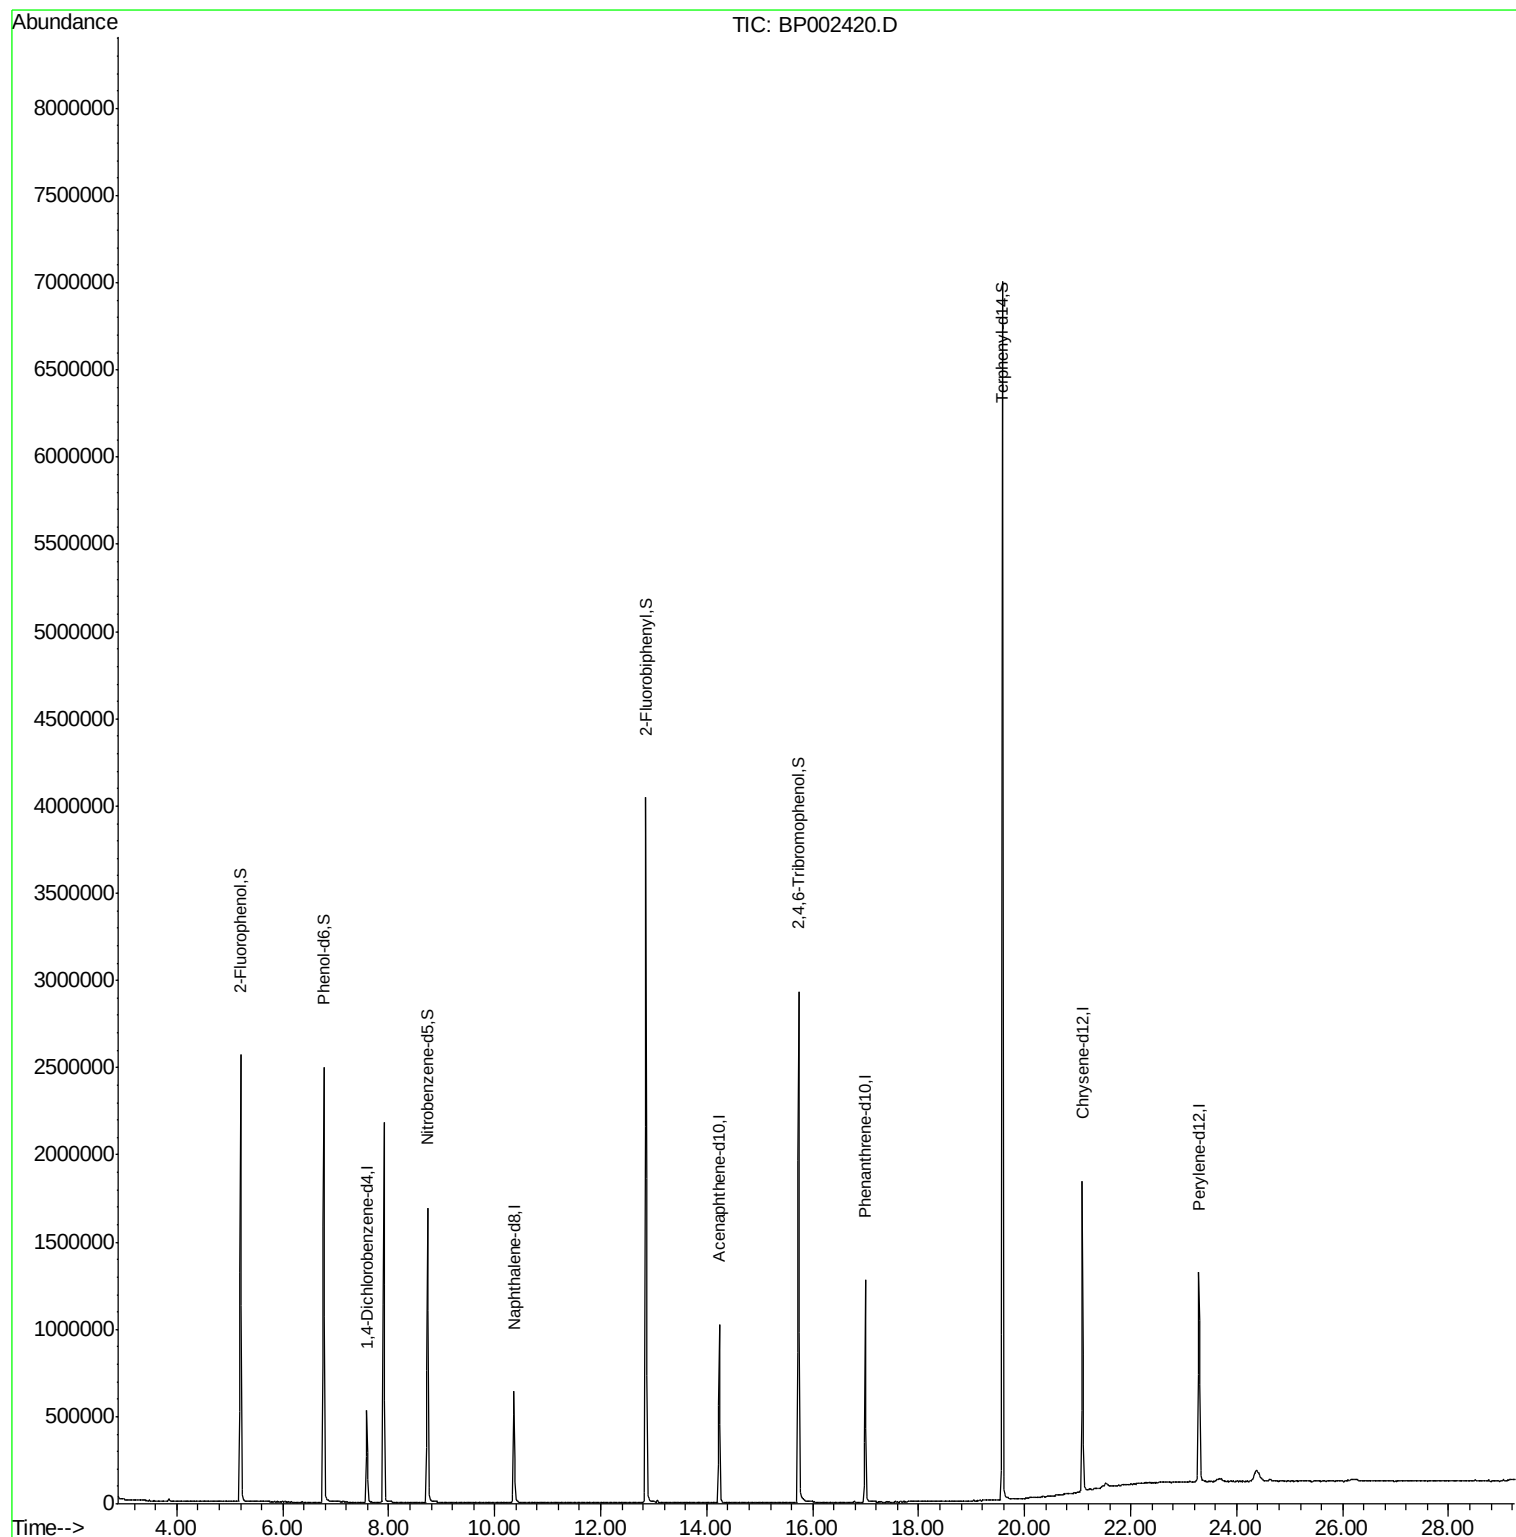

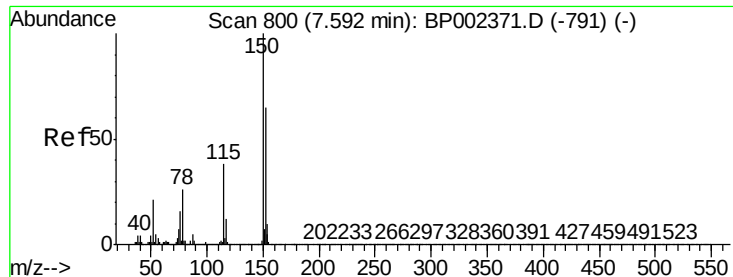


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.59 min Scan# 799
Delta R.T. -0.01 min
Lab File: BP002420.D
Acq: 17 Jun 2020 15:44

Instrument :
BNA_P
ClientSampleId :
PB129590BL

Tot Ion:152 Resp: 134952
Ion Ratio Lower Upper
152 100
150 159.3 124.0 186.0
115 59.5 47.4 71.0

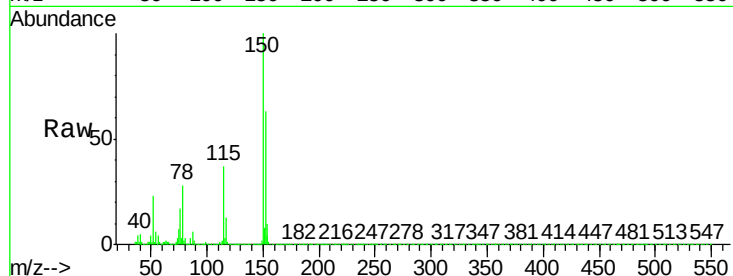


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

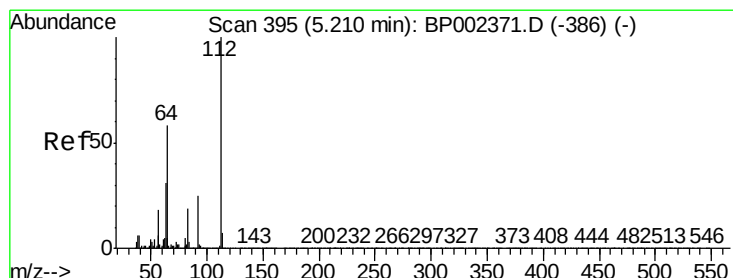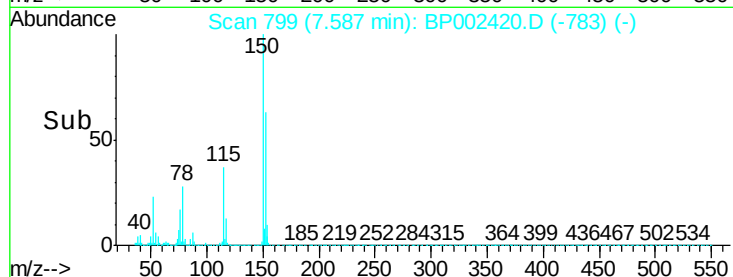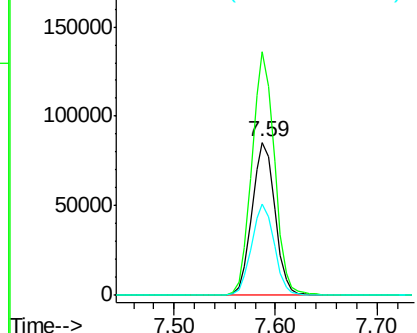



#5


2-Fluorophenol
Concen: 148.826 ng
RT: 5.20 min Scan# 394
Delta R.T. -0.01 min
Lab File: BP002420.D
Acq: 17 Jun 2020 15:44

Tgt Ion:112 Resp: 1085396
Ion Ratio Lower Upper
112 100
64 59.4 46.2 69.2
63 31.7 24.5 36.7

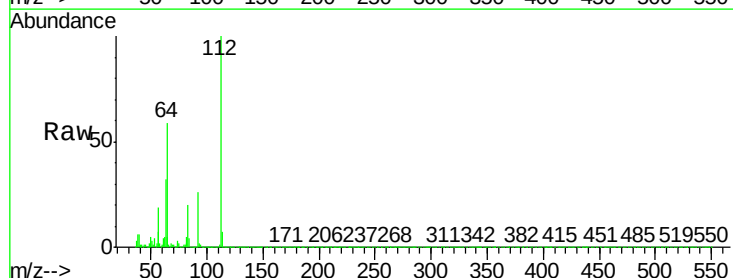

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BP0
Ion 63.00 (62.70 to 63.70): BP0

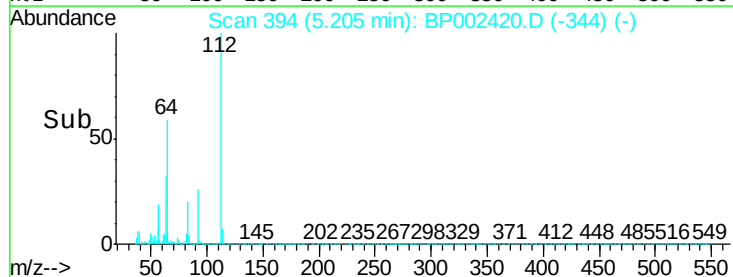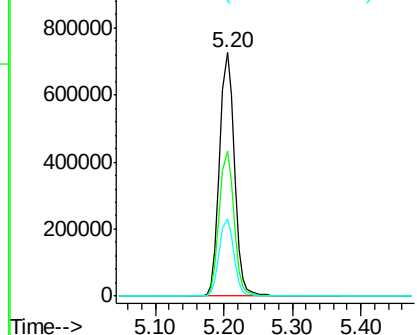

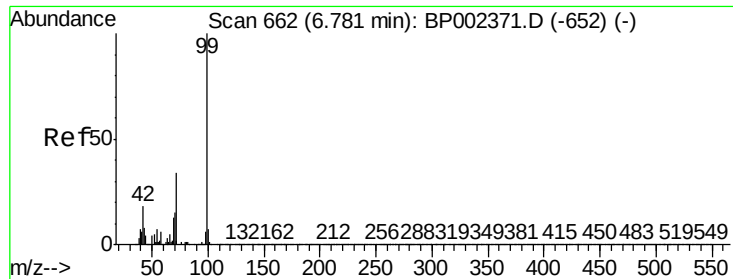

#7

Phenol-d6

Concen: 148.567 ng

RT: 6.78 min Scan# 661

Delta R.T. -0.01 min

Lab File: BP002420.D

Acq: 17 Jun 2020 15:44

Instrument :


BNA_P

ClientSampleId :

PB129590BL

Tot Ion: 99 Resp: 1442580




Ion	Ratio	Lower	Upper
99	100		
42	17.8	14.6	22.0
71	33.5	27.2	40.8

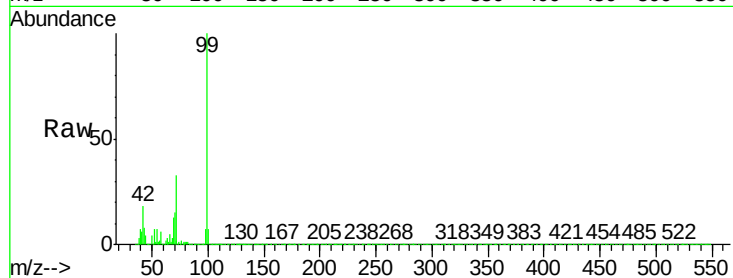

Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

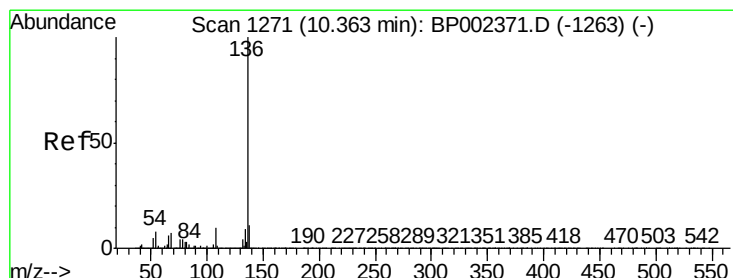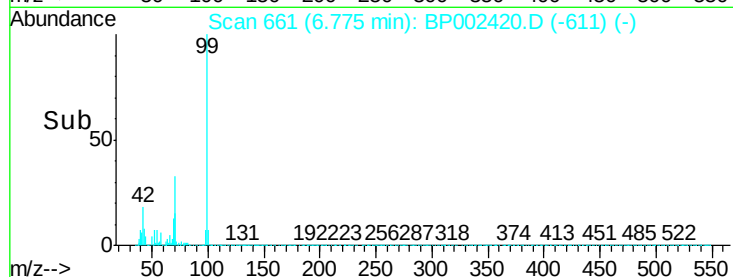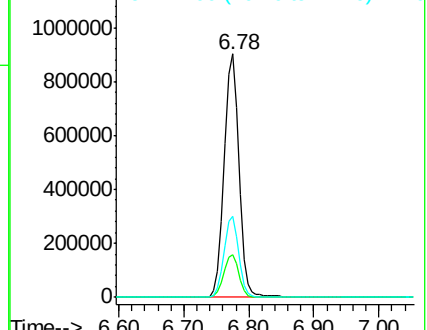

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.36 min Scan# 1270


Delta R.T. -0.01 min

Lab File: BP002420.D

Acq: 17 Jun 2020 15:44

Tgt Ion: 136 Resp: 546505

Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.8	13.2
54	8.4	6.4	9.6
68	6.9	5.6	8.4


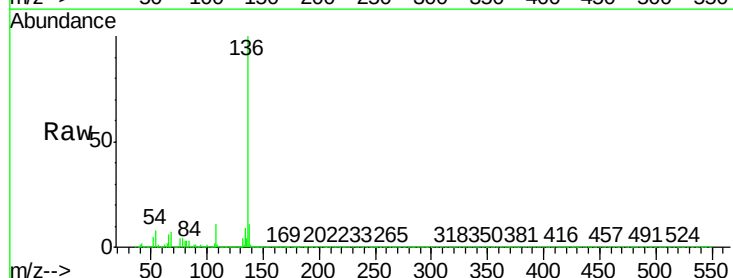



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0



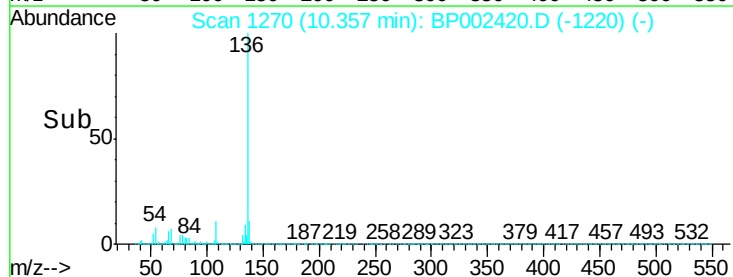
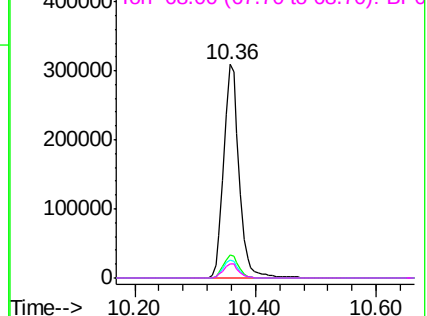


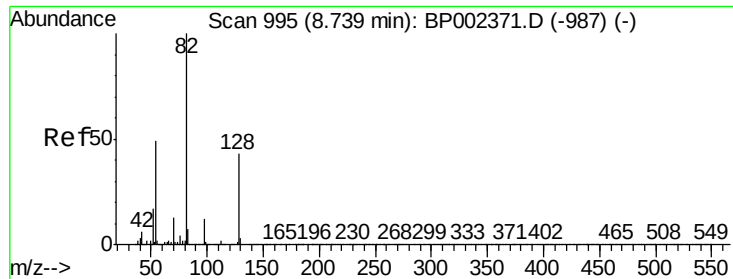

#23
 Nitrobenzene-d5
 Concen: 107.463 ng
 RT: 8.73 min Scan# 993
 Delta R.T. -0.01 min
 Lab File: BP002420.D
 Acq: 17 Jun 2020 15:44




Instrument :
 BNA_P
 ClientSampleId :
 PB129590BL


Tot Ion	82	Resp	983429
Ion Ratio	Lower	Upper	
82	100		
128	39.9	34.5	51.7
54	48.5	39.4	59.2

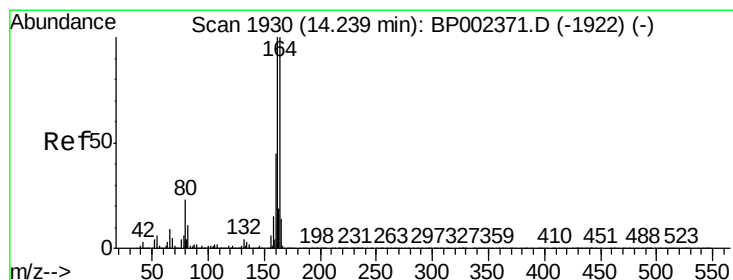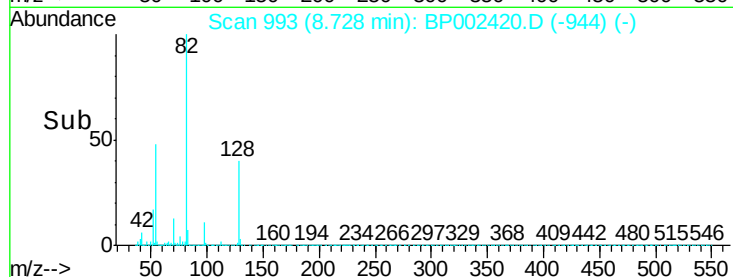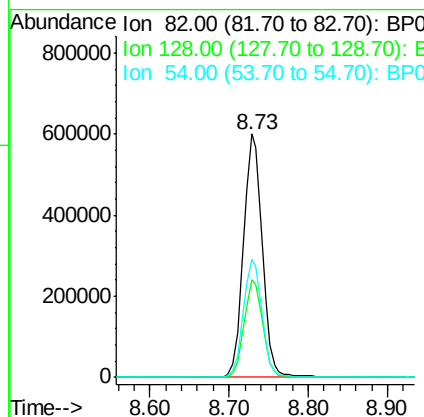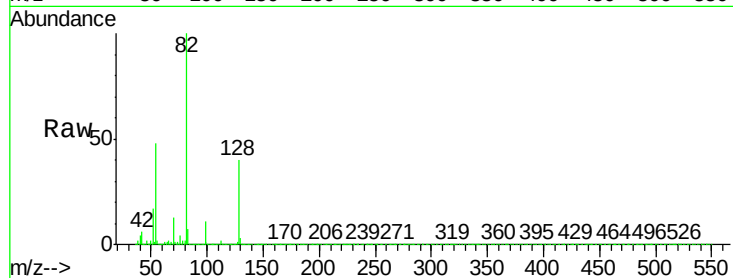

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.23 min Scan# 1929
 Delta R.T. -0.01 min
 Lab File: BP002420.D
 Acq: 17 Jun 2020 15:44

Tgt Ion	164	Resp	341647
Ion Ratio	Lower	Upper	
164	100		
162	101.8	79.8	119.8
160	44.1	36.2	54.2

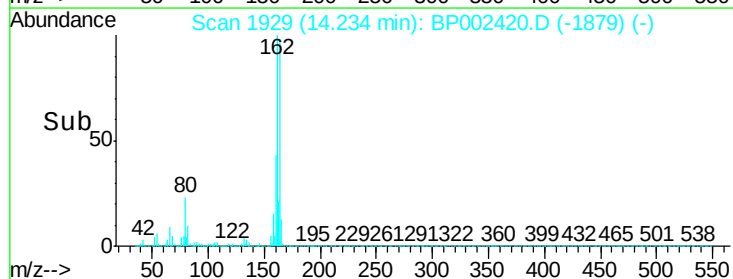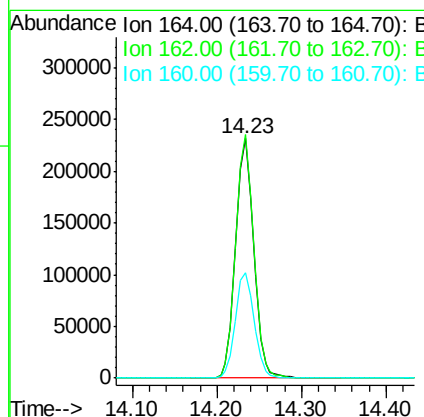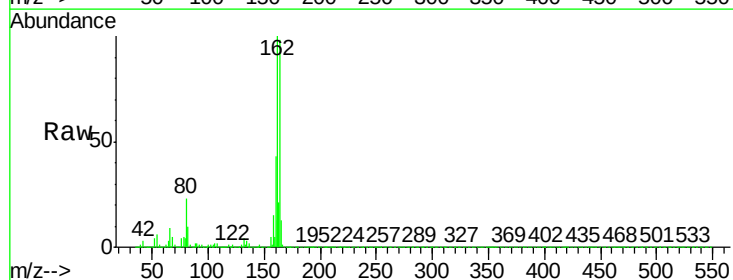


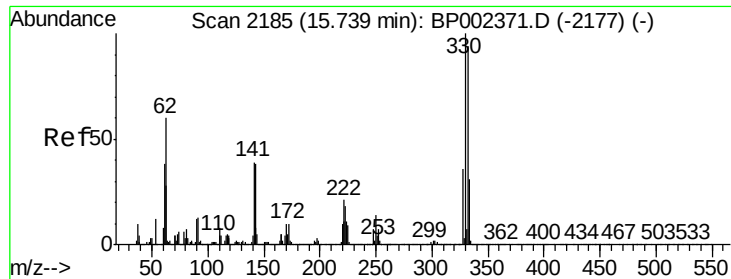




#42
2,4,6-Tribromophenol
Concen: 164.090 ng
RT: 15.73 min Scan# 2184
Delta R.T. -0.01 min
Lab File: BP002420.D
Acq: 17 Jun 2020 15:44

Instrument :
BNA_P
ClientSampleId :
PB129590BL

Tot Ion:330 Resp: 536742
Ion Ratio Lower Upper
330 100
332 95.5 76.6 115.0
141 36.8 30.3 45.5

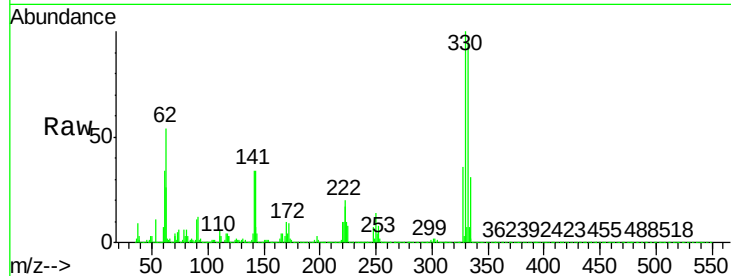


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

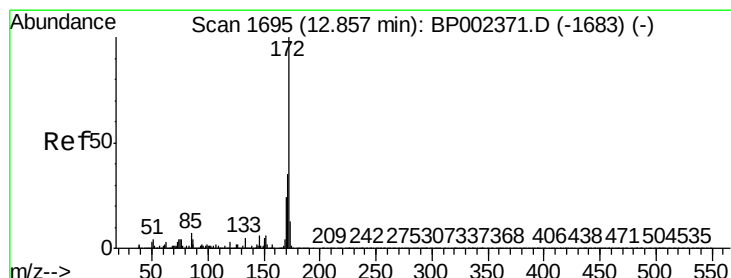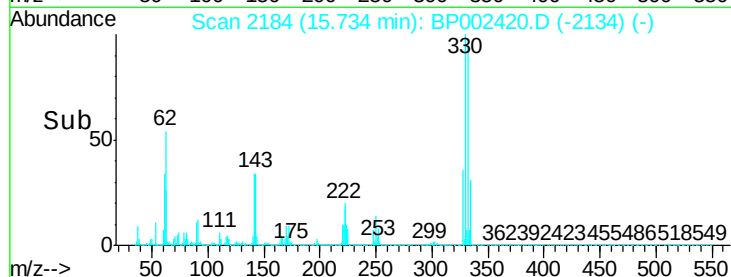
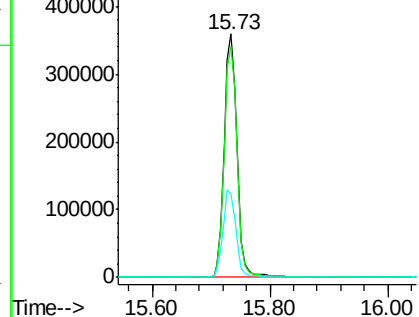



#45
2-Fluorobiphenyl
Concen: 103.496 ng
RT: 12.85 min Scan# 1694
Delta R.T. -0.00 min
Lab File: BP002420.D
Acq: 17 Jun 2020 15:44

Tgt Ion:172 Resp: 2102925
Ion Ratio Lower Upper
172 100
171 35.2 27.8 41.8
170 23.8 19.0 28.6

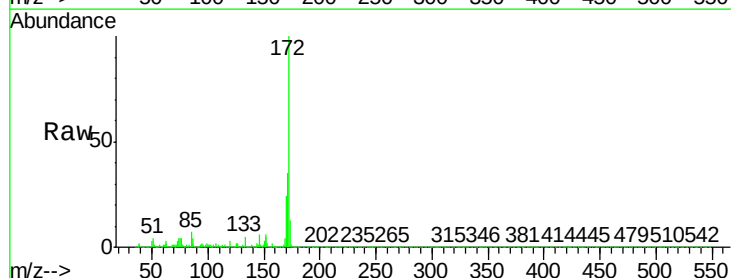

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

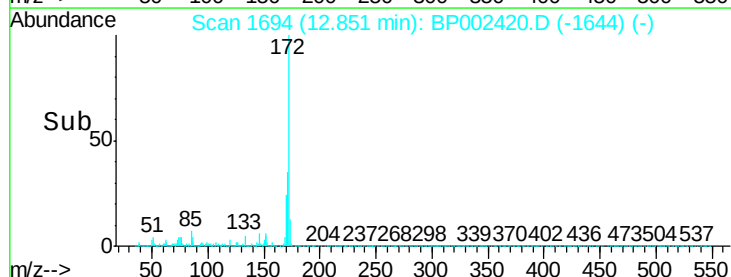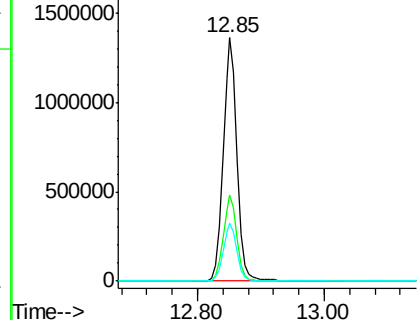


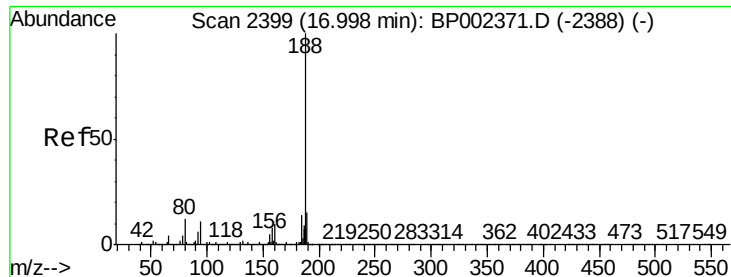




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.99 min Scan# 2398
Delta R.T. -0.01 min
Lab File: BP002420.D
Acq: 17 Jun 2020 15:44

Instrument :
BNA_P
ClientSampleId :
PB129590BL

Tot Ion:188 Resp: 776432
Ion Ratio Lower Upper
188 100
94 10.4 8.5 12.7
80 11.1 9.4 14.0

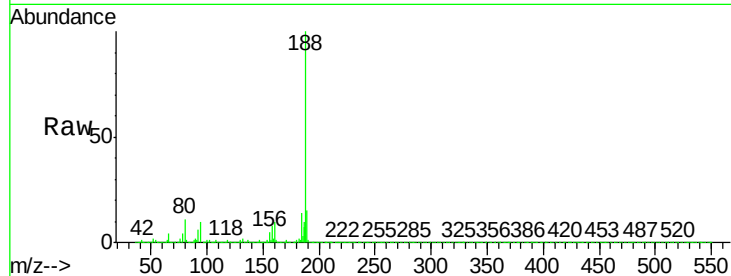


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BP0
Ion 80.00 (79.70 to 80.70): BP0

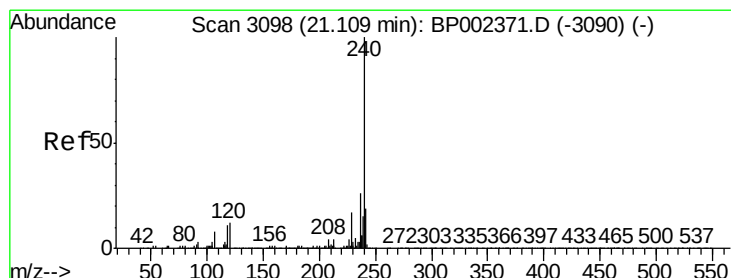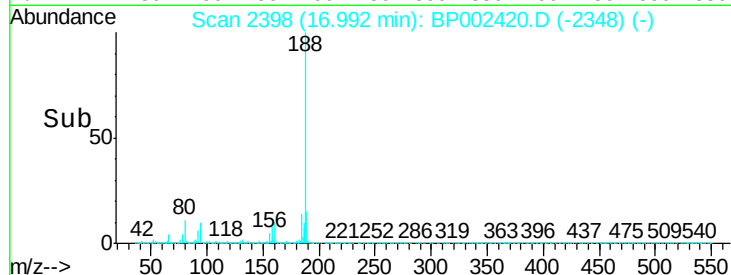
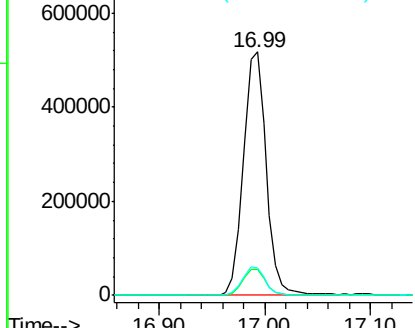



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.09 min Scan# 3095
Delta R.T. -0.02 min
Lab File: BP002420.D
Acq: 17 Jun 2020 15:44

Tgt Ion:240 Resp: 804286
Ion Ratio Lower Upper
240 100
120 12.2 9.3 13.9
236 26.4 21.0 31.6

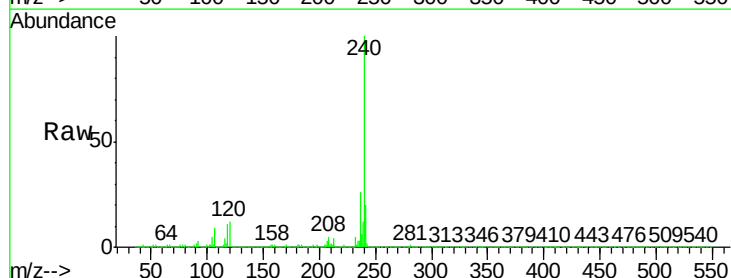

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

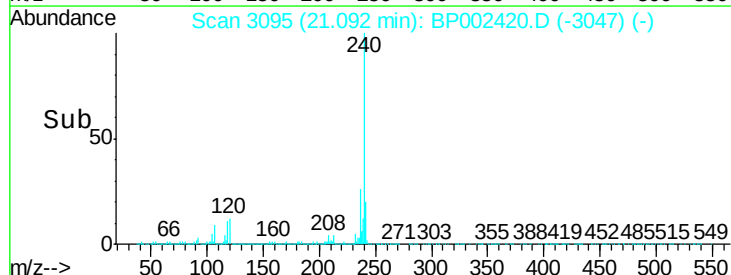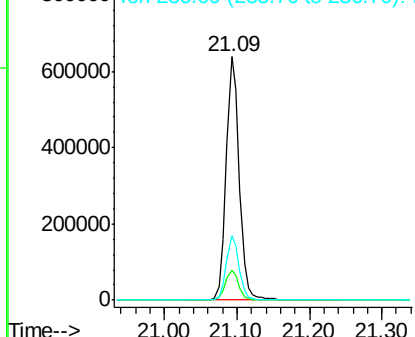

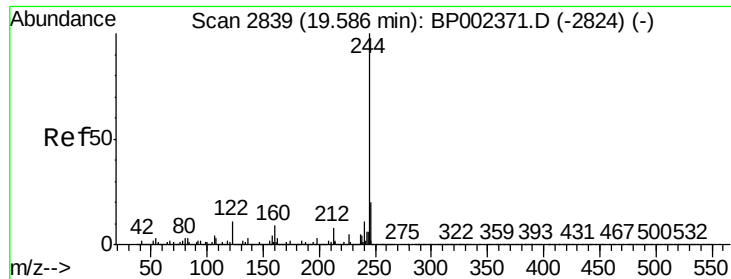

#79

Terphenyl-d14

Concen: 122.462 ng

RT: 19.58 min Scan# 2838

Delta R.T. -0.00 min

Lab File: BP002420.D

Acq: 17 Jun 2020 15:44

Instrument :

BNA_P

ClientSampleId :

PB129590BL


Tot Ion:244 Resp: 3449108

Ion Ratio Lower Upper

244 100

212 8.1 6.6 10.0




122 10.6 8.8 13.2

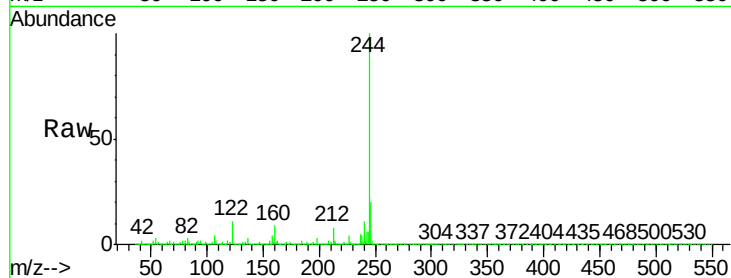

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

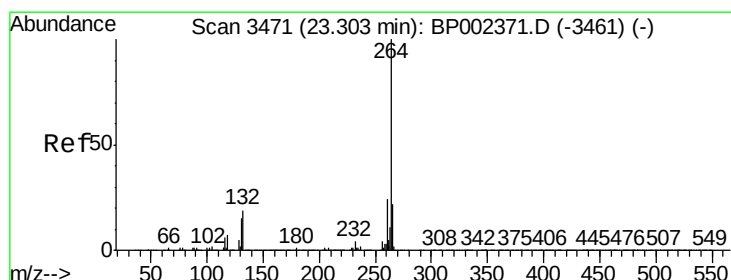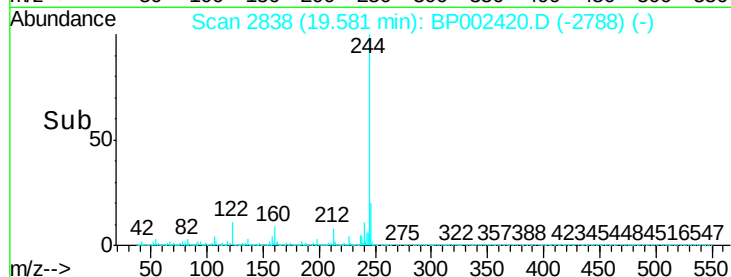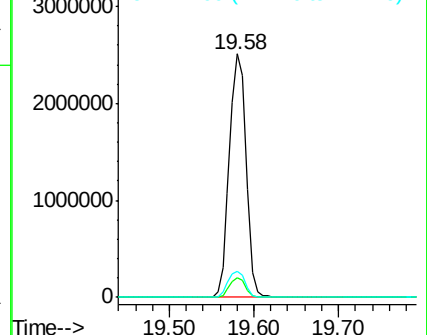

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.29 min Scan# 3469

Delta R.T. -0.01 min

Lab File: BP002420.D

Acq: 17 Jun 2020 15:44


Tgt Ion:264 Resp: 844770

Ion Ratio Lower Upper

264 100

260 24.3 19.4 29.0

265 21.6 17.4 26.2

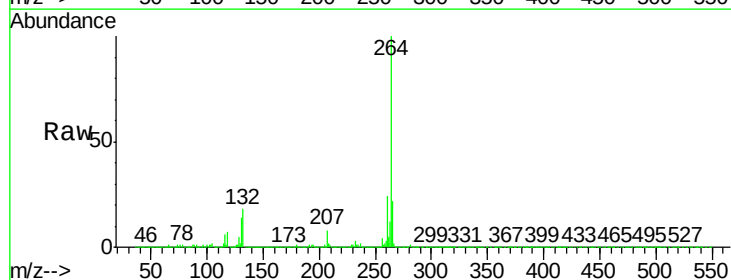

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

