

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061720\
 Data File : BP002424.D
 Acq On : 17 Jun 2020 18:01
 Operator : CG/JU
 Sample : PB129590BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129590BL

Quant Time: Jun 18 00:59:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	146933	20.00	ng	0.00
21) Naphthalene-d8	10.36	136	601661	20.00	ng	0.00
39) Acenaphthene-d10	14.23	164	373200	20.00	ng	0.00
64) Phenanthrene-d10	16.99	188	846585	20.00	ng	0.00
76) Chrysene-d12	21.09	240	866420	20.00	ng	-0.02
86) Perylene-d12	23.29	264	921526	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.20	112	1031605	129.92	ng	0.00
7) Phenol-d6	6.78	99	1367890	129.39	ng	0.00
23) Nitrobenzene-d5	8.73	82	925461	91.86	ng	-0.01
42) 2,4,6-Tribromophenol	15.73	330	495665	138.72	ng	0.00
45) 2-Fluorobiphenyl	12.85	172	1988028	89.57	ng	0.00
79) Terphenyl-d14	19.58	244	3185640	99.12	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061720\
Data File : BP002424.D
Acq On : 17 Jun 2020 18:01
Operator : CG/JU
Sample : PB129590BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129590BL

Quant Time: Jun 18 00:59:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

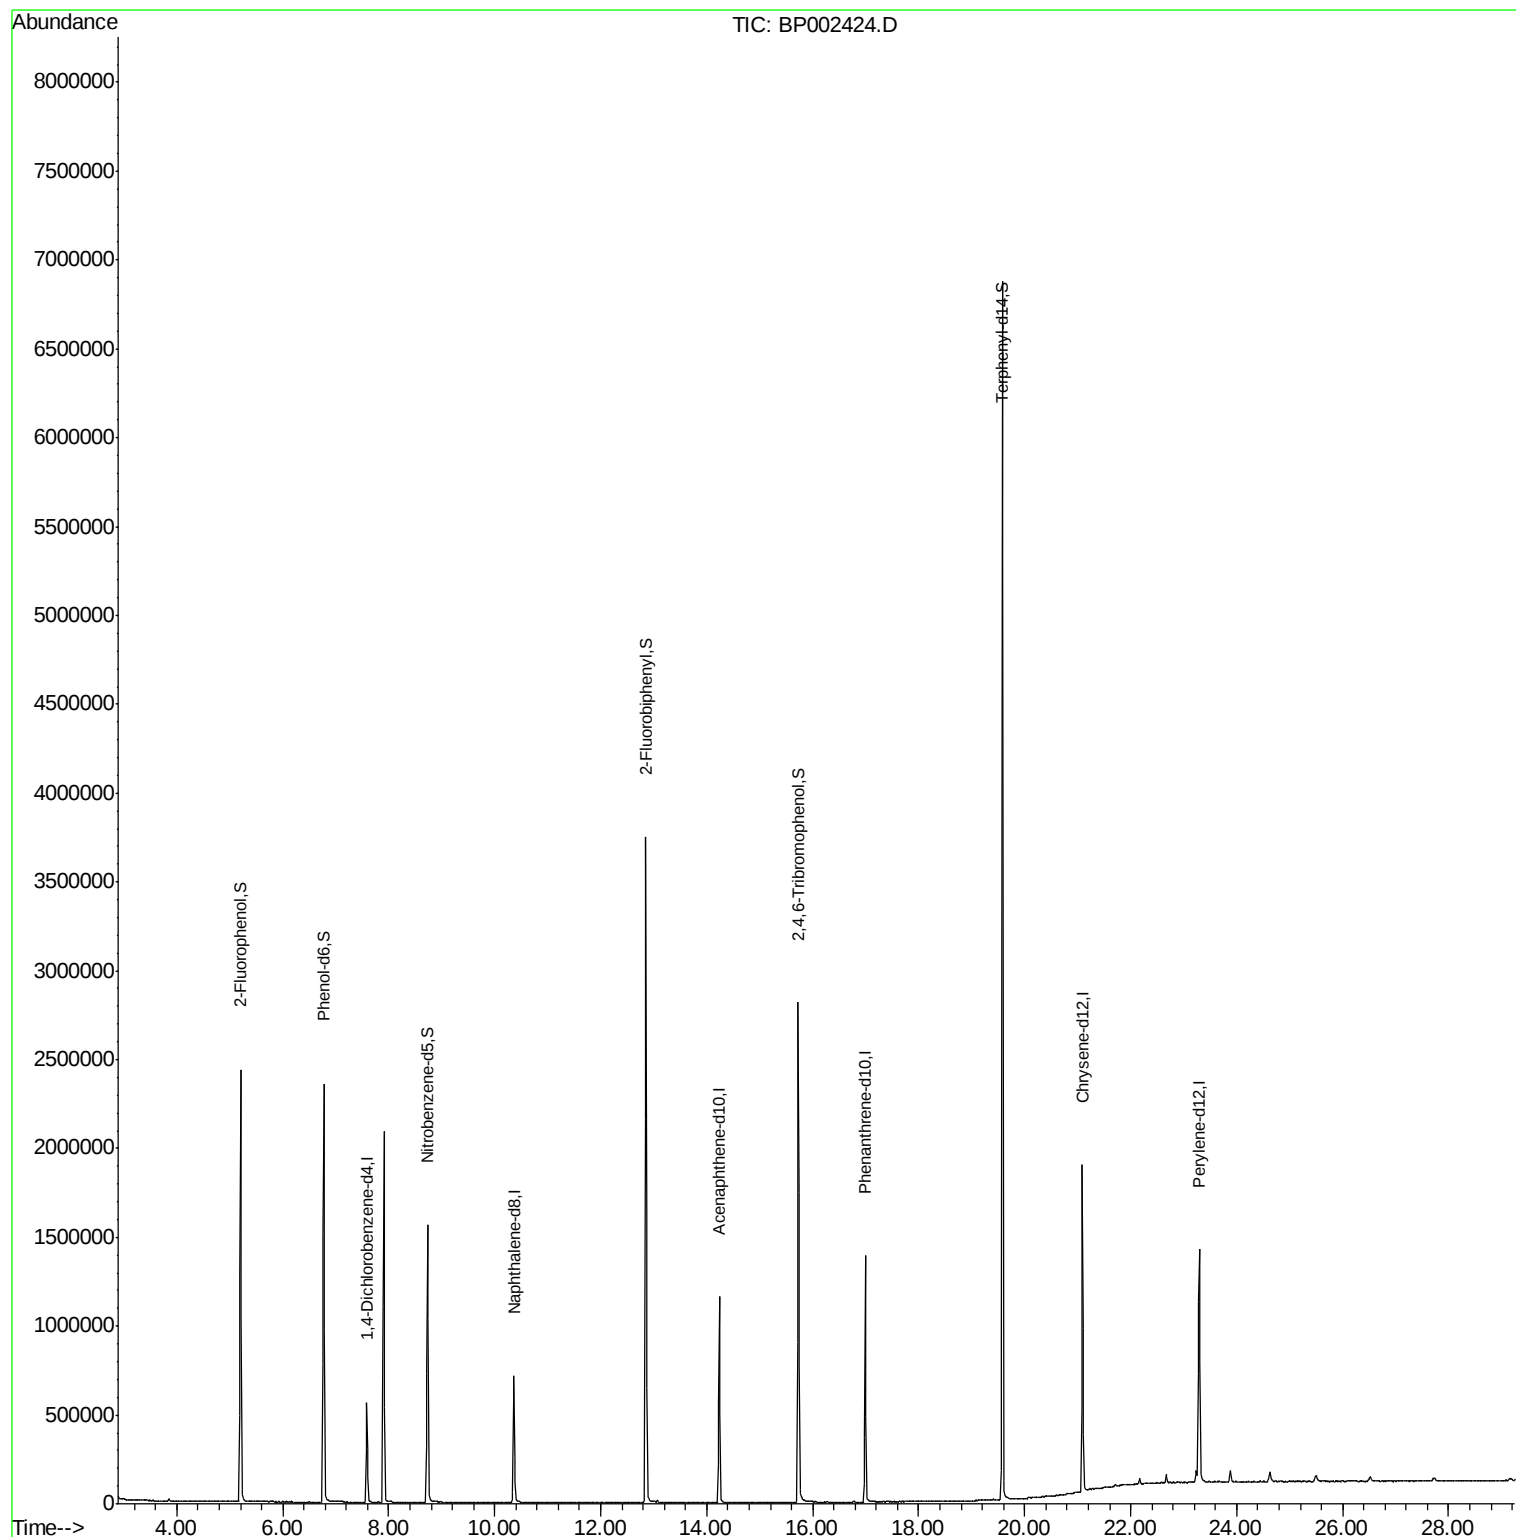

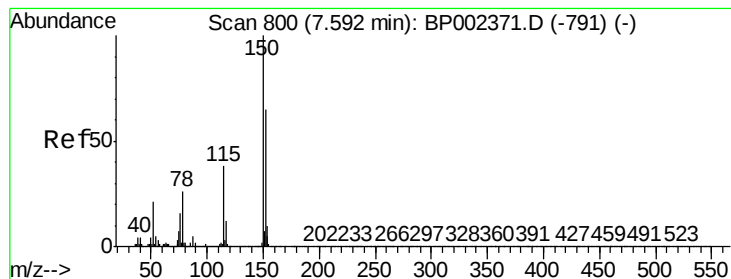

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 7.59 min Scan# 799

Delta R.T. -0.01 min

Lab File: BP002424.D

Acq: 17 Jun 2020 18:01

Instrument :

BNA_P

ClientSampleId :

PB129590BL


Tot Ion:152 Resp: 146933

Ion Ratio Lower Upper

152 100

150 160.4 124.0 186.0




115 60.7 47.4 71.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

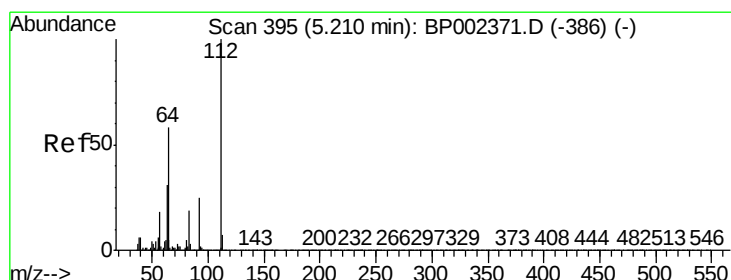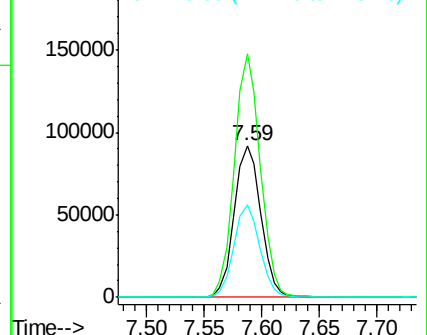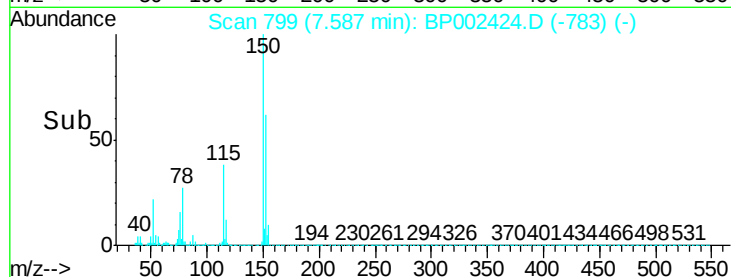

#5

2-Fluorophenol

Concen: 129.916 ng

RT: 5.20 min Scan# 394

Delta R.T. -0.01 min

Lab File: BP002424.D

Acq: 17 Jun 2020 18:01


Tgt Ion:112 Resp: 1031605

Ion Ratio Lower Upper

112 100

64 59.4 46.2 69.2



63 31.0 24.5 36.7




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

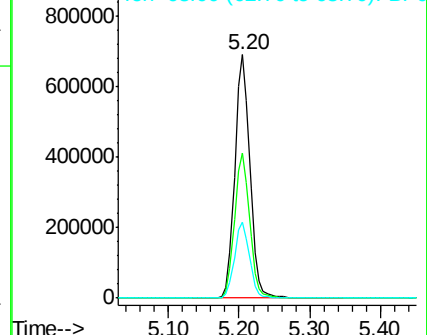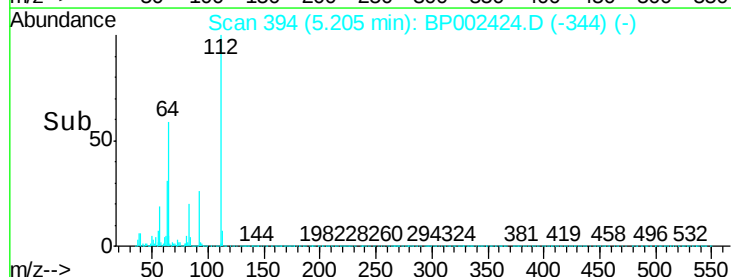

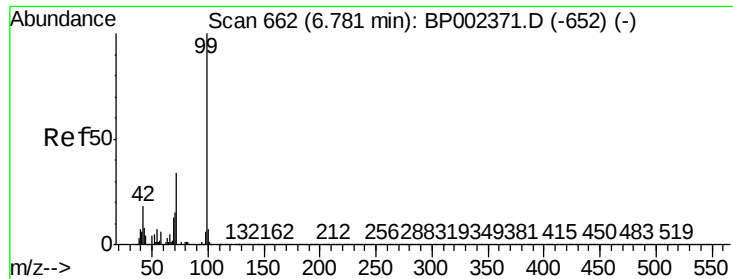

#7

Phenol-d6

Concen: 129.388 ng

RT: 6.78 min Scan# 661

Delta R.T. -0.01 min

Lab File: BP002424.D

Acq: 17 Jun 2020 18:01

Instrument :


BNA_P

ClientSampled :

PB129590BL

Tot Ion: 99 Resp: 1367890




Ion	Ratio	Lower	Upper
99	100		
42	18.1	14.6	22.0
71	33.9	27.2	40.8

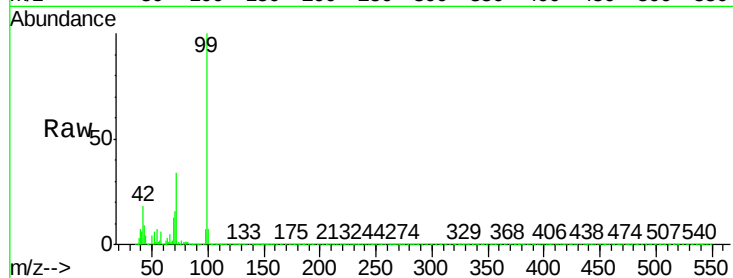

Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

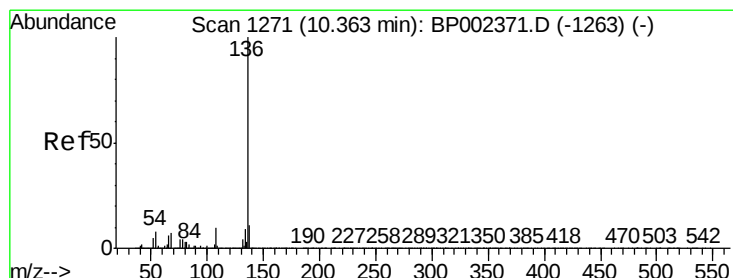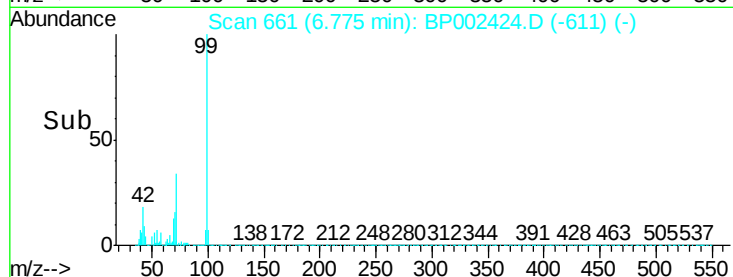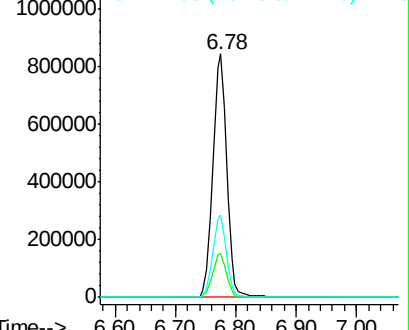

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.36 min Scan# 1270


Delta R.T. -0.01 min

Lab File: BP002424.D

Acq: 17 Jun 2020 18:01

Tgt Ion: 136 Resp: 601661

Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.8	13.2
54	8.4	6.4	9.6
68	7.3	5.6	8.4


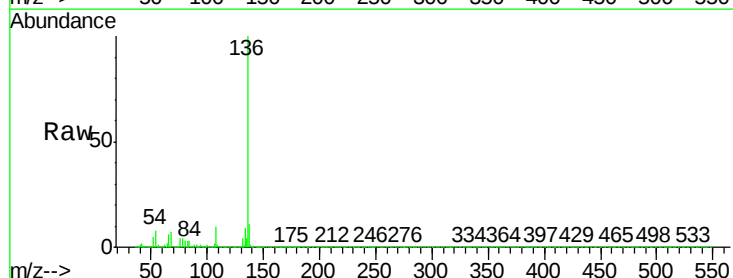



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0



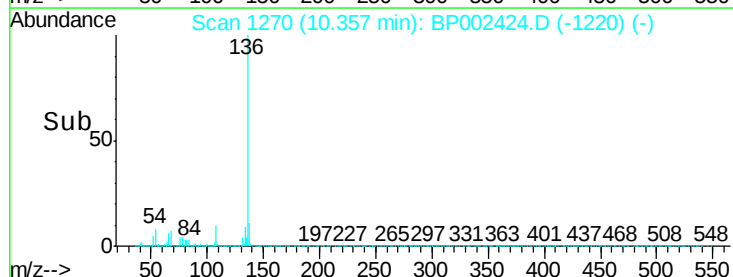
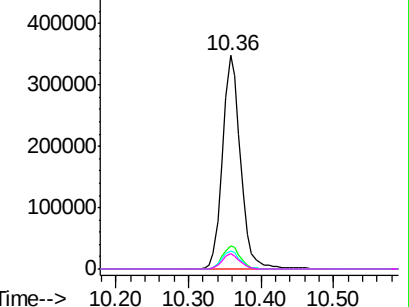


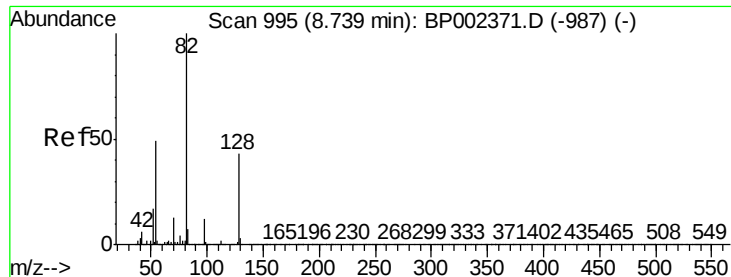

#23
Nitrobenzene-d5
Concen: 91.858 ng
RT: 8.73 min Scan# 993
Delta R.T. -0.01 min
Lab File: BP002424.D
Acq: 17 Jun 2020 18:01




Instrument :
BNA_P
ClientSampleId :
PB129590BL


Tot Ion	82	Resp	925461
Ion Ratio	Lower	Upper	
82	100		
128	40.8	34.5	51.7
54	49.3	39.4	59.2

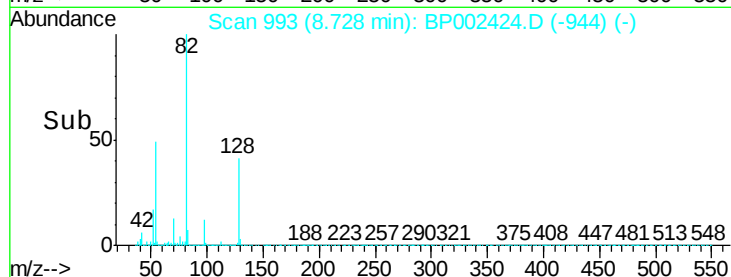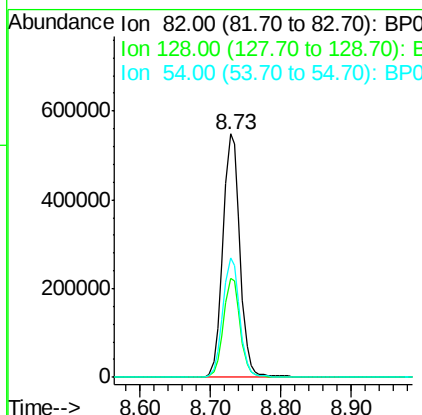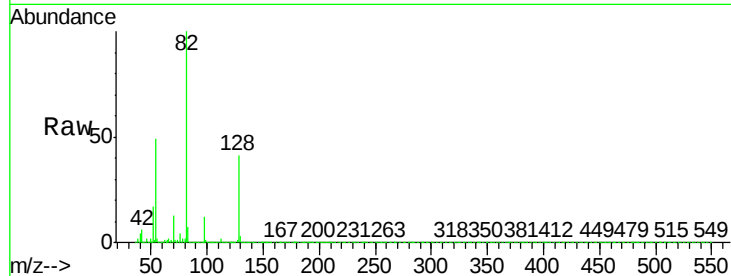

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.23 min Scan# 1929
Delta R.T. -0.01 min
Lab File: BP002424.D
Acq: 17 Jun 2020 18:01

Tgt Ion	164	Resp	373200
Ion Ratio	Lower	Upper	
164	100		
162	100.0	79.8	119.8
160	45.7	36.2	54.2


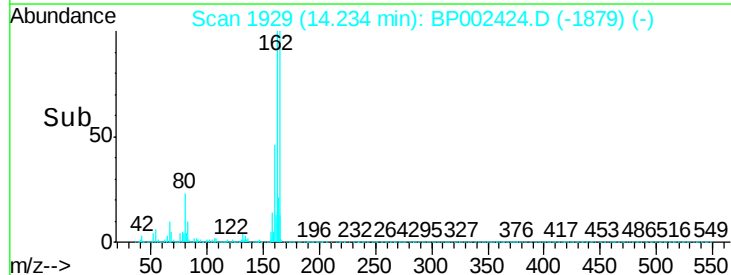
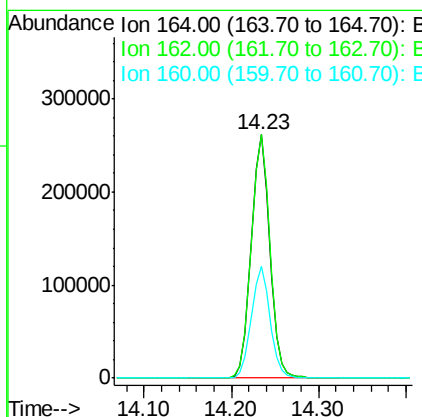



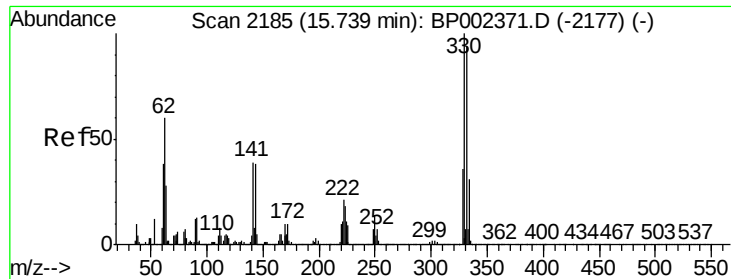

#42
 2,4,6-Tribromophenol
 Concen: 138.720 ng
 RT: 15.73 min Scan# 2184
 Delta R.T. -0.01 min
 Lab File: BP002424.D
 Acq: 17 Jun 2020 18:01




Instrument :
 BNA_P
 ClientSampleId :
 PB129590BL


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.4	76.6	115.0
141	37.4	30.3	45.5

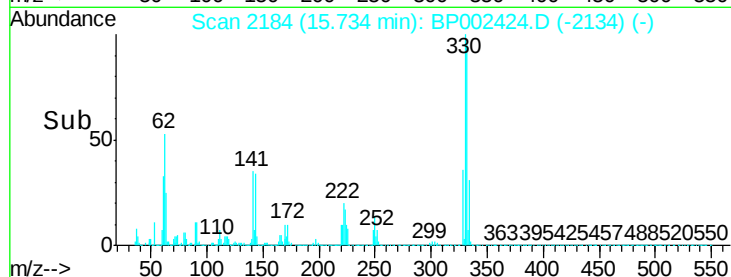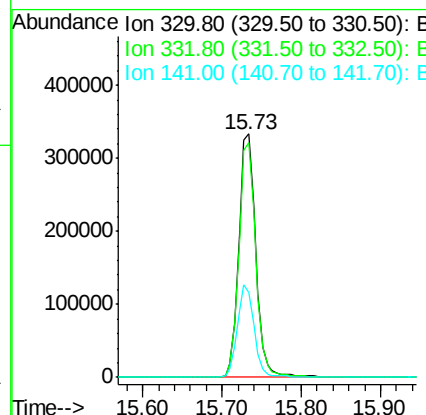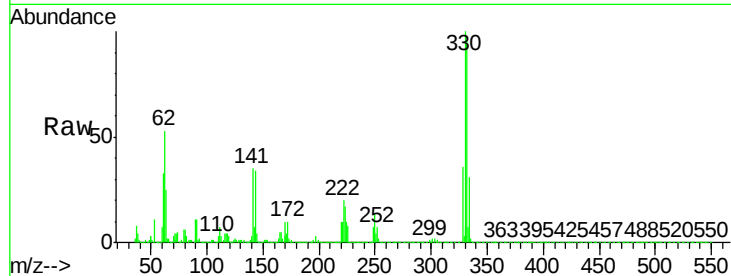

#45
 2-Fluorobiphenyl
 Concen: 89.569 ng
 RT: 12.85 min Scan# 1694
 Delta R.T. -0.00 min
 Lab File: BP002424.D
 Acq: 17 Jun 2020 18:01

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.1	27.8	41.8
170	23.5	19.0	28.6


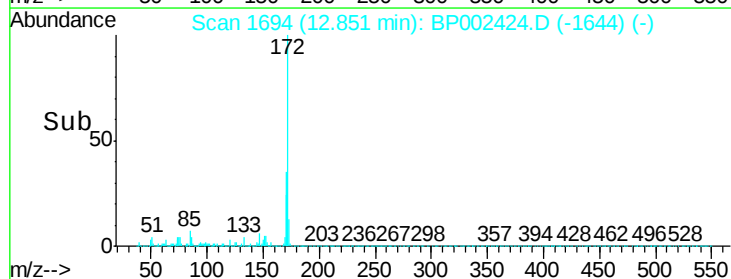
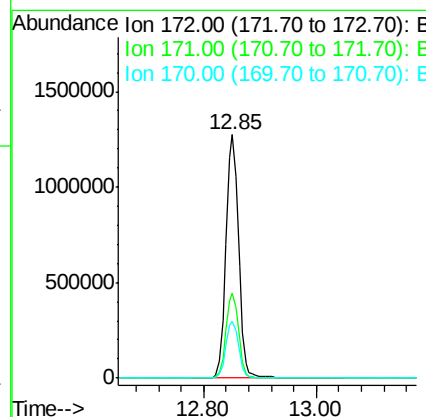



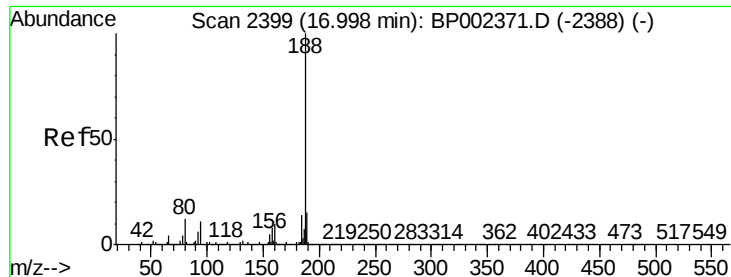

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.99 min Scan# 2398
Delta R.T. -0.01 min
Lab File: BP002424.D
Acq: 17 Jun 2020 18:01




Instrument :
BNA_P
ClientSampleId :
PB129590BL


Tot Ion:188 Resp: 846585
Ion Ratio Lower Upper
188 100
94 10.5 8.5 12.7
80 11.2 9.4 14.0

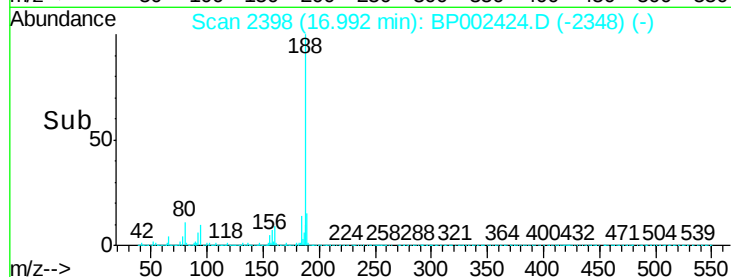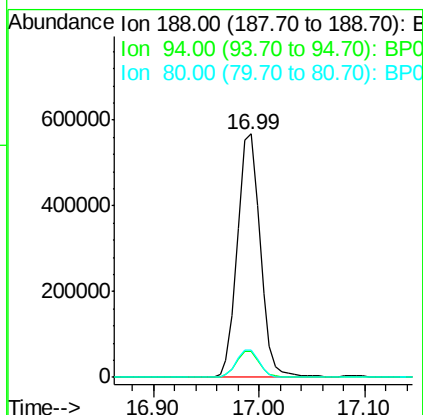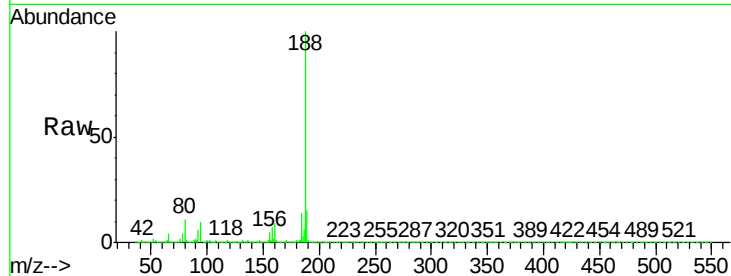

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.09 min Scan# 3095
Delta R.T. -0.02 min
Lab File: BP002424.D
Acq: 17 Jun 2020 18:01

Tgt Ion:240 Resp: 866420
Ion Ratio Lower Upper
240 100
120 12.8 9.3 13.9
236 25.7 21.0 31.6

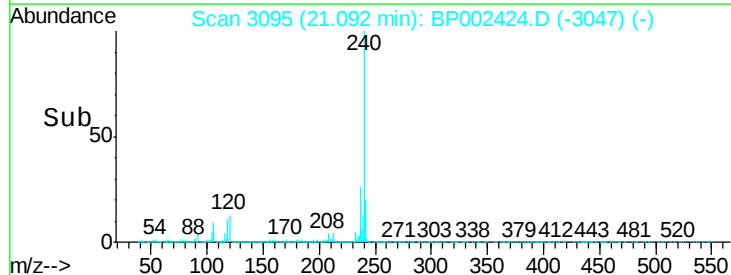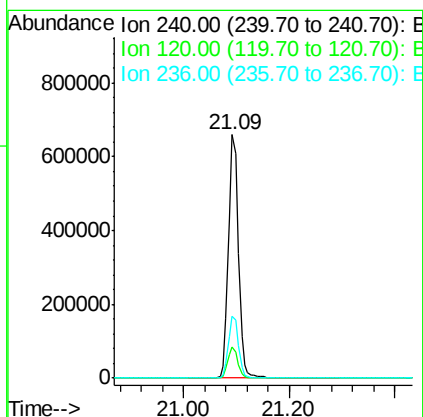

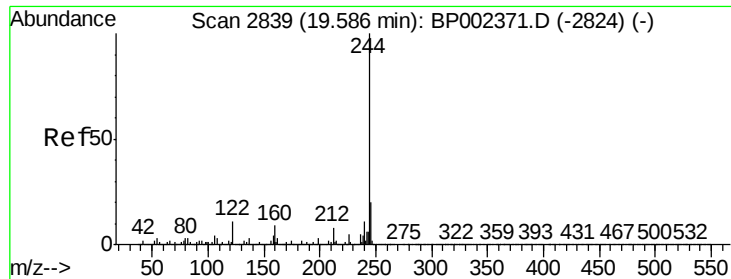

#79

Terphenyl-d14

Concen: 99.117 ng

RT: 19.58 min Scan# 2838

Delta R.T. -0.00 min

Lab File: BP002424.D

Acq: 17 Jun 2020 18:01

Instrument :

BNA_P

ClientSampleId :

PB129590BL


Tot Ion:244 Resp: 3185640

Ion Ratio Lower Upper

244 100

212 7.9 6.6 10.0




122 10.5 8.8 13.2

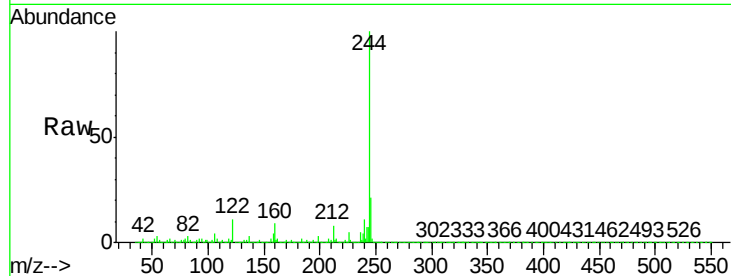

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

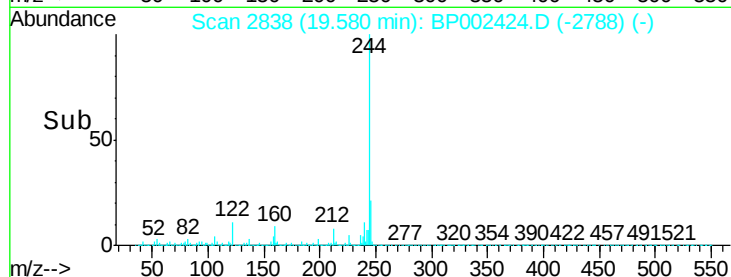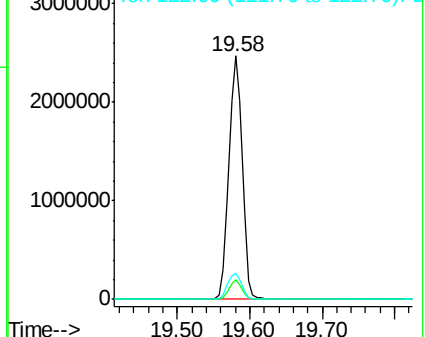

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.29 min Scan# 3469

Delta R.T. -0.01 min

Lab File: BP002424.D

Acq: 17 Jun 2020 18:01


Tgt Ion:264 Resp: 921526

Ion Ratio Lower Upper

264 100

260 24.2 19.4 29.0

265 21.4 17.4 26.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

