

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP061720\  
 Data File : BP002420.D  
 Acq On : 17 Jun 2020 15:44  
 Operator : CG/JU  
 Sample : PB129590BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 PB129590BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP060520.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.205       | 387           | 394         | 415          | rBV      | 2565190        | 3814195       | 40.42%          | 8.622%        |
| 2         | 6.775       | 653           | 661         | 682          | rBV      | 2495263        | 4011912       | 42.52%          | 9.069%        |
| 3         | 7.587       | 792           | 799         | 811          | rBV      | 524301         | 815214        | 8.64%           | 1.843%        |
| 4         | 7.905       | 844           | 853         | 875          | rBV      | 2174445        | 3524311       | 37.35%          | 7.967%        |
| 5         | 8.728       | 985           | 993         | 1012         | rBV      | 1689836        | 2802563       | 29.70%          | 6.335%        |
| 6         | 10.357      | 1262          | 1270        | 1290         | rBV      | 637098         | 1134290       | 12.02%          | 2.564%        |
| 7         | 12.851      | 1686          | 1694        | 1717         | rBV      | 4039748        | 6169363       | 65.39%          | 13.946%       |
| 8         | 14.234      | 1922          | 1929        | 1944         | rBV      | 1022053        | 1540728       | 16.33%          | 3.483%        |
| 9         | 15.734      | 2176          | 2184        | 2208         | rBV      | 2929481        | 4564197       | 48.37%          | 10.317%       |
| 10        | 16.992      | 2391          | 2398        | 2412         | rBV      | 1271942        | 1915345       | 20.30%          | 4.330%        |
| 11        | 19.581      | 2832          | 2838        | 2861         | rBV      | 6982505        | 9435433       | 100.00%         | 21.328%       |
| 12        | 21.092      | 3090          | 3095        | 3109         | rBV      | 1779070        | 2247457       | 23.82%          | 5.080%        |
| 13        | 23.286      | 3462          | 3468        | 3482         | rVB      | 1193886        | 2263781       | 23.99%          | 5.117%        |




Sum of corrected areas: 44238789

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061720\  
Data File : BP002420.D  
Acq On : 17 Jun 2020 15:44  
Operator : CG/JU  
Sample : PB129590BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB129590BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

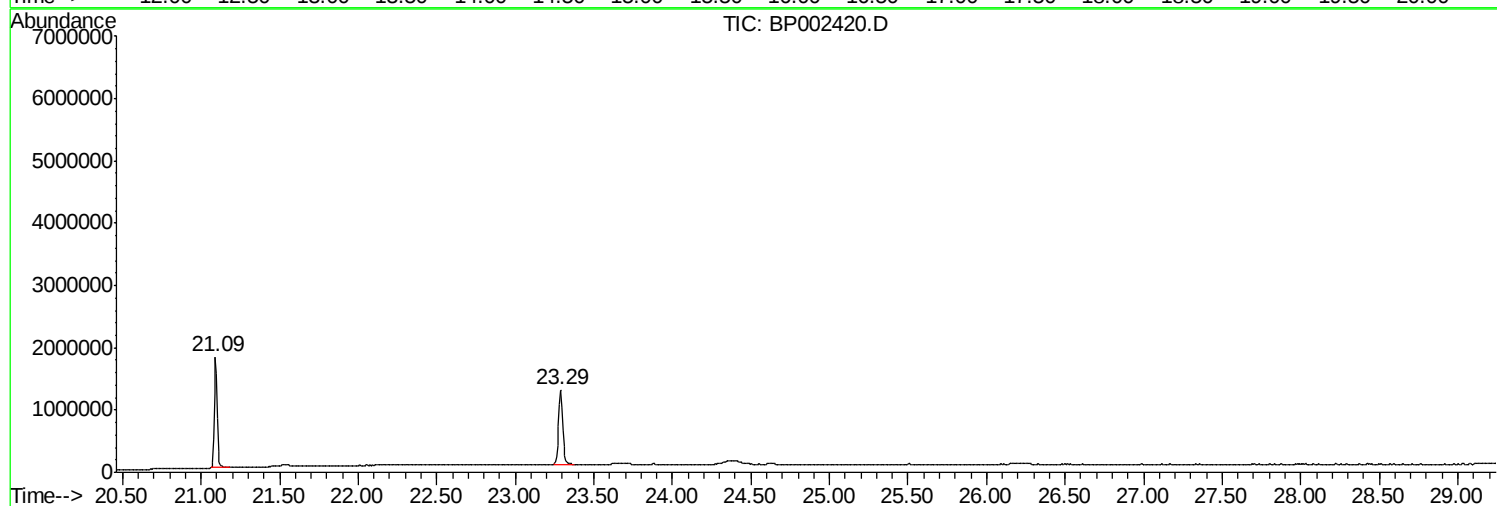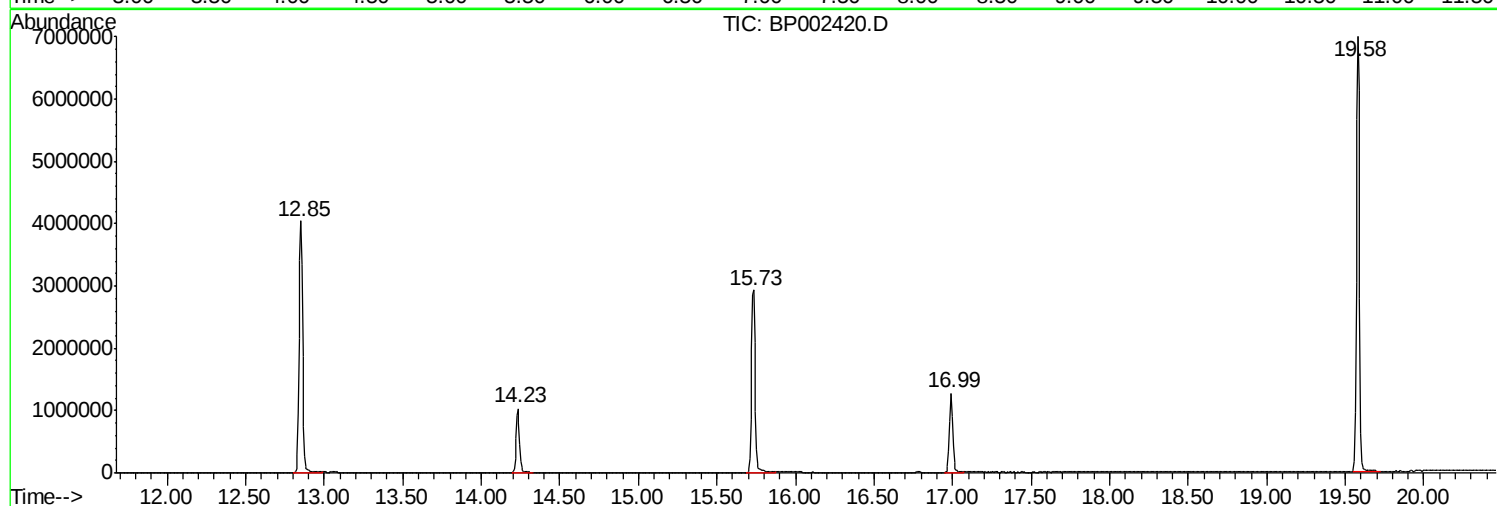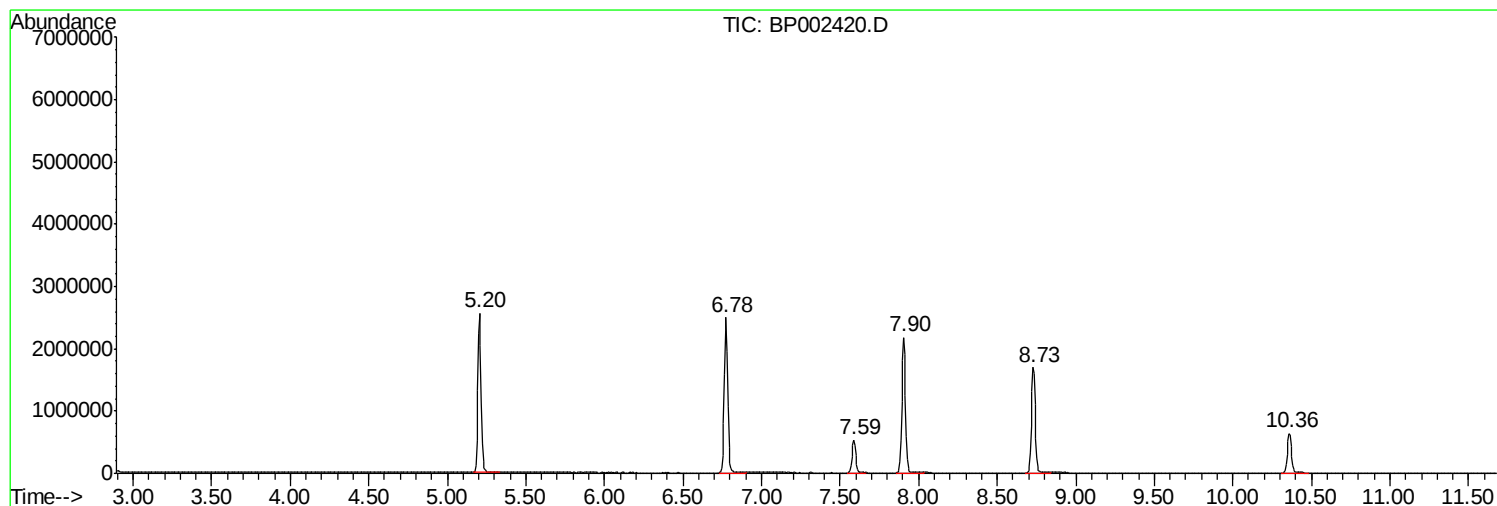

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP061720\  
Data File : BP002420.D  
Acq On : 17 Jun 2020 15:44  
Operator : CG/JU  
Sample : PB129590BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB129590BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP060520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP061720\  
Data File : BP002420.D  
Acq On : 17 Jun 2020 15:44  
Operator : CG/JU  
Sample : PB129590BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB129590BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP060520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |