

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061720\
 Data File : BP002425.D
 Acq On : 17 Jun 2020 18:35
 Operator : CG/JU
 Sample : L3020-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FD-02_061620

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.205	387	394	411	rBV	1872360	2776666	40.72%	7.653%
2	6.769	653	660	680	rBV	1818278	2987850	43.82%	8.235%
3	7.587	791	799	809	rBV	555430	865086	12.69%	2.384%
4	7.905	845	853	864	rBV	1624372	2587177	37.95%	7.131%
5	8.728	985	993	1010	rBV	1240265	2037099	29.88%	5.615%
6	10.357	1262	1270	1287	rBV	684890	1204427	17.66%	3.320%
7	12.851	1686	1694	1714	rBV	3053914	4760796	69.82%	13.122%
8	13.698	1832	1838	1850	rBV	161866	263144	3.86%	0.725%
9	14.234	1922	1929	1952	rBV	1084924	1614868	23.68%	4.451%
10	15.728	2173	2183	2213	rBV	2189349	3356341	49.23%	9.251%
11	16.992	2389	2398	2411	rBV	1309646	1964745	28.82%	5.415%
12	17.922	2551	2556	2562	rBV	55470	81730	1.20%	0.225%
13	19.398	2803	2807	2821	rBV	39756	86465	1.27%	0.238%
14	19.581	2832	2838	2850	rBV	5512675	6818195	100.00%	18.793%
15	20.851	3049	3054	3059	rBV	79940	146896	2.15%	0.405%
16	21.092	3090	3095	3106	rBV	1762794	2247375	32.96%	6.194%
17	22.169	3275	3278	3284	rVB2	60380	80526	1.18%	0.222%
18	22.674	3360	3364	3368	rVB2	54184	76744	1.13%	0.212%
19	23.286	3462	3468	3484	rVB	1204728	2324362	34.09%	6.407%




Sum of corrected areas: 36280492

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061720\
Data File : BP002425.D
Acq On : 17 Jun 2020 18:35
Operator : CG/JU
Sample : L3020-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FD-02_061620

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

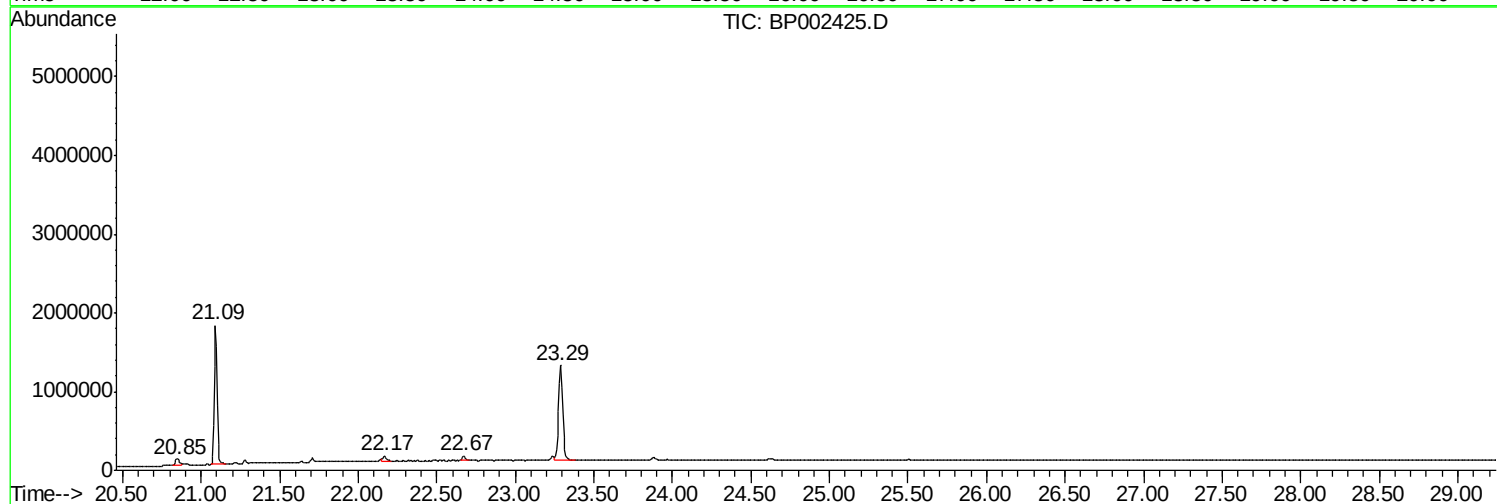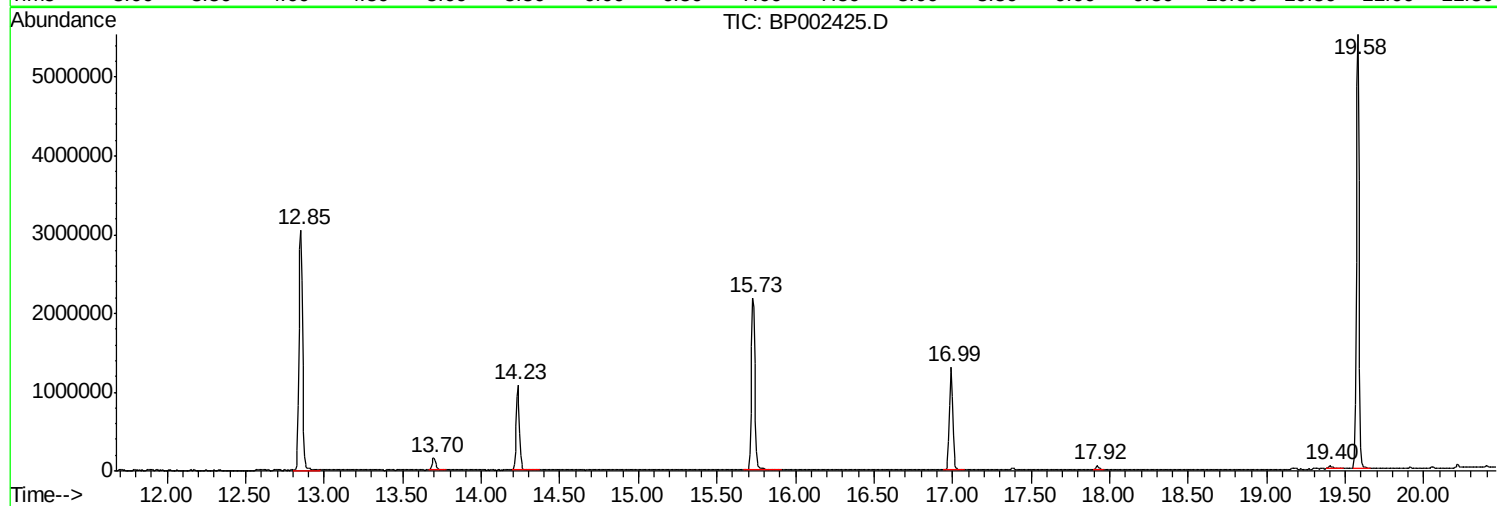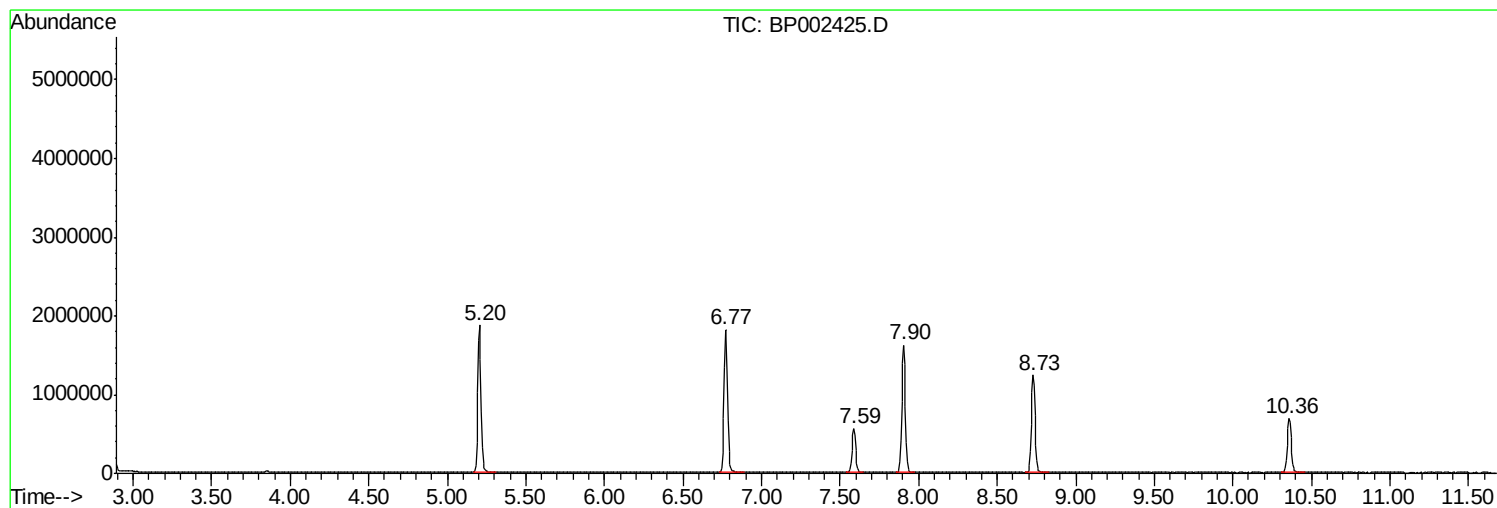

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061720\
Data File : BP002425.D
Acq On : 17 Jun 2020 18:35
Operator : CG/JU
Sample : L3020-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FD-02_061620

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061720\
Data File : BP002425.D
Acq On : 17 Jun 2020 18:35
Operator : CG/JU
Sample : L3020-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FD-02_061620

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc