


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061720\
 Data File : BP002418.D
 Acq On : 17 Jun 2020 14:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:08:53 2020

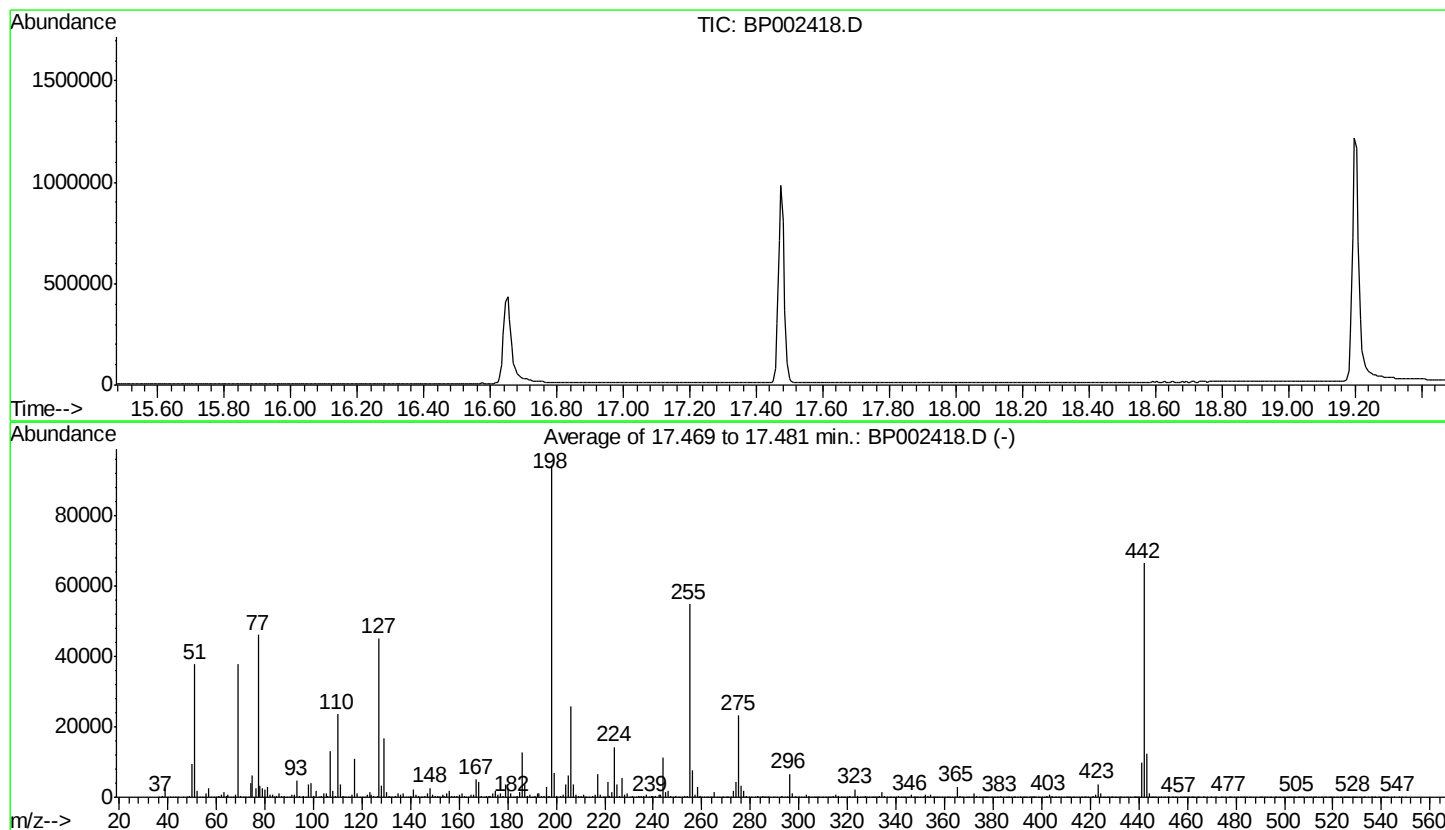

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	37742	PASS
68	69	0.00	2	1.7	640	PASS
69	198	0.00	100	40.0	37590	PASS
70	69	0.00	2	0.6	228	PASS
127	198	10	80	47.8	44971	PASS
197	198	0.00	2	0.5	441	PASS
198	198	100	100	100.0	94034	PASS
199	198	5	9	7.5	7042	PASS
275	198	10	60	24.7	23221	PASS
365	198	1	100	3.1	2960	PASS
441	198	0.01	100	10.3	9662	PASS
442	198	50	100	70.5	66321	PASS
443	442	15	24	18.6	12350	PASS