
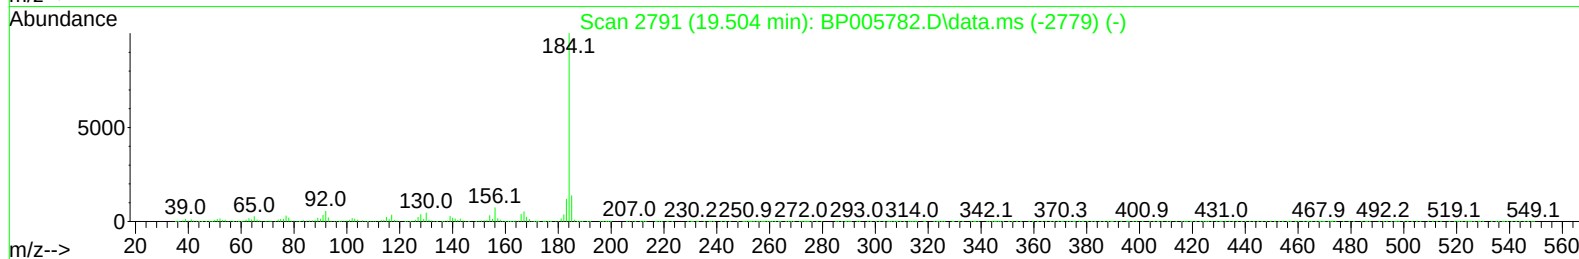
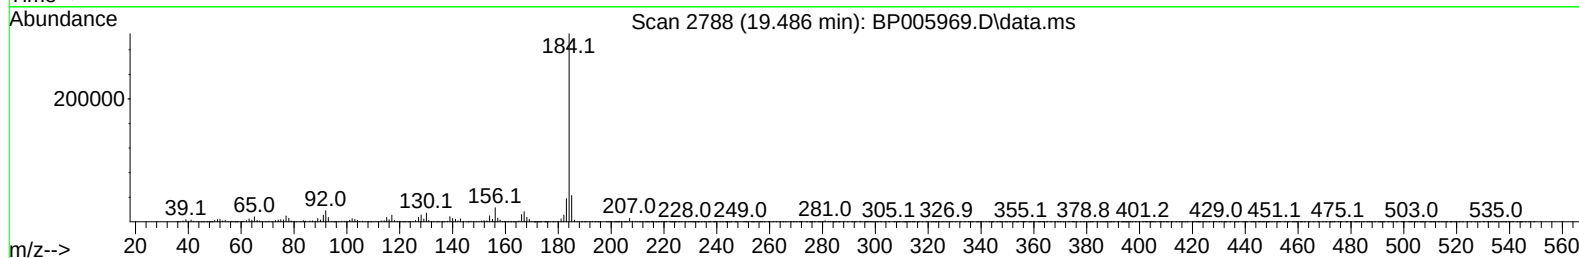


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061821\
 Data File : BP005969.D
 Acq On : 18 Jun 2021 13:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 14:34:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 11:35:30 2021
 Response via : Initial Calibration

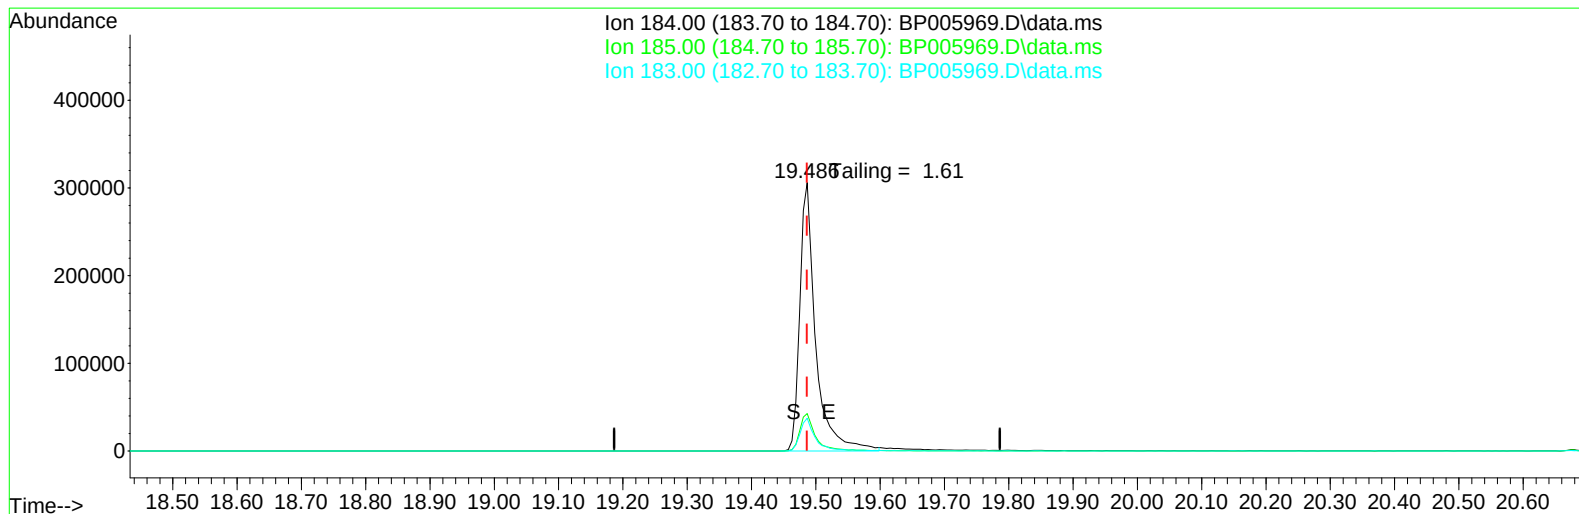




TIC: BP005969.D\data.ms

(77) Benzidine**19.486min (+ 0.000) 22106.88 ng****response 535440**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.97
183.00	11.90	12.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061821\
Data File : BP005969.D
Acq On : 18 Jun 2021 13:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 14:34:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 11:35:30 2021
Response via : Initial Calibration

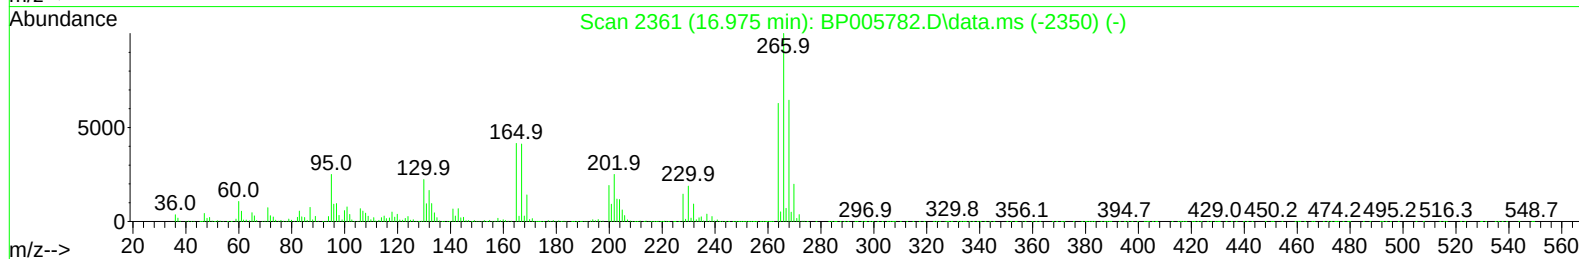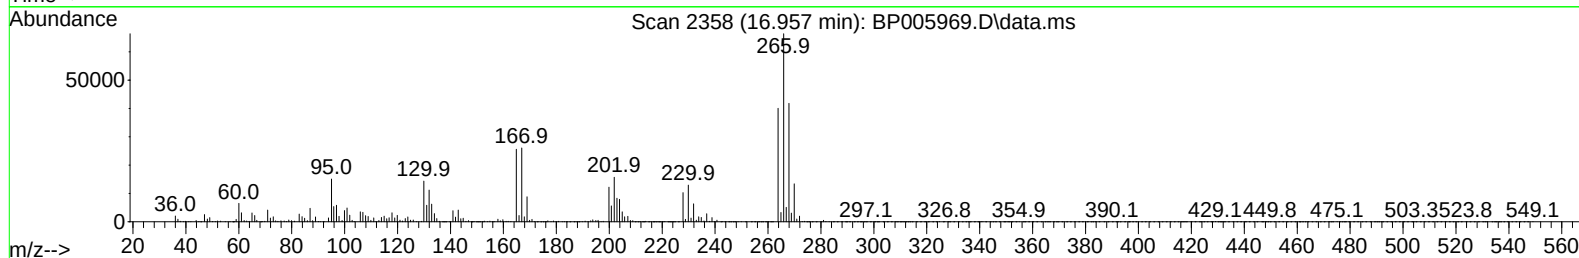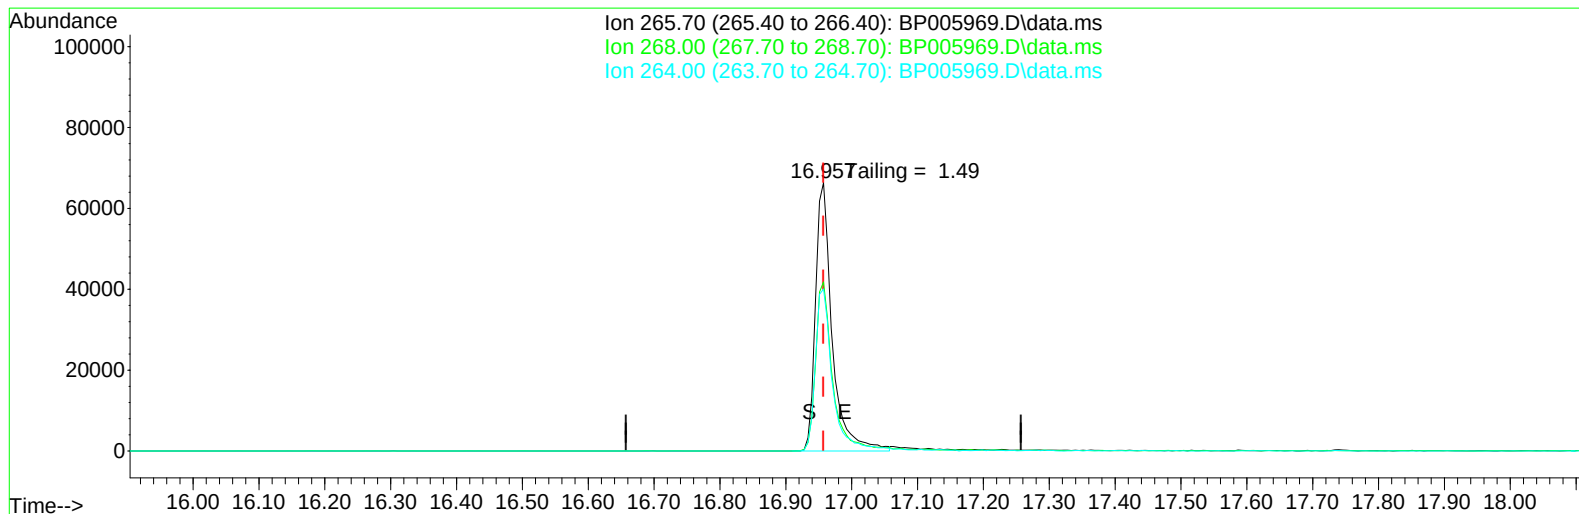

TIC: BP005969.D\data.ms

(70) Pentachlorophenol (C)

16.957min (+ 0.000) 867952.47 ng

response 118797

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.02
264.00	62.90	60.38
0.00	0.00	0.00