
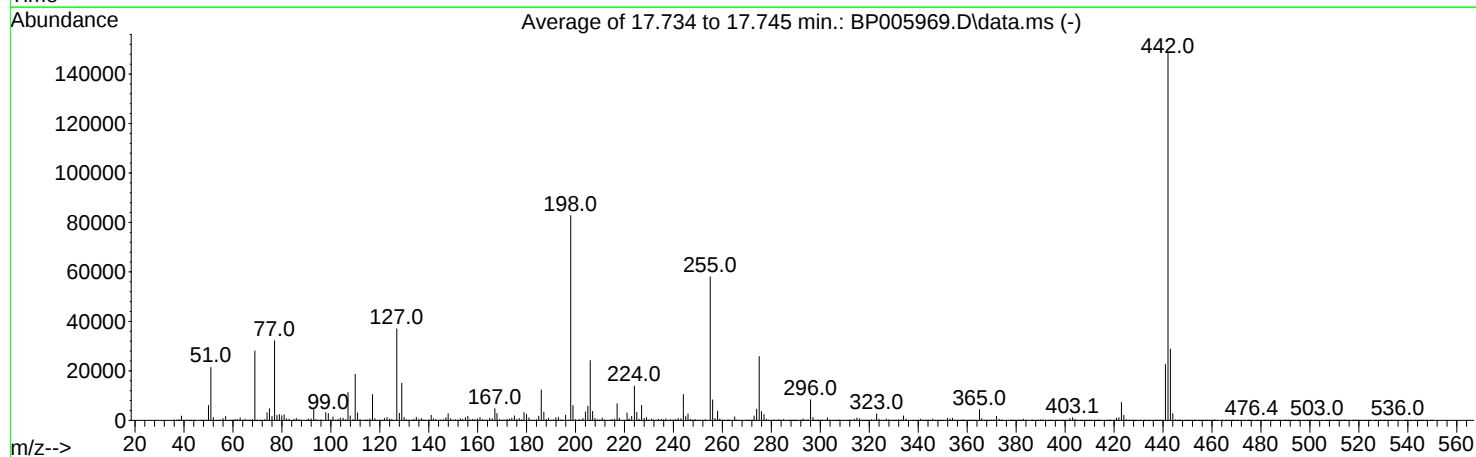


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061821\
 Data File : BP005969.D
 Acq On : 18 Jun 2021 13:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 16 11:35:30 2021

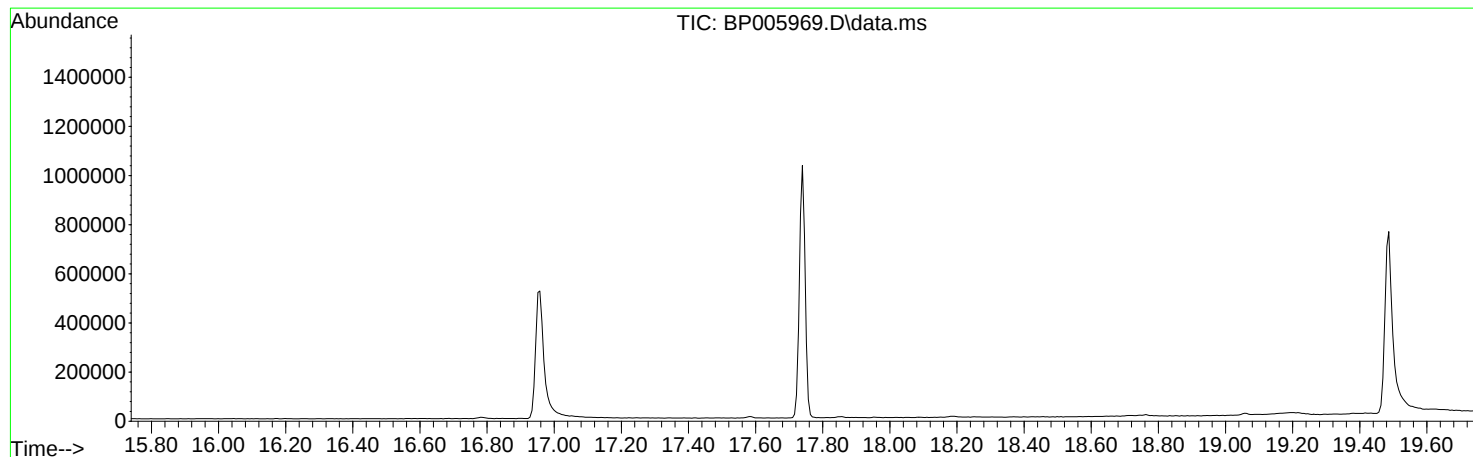

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.9	21442	PASS
68	69	0.00	2	1.2	350	PASS
69	198	0.00	100	33.9	28082	PASS
70	69	0.00	2	0.5	145	PASS
127	198	10	80	44.7	36997	PASS
197	198	0.00	2	0.2	194	PASS
198	198	100	100	100.0	82784	PASS
199	198	5	9	7.2	5996	PASS
275	198	10	60	31.2	25808	PASS
365	198	1	100	5.3	4347	PASS
441	198	0.01	100	27.3	22615	PASS
442	442	100	100	100.0	148715	PASS
443	442	15	24	19.3	28765	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/18/2021	BNA_P	<u>BP005969.D</u>
Compound Name	Response	Retention Time
DDT	323399	20.67
DDD	7499	20.25
DDE	1705	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9204	332603	2.77

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061821\
 Data File : BP005969.D
 Acq On : 18 Jun 2021 13:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 18 14:34:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 11:35:30 2021
 Response via : Initial Calibration

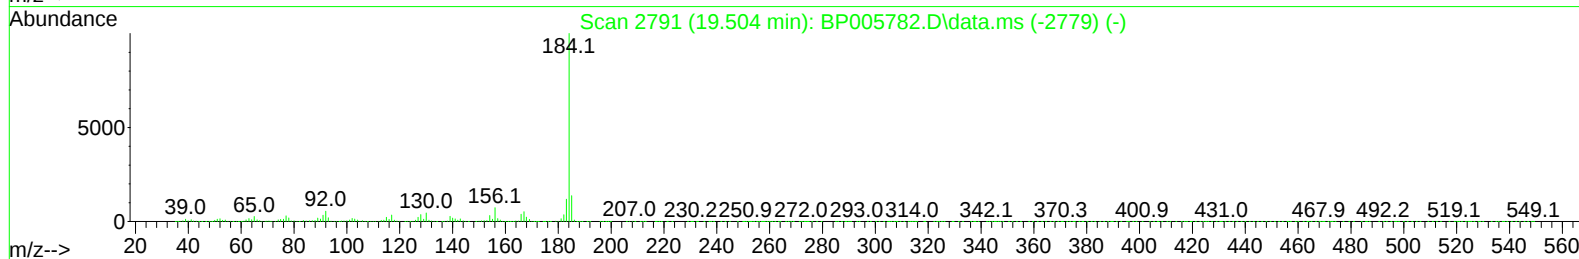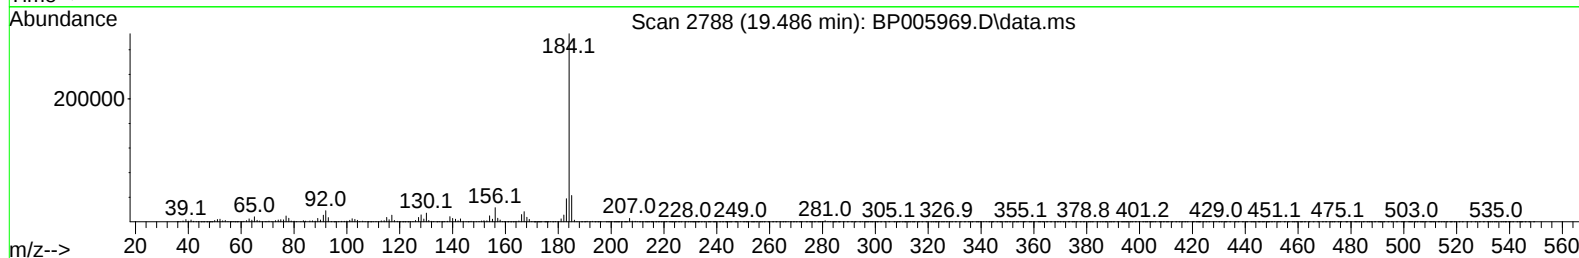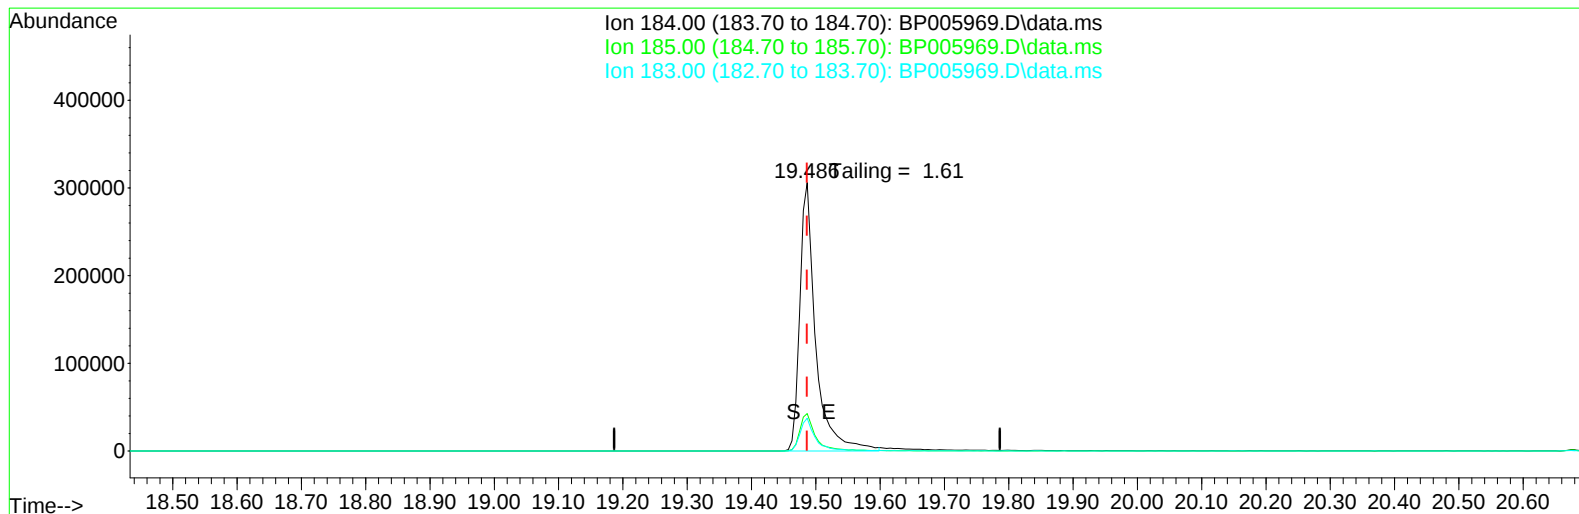

TIC: BP005969.D\data.ms

(77) Benzidine

19.486min (+ 0.000) 22106.88 ng




response 535440

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.97
183.00	11.90	12.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061821\
Data File : BP005969.D
Acq On : 18 Jun 2021 13:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 18 14:34:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 11:35:30 2021
Response via : Initial Calibration

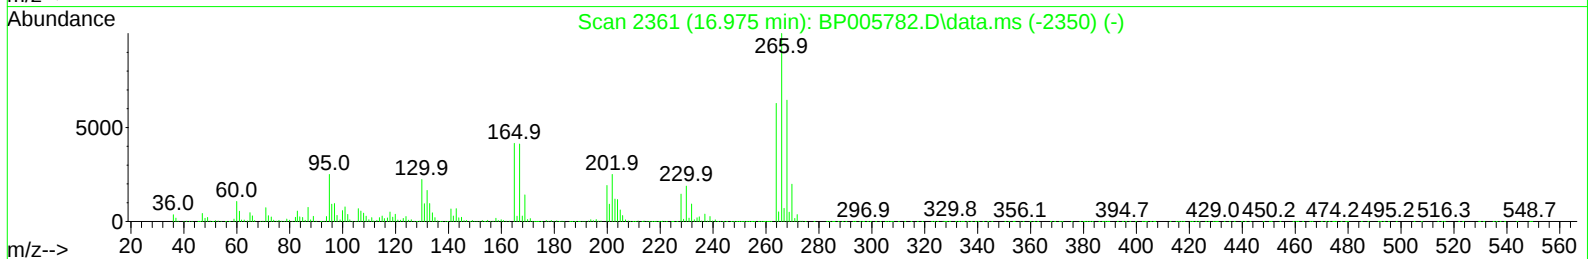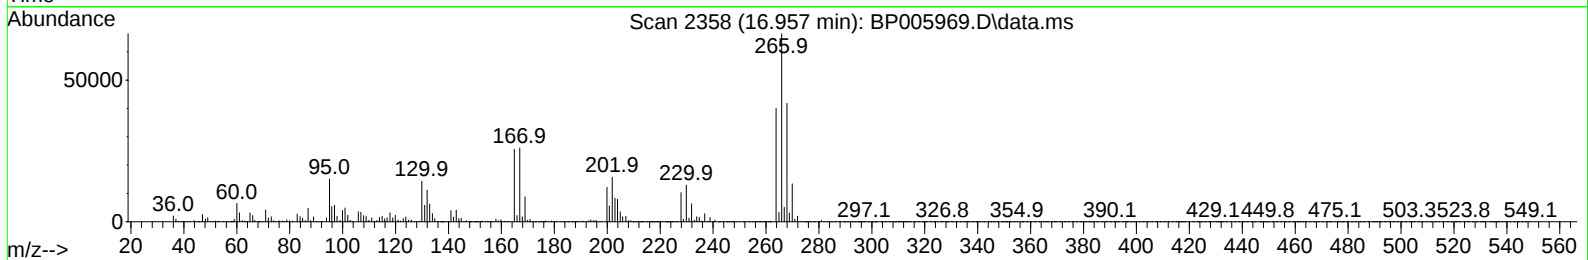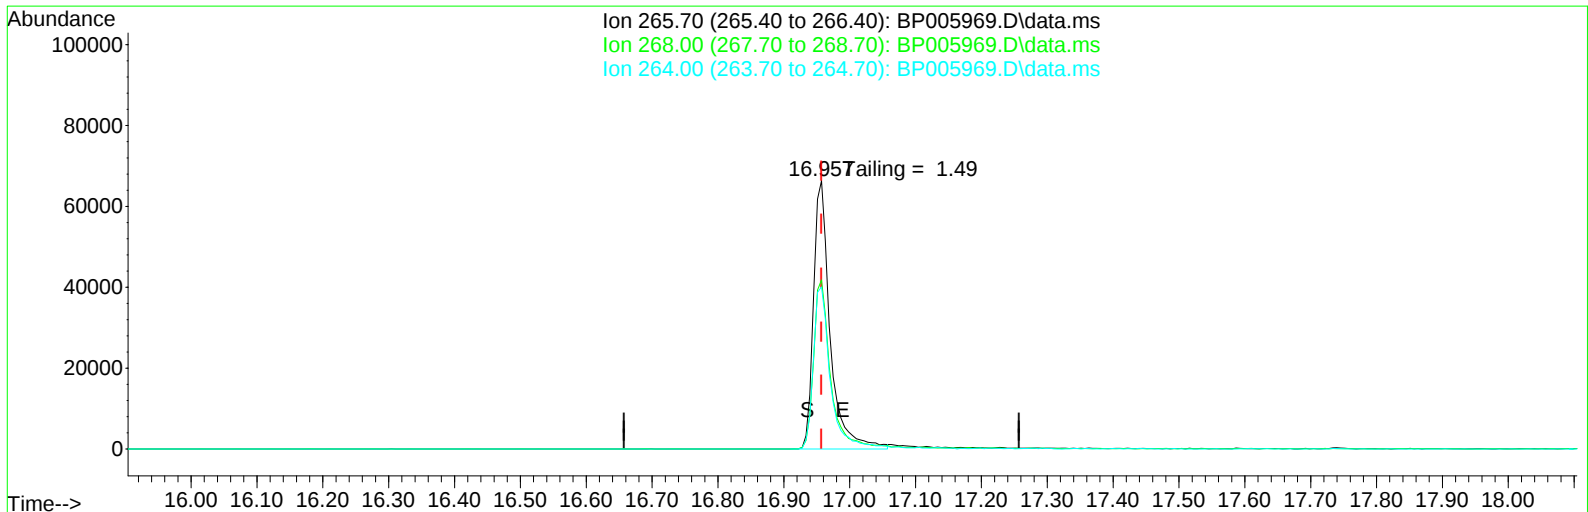

TIC: BP005969.D\data.ms

(70) Pentachlorophenol (C)

16.957min (+ 0.000) 867952.47 ng

response 118797

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.02
264.00	62.90	60.38
0.00	0.00	0.00