

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061923\
 Data File : BP015605.D
 Acq On : 19 Jun 2023 16:04
 Operator : MA/JU
 Sample : PB153448BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK448

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	43	rVB	27786	36161	0.74%	0.082%
2	3.846	109	112	135	rBV	366959	673741	13.86%	1.533%
3	4.176	165	168	174	rVB3	6587	8718	0.18%	0.020%
4	7.240	683	689	707	rBV	530466	909576	18.72%	2.070%
5	7.405	710	717	730	rBV	424321	682598	14.05%	1.553%
6	7.611	745	752	763	rBV	565302	918531	18.90%	2.090%
7	8.081	825	832	843	rBV	420042	698683	14.38%	1.590%
8	8.799	947	954	966	rBV	707833	1239986	25.52%	2.821%
9	9.264	1026	1033	1050	rBV	580793	1012839	20.84%	2.305%
10	9.411	1055	1058	1064	rVB8	3142	4910	0.10%	0.011%
11	9.987	1148	1156	1168	rBV	513515	911852	18.76%	2.075%
12	10.534	1240	1249	1267	rBV	660305	1330634	27.38%	3.028%
13	10.910	1305	1313	1321	rBV	673545	1147704	23.62%	2.611%
14	11.052	1329	1337	1357	rBV	688633	1395984	28.73%	3.176%
15	12.493	1577	1582	1592	rBV2	12339	23984	0.49%	0.055%
16	12.787	1626	1632	1639	rVB10	4205	7549	0.16%	0.017%
17	13.546	1753	1761	1762	rBV8	3554	6242	0.13%	0.014%
18	13.610	1767	1772	1781	rVV2	25971	47329	0.97%	0.108%
19	14.134	1852	1861	1877	rBV	1613433	2339645	48.14%	5.324%
20	14.422	1903	1910	1932	rBV	1772506	2616216	53.83%	5.953%
21	14.728	1953	1962	1969	rBV	1156876	1744433	35.90%	3.969%
22	14.793	1969	1973	1980	rVB6	7256	13194	0.27%	0.030%
23	14.946	1993	1999	2025	rBV	309993	945511	19.46%	2.151%
24	15.369	2065	2071	2074	rBV8	4259	7271	0.15%	0.017%
25	15.540	2096	2100	2103	rBV	5318	6001	0.12%	0.014%
26	15.716	2121	2130	2137	rBV	2151503	3258710	67.06%	7.415%
27	15.769	2137	2139	2145	rVV4	19801	28367	0.58%	0.065%
28	15.846	2146	2152	2168	rBV	737879	1149018	23.64%	2.614%
29	15.957	2168	2171	2174	rBV5	8262	11418	0.23%	0.026%
30	16.351	2234	2238	2242	rVB7	3883	5717	0.12%	0.013%
31	16.498	2261	2263	2269	rVB6	3743	5790	0.12%	0.013%
32	16.663	2286	2291	2297	rBV9	6082	11554	0.24%	0.026%
33	16.781	2307	2311	2314	rBV6	4443	5876	0.12%	0.013%
34	16.940	2334	2338	2340	rBV5	4731	7132	0.15%	0.016%
35	17.163	2372	2376	2381	rVB8	4307	7000	0.14%	0.016%
36	17.275	2392	2395	2403	rVB7	4791	8666	0.18%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061923\
 Data File : BP015605.D
 Acq On : 19 Jun 2023 16:04
 Operator : MA/JU
 Sample : PB153448BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK448

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	17.481	2424	2430	2441	rBV	1631799	2344439	48.24%	5.334%
38	17.581	2441	2447	2459	rVV	2608253	3796570	78.12%	8.639%
39	17.904	2500	2502	2506	rVB4	5609	5549	0.11%	0.013%
40	18.128	2537	2540	2544	rVB6	4219	6884	0.14%	0.016%
41	18.351	2576	2578	2584	rVB5	4113	6146	0.13%	0.014%
42	18.416	2586	2589	2592	rVB	8564	9165	0.19%	0.021%
43	19.381	2749	2753	2758	rBV2	42308	58734	1.21%	0.134%
44	19.451	2761	2765	2770	rBV2	40000	65483	1.35%	0.149%
45	19.804	2819	2825	2838	rBV	3458175	4859700	100.00%	11.058%
46	20.716	2978	2980	2985	rVB3	44968	47863	0.98%	0.109%
47	21.563	3119	3124	3134	rBV	1832746	2591145	53.32%	5.896%
48	23.945	3521	3529	3546	rVB2	2109059	4463273	91.84%	10.156%
49	24.110	3550	3557	3566	rVB	1116185	2465352	50.73%	5.610%




Sum of corrected areas: 43948843

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061923\
Data File : BP015605.D
Acq On : 19 Jun 2023 16:04
Operator : MA/JU
Sample : PB153448BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

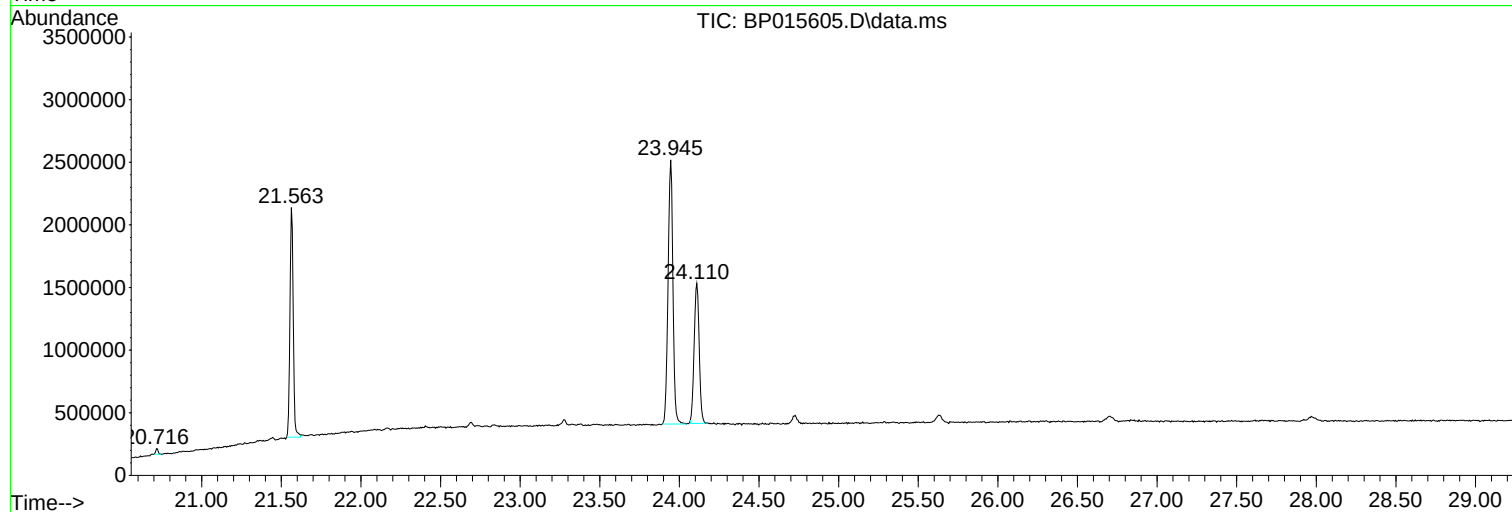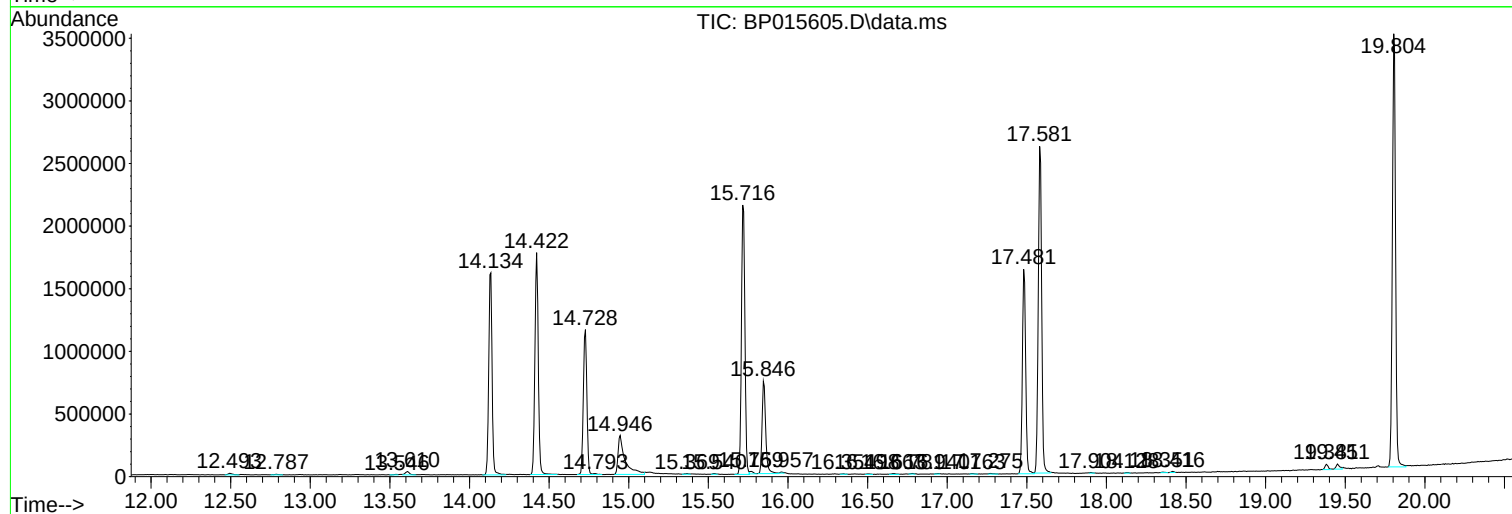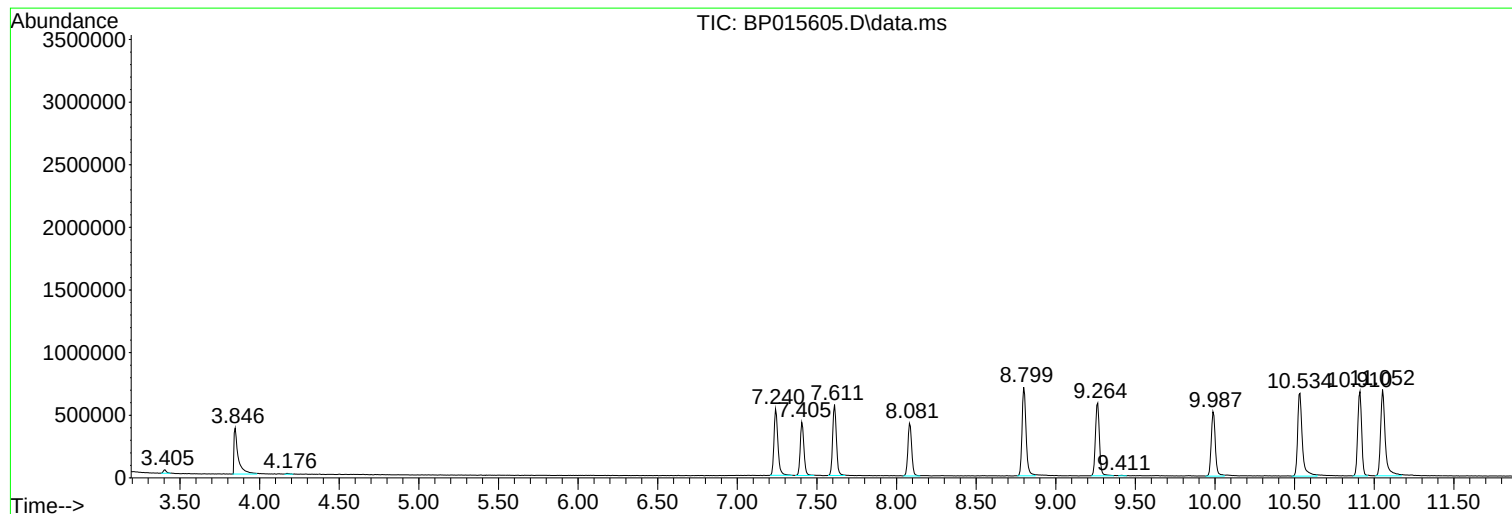

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061923\
Data File : BP015605.D
Acq On : 19 Jun 2023 16:04
Operator : MA/JU
Sample : PB153448BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061923\
Data File : BP015605.D
Acq On : 19 Jun 2023 16:04
Operator : MA/JU
Sample : PB153448BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------