








Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062023\  
 Data File : BP015625.D  
 Acq On : 20 Jun 2023 17:03  
 Operator : MA/JU  
 Sample : 03080-07  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCFH6

Manual IntegrationsAPPROVED

Quant Time: Jun 20 23:11:04 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jun 15 05:36:46 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh  
 Patel

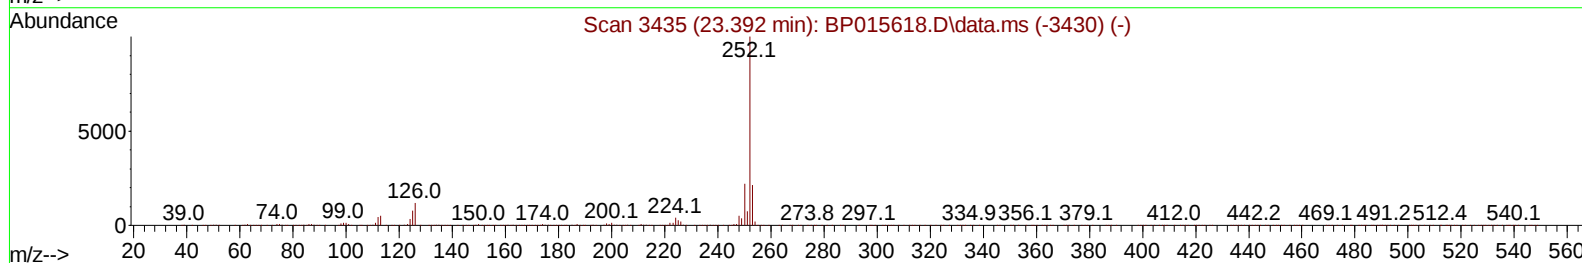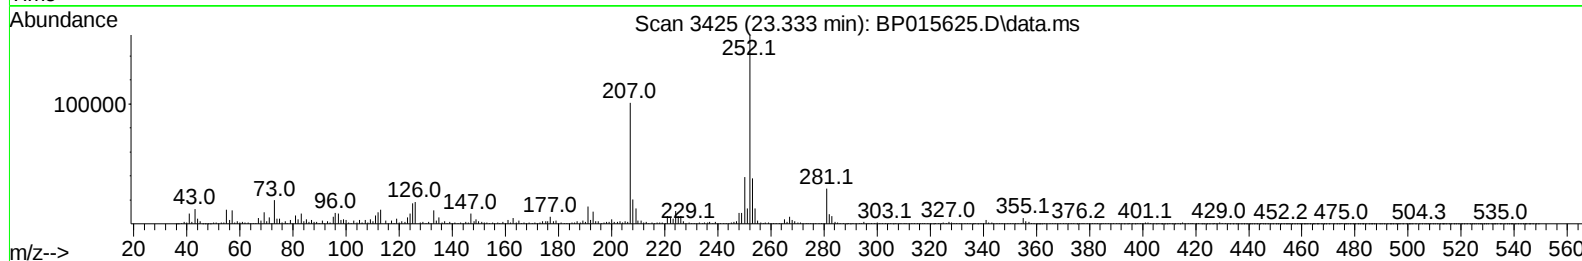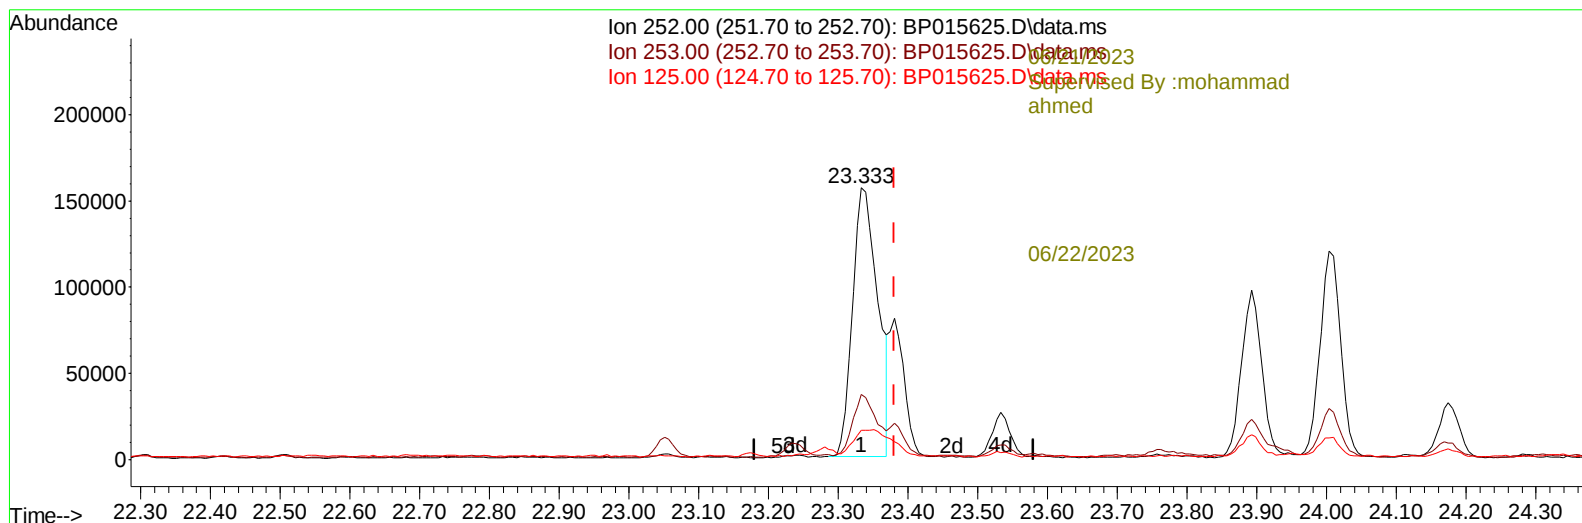

TIC: BP015625.D\data.ms

(91) Benzo(k)fluoranthene

23.333min (-0.047) 8.90 ng/u1

response 392649

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 22.10  | 23.99  |
| 125.00 | 9.10   | 10.78  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062023\  
 Data File : BP015625.D  
 Acq On : 20 Jun 2023 17:03  
 Operator : MA/JU  
 Sample : 03080-07  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCFH6

Manual IntegrationsAPPROVED

Quant Time: Jun 20 23:11:04 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jun 15 05:36:46 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh  
 Patel

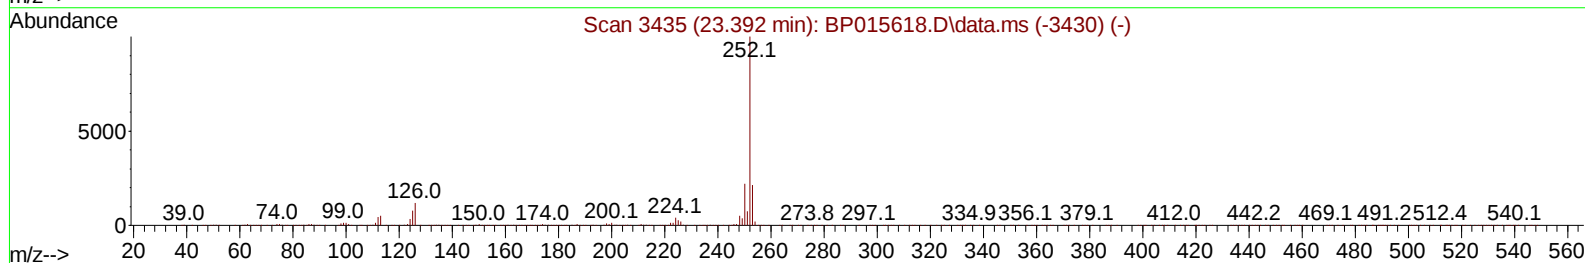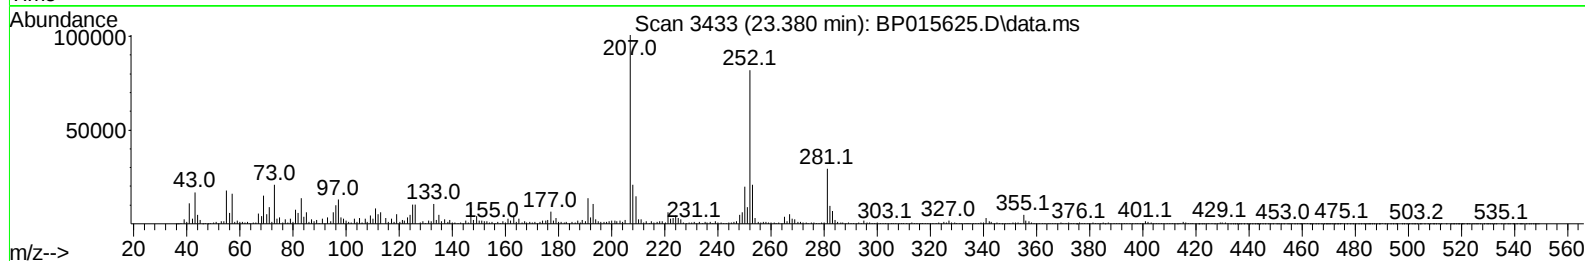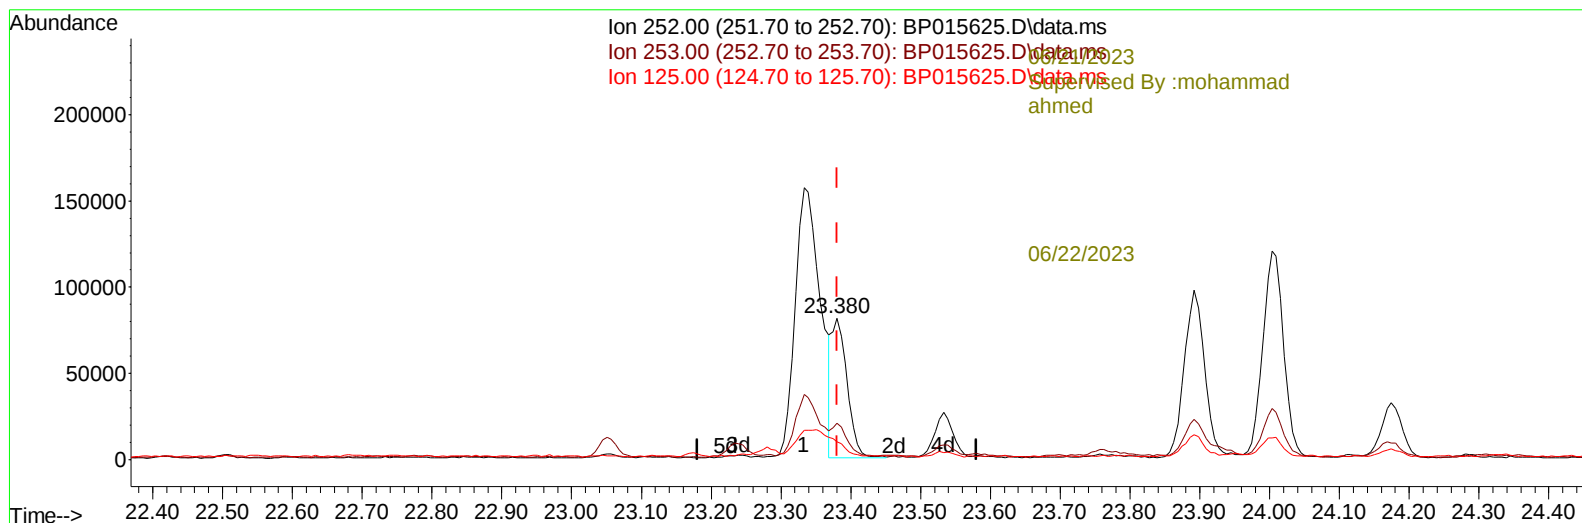

TIC: BP015625.D\data.ms

**(91) Benzo(k)fluoranthene**

**23.380min (-0.000) 2.76 ng/u1 m**

**response 121837**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 22.10  | 25.57  |
| 125.00 | 9.10   | 12.42# |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062023\  
 Data File : BP015625.D  
 Acq On : 20 Jun 2023 17:03  
 Operator : MA/JU  
 Sample : 03080-07  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCFH6

Manual IntegrationsAPPROVED

Quant Time: Jun 20 23:11:37 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jun 15 05:36:46 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh  
 Patel

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----06/21/2023               |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.087  | 152  | 86022    | 20.000 | ng/ul  | 0.00     |
| 20) Naphthalene-d8            | 10.910 | 136  | 381570   | 20.000 | ng/ul  | 0.00     |
| 38) Acenaphthene-d10          | 14.728 | 164  | 257733   | 20.000 | ng/ul  | 0.00     |
| 64) Phenanthrene-d10          | 17.486 | 188  | 619053   | 20.000 | ng/ul  | 0.00     |
| 79) Chrysene-d12              | 21.569 | 240  | 644058   | 20.000 | ng/ul  | 0.00     |
| 88) Perylene-d12              | 24.121 | 264  | 706905   | 20.000 | ng/ul  | 0.00     |
| -----06/22/2023               |        |      |          |        |        |          |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8             | 3.405  | 96   | 6058     | 2.608  | ng/uL  | 0.00     |
| 4) Pyridine-d5                | 3.852  | 84   | 75974    | 12.591 | ng/ul  | 0.00     |
| 7) Phenol-d5                  | 7.252  | 99   | 154839   | 19.538 | ng/ul  | 0.01     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.410  | 67   | 96729    | 20.438 | ng/ul  | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.610  | 132  | 123004   | 21.408 | ng/ul  | 0.00     |
| 15) 4-Methylphenol-d8         | 8.804  | 113  | 111080   | 17.079 | ng/ul  | 0.00     |
| 21) Nitrobenzene-d5           | 9.263  | 128  | 62920    | 21.003 | ng/ul  | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.993  | 143  | 73622    | 21.520 | ng/ul  | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.540 | 165  | 126923   | 20.338 | ng/ul  | 0.00     |
| 31) 4-Chloroaniline-d4        | 11.063 | 131  | 125118   | 13.968 | ng/ul  | 0.00     |
| 46) Dimethylphthalate-d6      | 14.134 | 166  | 456366   | 22.455 | ng/ul  | 0.00     |
| 49) Acenaphthylene-d8         | 14.422 | 160  | 517764   | 23.298 | ng/ul  | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.963 | 143  | 57243m   | 15.728 | ng/ul  | 0.03     |
| 60) Fluorene-d10              | 15.722 | 176  | 400311   | 23.357 | ng/ul  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.857 | 200  | 60179    | 15.345 | ng/ul  | 0.00     |
| 73) Anthracene-d10            | 17.586 | 188  | 655395   | 23.269 | ng/ul  | 0.00     |
| 81) Pyrene-d10                | 19.810 | 212  | 898929   | 26.078 | ng/ul  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.951 | 264  | 868065   | 24.474 | ng/ul  | 0.00     |
| -----                         |        |      |          |        |        |          |
| Target Compounds              |        |      |          |        |        | Qvalue   |
| 72) Phenanthrene              | 17.528 | 178  | 119129   | 3.586  | ng/ul  | 98       |
| 80) Fluoranthene              | 19.486 | 202  | 397363   | 9.463  | ng/ul  | 98       |
| 82) Pyrene                    | 19.839 | 202  | 335081   | 7.713  | ng/ul  | 98       |
| 85) Benzo(a)anthracene        | 21.551 | 228  | 213732   | 4.747  | ng/ul  | 99       |
| 87) Chrysene                  | 21.610 | 228  | 240760   | 5.657  | ng/ul  | 96       |
| 90) Benzo(b)fluoranthene      | 23.333 | 252  | 392649   | 8.605  | ng/ul  | 95       |
| 91) Benzo(k)fluoranthene      | 23.380 | 252  | 121837m  | 2.762  | ng/ul  |          |
| 93) Benzo(a)pyrene            | 24.004 | 252  | 246146   | 6.187  | ng/ul  | 97       |
| 94) Indeno(1,2,3-cd)pyrene    | 26.815 | 276  | 201173   | 3.907  | ng/ul  | 95       |
| 95) Dibenzo(a,h)anthracene    | 26.821 | 278  | 50663    | 1.208  | ng/ul# | 75       |
| 96) Benzo(g,h,i)perylene      | 27.656 | 276  | 186804   | 4.403  | ng/ul  | 99       |
| -----                         |        |      |          |        |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062023\  
Data File : BP015625.D  
Acq On : 20 Jun 2023 17:03  
Operator : MA/JU  
Sample : 03080-07  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DCFH6

Manual IntegrationsAPPROVED

Quant Time: Jun 20 23:11:37 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Jun 15 05:36:46 2023  
Response via : Initial Calibration

Reviewed By :Yogesh  
Patel

