




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:04:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

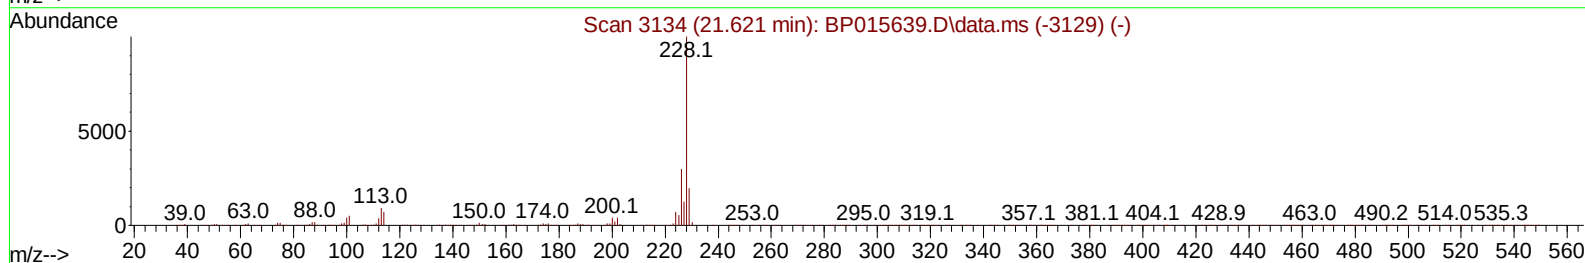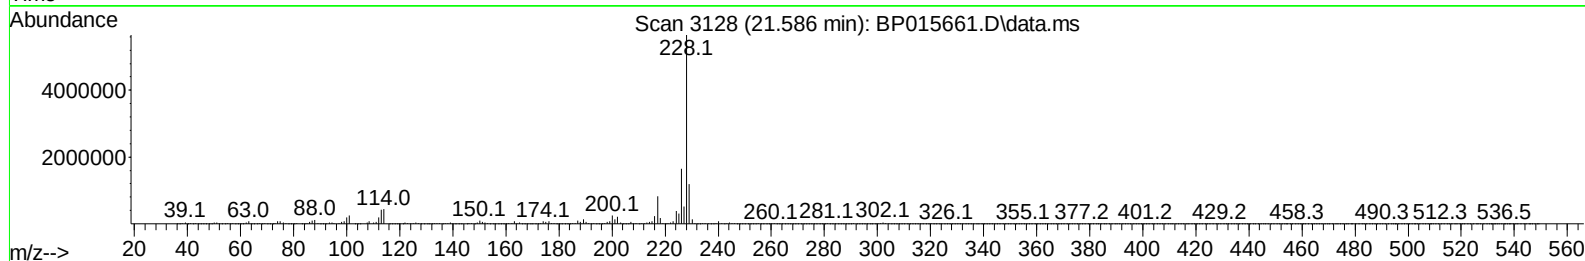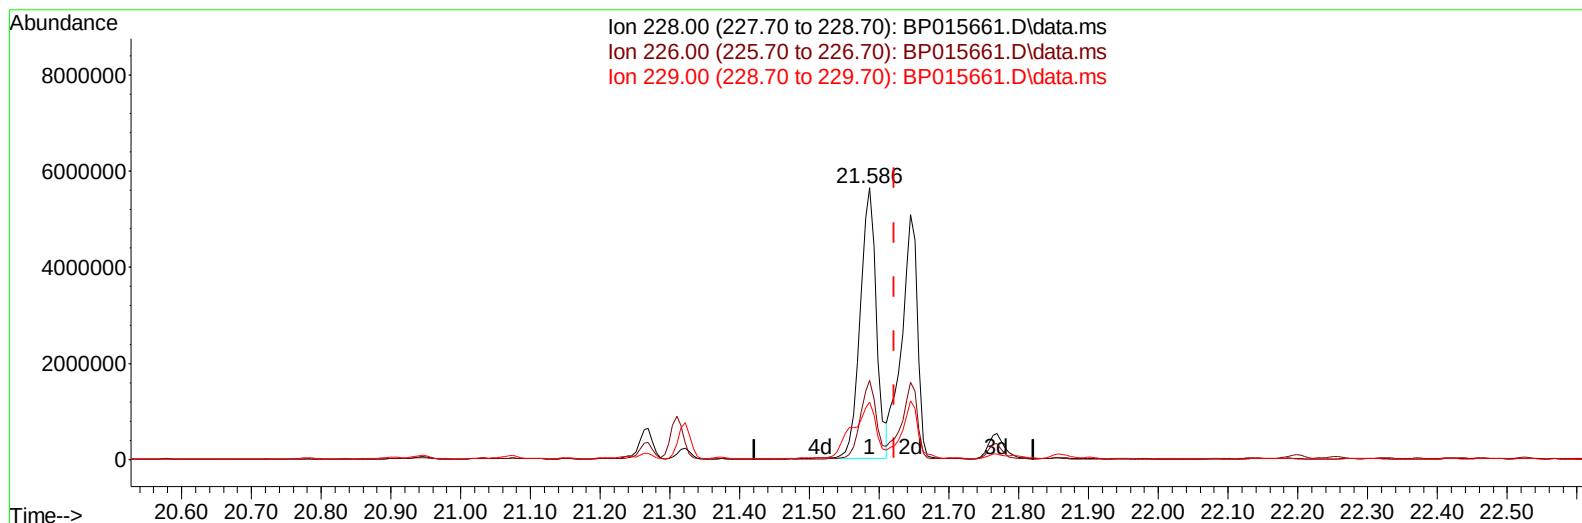

TIC: BP015661.D\data.ms

(87) Chrysene

21.586min (-0.035) 301.32 ng/ul

response 9050278

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.90	29.14
229.00	18.90	21.05
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:04:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

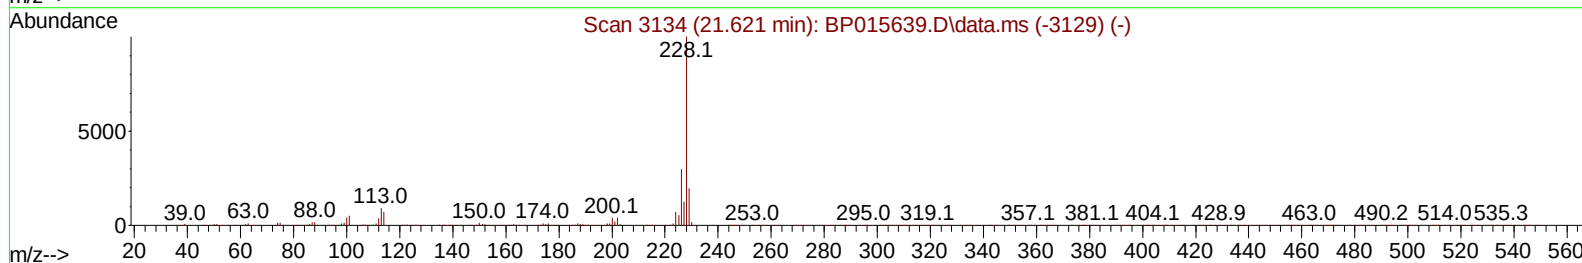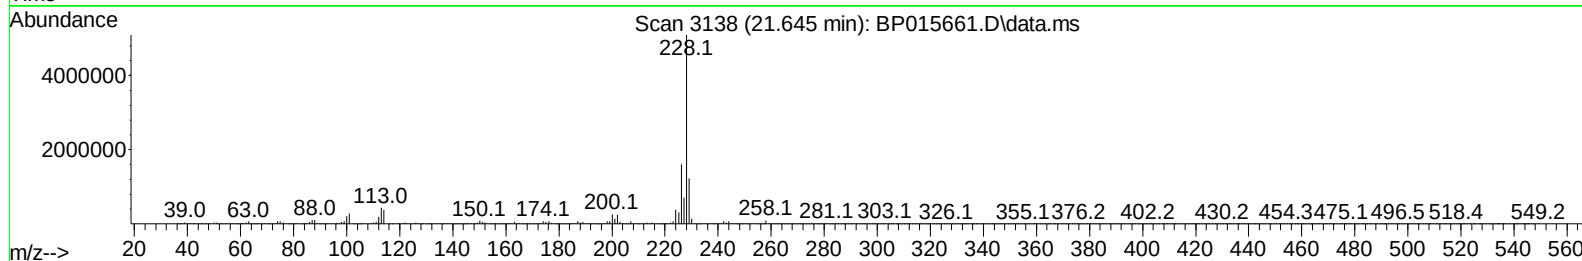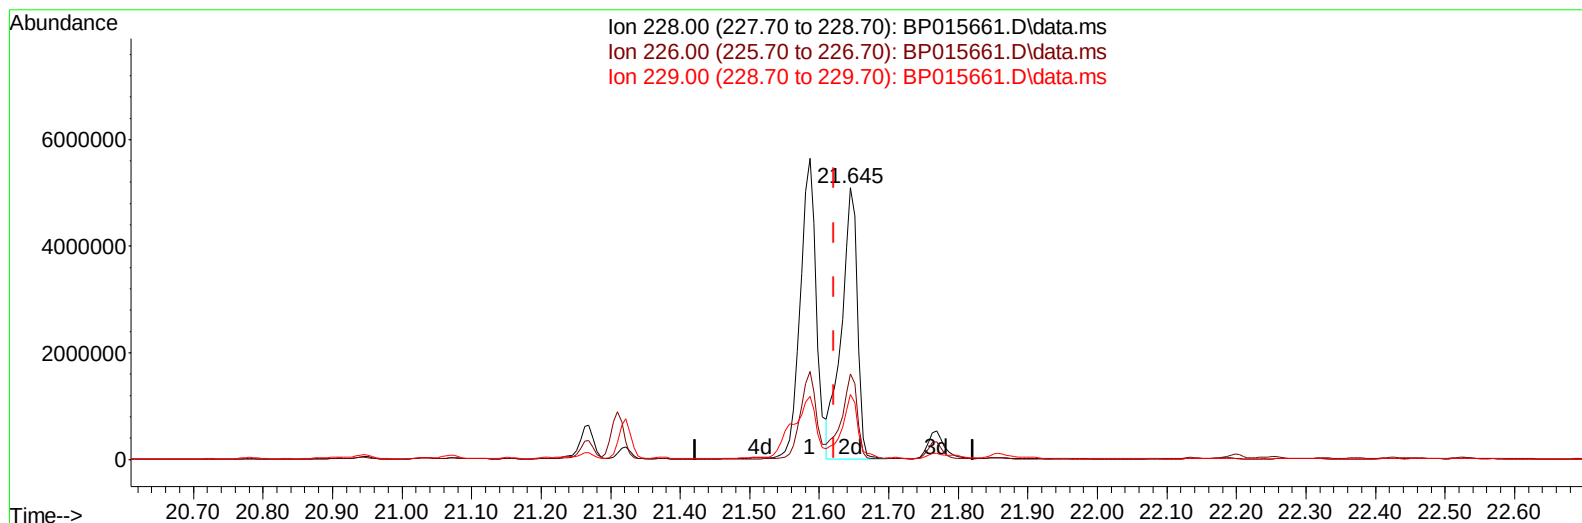

TIC: BP015661.D\data.ms

(87) Chrysene

21.645min (+ 0.024) 271.25 ng/ul m

response 8147009

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.90	31.51
229.00	18.90	23.97#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:04:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

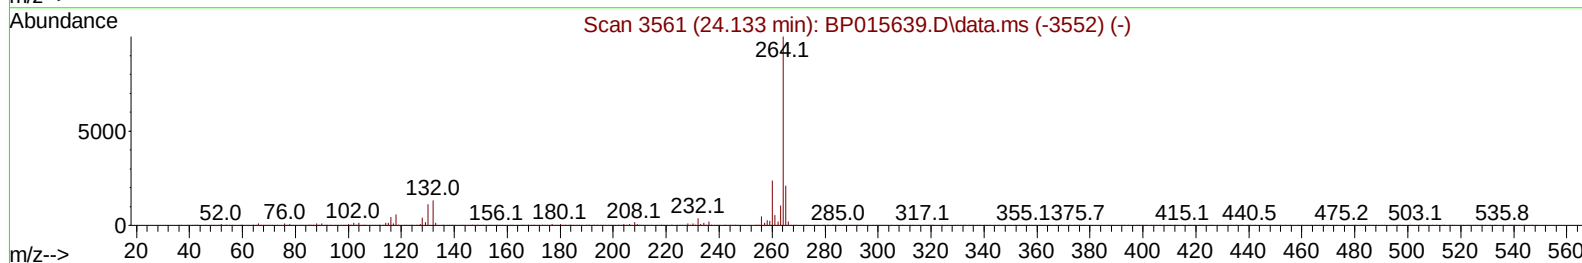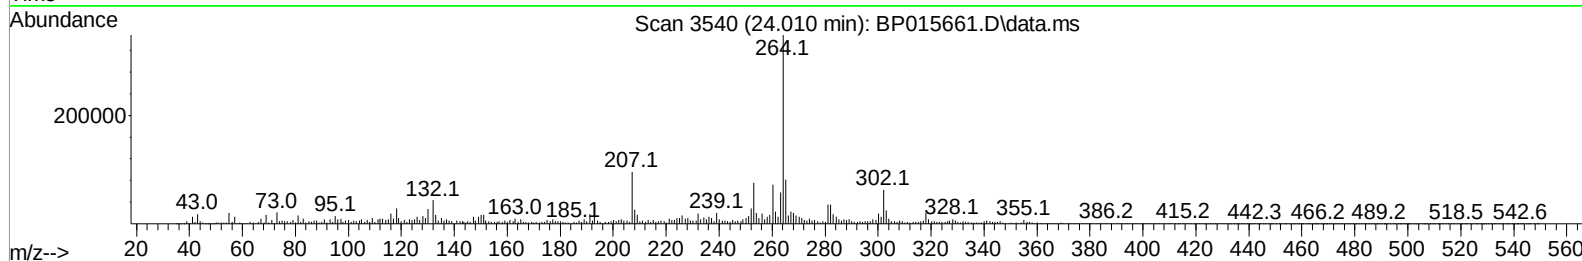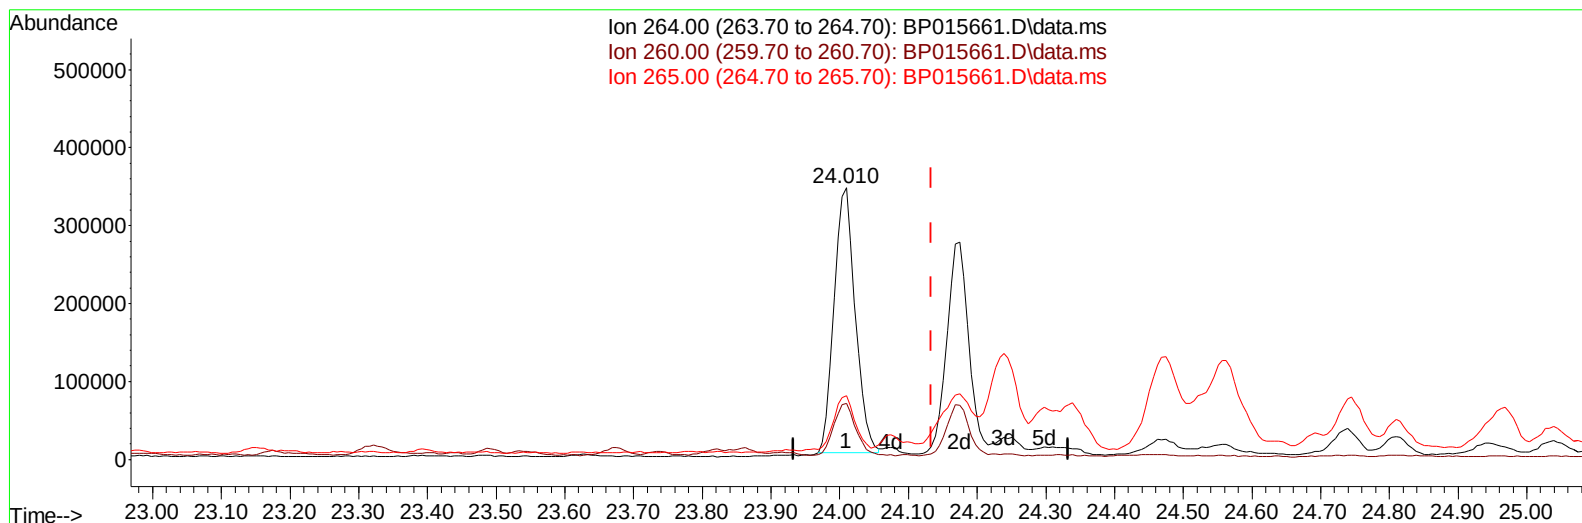

TIC: BP015661.D\data.ms

(88) Perylene-d12 (I)

24.010min (-0.123) 20.00 ng/ul

response 722404

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	24.20	20.72
265.00	21.50	23.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:04:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

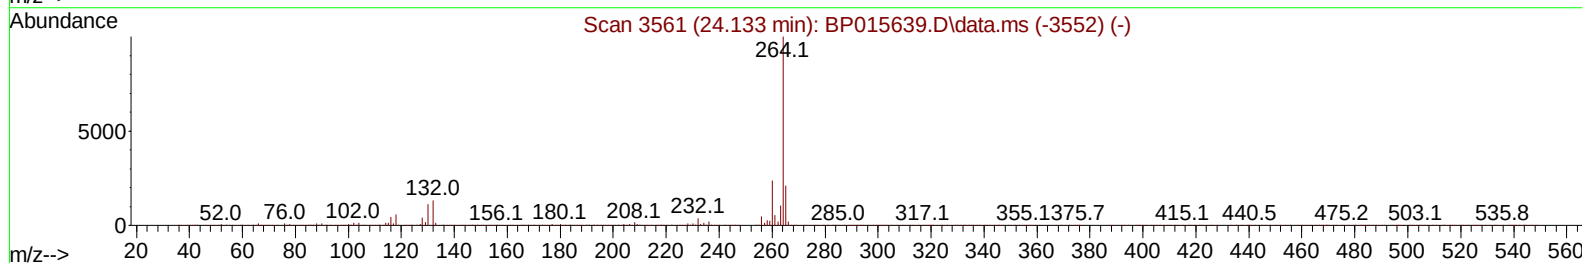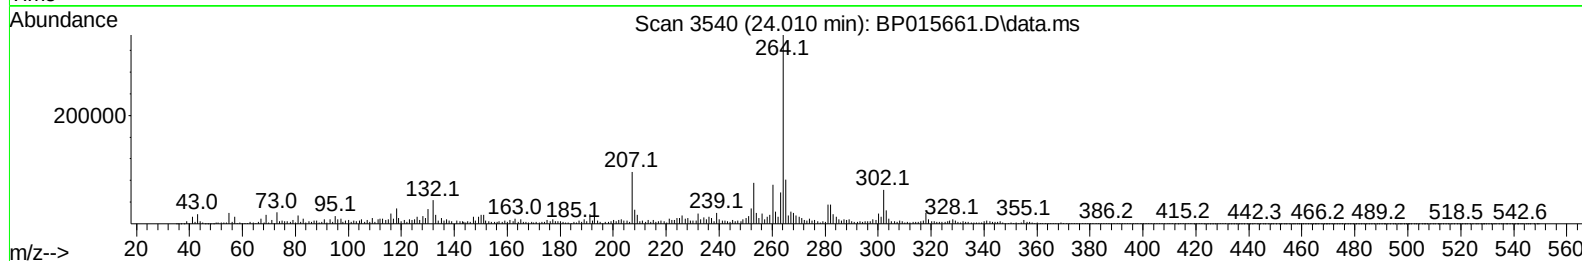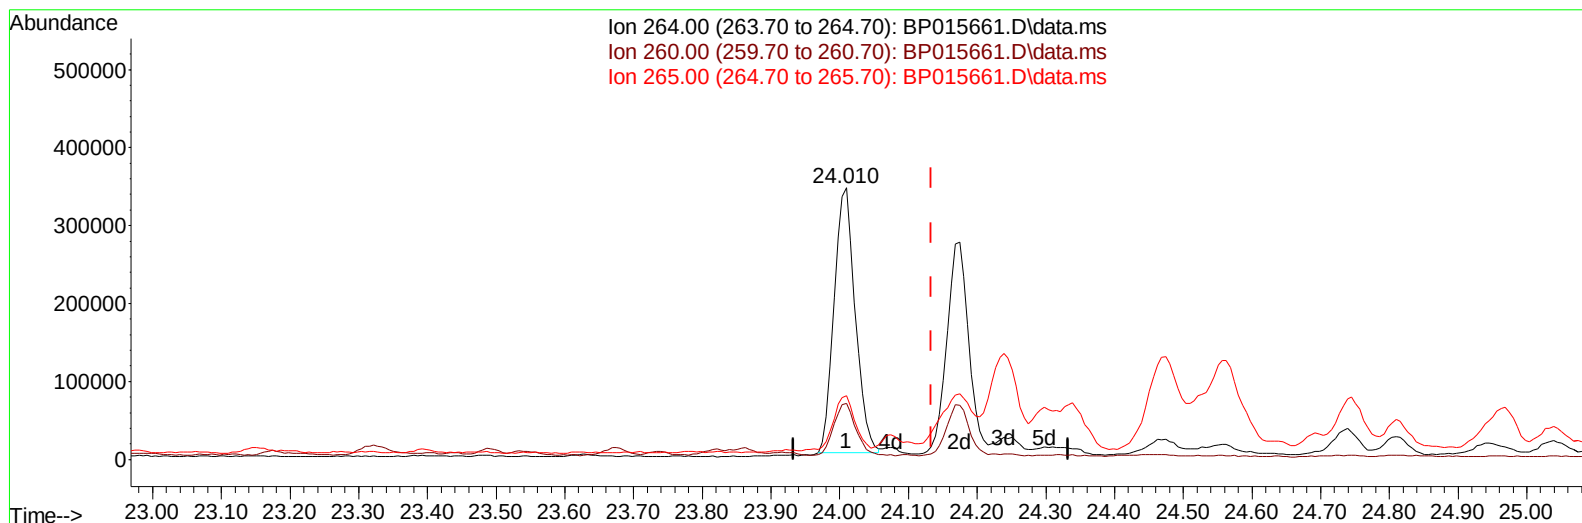

TIC: BP015661.D\data.ms

(88) Perylene-d12 (I)

24.010min (-0.123) 20.00 ng/ul

response 722404

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	24.20	20.72
265.00	21.50	23.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:04:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

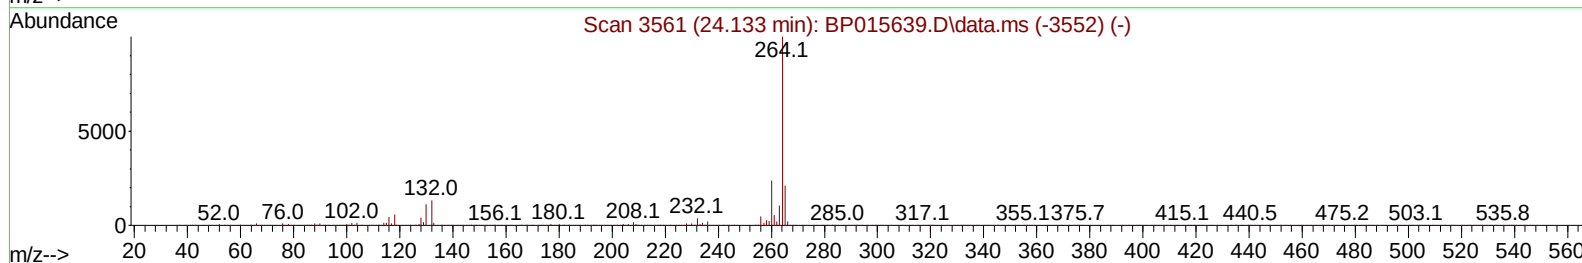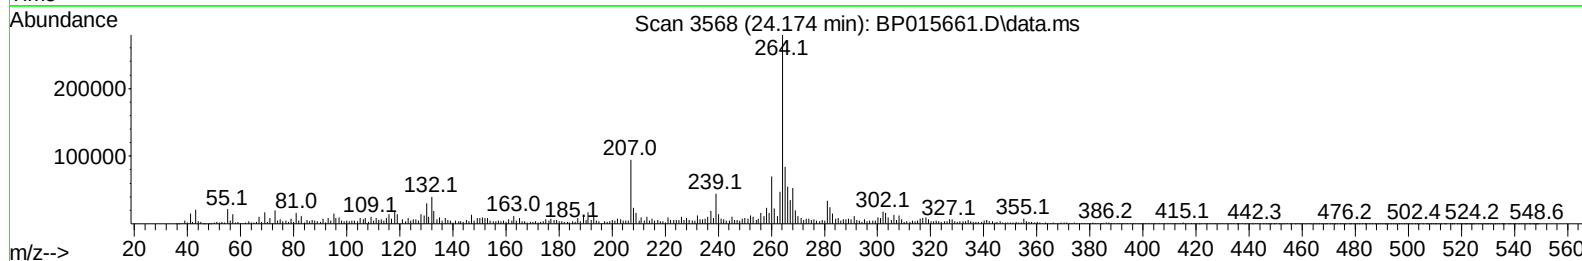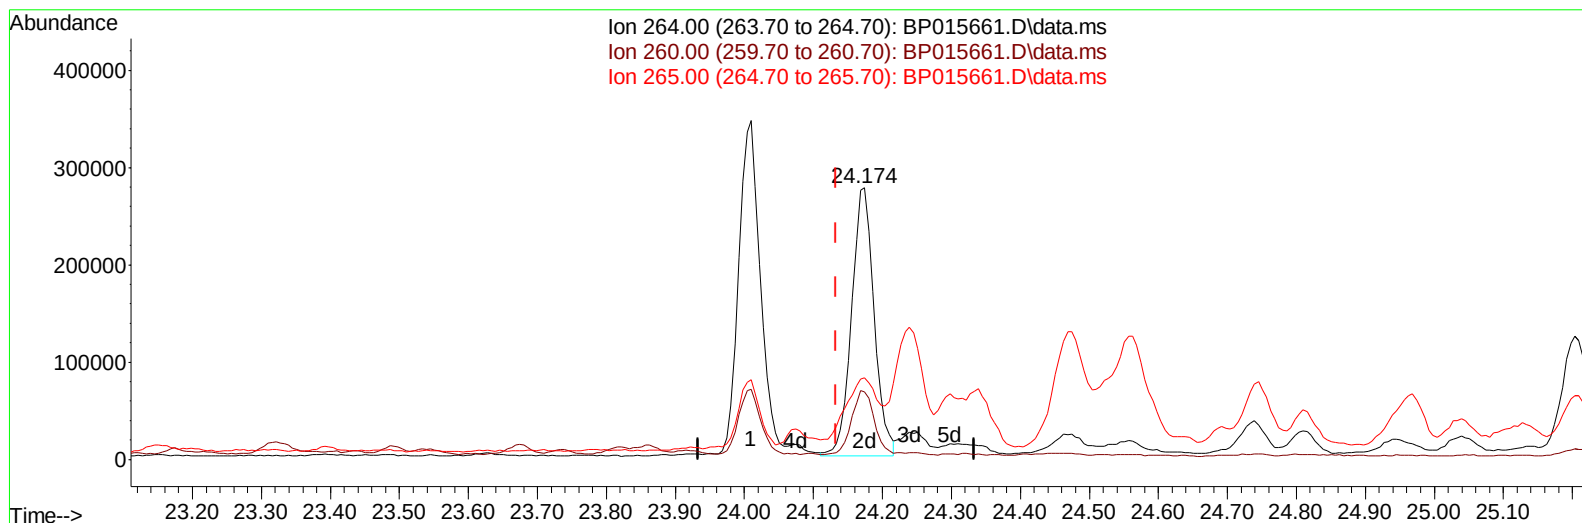

TIC: BP015661.D\data.ms

(88) Perylene-d12 (I)

24.174min (+ 0.041) 20.00 ng/ul m

response 627346

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	24.20	25.00
265.00	21.50	30.10#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015661.D
Acq On : 22 Jun 2023 22:59
Operator : MA/JU
Sample : 03083-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

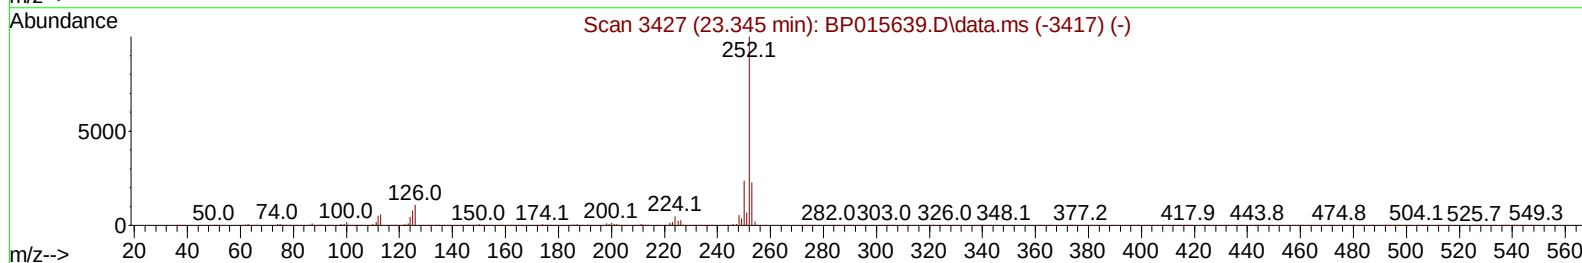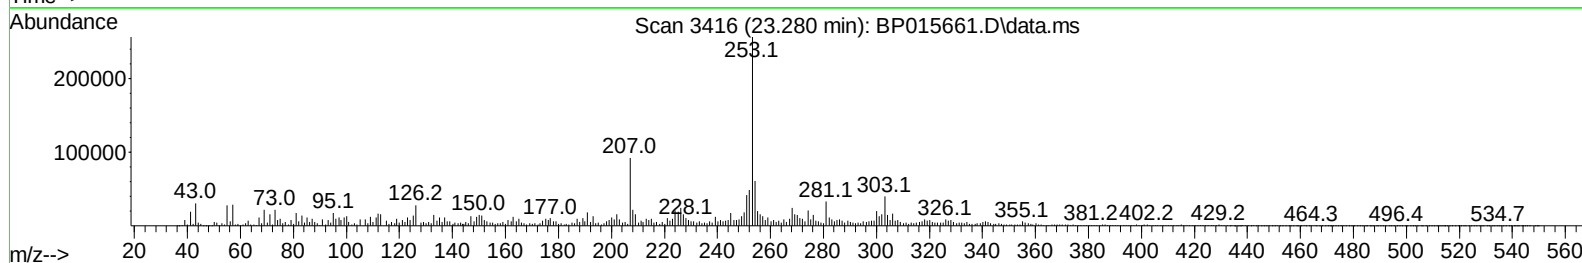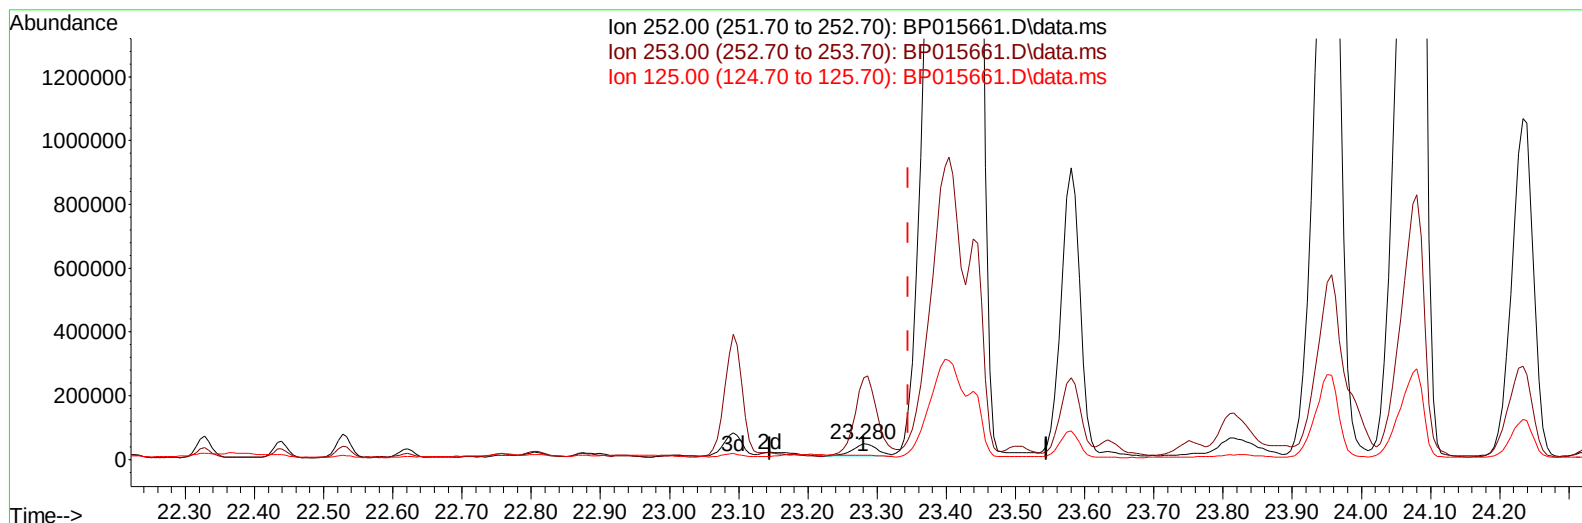

TIC: BP015661.D\data.ms

(90) Benzo(b)fluoranthene

23.280min (-0.064) 2.41 ng/u1

response 97559

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.80	528.19#
125.00	9.10	27.85#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015661.D
Acq On : 22 Jun 2023 22:59
Operator : MA/JU
Sample : 03083-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

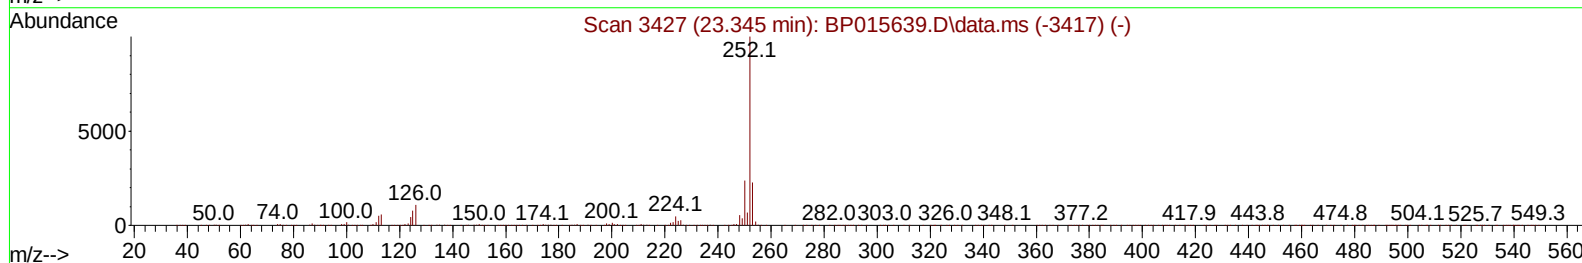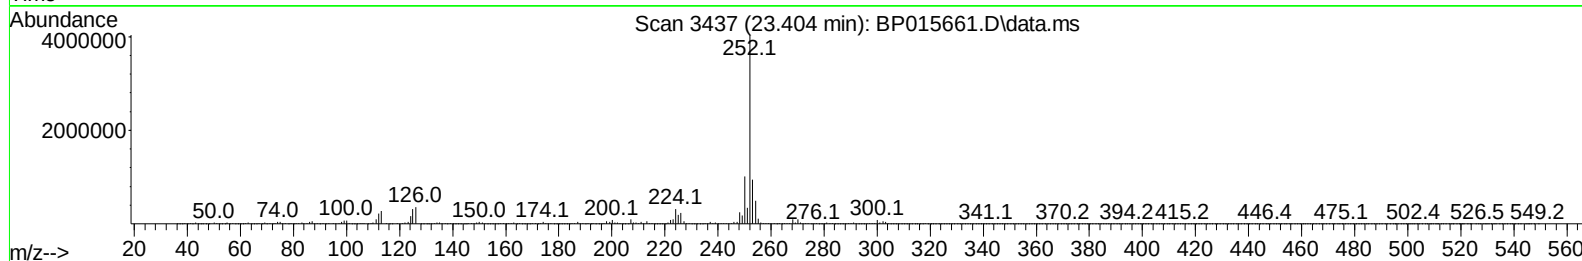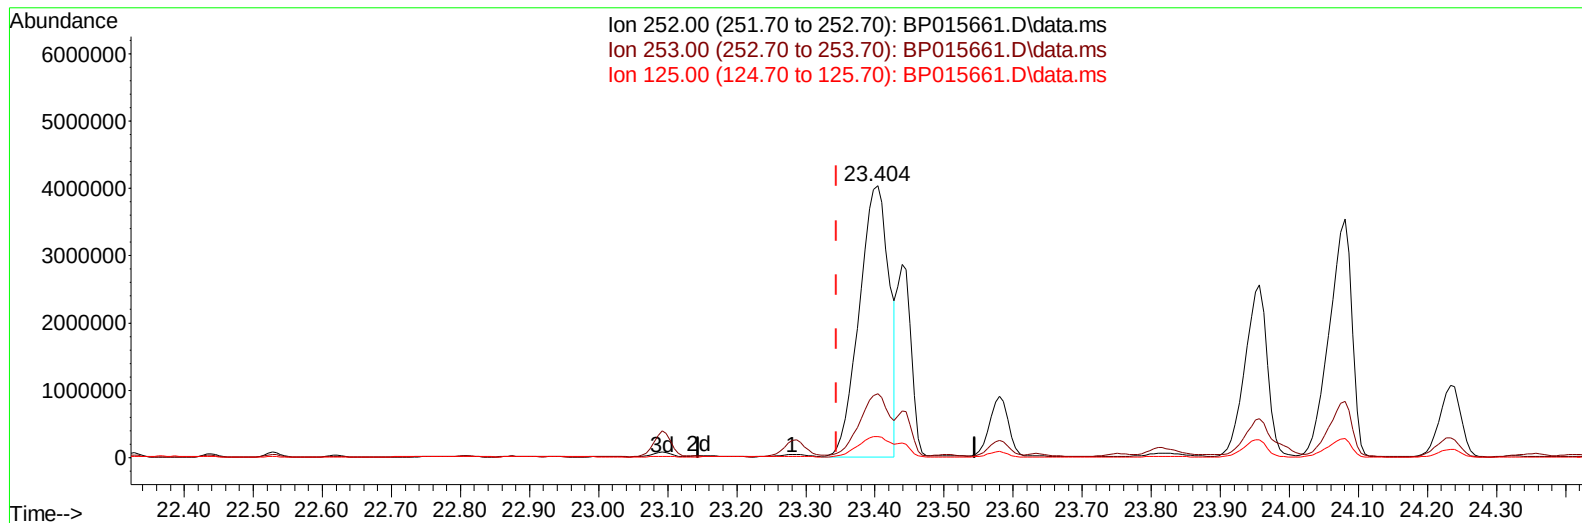

TIC: BP015661.D\data.ms

(90) Benzo(b)fluoranthene

23.404min (+ 0.059) 300.03 ng/ul m

response 12149756

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.80	23.52
125.00	9.10	7.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

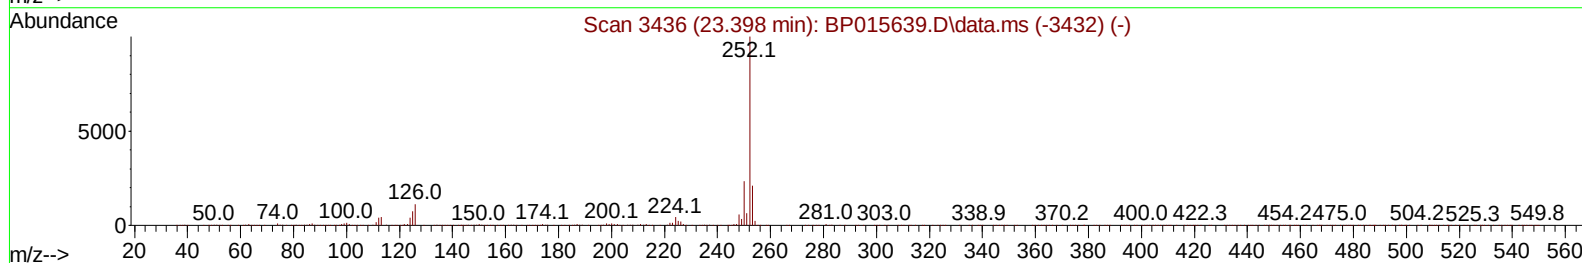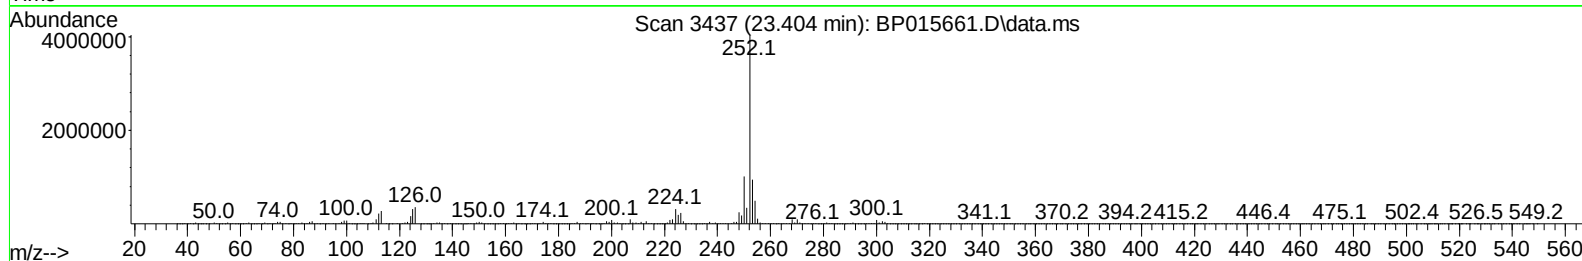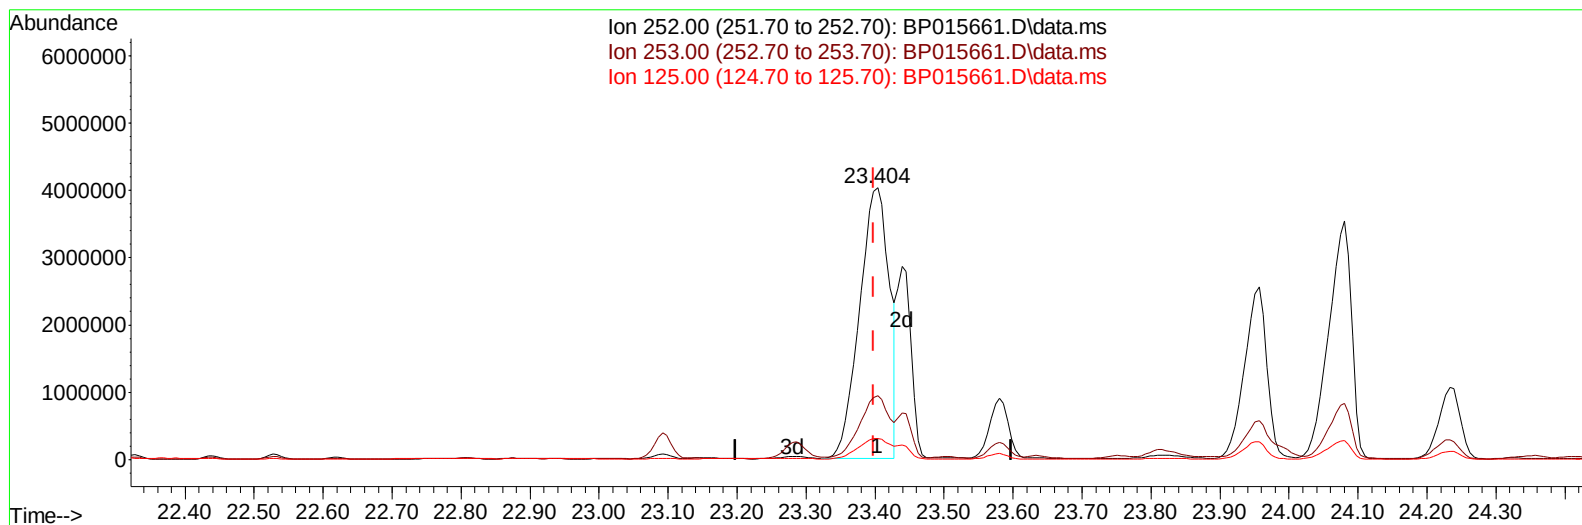

TIC: BP015661.D\data.ms

(91) Benzo(k)fluoranthene

23.404min (+ 0.006) 308.70 ng/uL

response 12084102

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.10	23.52
125.00	9.10	7.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

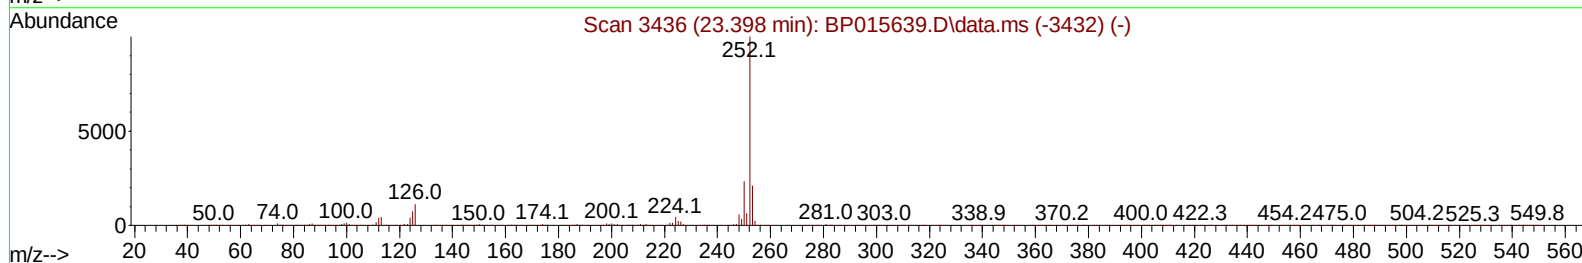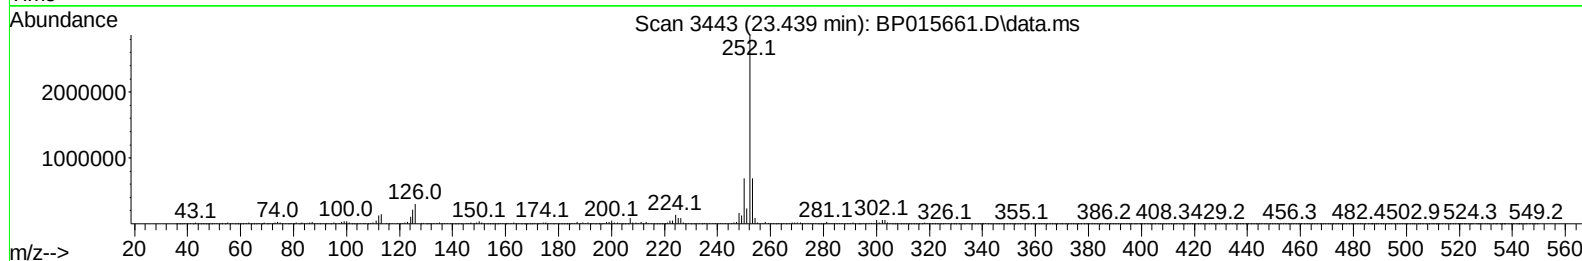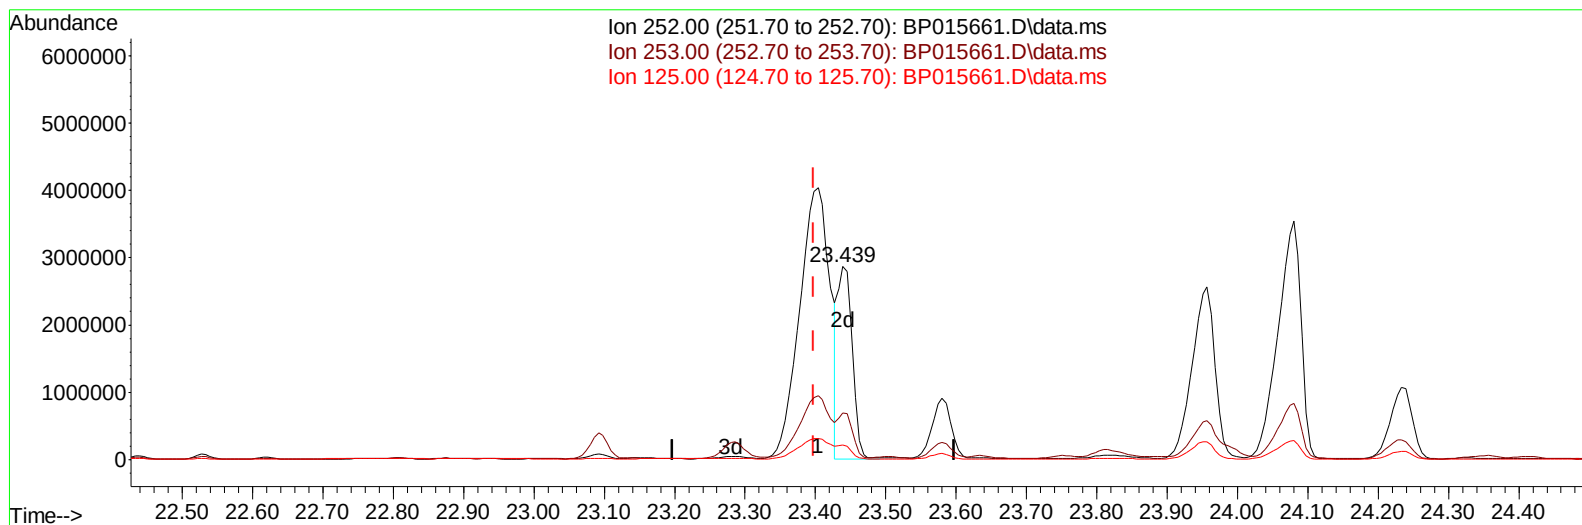

TIC: BP015661.D\data.ms

(91) Benzo(k)fluoranthene

23.439min (+ 0.041) 103.84 ng/ul m

response 4064926

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.10	24.15
125.00	9.10	7.49
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

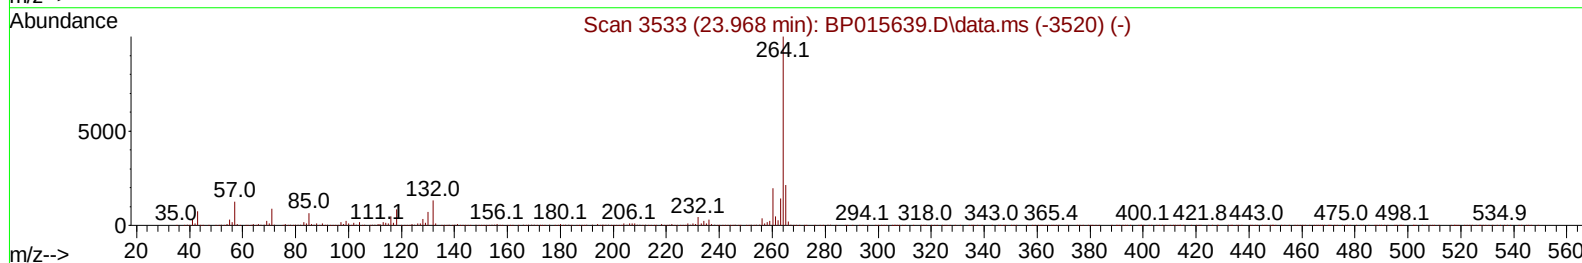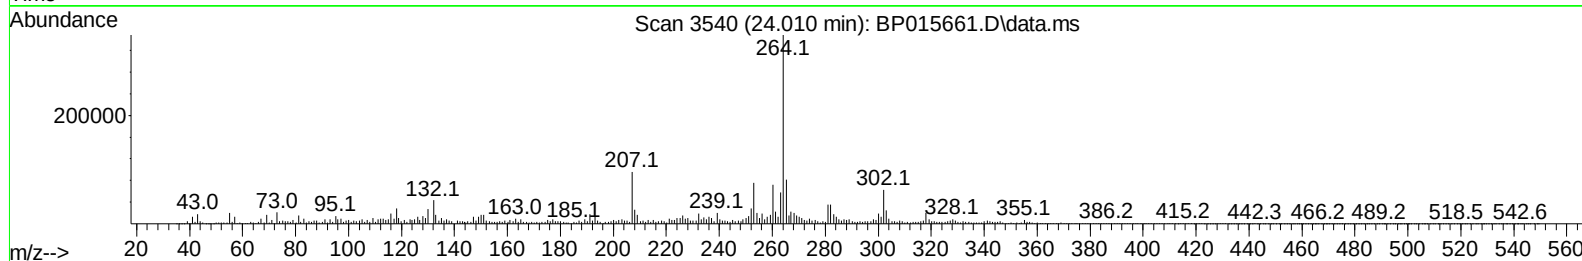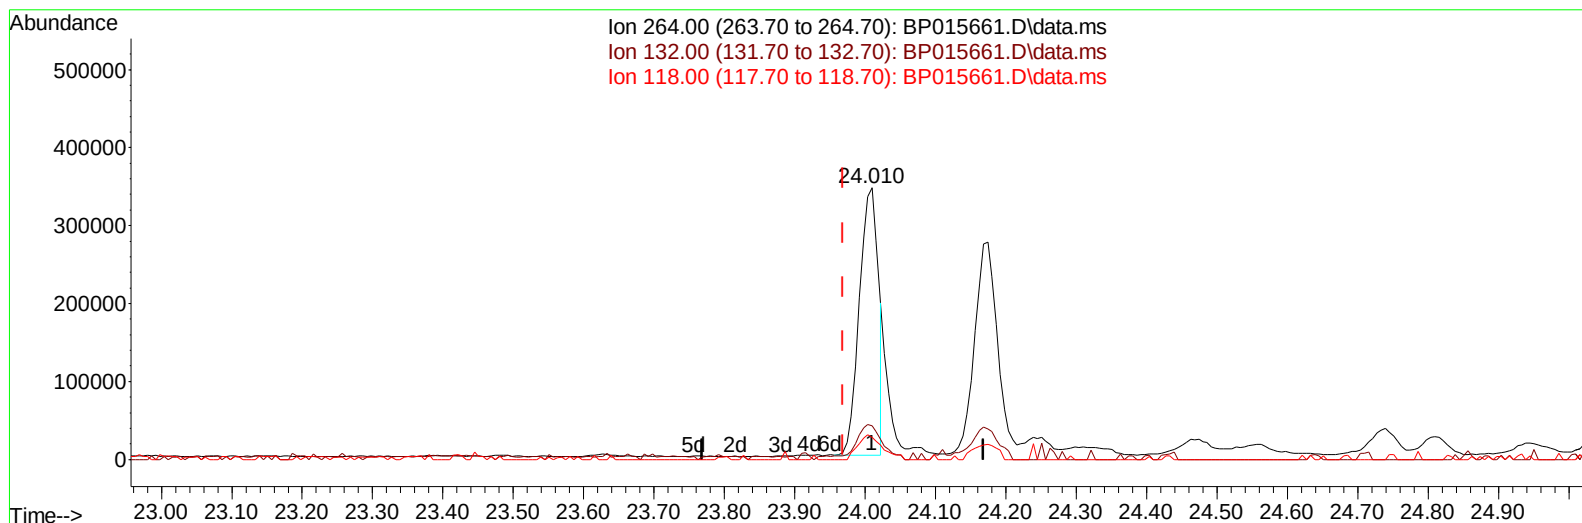

TIC: BP015661.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

24.010min (+ 0.041) 20.29 ng/ul

response 638739

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	15.00	12.45
118.00	9.10	8.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015661.D
Acq On : 22 Jun 2023 22:59
Operator : MA/JU
Sample : 03083-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

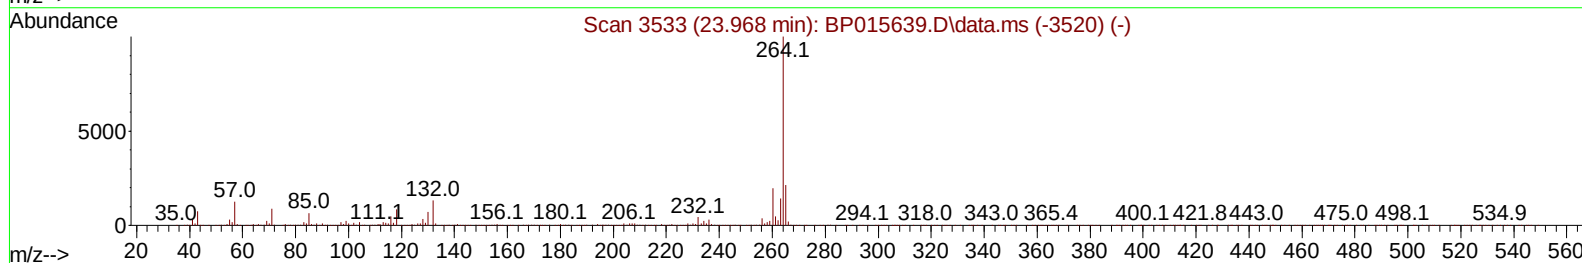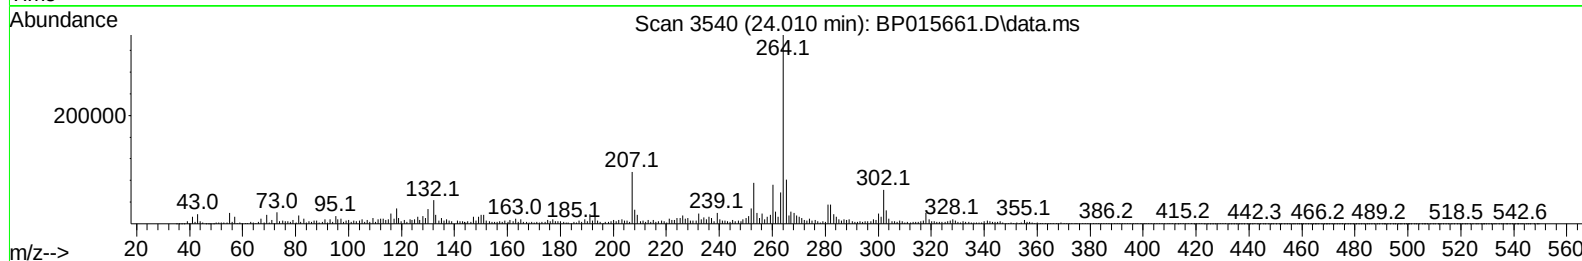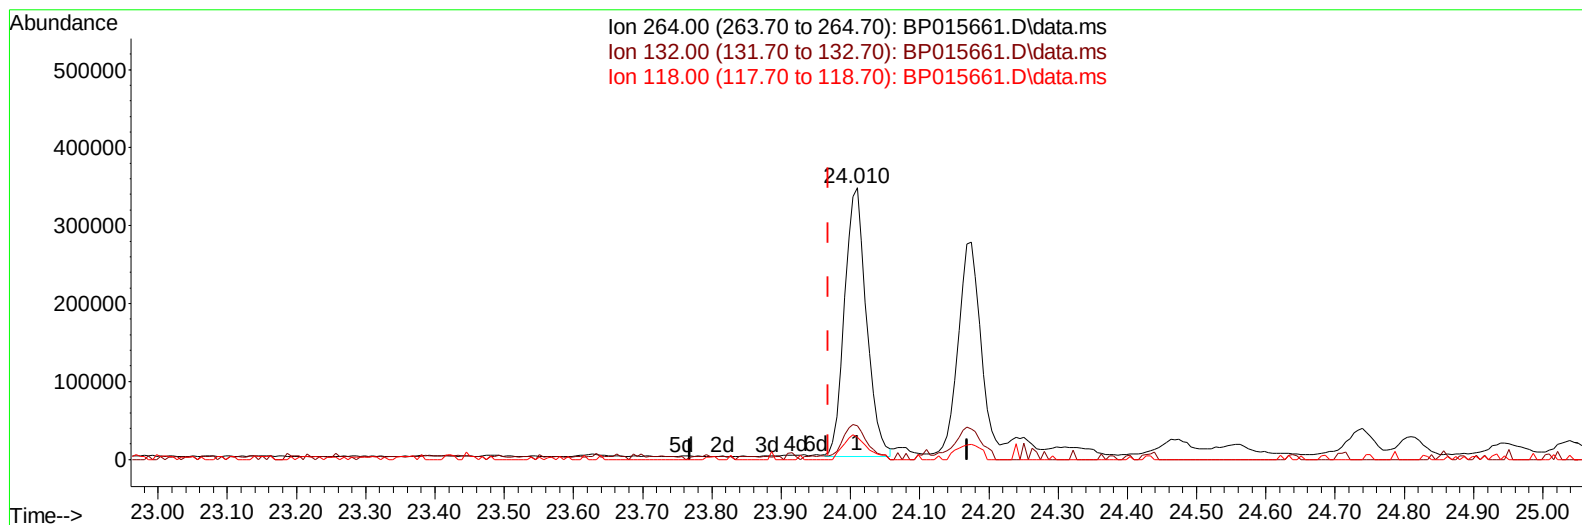

TIC: BP015661.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

24.010min (+ 0.041) 23.86 ng/ul m

response 751049

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	15.00	12.45
118.00	9.10	8.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

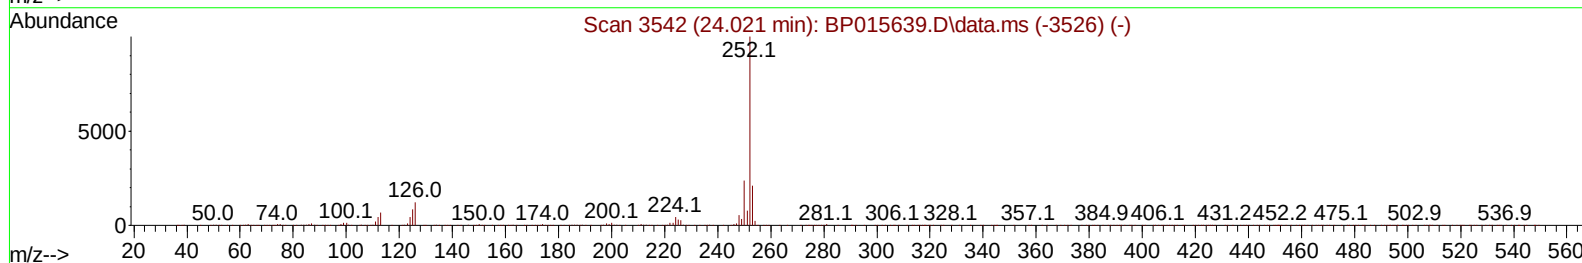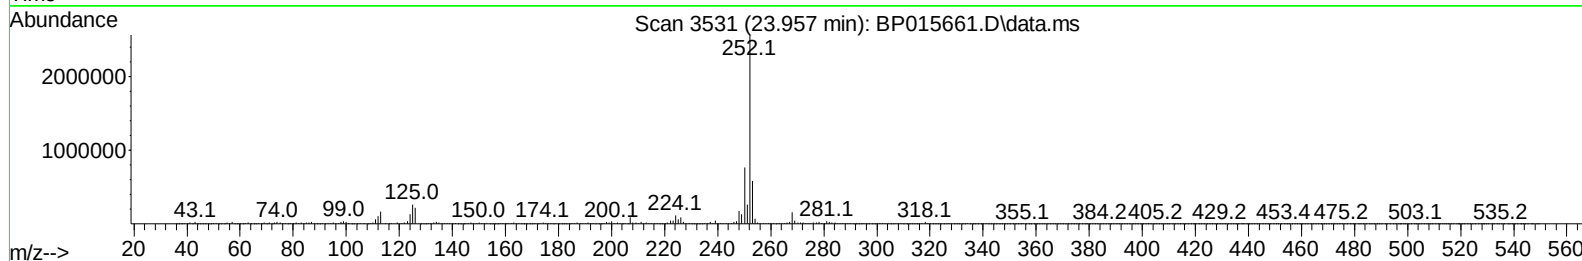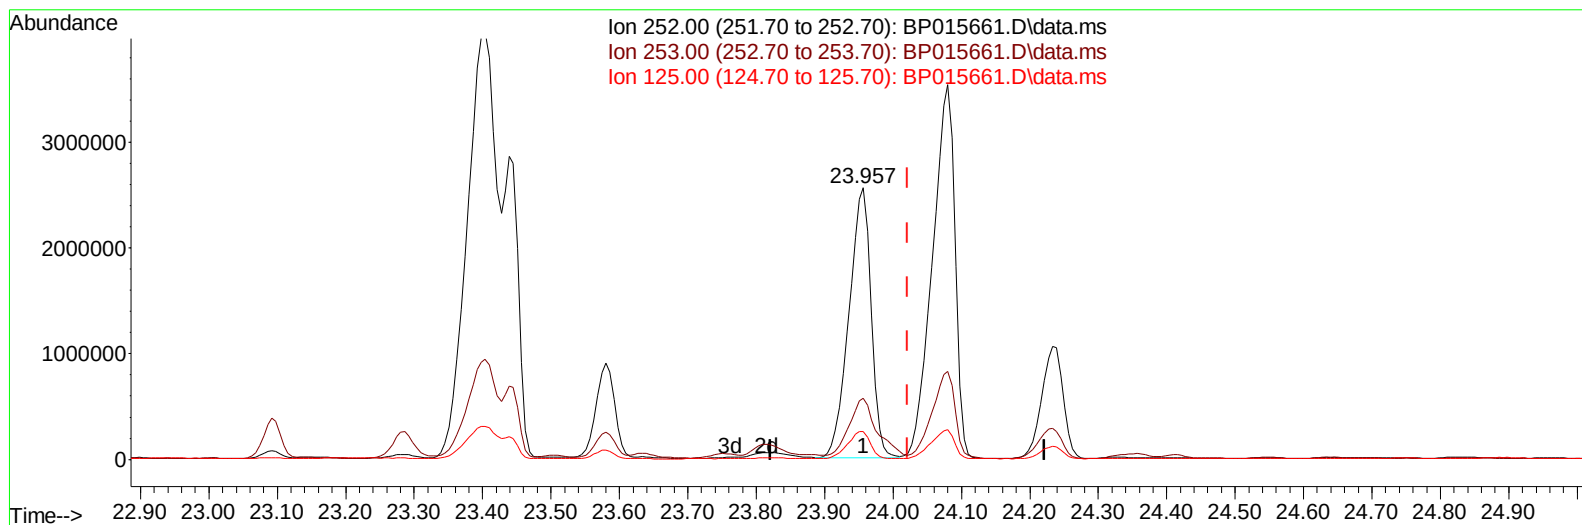

TIC: BP015661.D\data.ms

(93) Benzo(a)pyrene (C)

23.957min (-0.064) 162.64 ng/ul

response 5742121

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.20	22.55
125.00	10.10	10.32
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

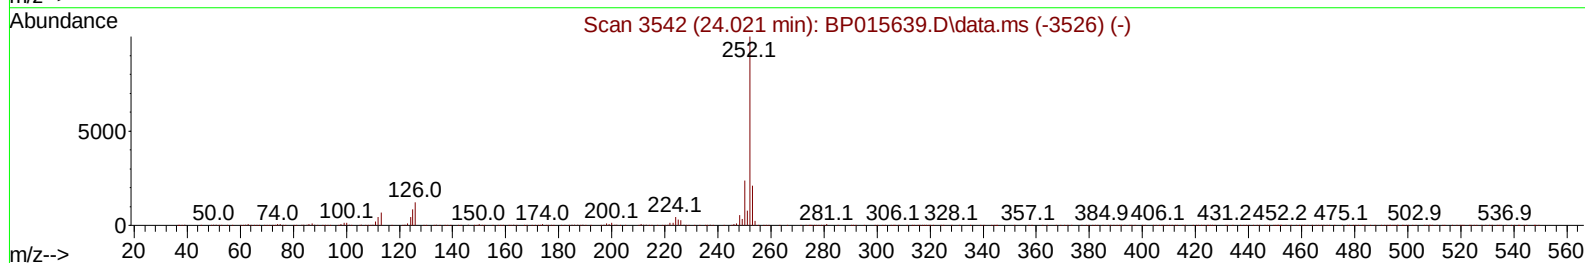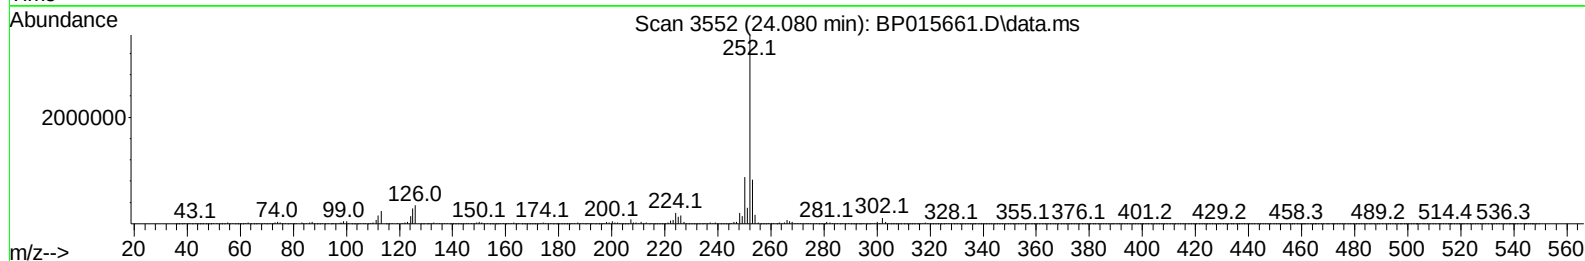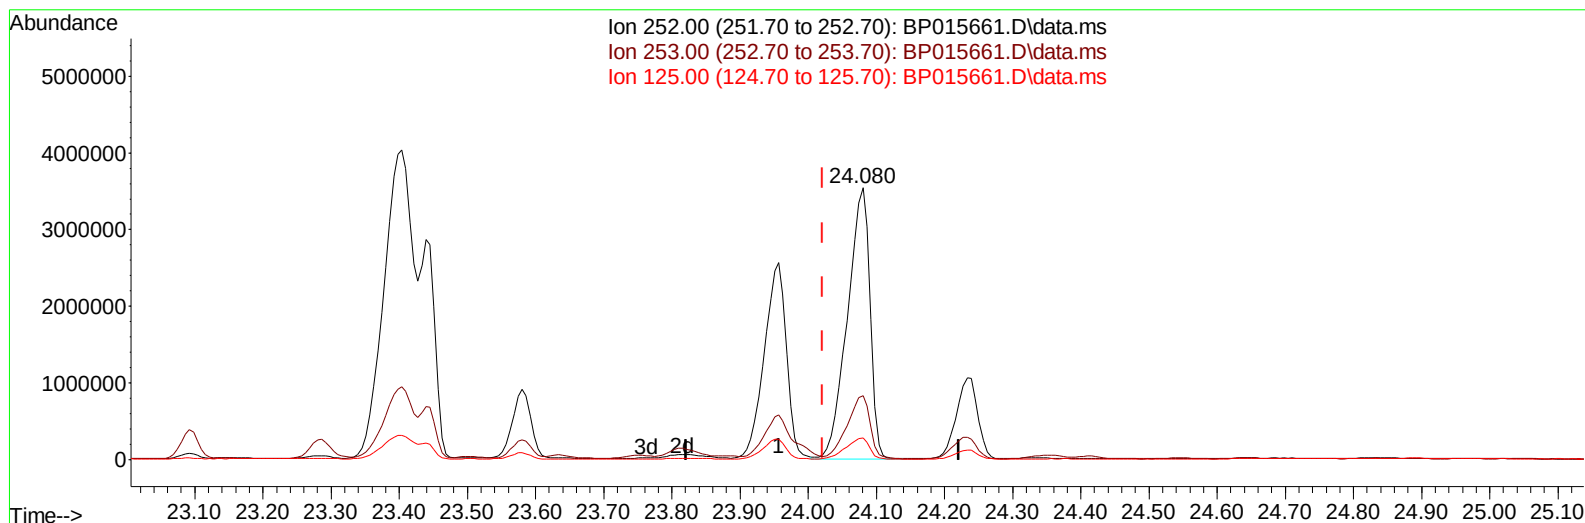

TIC: BP015661.D\data.ms

(93) Benzo(a)pyrene (C)

24.080min (+ 0.059) 230.60 ng/ul m

response 8141495

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.20	23.43
125.00	10.10	8.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015661.D
Acq On : 22 Jun 2023 22:59
Operator : MA/JU
Sample : 03083-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

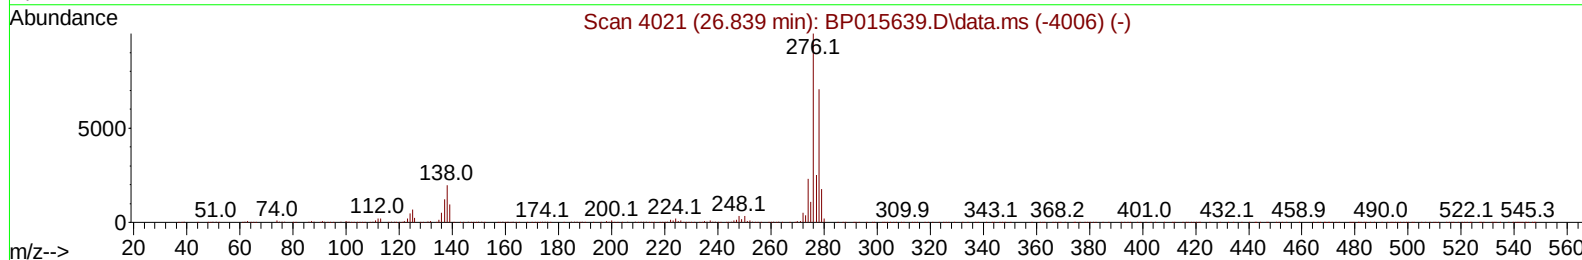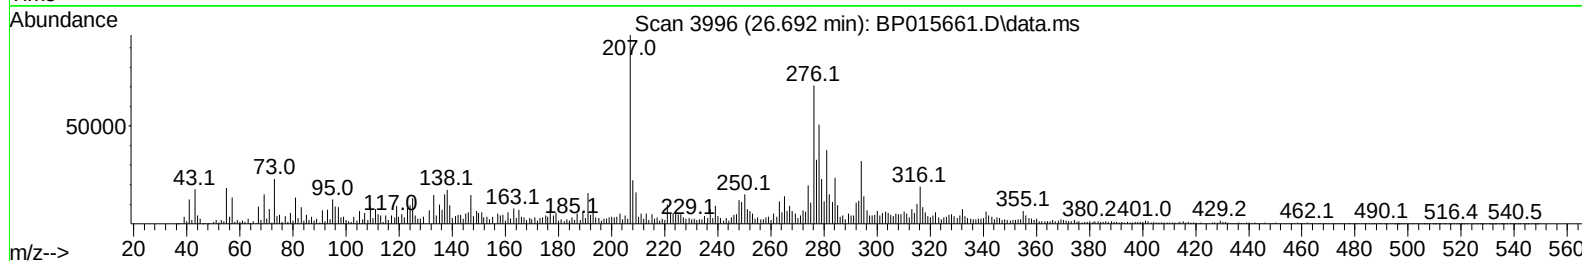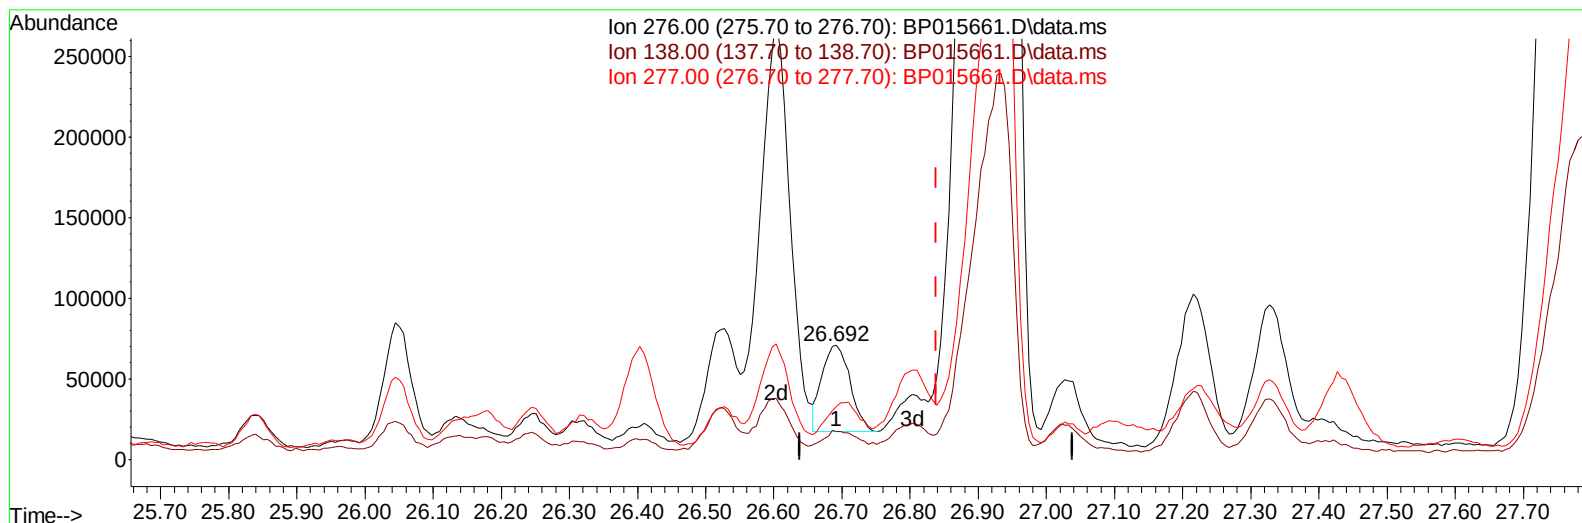

TIC: BP015661.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

26.692min (-0.147) 3.34 ng/u1

response 152684

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	21.60	24.73
277.00	25.20	46.17#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

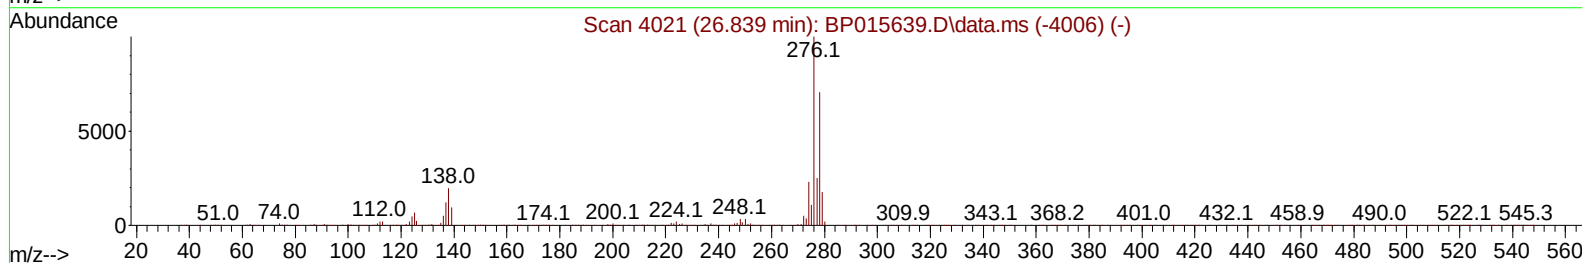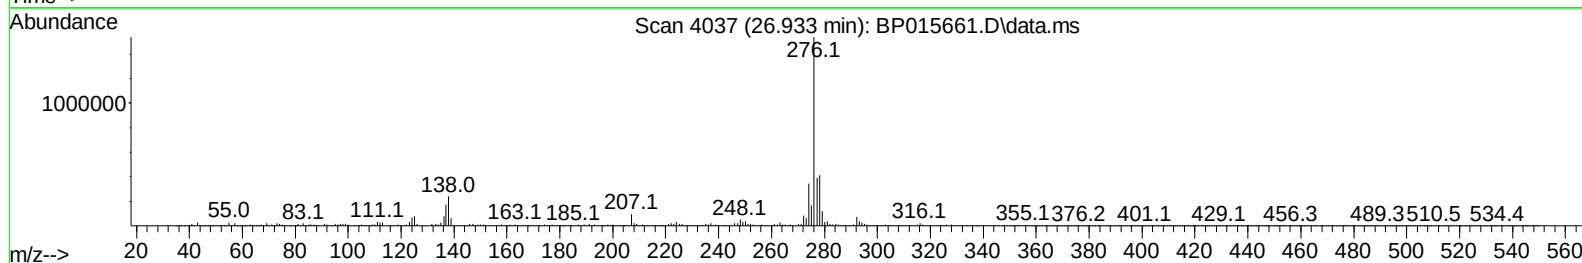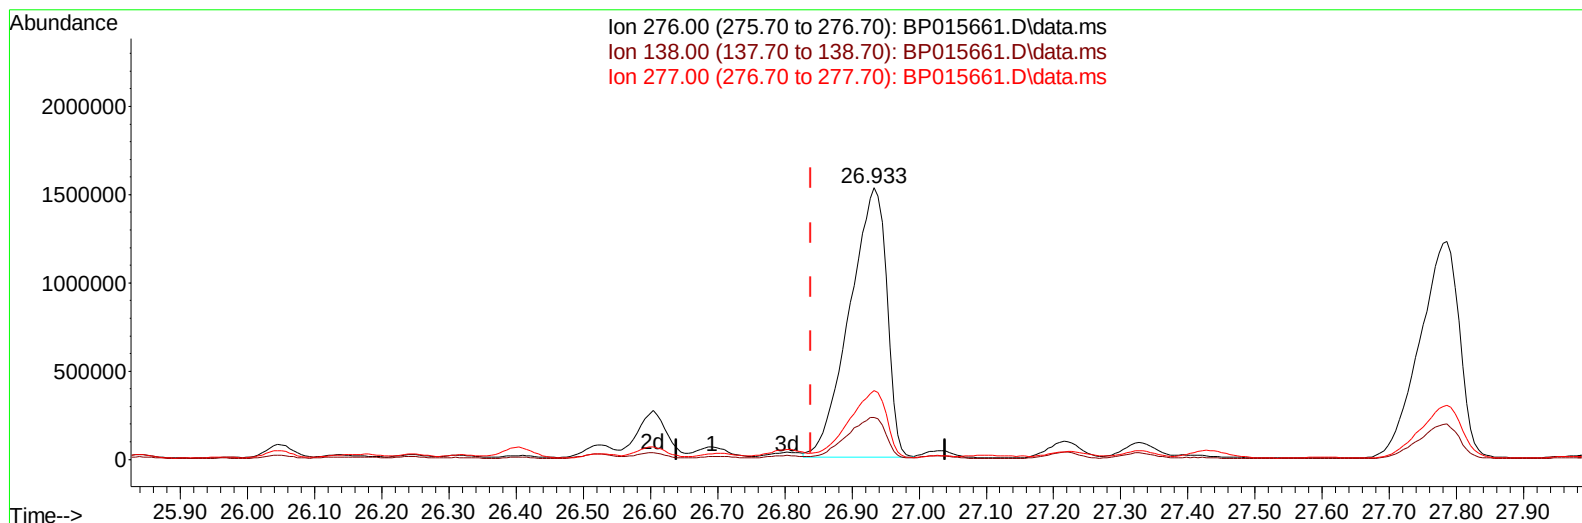

TIC: BP015661.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

26.933min (+ 0.094) 128.40 ng/ul m

response 5866890

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	21.60	15.57#
277.00	25.20	25.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015661.D
Acq On : 22 Jun 2023 22:59
Operator : MA/JU
Sample : 03083-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:05:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

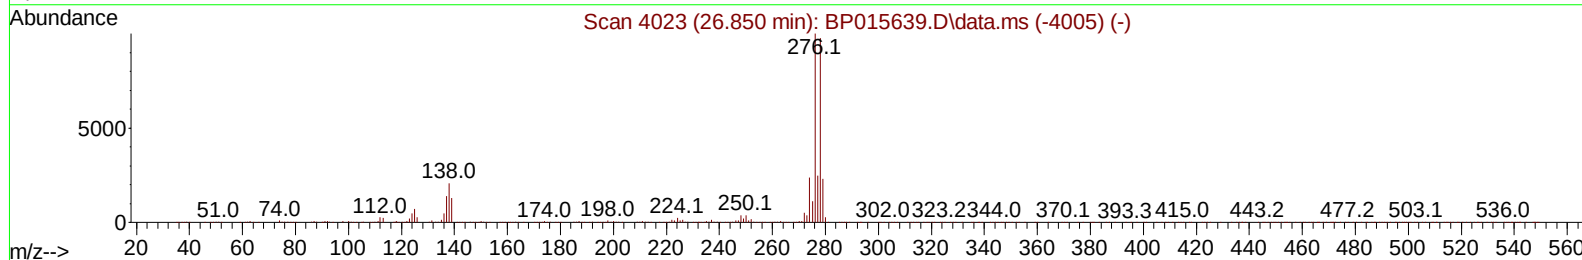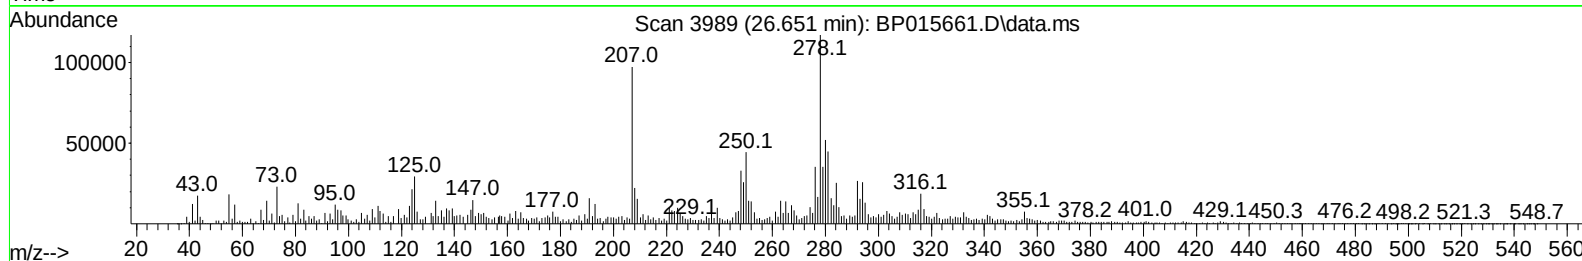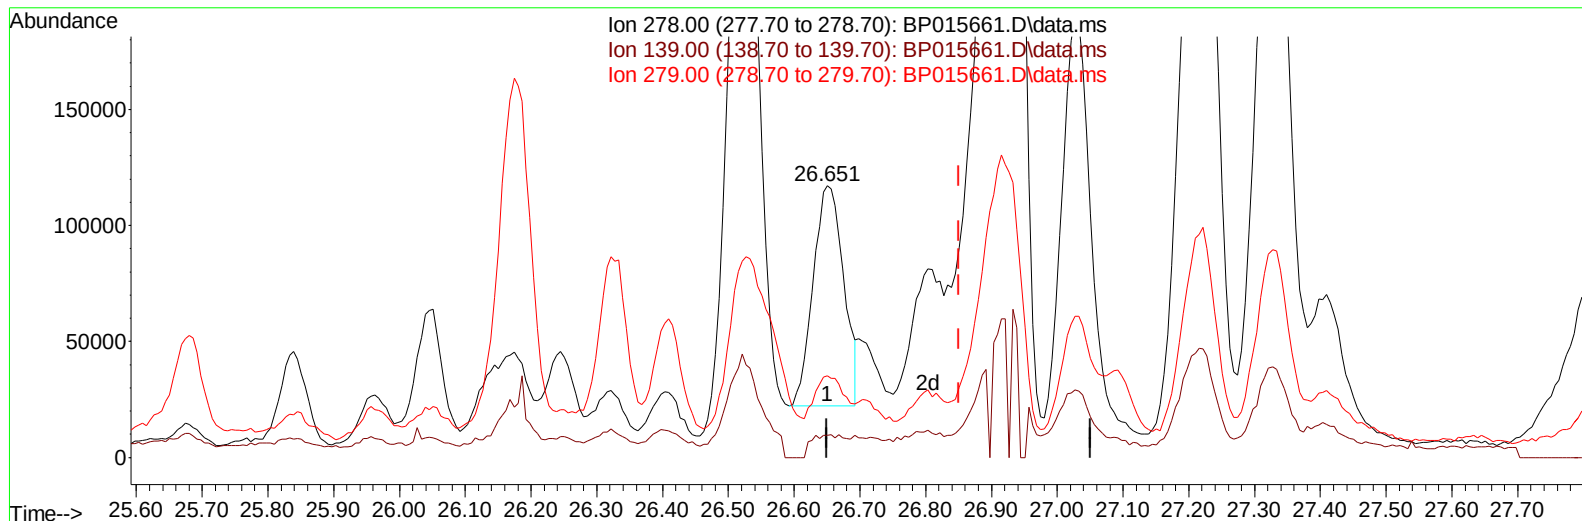

TIC: BP015661.D\data.ms

(95) Dibenzo(a,h)anthracene

26.651min (-0.200) 8.24 ng/u1

response 306562

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	14.20	8.20#
279.00	23.40	30.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:07:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

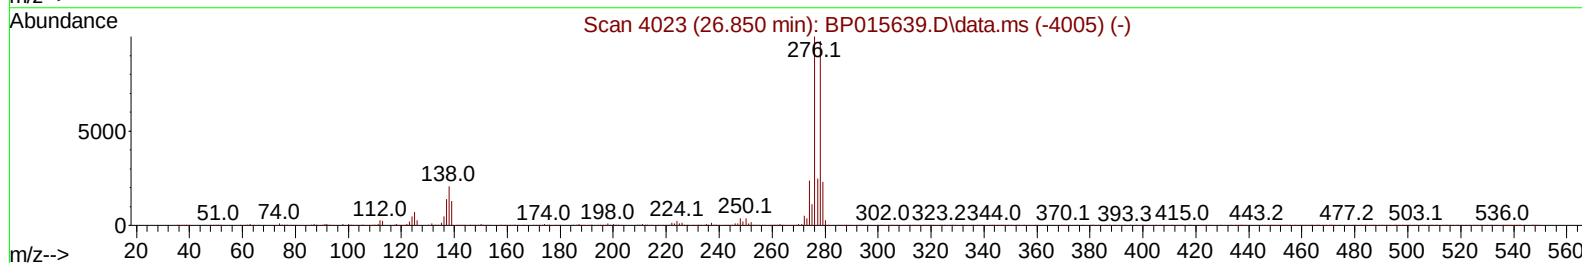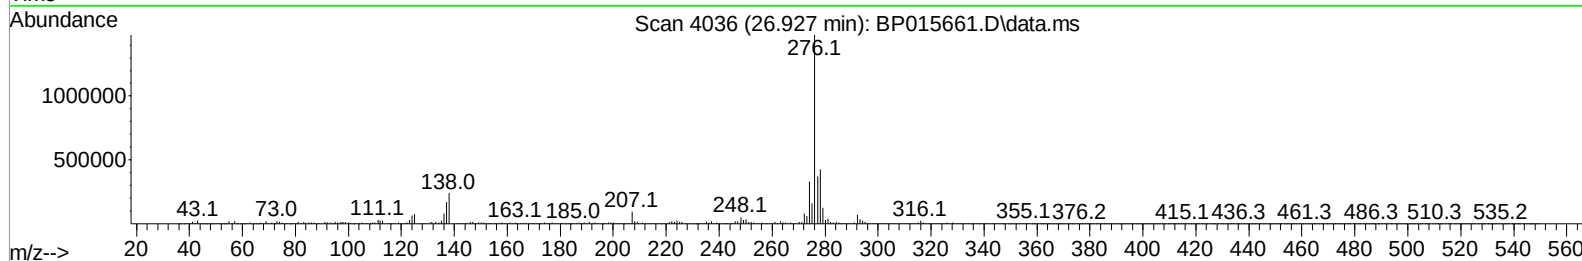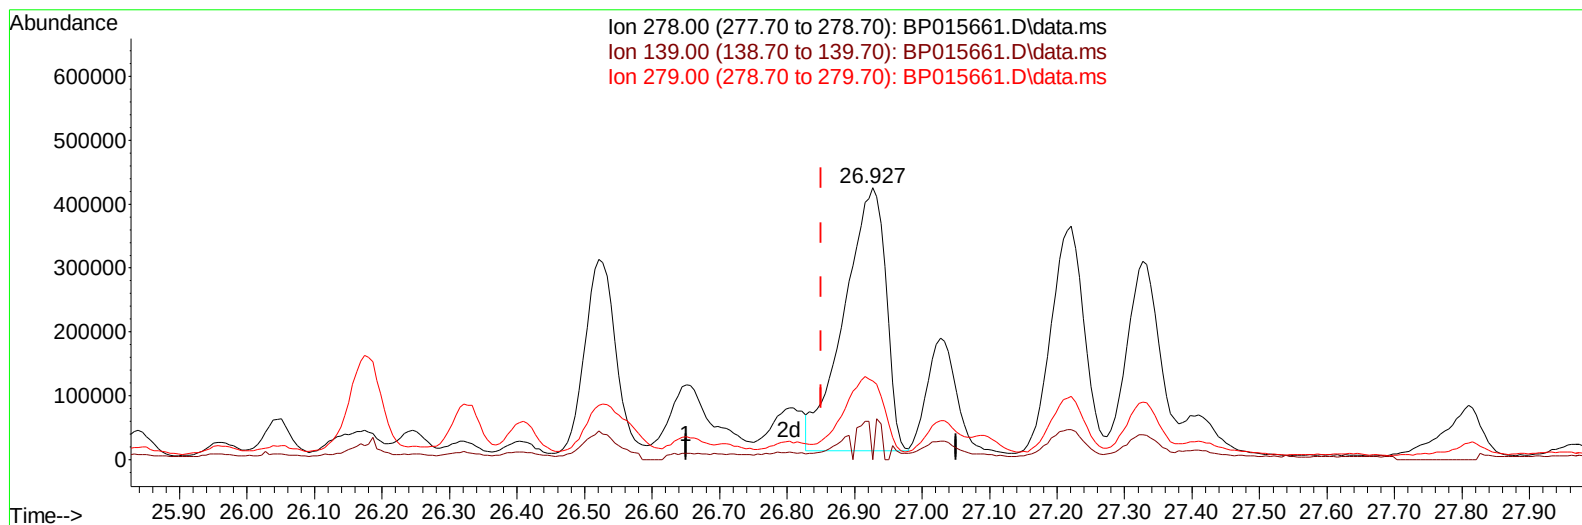

TIC: BP015661.D\data.ms

(95) Dibenzo(a,h)anthracene

26.927min (+ 0.077) 47.56 ng/ul m

response 1770608

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	14.20	0.00#
279.00	23.40	28.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015661.D
Acq On : 22 Jun 2023 22:59
Operator : MA/JU
Sample : 03083-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:07:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

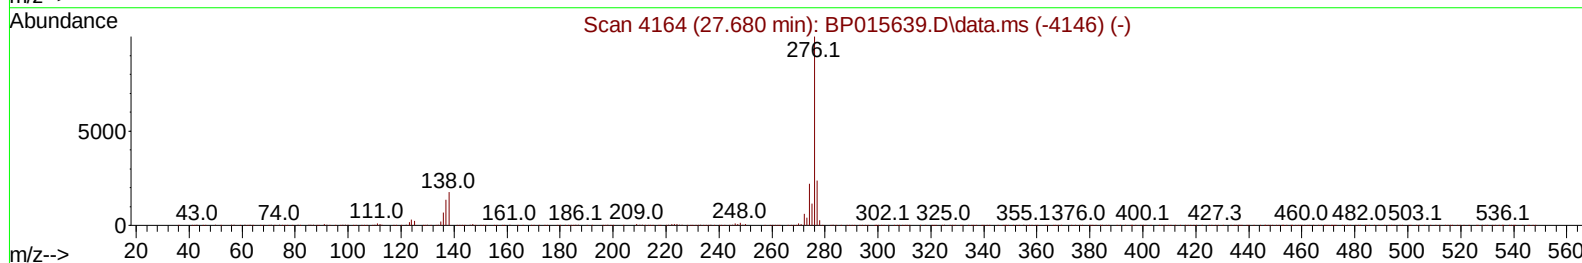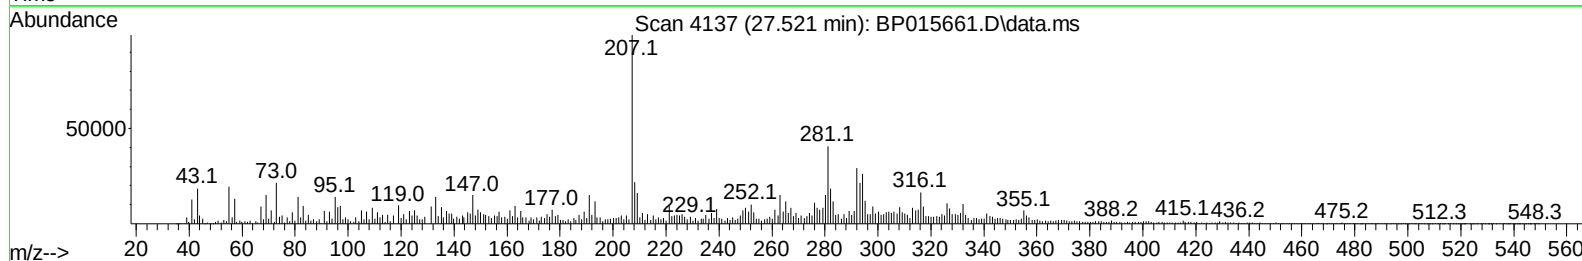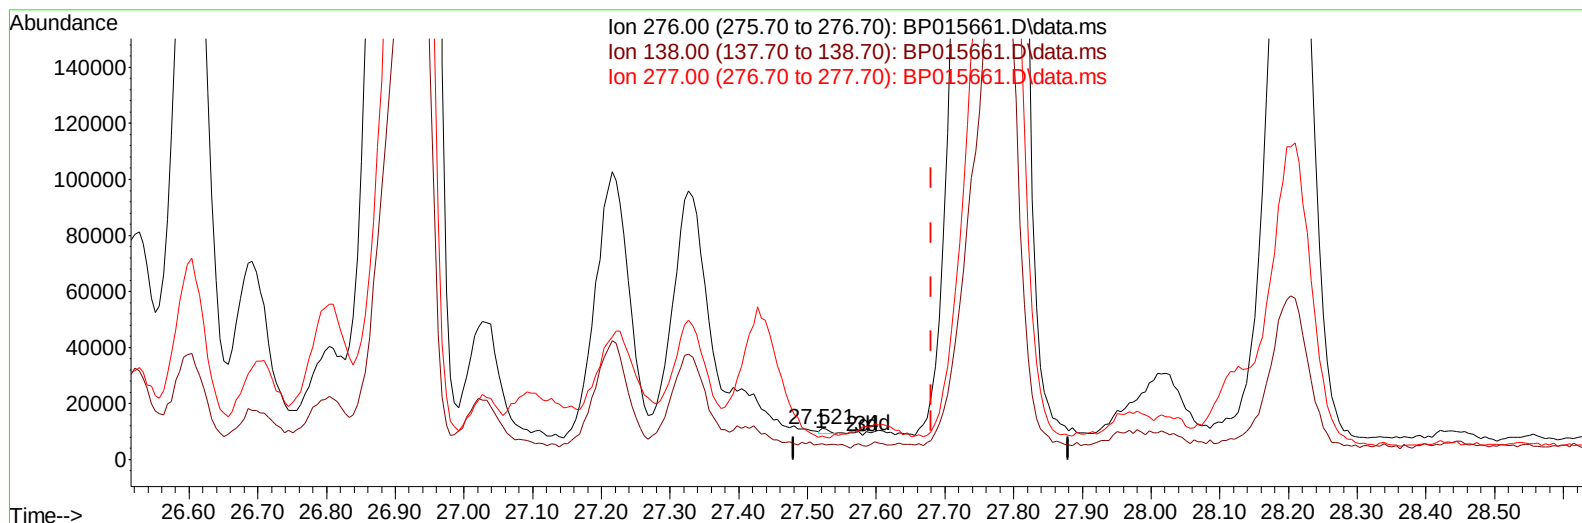

TIC: BP015661.D\data.ms

(96) Benzo(g,h,i)perylene

27.521min (-0.159) 0.04 ng/u1

response 1445

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	19.50	49.82#
277.00	23.80	74.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:07:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

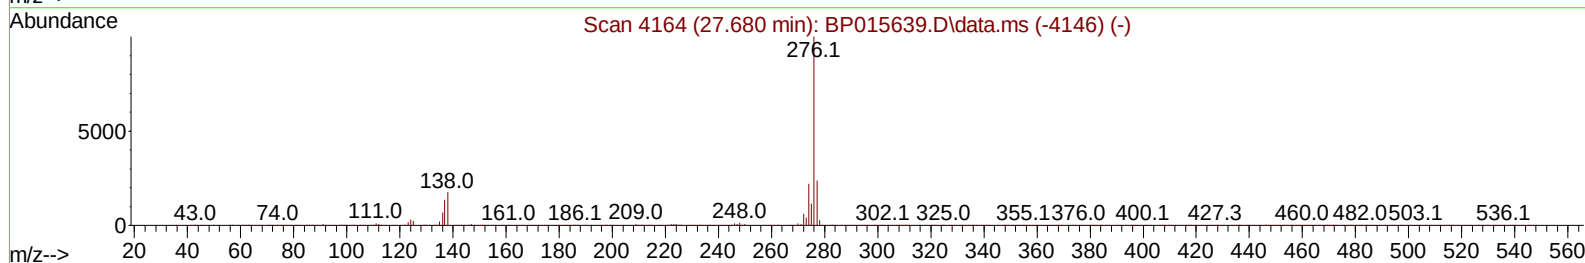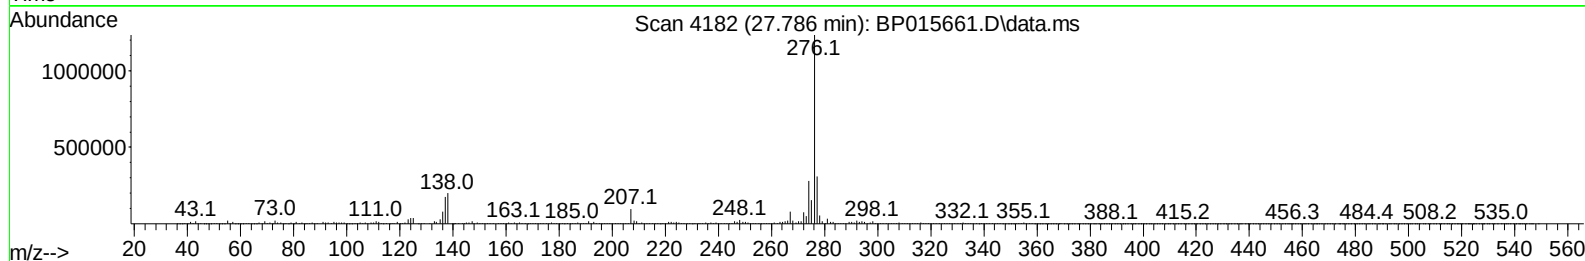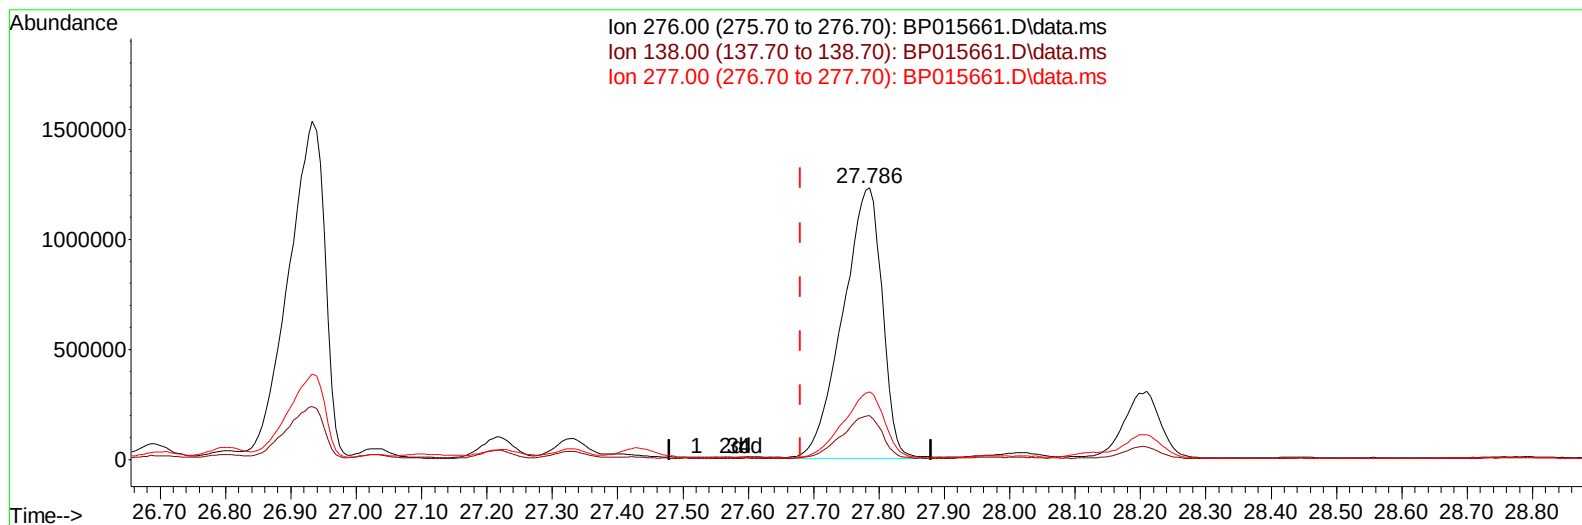

TIC: BP015661.D\data.ms

(96) Benzo(g,h,i)perylene

27.786min (+ 0.106) 135.26 ng/ul m

response 5093047

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	19.50	16.23
277.00	23.80	24.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015661.D
 Acq On : 22 Jun 2023 22:59
 Operator : MA/JU
 Sample : 03083-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2

Manual IntegrationsAPPROVED

Quant Time: Jun 23 00:07:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :mohammad ahmed 06/23/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.081	152		104713	20.000	ng/ul	0.00
20) Naphthalene-d8	10.910	136		365223	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.734	164		210031	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188		465708	20.000	ng/ul	0.00
79) Chrysene-d12	21.604	240		454548	20.000	ng/ul	0.02
88) Perylene-d12	24.174	264		627346m	20.000	ng/ul	0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.399	96		7825	2.767	ng/uL	0.00
4) Pyridine-d5	3.870	84		15970	2.174	ng/ul	0.03
7) Phenol-d5	7.252	99		159034	16.486	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.405	67		95744	16.619	ng/ul	0.00
11) 2-Chlorophenol-d4	7.611	132		137599	19.673	ng/ul	0.00
15) 4-Methylphenol-d8	8.810	113		122046	15.415	ng/ul	0.00
21) Nitrobenzene-d5	9.263	128		60651	21.152	ng/ul	0.00
24) 2-Nitrophenol-d4	9.993	143		70400	21.499	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.546	165		120119	20.110	ng/ul	0.01
31) 4-Chloroaniline-d4	11.069	131		105558	12.312	ng/ul	0.02
46) Dimethylphthalate-d6	14.134	166		401171	24.222	ng/ul	0.00
49) Acenaphthylene-d8	14.428	160		458071	25.294	ng/ul	0.00
54) 4-Nitrophenol-d4	14.975	143		32080	10.816	ng/ul	0.02
60) Fluorene-d10	15.728	176		346625	24.818	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200		28339	9.605	ng/ul	0.02
73) Anthracene-d10	17.598	188		558612	26.363	ng/ul	0.00
81) Pyrene-d10	19.828	212		651118	26.764	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.010	264		751049m	23.860	ng/ul	0.04
Target Compounds							
						Qvalue	
30) Naphthalene	10.963	128		153416	7.752	ng/ul	99
36) 2-Methylnaphthalene	12.569	142		57227	4.113	ng/ul	97
37) 1-Methylnaphthalene	12.781	142		61843	4.415	ng/ul	98
50) Acenaphthylene	14.457	152		144268	7.194	ng/ul	97
52) Acenaphthene	14.798	153		396000	28.565	ng/ul	99
61) Fluorene	15.781	166		381992	23.849	ng/ul	98
72) Phenanthrene	17.551	178		7459224	298.467	ng/ul	99
74) Anthracene	17.634	178		1963311	77.425	ng/ul	100
80) Fluoranthene	19.516	202		15076635	508.761	ng/ul	98
82) Pyrene	19.875	202		13172675	429.655	ng/ul#	94
85) Benzo(a)anthracene	21.586	228		9080023	285.747	ng/ul	97
87) Chrysene	21.645	228		8147009m	271.245	ng/ul	
90) Benzo(b)fluoranthene	23.404	252		12149756m	300.029	ng/ul	
91) Benzo(k)fluoranthene	23.439	252		4064926m	103.843	ng/ul	
93) Benzo(a)pyrene	24.080	252		8141495m	230.598	ng/ul	
94) Indeno(1,2,3-cd)pyrene	26.933	276		5866890m	128.401	ng/ul	
95) Dibenzo(a,h)anthracene	26.927	278		1770608m	47.565	ng/ul	
96) Benzo(g,h,i)perylene	27.786	276		5093047m	135.256	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015661.D
Acq On : 22 Jun 2023 22:59
Operator : MA/JU
Sample : 03083-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :mohammad ahmed 06/23/2023

Quant Time: Jun 23 00:07:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

