

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015640.D
 Acq On : 22 Jun 2023 11:10
 Operator : MA/JU
 Sample : PB153402BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK402

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	42	rVB	38290	51850	1.44%	0.144%
2	3.840	108	111	123	rBV	429040	672156	18.70%	1.866%
3	4.164	164	166	170	rBV3	4854	7854	0.22%	0.022%
4	4.258	179	182	185	rBV5	3195	5058	0.14%	0.014%
5	7.175	675	678	681	rBV5	2495	4032	0.11%	0.011%
6	7.240	681	689	708	rVV	505089	938708	26.12%	2.606%
7	7.405	711	717	728	rVV	436102	708564	19.72%	1.967%
8	7.605	744	751	767	rBV	570979	992895	27.63%	2.757%
9	8.081	825	832	842	rBV	357708	615242	17.12%	1.708%
10	8.799	948	954	972	rBV	656062	1239142	34.48%	3.440%
11	9.258	1023	1032	1051	rBV	577617	1046591	29.12%	2.906%
12	9.987	1149	1156	1175	rBV	492607	924321	25.72%	2.566%
13	10.534	1242	1249	1270	rBV	583420	1229761	34.22%	3.414%
14	10.910	1305	1313	1325	rBV	516701	918618	25.56%	2.551%
15	11.057	1330	1338	1363	rBV	561457	1319007	36.70%	3.662%
16	12.434	1568	1572	1576	rVB7	2745	3949	0.11%	0.011%
17	12.522	1580	1587	1593	rVV7	8061	18299	0.51%	0.051%
18	13.610	1766	1772	1778	rBV4	12937	21826	0.61%	0.061%
19	13.963	1827	1832	1835	rBV7	2242	4313	0.12%	0.012%
20	14.134	1854	1861	1877	rBV	1486671	2174557	60.51%	6.038%
21	14.428	1902	1911	1929	rBV	1538557	2405845	66.94%	6.680%
22	14.540	1929	1930	1934	rVB3	4614	4827	0.13%	0.013%
23	14.728	1955	1962	1974	rBV	861908	1306303	36.35%	3.627%
24	14.951	1993	2000	2021	rBV	362545	954665	26.56%	2.651%
25	15.728	2125	2132	2147	rBV	1872595	2910092	80.97%	8.080%
26	15.863	2149	2155	2169	rBV	436962	867937	24.15%	2.410%
27	16.928	2332	2336	2340	rBV7	3779	6136	0.17%	0.017%
28	17.281	2394	2396	2401	rVB6	4311	4356	0.12%	0.012%
29	17.398	2412	2416	2418	rBV5	2740	3997	0.11%	0.011%
30	17.492	2425	2432	2442	rBV	1117662	1607471	44.73%	4.463%
31	17.592	2442	2449	2467	rVV	2113128	3174681	88.33%	8.814%
32	18.104	2534	2536	2539	rBV4	3836	3655	0.10%	0.010%
33	18.369	2577	2581	2588	rBV6	25514	71627	1.99%	0.199%
34	19.398	2752	2756	2761	rBV	28541	37328	1.04%	0.104%
35	19.469	2765	2768	2776	rVB3	21924	36376	1.01%	0.101%
36	19.816	2822	2827	2842	rBV	2506075	3593941	100.00%	9.979%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015640.D
Acq On : 22 Jun 2023 11:10
Operator : MA/JU
Sample : PB153402BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK402

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	21.339	3083	3086	3094	rVB2	78799	127607	3.55%	0.354%
38	21.580	3122	3127	3137	rBV	1054706	1579185	43.94%	4.385%
39	23.969	3526	3533	3547	rVB	1470990	3112863	86.61%	8.643%
40	24.139	3556	3562	3572	rVB	586914	1311088	36.48%	3.640%




Sum of corrected areas: 36016723

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015640.D
Acq On : 22 Jun 2023 11:10
Operator : MA/JU
Sample : PB153402BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

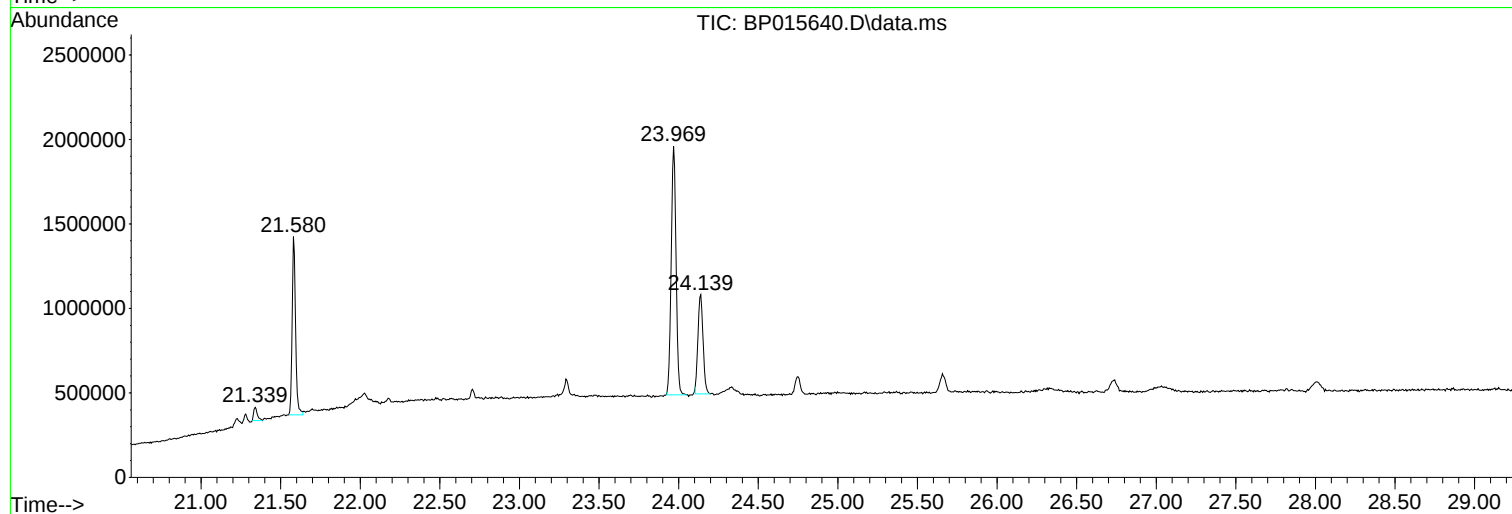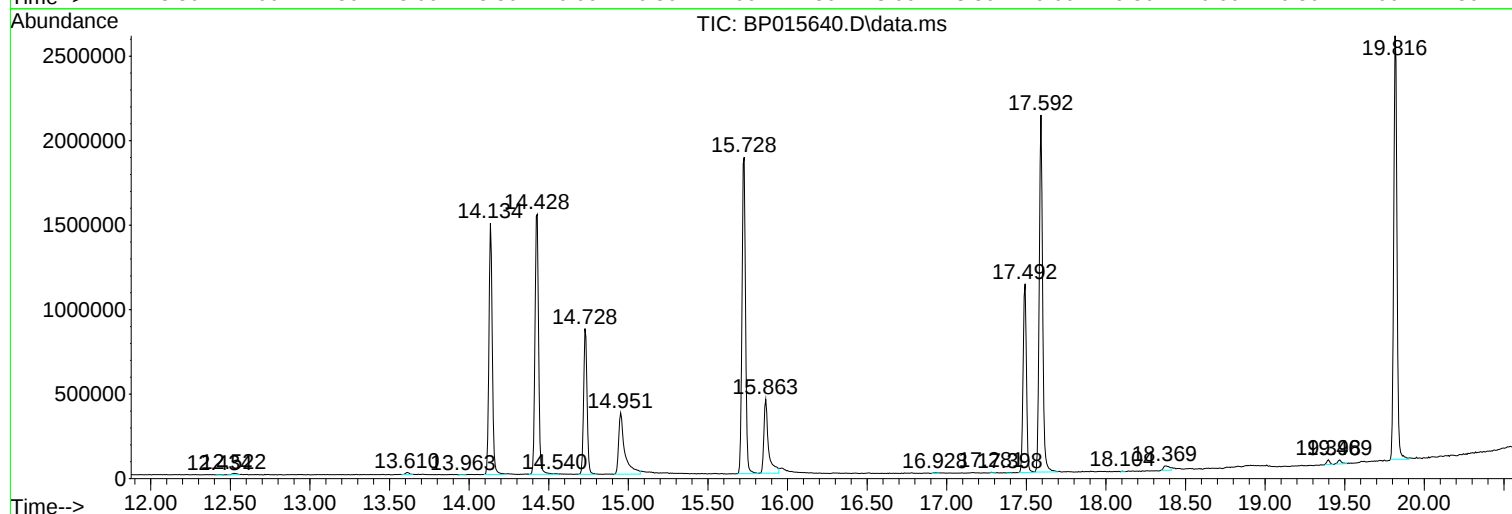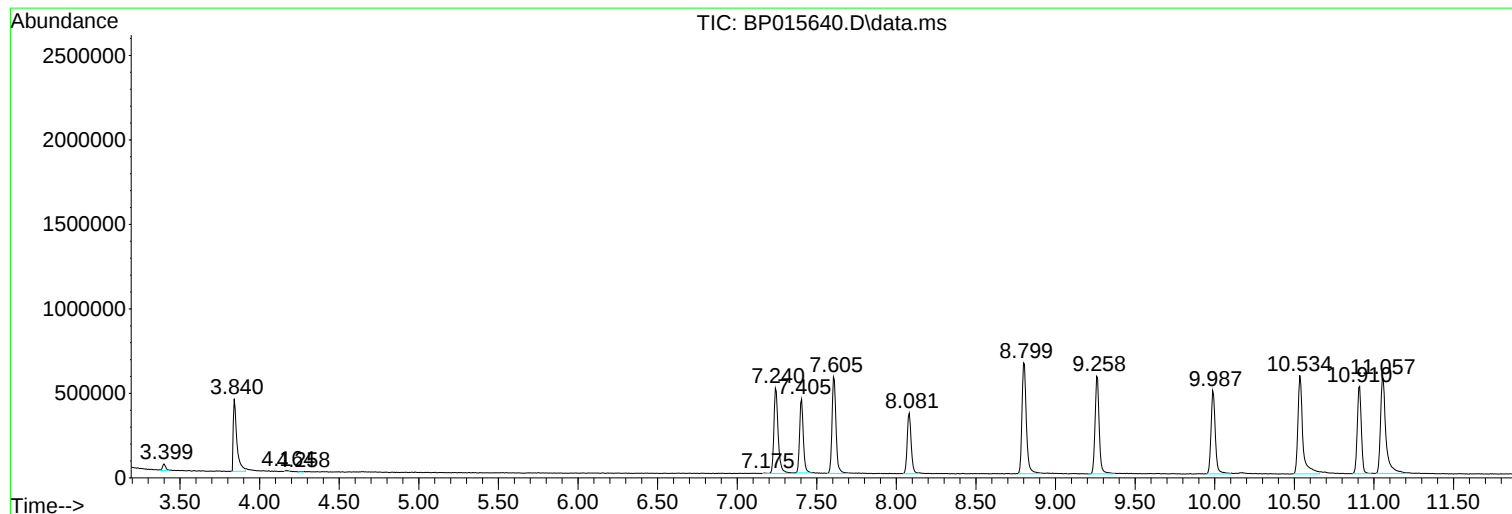

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015640.D
Acq On : 22 Jun 2023 11:10
Operator : MA/JU
Sample : PB153402BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015640.D
Acq On : 22 Jun 2023 11:10
Operator : MA/JU
Sample : PB153402BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------