

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
 Data File : BP015655.D
 Acq On : 22 Jun 2023 19:37
 Operator : MA/JU
 Sample : PB153402BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK402

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	42	rVB	39787	52136	1.75%	0.148%
2	3.840	108	111	129	rBV	464833	738792	24.75%	2.096%
3	4.170	165	167	170	rVB2	7795	7506	0.25%	0.021%
4	7.240	683	689	705	rBV	588629	1080100	36.19%	3.064%
5	7.399	710	716	729	rVV	485206	812765	27.23%	2.306%
6	7.605	744	751	766	rBV	663199	1121787	37.59%	3.182%
7	7.834	788	790	794	rBV5	2405	3535	0.12%	0.010%
8	8.081	824	832	844	rBV	412393	701647	23.51%	1.990%
9	8.540	906	910	913	rBV6	1764	3006	0.10%	0.009%
10	8.799	947	954	973	rBV	775704	1446769	48.48%	4.104%
11	9.257	1025	1032	1049	rBV	654915	1188127	39.81%	3.370%
12	9.875	1134	1137	1143	rVB7	1840	3622	0.12%	0.010%
13	9.987	1149	1156	1177	rBV	572721	1051591	35.24%	2.983%
14	10.181	1186	1189	1195	rBV8	3085	6491	0.22%	0.018%
15	10.534	1241	1249	1273	rBV	705507	1467309	49.16%	4.162%
16	10.904	1305	1312	1325	rBV	604744	1048929	35.15%	2.976%
17	11.052	1329	1337	1368	rBV	635081	1514518	50.75%	4.296%
18	12.528	1580	1588	1597	rBV3	8787	23525	0.79%	0.067%
19	13.610	1764	1772	1778	rVB2	13846	24041	0.81%	0.068%
20	13.710	1786	1789	1796	rVB8	2035	3360	0.11%	0.010%
21	14.134	1853	1861	1878	rBV	1467076	2255338	75.57%	6.398%
22	14.245	1878	1880	1884	rVB5	3647	4597	0.15%	0.013%
23	14.422	1902	1910	1925	rBV2	1656448	2582342	86.53%	7.325%
24	14.728	1956	1962	1972	rBV	920905	1391523	46.63%	3.947%
25	14.957	1994	2001	2022	rBV	260431	792878	26.57%	2.249%
26	15.722	2125	2131	2147	rBV	1969702	2984489	100.00%	8.466%
27	15.863	2149	2155	2170	rVV	395307	742292	24.87%	2.106%
28	15.969	2170	2173	2186	rVB7	17515	40977	1.37%	0.116%
29	17.169	2372	2377	2380	rBV7	3356	5624	0.19%	0.016%
30	17.492	2425	2432	2442	rBV	980862	1466901	49.15%	4.161%
31	17.592	2442	2449	2468	rVV	1873490	2879374	96.48%	8.168%
32	19.463	2765	2767	2773	rVB	15284	20416	0.68%	0.058%
33	19.816	2822	2827	2838	rBV	1891978	2654266	88.94%	7.530%
34	21.580	3123	3127	3135	rBV	715655	1086108	36.39%	3.081%
35	23.968	3526	3533	3543	rVB2	1365779	2795509	93.67%	7.930%
36	24.139	3556	3562	3572	rVB	571225	1249261	41.86%	3.544%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015655.D
Acq On : 22 Jun 2023 19:37
Operator : MA/JU
Sample : PB153402BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK402

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 35251451

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015655.D
Acq On : 22 Jun 2023 19:37
Operator : MA/JU
Sample : PB153402BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

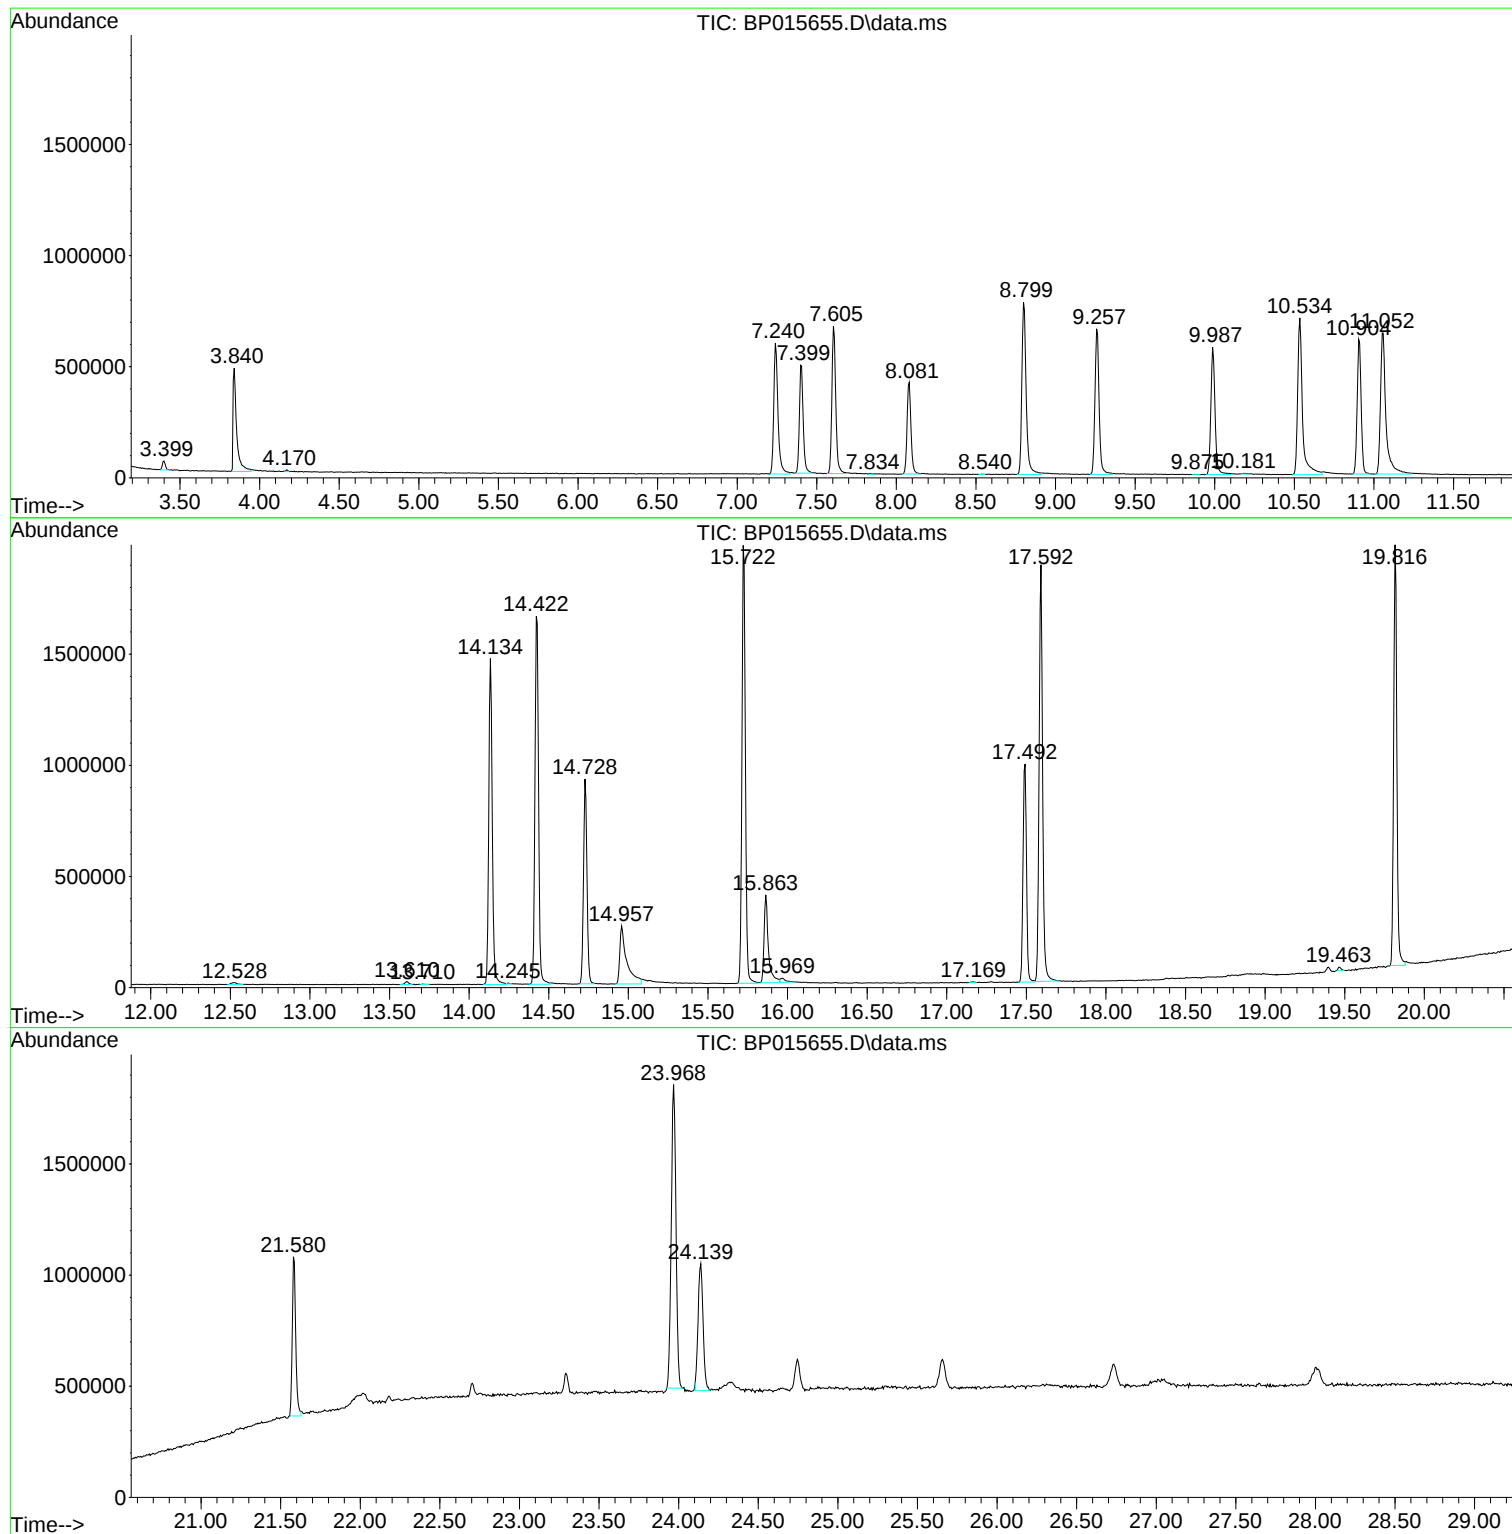

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015655.D
Acq On : 22 Jun 2023 19:37
Operator : MA/JU
Sample : PB153402BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062223\
Data File : BP015655.D
Acq On : 22 Jun 2023 19:37
Operator : MA/JU
Sample : PB153402BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------