




Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062323\  
 Data File : BP015670.D  
 Acq On : 23 Jun 2023 14:23  
 Operator : MA/JU  
 Sample : 03084-19  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCFN6

Manual IntegrationsAPPROVED

Quant Time: Jun 23 22:34:56 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jun 22 22:01:49 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023  
 Supervised By :mohammad ahmed 06/27/2023

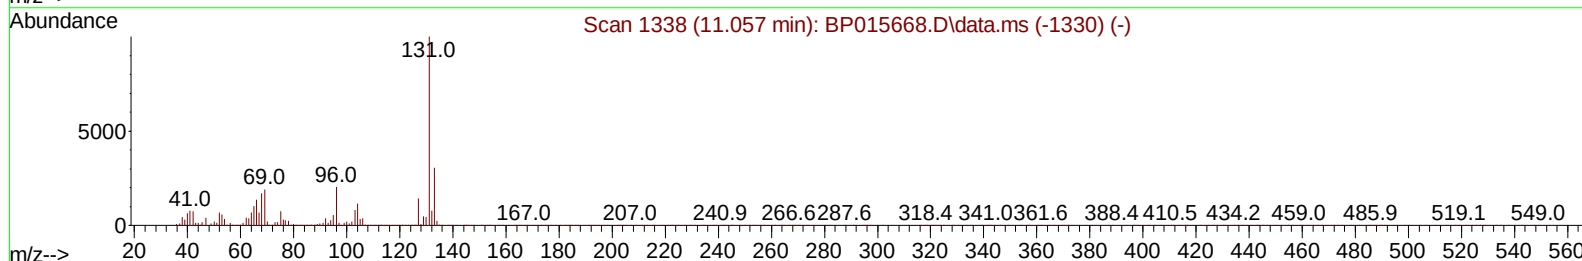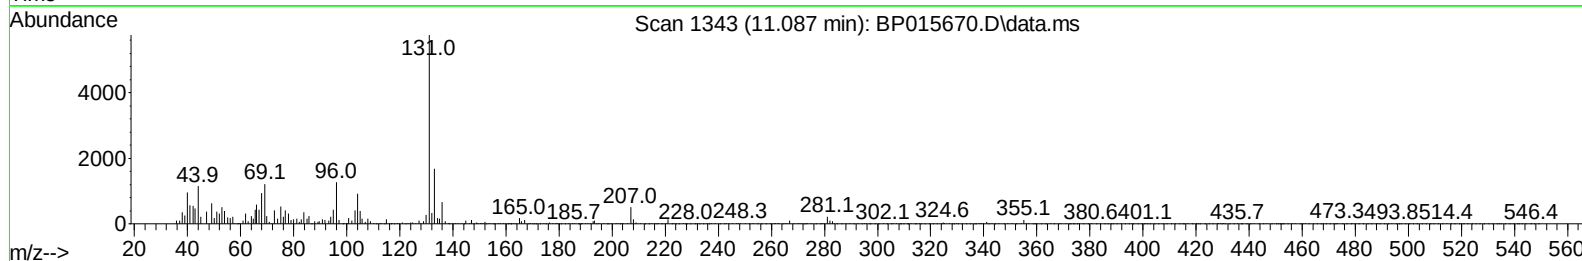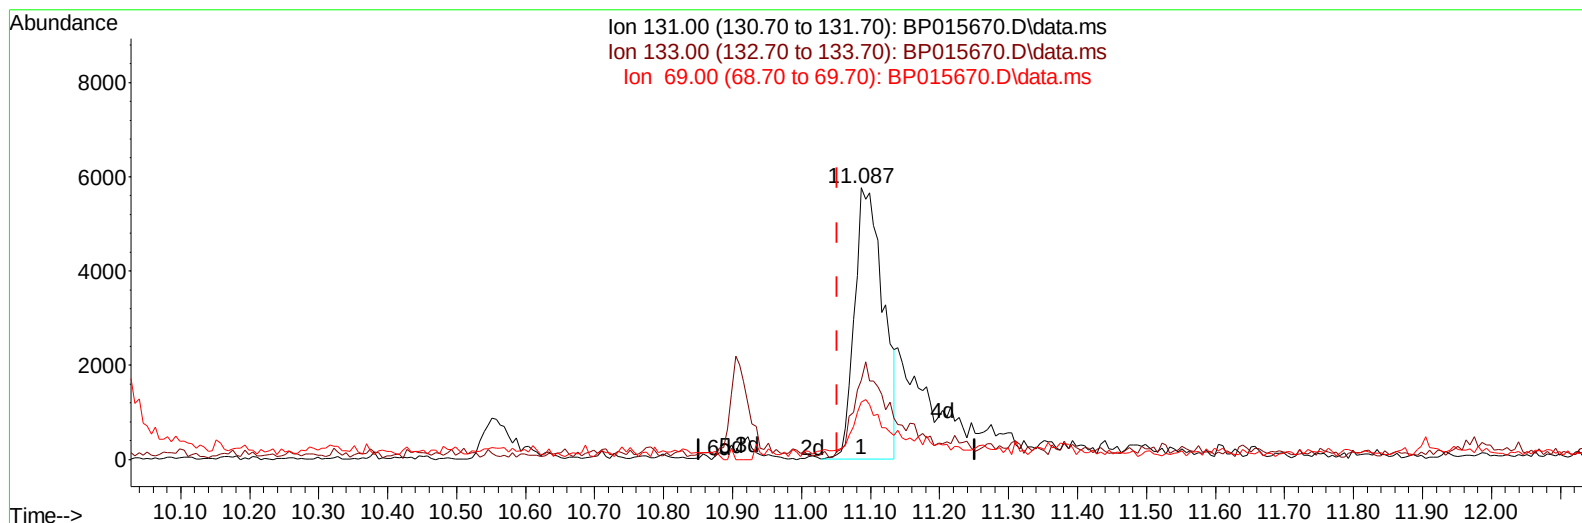

TIC: BP015670.D\data.ms

**(31) 4-Chloroaniline-d4 (S)**

**11.087min (+ 0.035) 1.42 ng/uI**

**response 16613**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 131.00 | 100.00 | 100.00 |
| 133.00 | 32.20  | 29.20  |
| 69.00  | 18.30  | 21.08  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062323\  
Data File : BP015670.D  
Acq On : 23 Jun 2023 14:23  
Operator : MA/JU  
Sample : 03084-19  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DCFN6

Manual IntegrationsAPPROVED

Quant Time: Jun 23 22:34:56 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Jun 22 22:01:49 2023  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023  
Supervised By :mohammad ahmed 06/27/2023

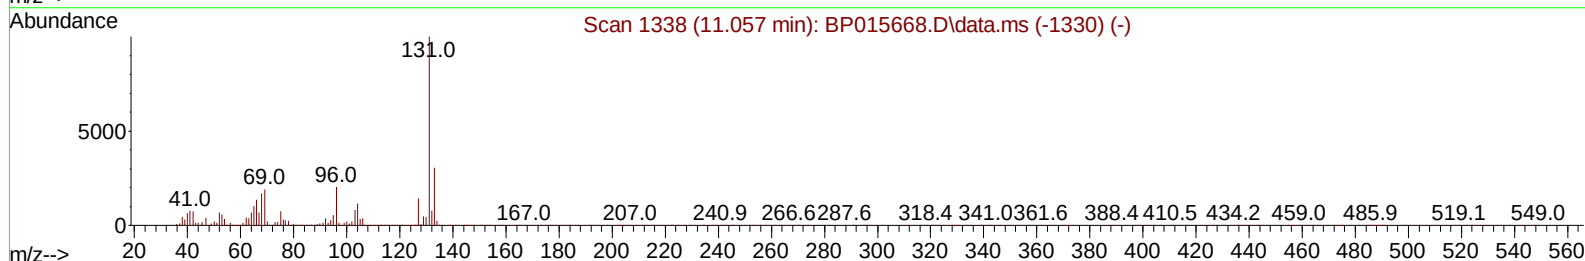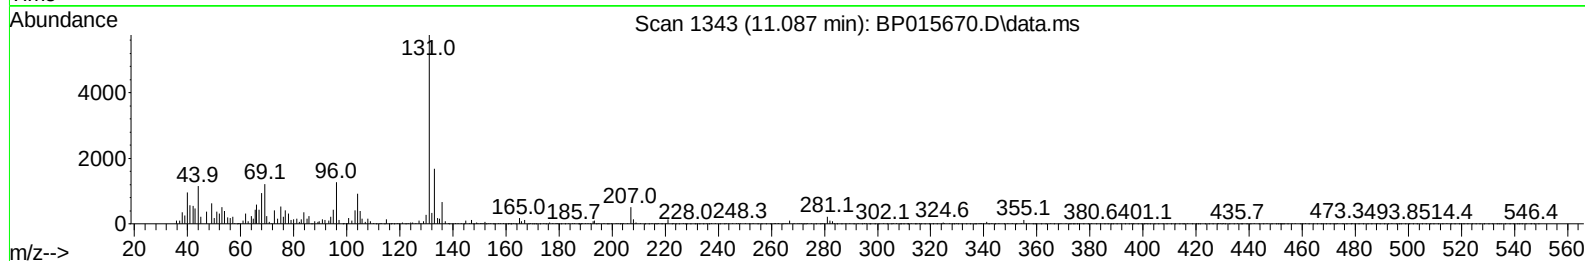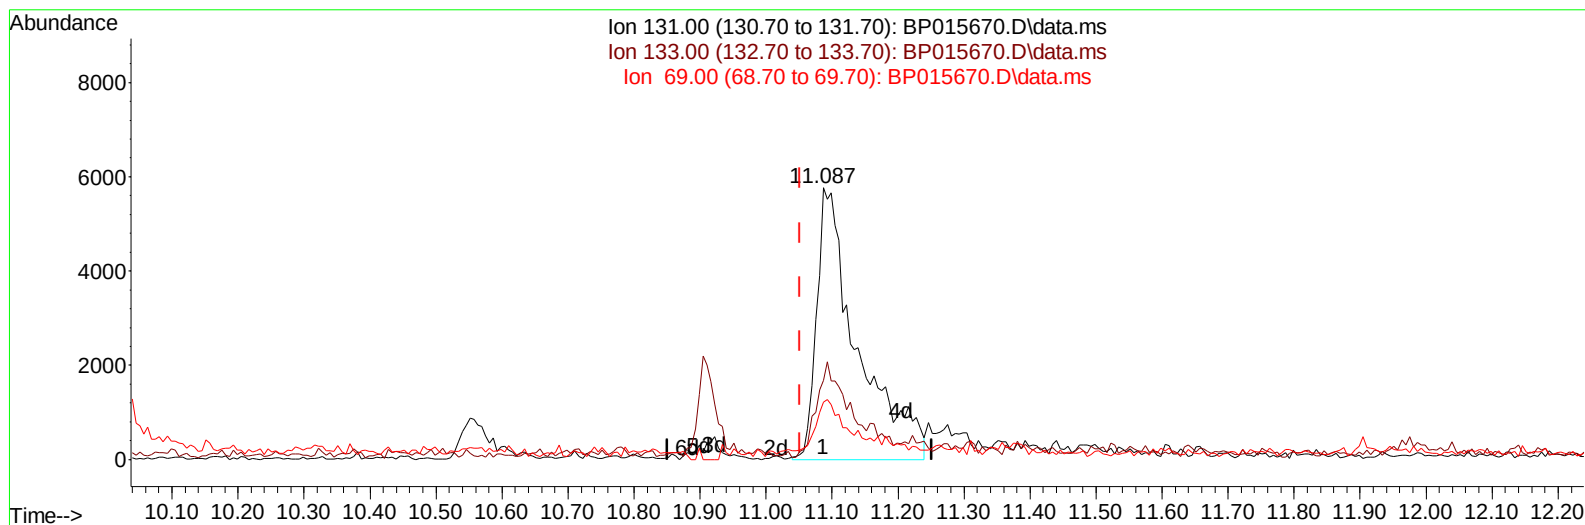

TIC: BP015670.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.087min (+ 0.035) 2.11 ng/ul m

response 24720

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 131.00 | 100.00 | 100.00 |
| 133.00 | 32.20  | 29.20  |
| 69.00  | 18.30  | 21.08  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062323\  
 Data File : BP015670.D  
 Acq On : 23 Jun 2023 14:23  
 Operator : MA/JU  
 Sample : 03084-19  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCFN6

Manual IntegrationsAPPROVED

Quant Time: Jun 23 22:34:56 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jun 22 22:01:49 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023  
 Supervised By :mohammad ahmed 06/27/2023

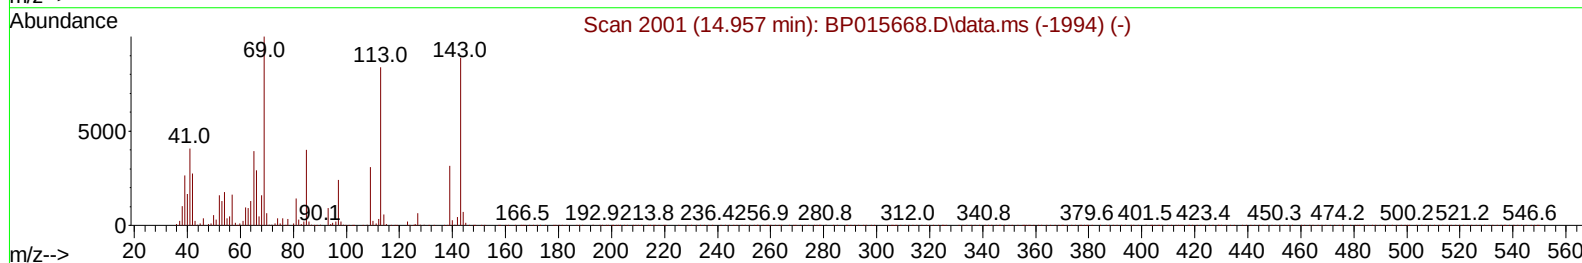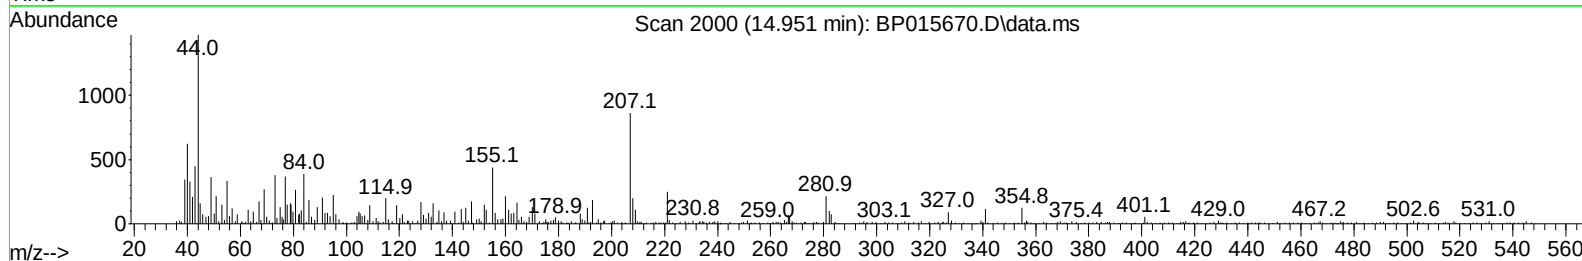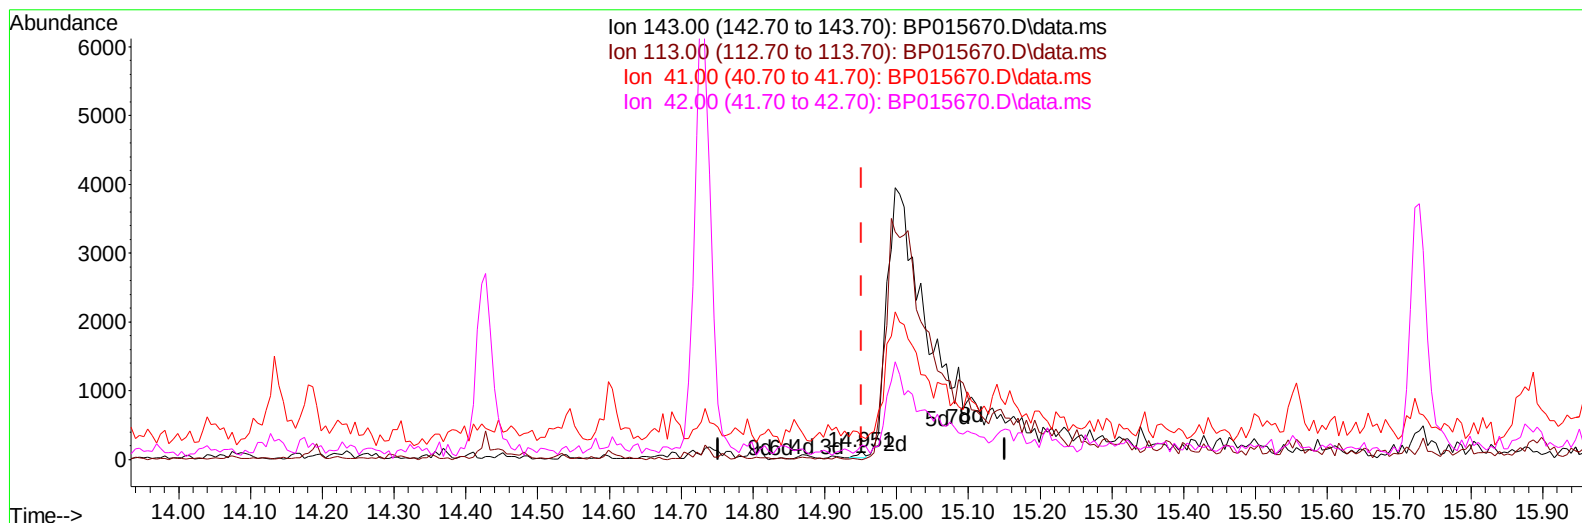

TIC: BP015670.D\data.ms

**(54) 4-Nitrophenol-d4 (S)**

**14.951min (+ 0.000) 0.02 ng/ul**

**response 67**

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 143.00 | 100.00 | 100.00  |
| 113.00 | 86.60  | 0.00#   |
| 41.00  | 42.20  | 282.76# |
| 42.00  | 29.40  | 178.45# |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062323\  
 Data File : BP015670.D  
 Acq On : 23 Jun 2023 14:23  
 Operator : MA/JU  
 Sample : 03084-19  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCFN6

Manual IntegrationsAPPROVED

Quant Time: Jun 23 22:44:52 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jun 22 22:01:49 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023  
 Supervised By :mohammad ahmed 06/27/2023

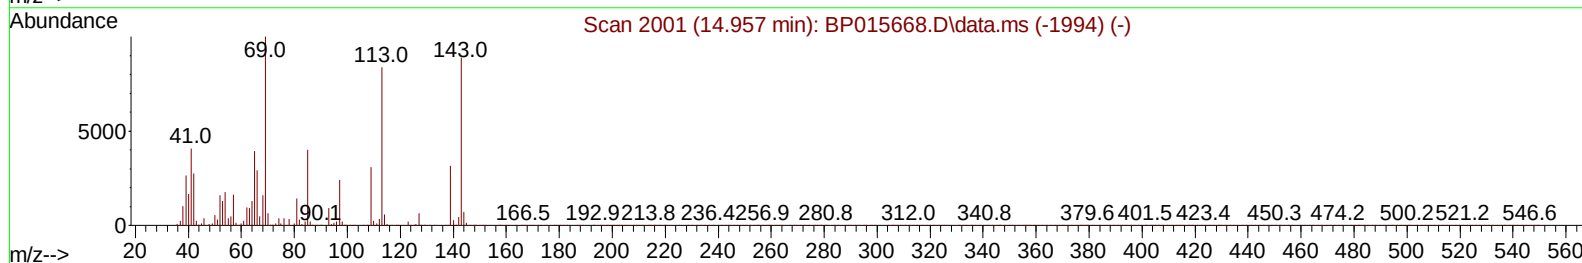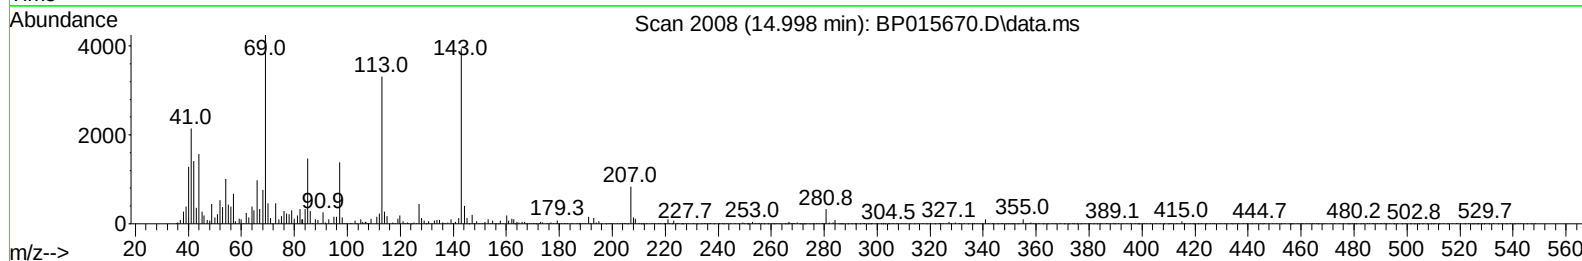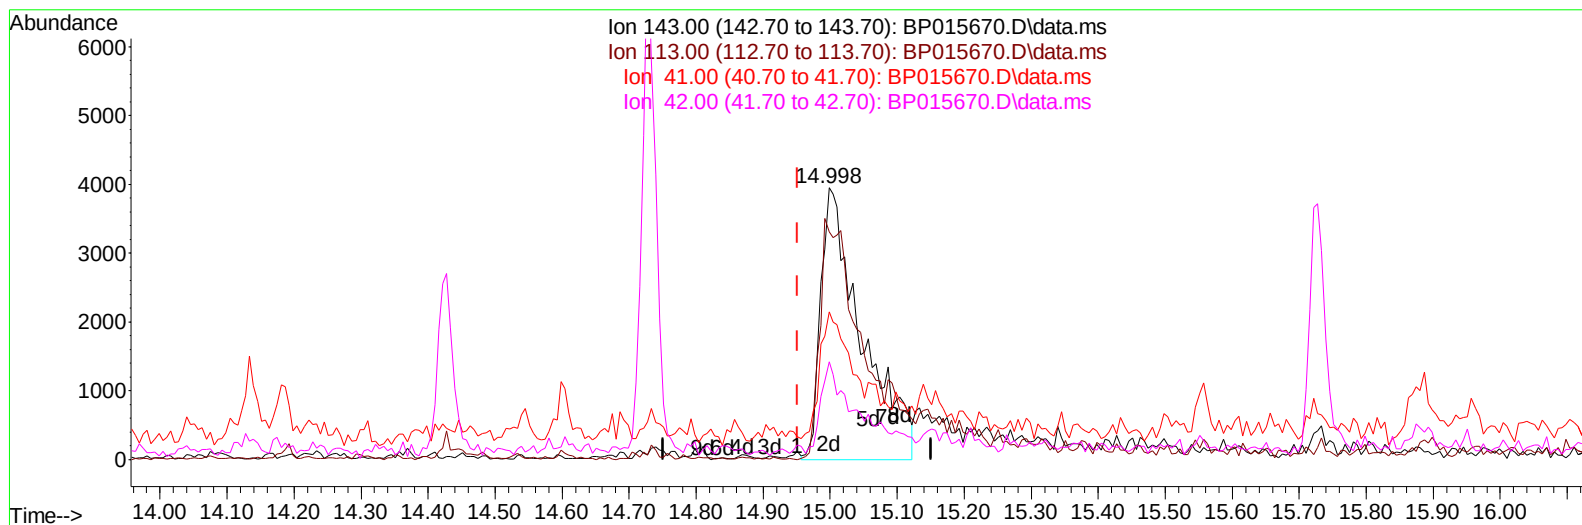

TIC: BP015670.D\data.ms

**(54) 4-Nitrophenol-d4 (S)**

**14.998min (+ 0.047) 4.40 ng/ul m**

**response 16725**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 143.00 | 100.00 | 100.00 |
| 113.00 | 86.60  | 83.86  |
| 41.00  | 42.20  | 54.36# |
| 42.00  | 29.40  | 35.86# |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062323\  
 Data File : BP015670.D  
 Acq On : 23 Jun 2023 14:23  
 Operator : MA/JU  
 Sample : 03084-19  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCFN6

Manual IntegrationsAPPROVED

Quant Time: Jun 23 22:46:00 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jun 22 22:01:49 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023  
 Supervised By :mohammad ahmed 06/27/2023

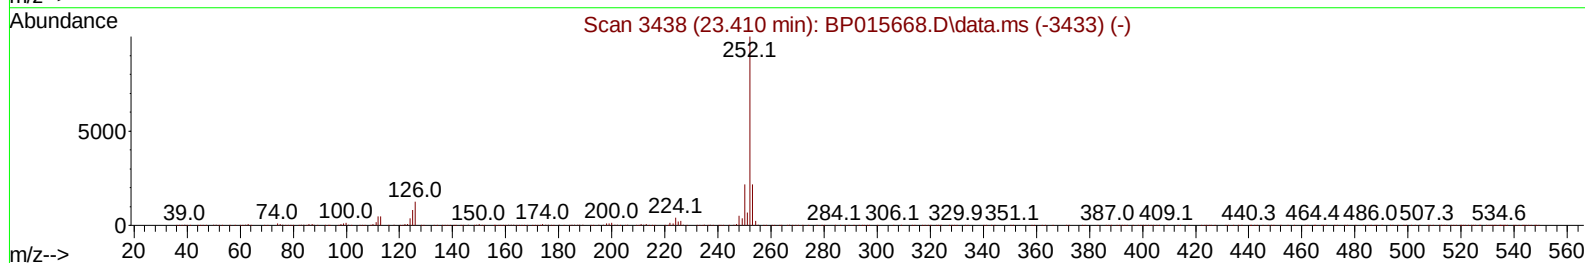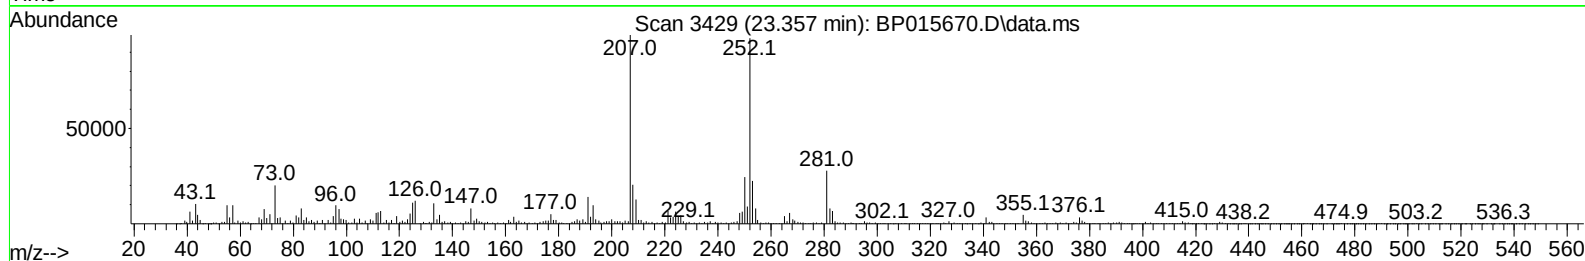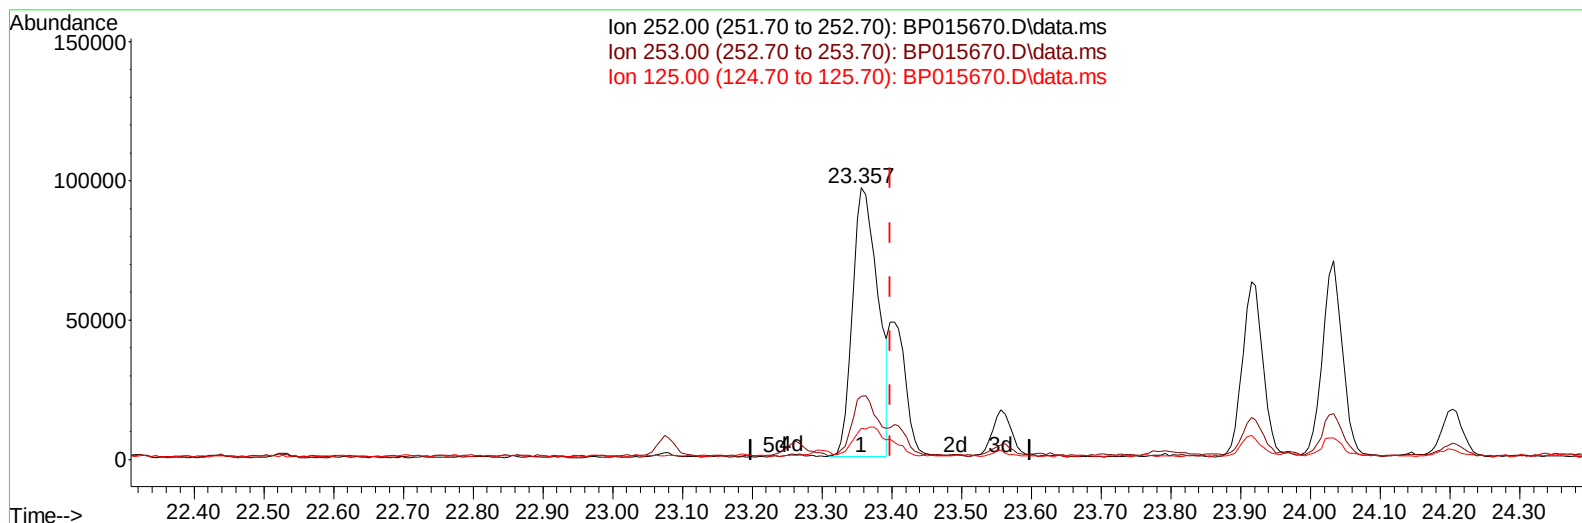

TIC: BP015670.D\data.ms

**(91) Benzo(k)fluoranthene**

**23.357min (-0.041) 5.72 ng/u1**

**response 244799**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 22.10  | 23.17  |
| 125.00 | 9.10   | 11.55# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062323\  
 Data File : BP015670.D  
 Acq On : 23 Jun 2023 14:23  
 Operator : MA/JU  
 Sample : 03084-19  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCFN6

Manual IntegrationsAPPROVED

Quant Time: Jun 23 22:46:00 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jun 22 22:01:49 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023  
 Supervised By :mohammad ahmed 06/27/2023

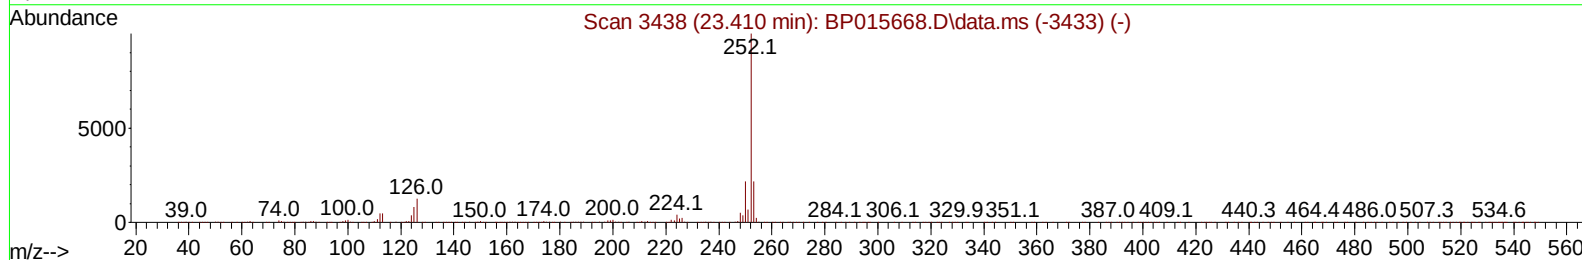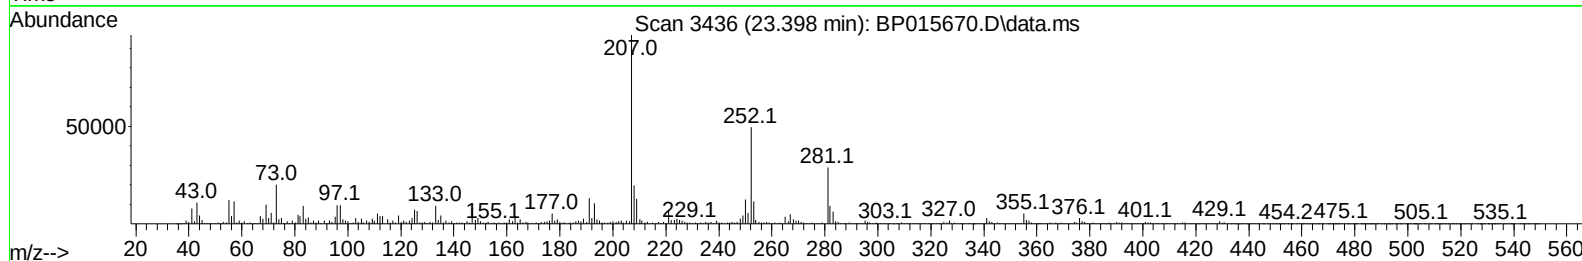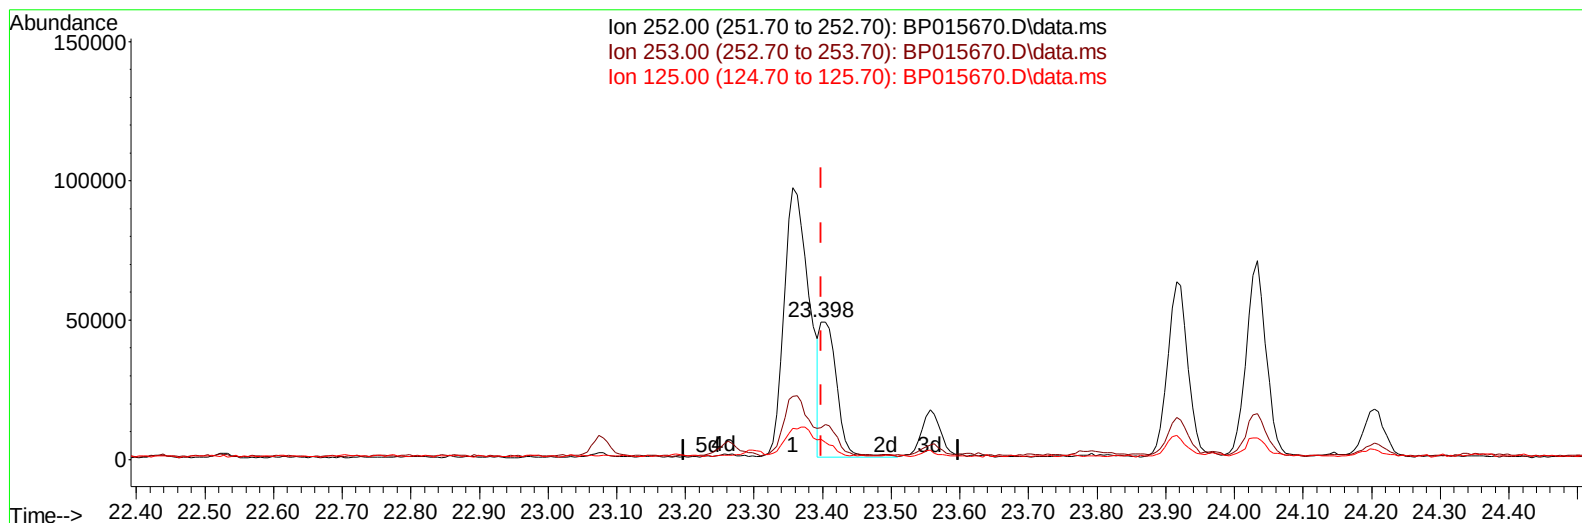

TIC: BP015670.D\data.ms

(91) Benzo(k)fluoranthene

23.398min (+ 0.000) 1.94 ng/ul m

response 83112

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 22.10  | 23.06  |
| 125.00 | 9.10   | 14.94# |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062323\  
 Data File : BP015670.D  
 Acq On : 23 Jun 2023 14:23  
 Operator : MA/JU  
 Sample : 03084-19  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCFN6

Manual IntegrationsAPPROVED

Quant Time: Jun 23 22:46:31 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Jun 22 22:01:49 2023  
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023  
 Supervised By :mohammad ahmed 06/27/2023

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----                         |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.081  | 152  | 133890   | 20.000 | ng/ul  | 0.00     |
| 20) Naphthalene-d8            | 10.910 | 136  | 499834   | 20.000 | ng/ul  | 0.00     |
| 38) Acenaphthene-d10          | 14.734 | 164  | 269426   | 20.000 | ng/ul  | 0.00     |
| 64) Phenanthrene-d10          | 17.492 | 188  | 537510   | 20.000 | ng/ul  | 0.00     |
| 79) Chrysene-d12              | 21.586 | 240  | 555229   | 20.000 | ng/ul  | 0.00     |
| 88) Perylene-d12              | 24.145 | 264  | 685907   | 20.000 | ng/ul  | 0.01     |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8             | 3.399  | 96   | 7054     | 1.951  | ng/uL  | 0.00     |
| 4) Pyridine-d5                | 0.000  | 84   | 0d       | 0.000  | ng/ul  |          |
| 7) Phenol-d5                  | 7.246  | 99   | 97463    | 7.901  | ng/ul  | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.405  | 67   | 73410    | 9.965  | ng/ul  | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.610  | 132  | 89445    | 10.002 | ng/ul  | 0.00     |
| 15) 4-Methylphenol-d8         | 8.816  | 113  | 40347    | 3.986  | ng/ul  | 0.01     |
| 21) Nitrobenzene-d5           | 9.263  | 128  | 41185    | 10.495 | ng/ul  | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.993  | 143  | 47075    | 10.505 | ng/ul  | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.557 | 165  | 68067    | 8.326  | ng/ul  | 0.02     |
| 31) 4-Chloroaniline-d4        | 11.087 | 131  | 24720m   | 2.107  | ng/ul  | 0.04     |
| 46) Dimethylphthalate-d6      | 14.140 | 166  | 245046   | 11.534 | ng/ul  | 0.00     |
| 49) Acenaphthylene-d8         | 14.428 | 160  | 276471   | 11.901 | ng/ul  | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.998 | 143  | 16725m   | 4.396  | ng/ul  | 0.05     |
| 60) Fluorene-d10              | 15.728 | 176  | 195792   | 10.928 | ng/ul  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.881 | 200  | 20583    | 6.045  | ng/ul  | 0.02     |
| 73) Anthracene-d10            | 17.592 | 188  | 283506   | 11.593 | ng/ul  | 0.00     |
| 81) Pyrene-d10                | 19.822 | 212  | 362602   | 12.202 | ng/ul  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.980 | 264  | 406060   | 11.799 | ng/ul  | 0.01     |
| Target Compounds              |        |      |          |        |        |          |
|                               |        |      |          |        | Qvalue |          |
| 72) Phenanthrene              | 17.533 | 178  | 57878    | 2.007  | ng/ul  | 99       |
| 80) Fluoranthene              | 19.492 | 202  | 259236   | 7.162  | ng/ul  | 99       |
| 82) Pyrene                    | 19.851 | 202  | 219643   | 5.865  | ng/ul  | 99       |
| 85) Benzo(a)anthracene        | 21.569 | 228  | 123892   | 3.192  | ng/ul  | 98       |
| 87) Chrysene                  | 21.627 | 228  | 162604   | 4.432  | ng/ul  | 96       |
| 90) Benzo(b)fluoranthene      | 23.357 | 252  | 244799   | 5.529  | ng/ul# | 96       |
| 91) Benzo(k)fluoranthene      | 23.398 | 252  | 83112m   | 1.942  | ng/ul  |          |
| 93) Benzo(a)pyrene            | 24.033 | 252  | 141159   | 3.657  | ng/ul  | 98       |
| 94) Indeno(1,2,3-cd)pyrene    | 26.856 | 276  | 120677   | 2.416  | ng/ul  | 97       |
| 96) Benzo(g,h,i)perylene      | 27.698 | 276  | 115490   | 2.805  | ng/ul  | 97       |
| -----                         |        |      |          |        |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP062323\  
Data File : BP015670.D  
Acq On : 23 Jun 2023 14:23  
Operator : MA/JU  
Sample : 03084-19  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DCFN6

## Manual IntegrationsAPPROVED

Quant Time: Jun 23 22:46:31 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP060723.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Jun 22 22:01:49 2023  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023  
Supervised By :mohammad ahmed 06/27/2023

