




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015693.D
 Acq On : 24 Jun 2023 03:54
 Operator : MA/JU
 Sample : 03085-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFN8

Manual IntegrationsAPPROVED

Quant Time: Jun 24 04:35:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023

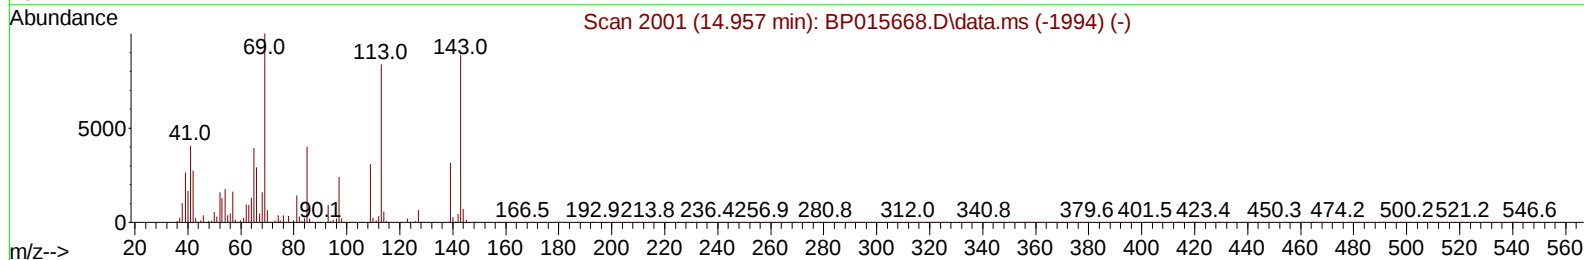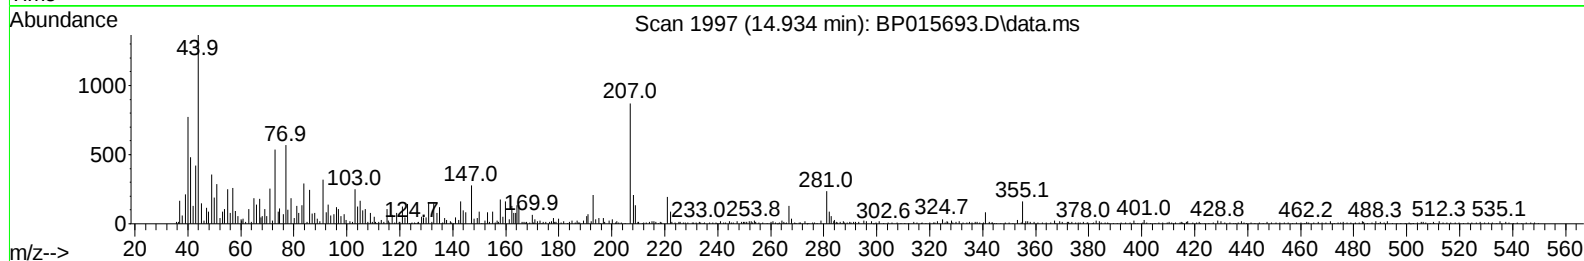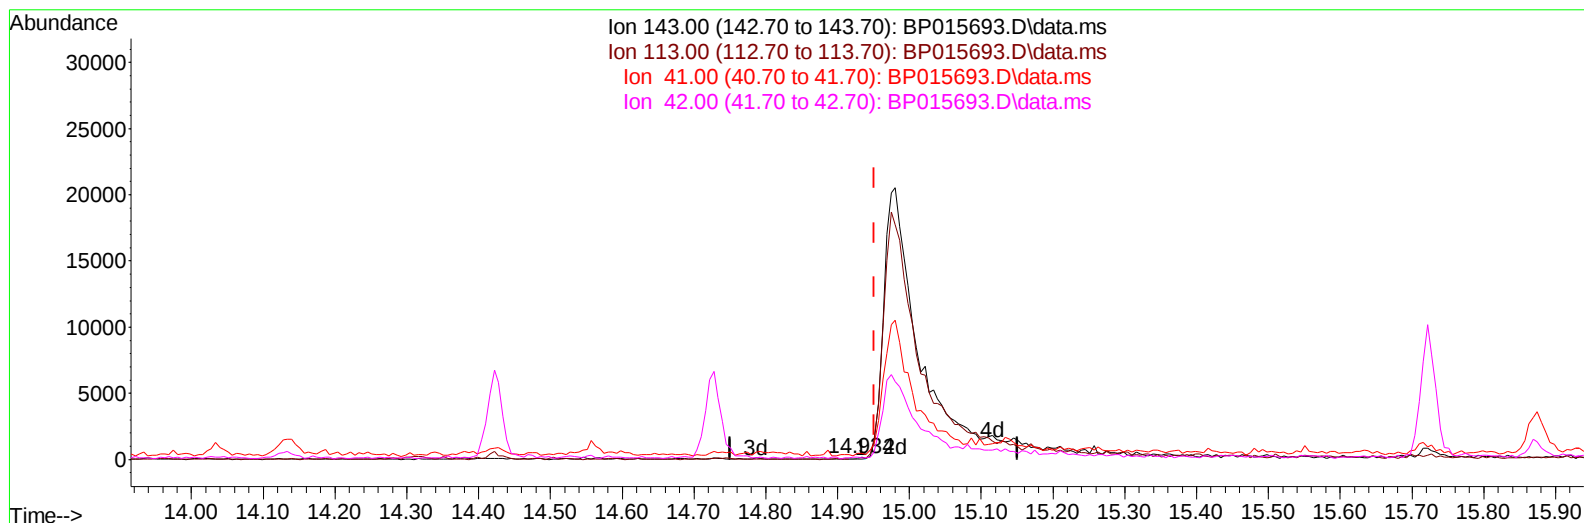

TIC: BP015693.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.934min (-0.018) 0.03 ng/u1

response 103

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	17.28#
41.00	42.20	298.15#
42.00	29.40	80.25#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015693.D
 Acq On : 24 Jun 2023 03:54
 Operator : MA/JU
 Sample : 03085-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFN8

Manual IntegrationsAPPROVED

Quant Time: Jun 24 04:35:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023

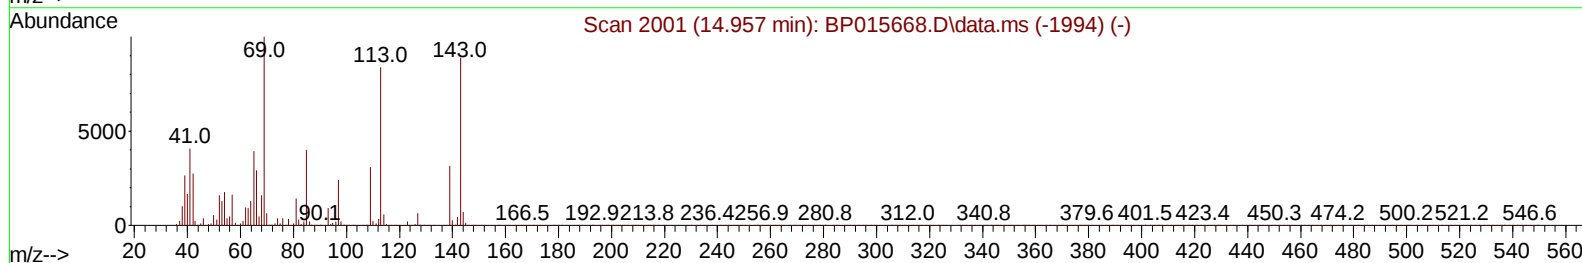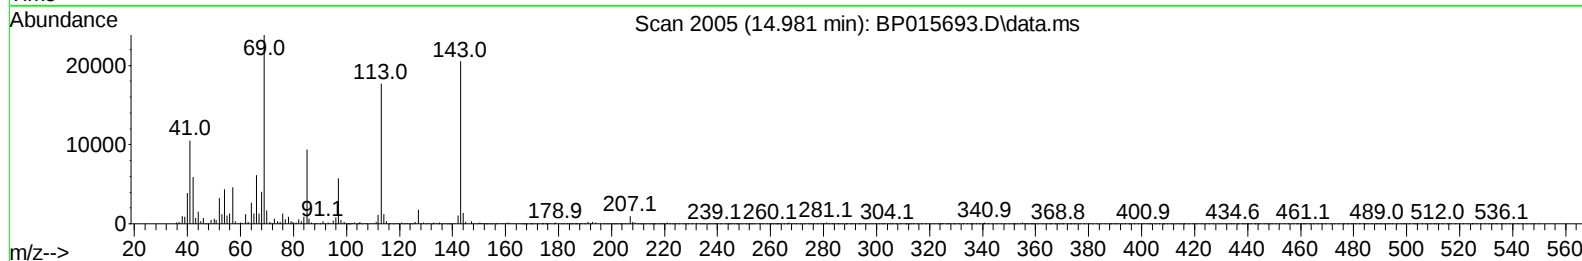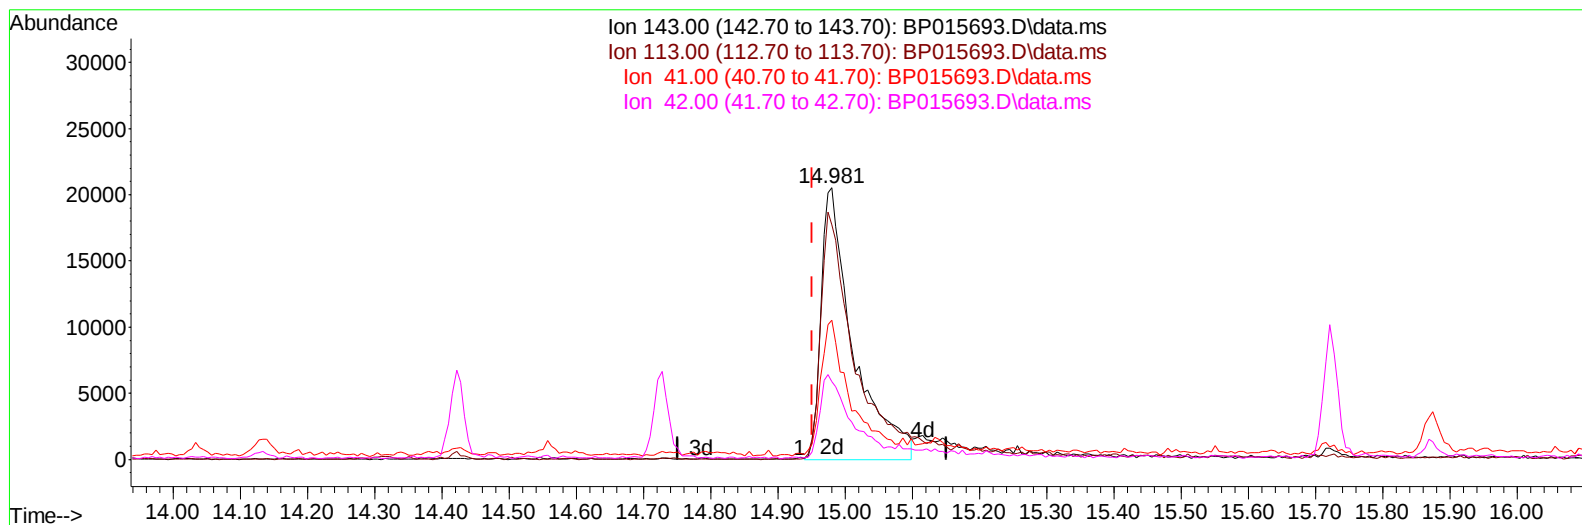

TIC: BP015693.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.981min (+ 0.029) 18.07 ng/ul m

response 68332

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	86.32
41.00	42.20	51.28#
42.00	29.40	28.58

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015693.D
 Acq On : 24 Jun 2023 03:54
 Operator : MA/JU
 Sample : 03085-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFN8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023

Quant Time: Jun 24 04:37:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.081	152	127437	20.000	ng/ul	0.00
20) Naphthalene-d8	10.904	136	469185	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.728	164	267805	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.486	188	595872	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	581857	20.000	ng/ul	0.00
88) Perylene-d12	24.139	264	703261	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	13998	4.067	ng/uL	0.00
4) Pyridine-d5	3.852	84	91384	10.223	ng/ul	0.01
7) Phenol-d5	7.246	99	230017	19.592	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	153909	21.951	ng/ul	0.00
11) 2-Chlorophenol-d4	7.604	132	194687	22.872	ng/ul	0.00
15) 4-Methylphenol-d8	8.804	113	127082	13.189	ng/ul	0.00
21) Nitrobenzene-d5	9.263	128	90867	24.668	ng/ul	0.00
24) 2-Nitrophenol-d4	9.993	143	106695	25.364	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	166879	21.747	ng/ul	0.01
31) 4-Chloroaniline-d4	11.075	131	141262	12.825	ng/ul	0.02
46) Dimethylphthalate-d6	14.134	166	569836	26.983	ng/ul	0.00
49) Acenaphthylene-d8	14.422	160	643400	27.863	ng/ul	0.00
54) 4-Nitrophenol-d4	14.981	143	68332m	18.069	ng/ul	0.03
60) Fluorene-d10	15.722	176	476724	26.770	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	64778	17.160	ng/ul	0.01
73) Anthracene-d10	17.592	188	703473	25.948	ng/ul	0.00
81) Pyrene-d10	19.816	212	959098	30.798	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	990294	28.064	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015693.D
Acq On : 24 Jun 2023 03:54
Operator : MA/JU
Sample : 03085-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFN8

Manual IntegrationsAPPROVED

Quant Time: Jun 24 04:37:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023

