




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015698.D
Acq On : 24 Jun 2023 07:16
Operator : MA/JU
Sample : 03085-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFQ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023

Quant Time: Jun 24 22:16:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

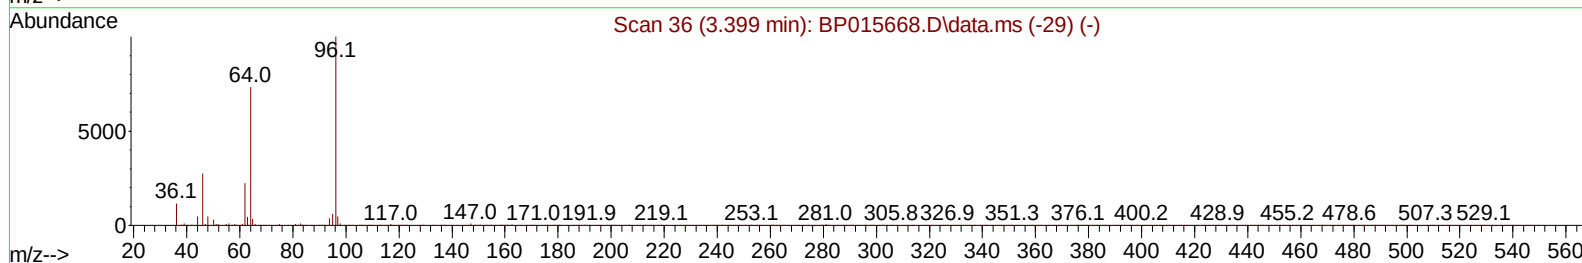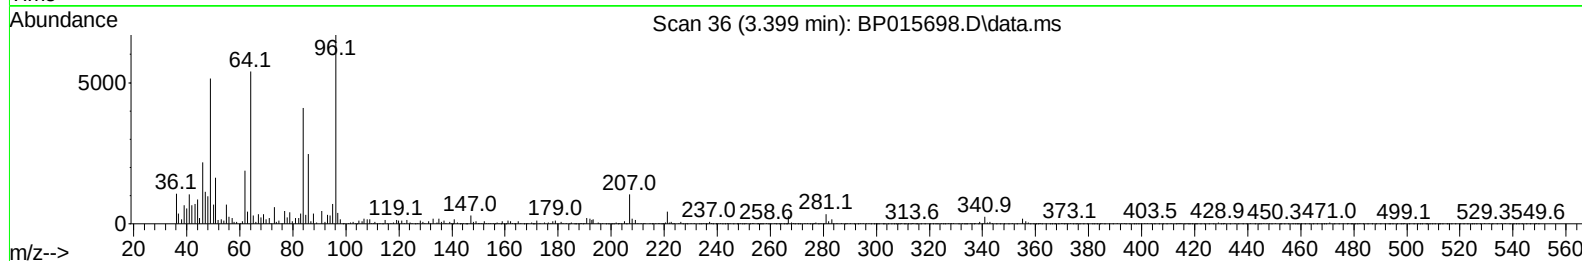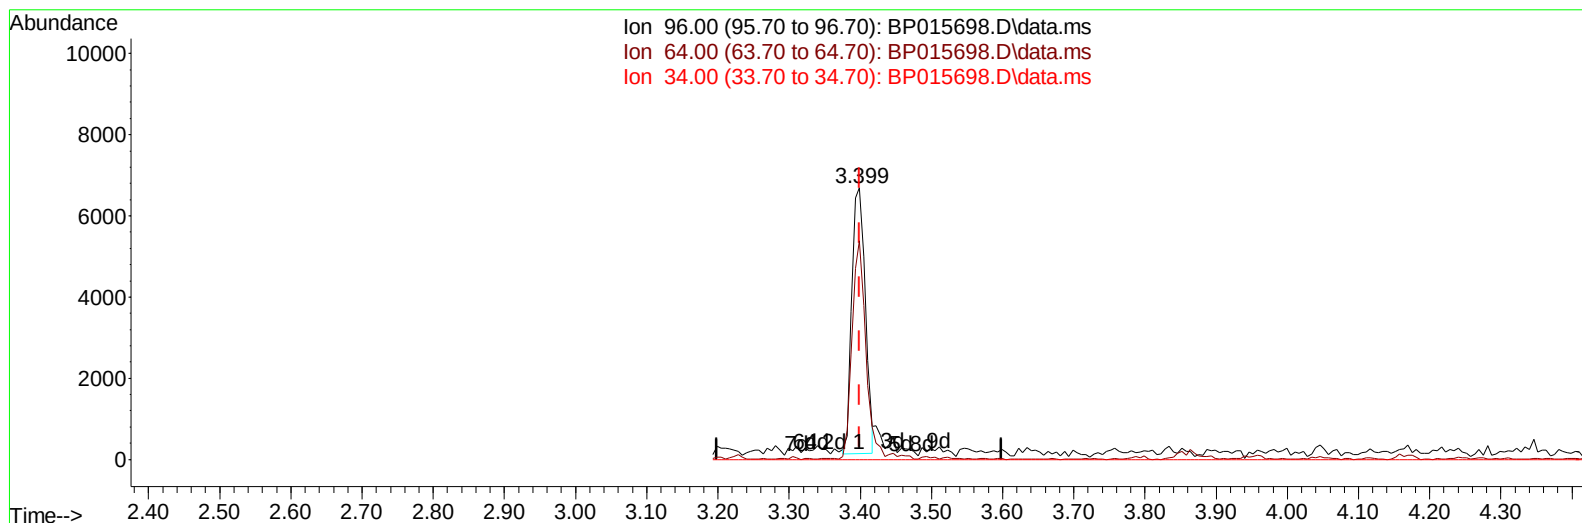

TIC: BP015698.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.399min (+ 0.000) 2.11 ng/uL****response 8685**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	75.60	80.52
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015698.D
Acq On : 24 Jun 2023 07:16
Operator : MA/JU
Sample : 03085-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFQ1

Manual IntegrationsAPPROVED

Quant Time: Jun 24 22:16:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023

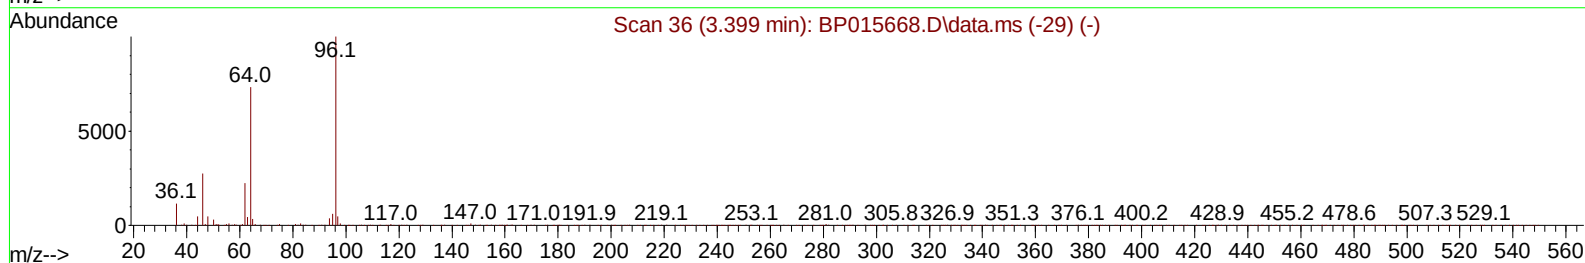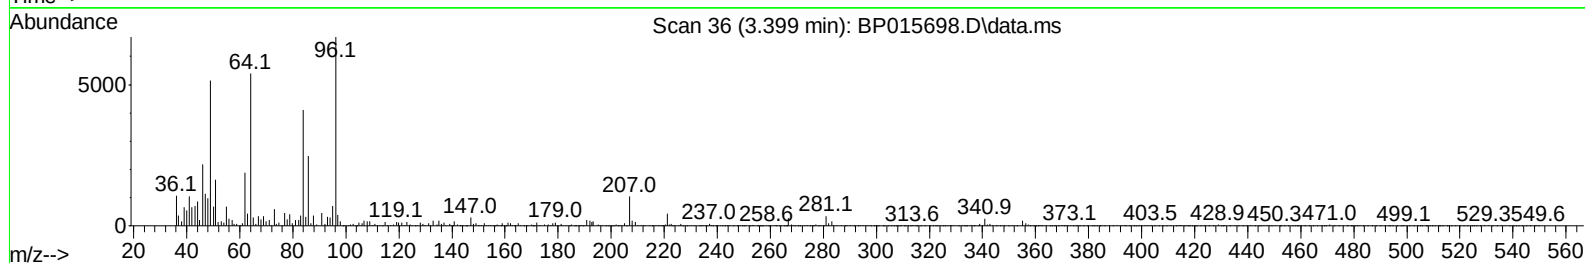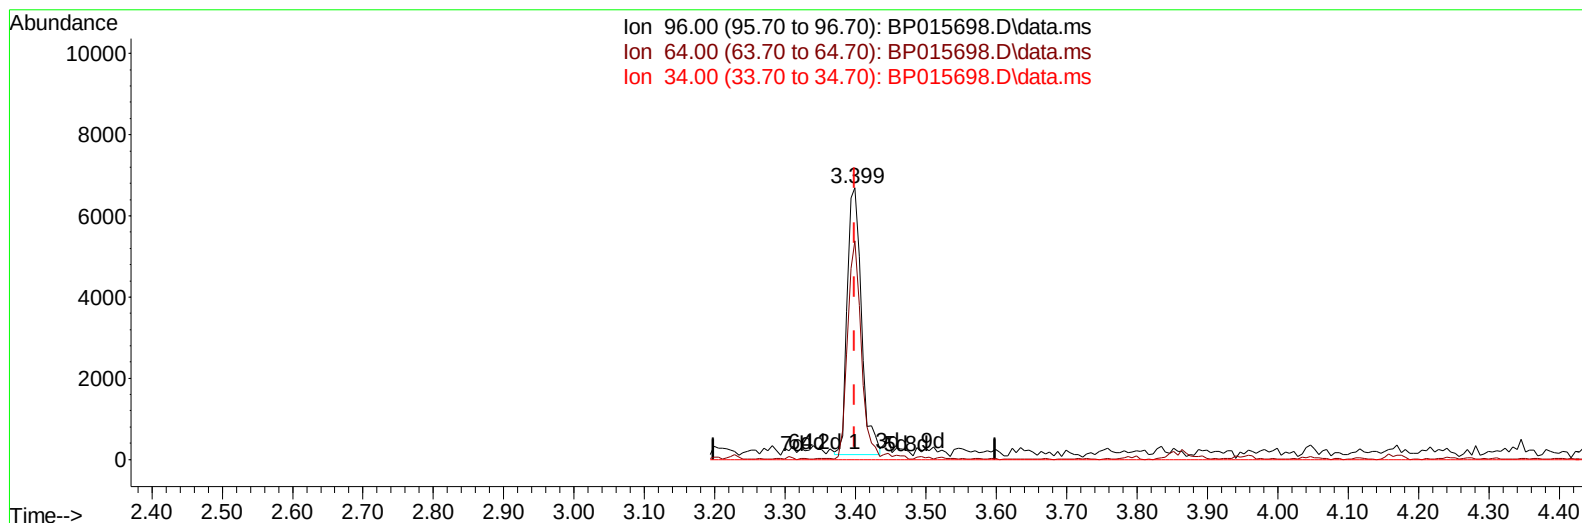

TIC: BP015698.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.399min (+ 0.000) 2.24 ng/uL m

response 9226

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	75.60	80.52
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015698.D
Acq On : 24 Jun 2023 07:16
Operator : MA/JU
Sample : 03085-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFQ1

Manual IntegrationsAPPROVED

Quant Time: Jun 24 22:55:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023

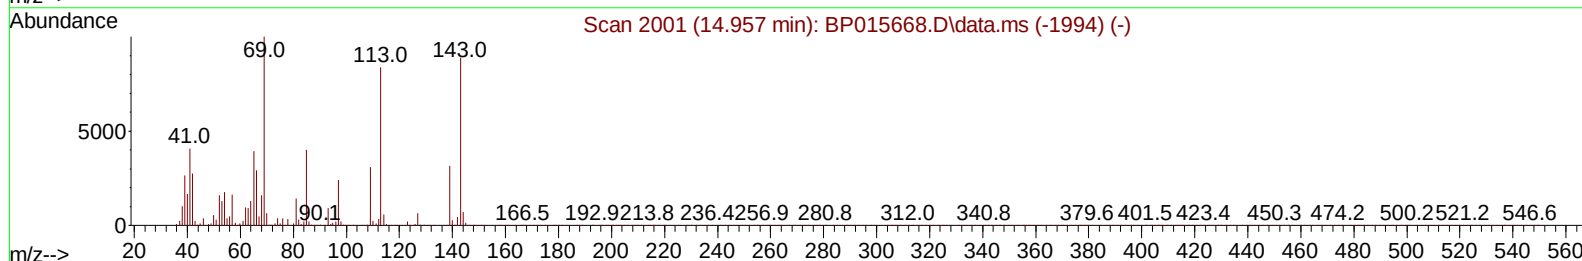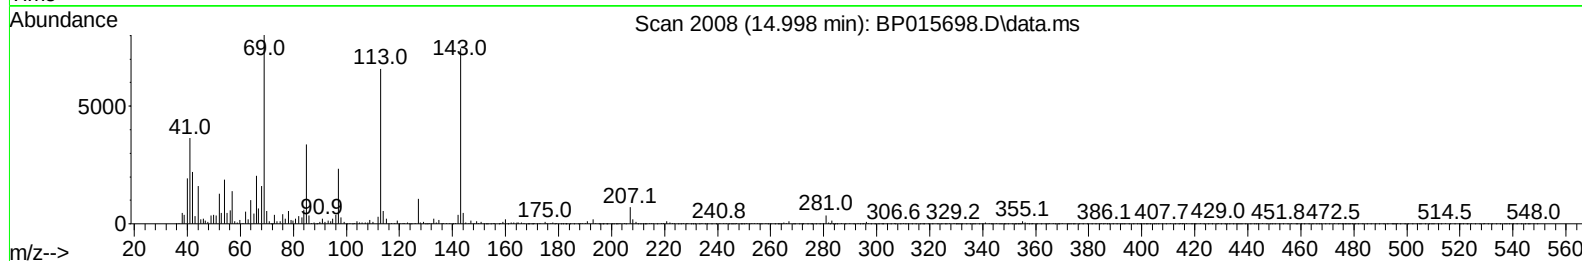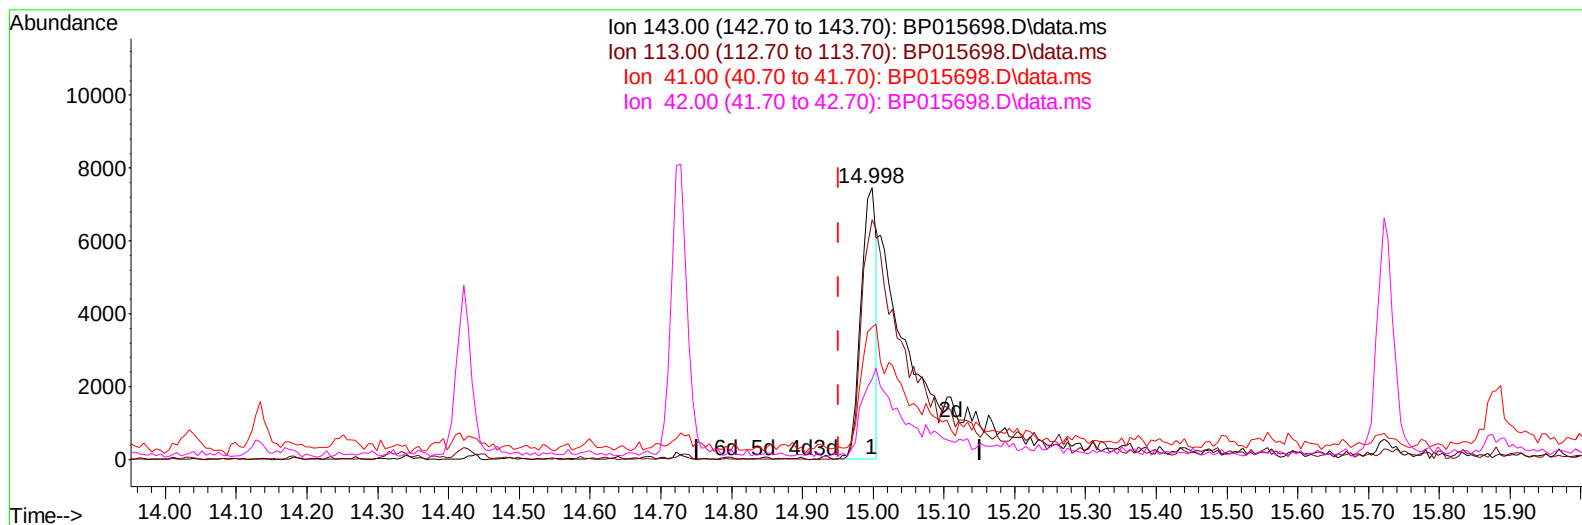

TIC: BP015698.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.998min (+ 0.047) 2.33 ng/ul

response 11291

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	88.23
41.00	42.20	48.75
42.00	29.40	29.57




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015698.D
Acq On : 24 Jun 2023 07:16
Operator : MA/JU
Sample : 03085-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFQ1

Manual IntegrationsAPPROVED

Quant Time: Jun 24 22:55:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023

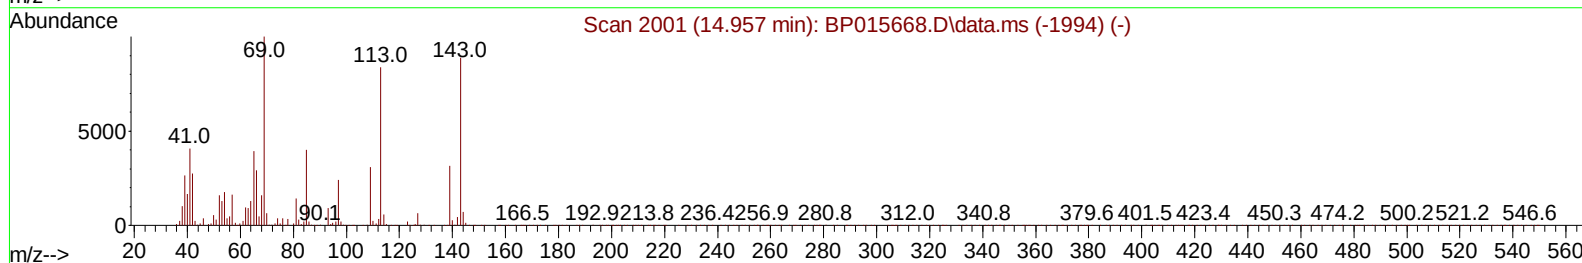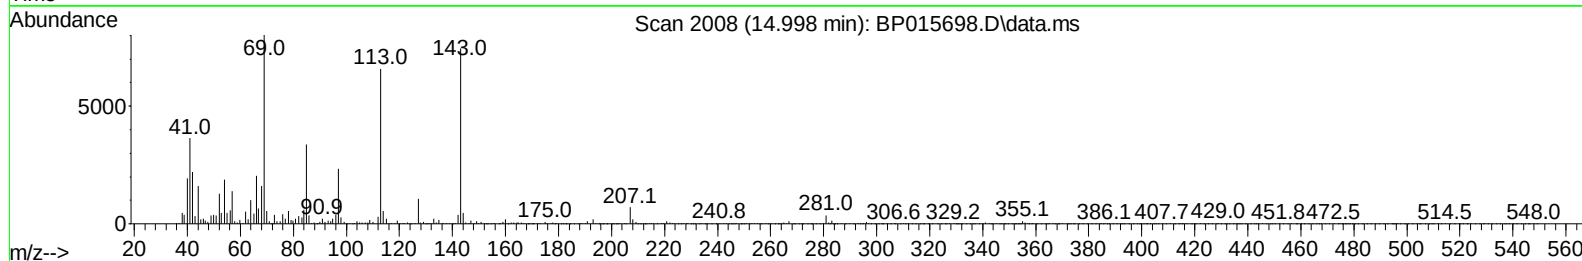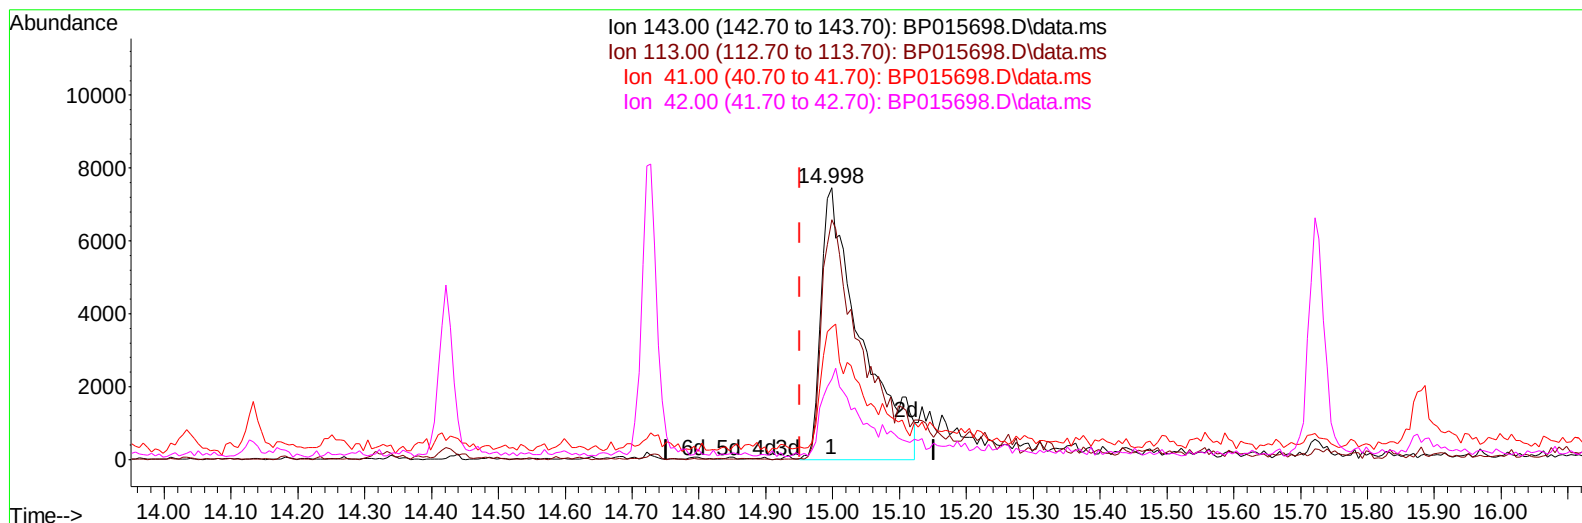

TIC: BP015698.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.998min (+ 0.047) 6.35 ng/ul m

response 30809

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	88.23
41.00	42.20	48.75
42.00	29.40	29.57

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015698.D
 Acq On : 24 Jun 2023 07:16
 Operator : MA/JU
 Sample : 03085-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFQ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023

Quant Time: Jun 24 22:57:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	152439	20.000	ng/ul	0.00
20) Naphthalene-d8	10.904	136	588270	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.728	164	343834	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.486	188	705725	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	666808	20.000	ng/ul	0.00
88) Perylene-d12	24.139	264	799746	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	9226m	2.241	ng/uL	0.00
4) Pyridine-d5	3.846	84	65077	6.086	ng/ul	0.00
7) Phenol-d5	7.246	99	165374	11.776	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	112755	13.444	ng/ul	0.00
11) 2-Chlorophenol-d4	7.605	132	144676	14.209	ng/ul	0.00
15) 4-Methylphenol-d8	8.805	113	124546	10.806	ng/ul	0.00
21) Nitrobenzene-d5	9.263	128	67173	14.544	ng/ul	0.00
24) 2-Nitrophenol-d4	9.993	143	75200	14.258	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	119928	12.465	ng/ul	0.01
31) 4-Chloroaniline-d4	11.069	131	123104	8.914	ng/ul	0.02
46) Dimethylphthalate-d6	14.134	166	413334	15.245	ng/ul	0.00
49) Acenaphthylene-d8	14.422	160	474378	16.001	ng/ul	0.00
54) 4-Nitrophenol-d4	14.998	143	30809m	6.345	ng/ul	0.05
60) Fluorene-d10	15.728	176	344270	15.057	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	39315	8.794	ng/ul	0.01
73) Anthracene-d10	17.592	188	492888	15.350	ng/ul	0.00
81) Pyrene-d10	19.816	212	632015	17.709	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	648559	16.162	ng/ul	0.00
Target Compounds						
					Qvalue	
72) Phenanthrene	17.533	178	67112	1.772	ng/ul	98
80) Fluoranthene	19.492	202	179759	4.135	ng/ul	98
82) Pyrene	19.845	202	112972	2.512	ng/ul	100
87) Chrysene	21.621	228	64701	1.468	ng/ul	97
90) Benzo(b)fluoranthene	23.351	252	72109	1.397	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015698.D
Acq On : 24 Jun 2023 07:16
Operator : MA/JU
Sample : 03085-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFQ1

Manual IntegrationsAPPROVED

Quant Time: Jun 24 22:57:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023

