




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015699.D
 Acq On : 24 Jun 2023 07:50
 Operator : MA/JU
 Sample : 03085-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFP6

Manual IntegrationsAPPROVED

Quant Time: Jun 24 22:16:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023

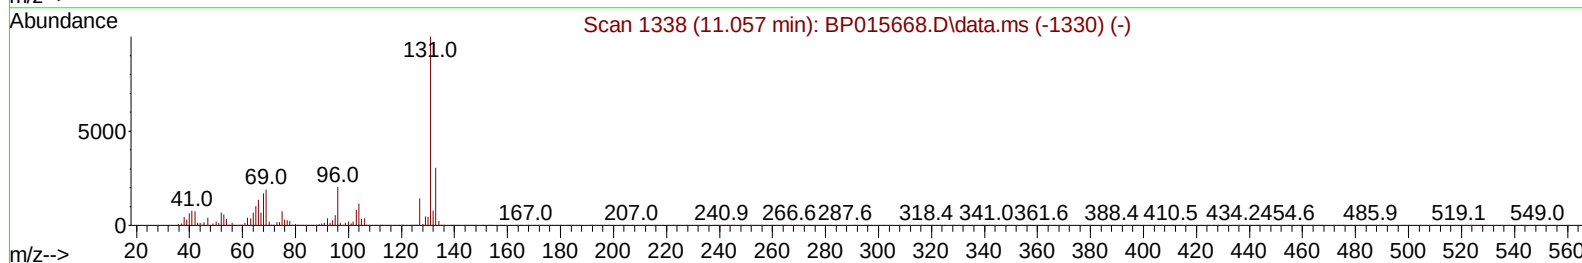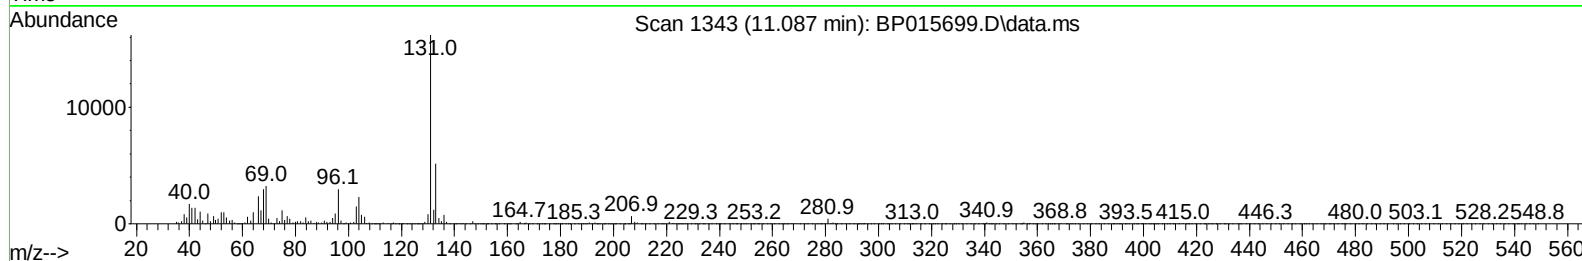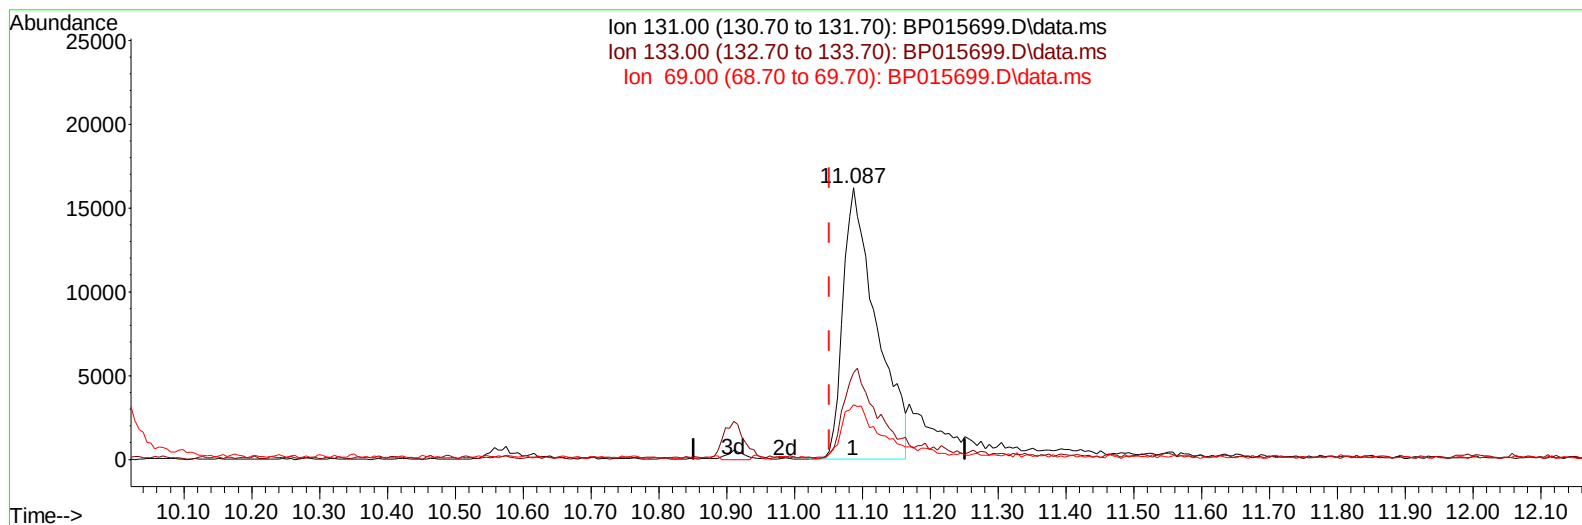

TIC: BP015699.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.087min (+ 0.035) 4.09 ng/ul

response 55173

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	31.99
69.00	18.30	20.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015699.D
Acq On : 24 Jun 2023 07:50
Operator : MA/JU
Sample : 03085-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFP6

Manual IntegrationsAPPROVED

Quant Time: Jun 24 22:16:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023

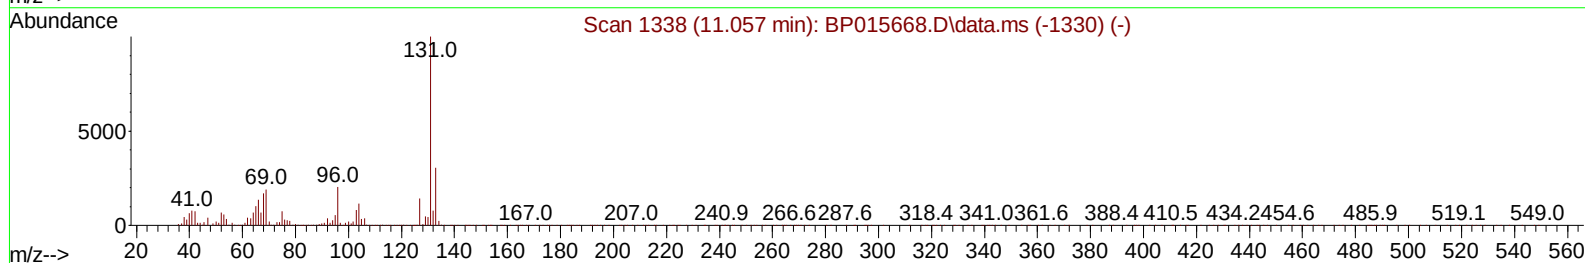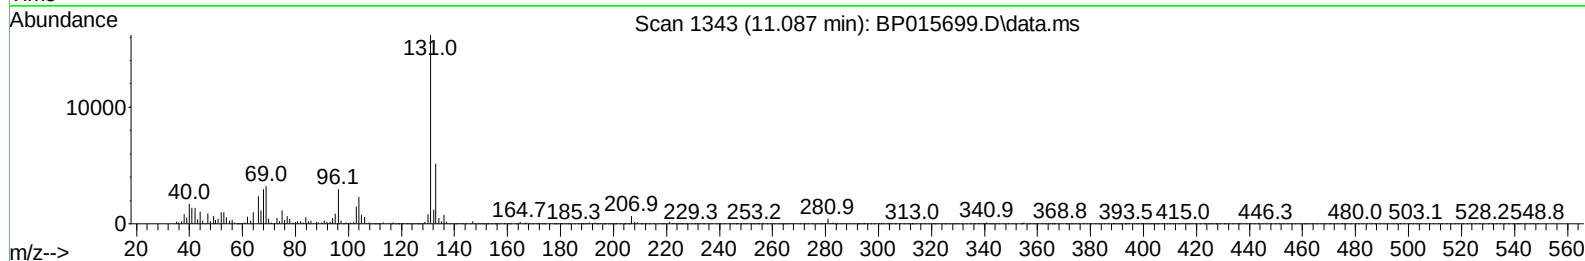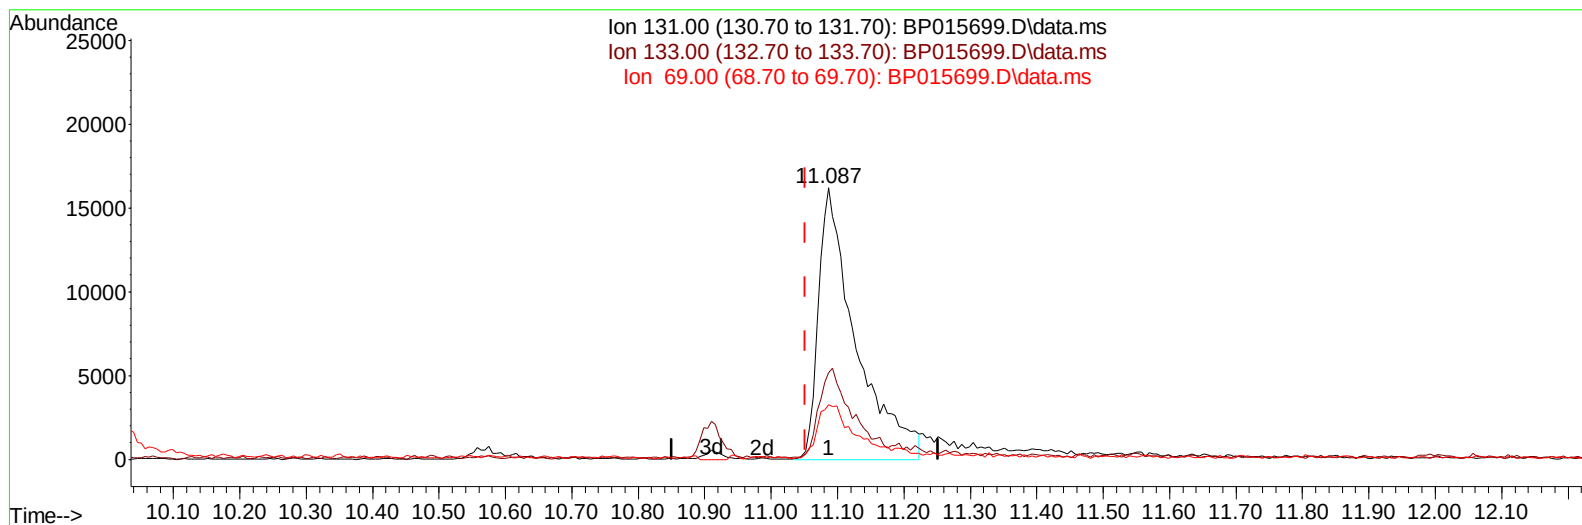

TIC: BP015699.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.087min (+ 0.035) 4.67 ng/ul m

response 62997

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	31.99
69.00	18.30	20.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015699.D
 Acq On : 24 Jun 2023 07:50
 Operator : MA/JU
 Sample : 03085-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFP6

Manual IntegrationsAPPROVED

Quant Time: Jun 24 22:16:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023

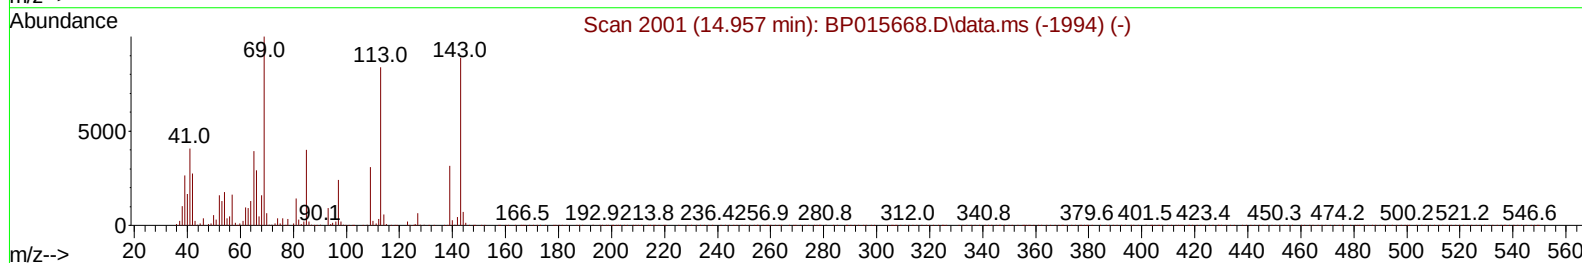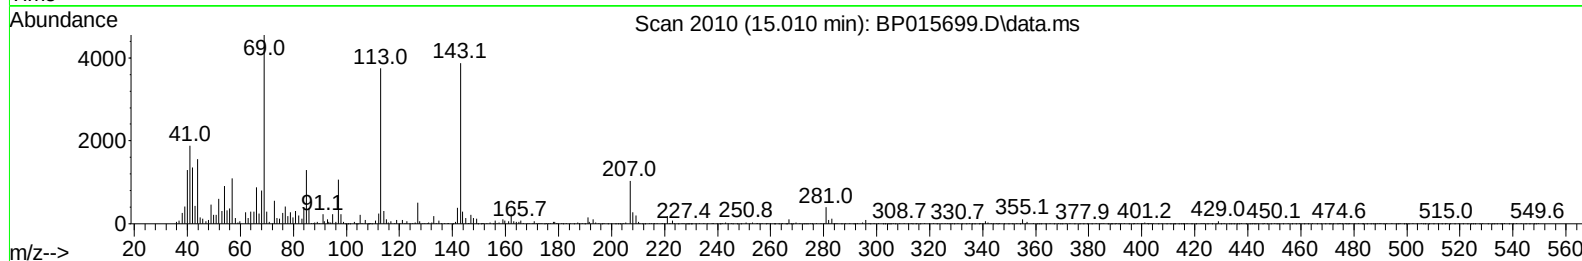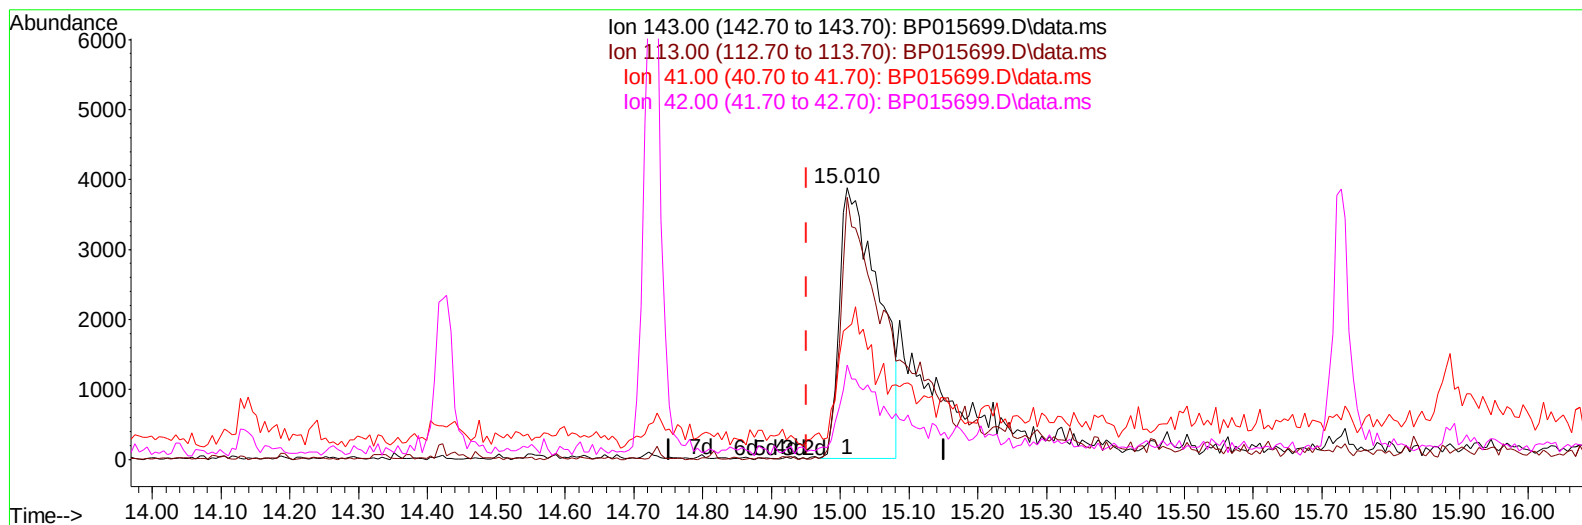

TIC: BP015699.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.010min (+ 0.059) 3.28 ng/ul

response 15194

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	96.47
41.00	42.20	48.40
42.00	29.40	34.90




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015699.D
 Acq On : 24 Jun 2023 07:50
 Operator : MA/JU
 Sample : 03085-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFP6

Manual IntegrationsAPPROVED

Quant Time: Jun 24 22:59:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023

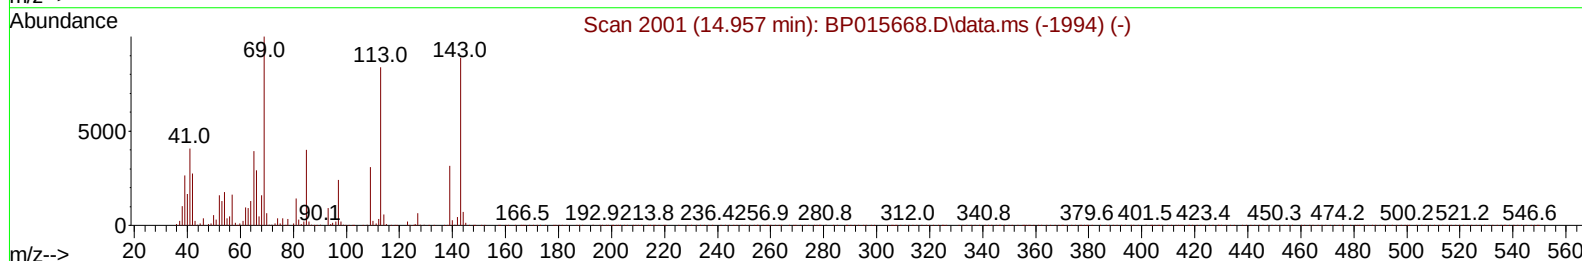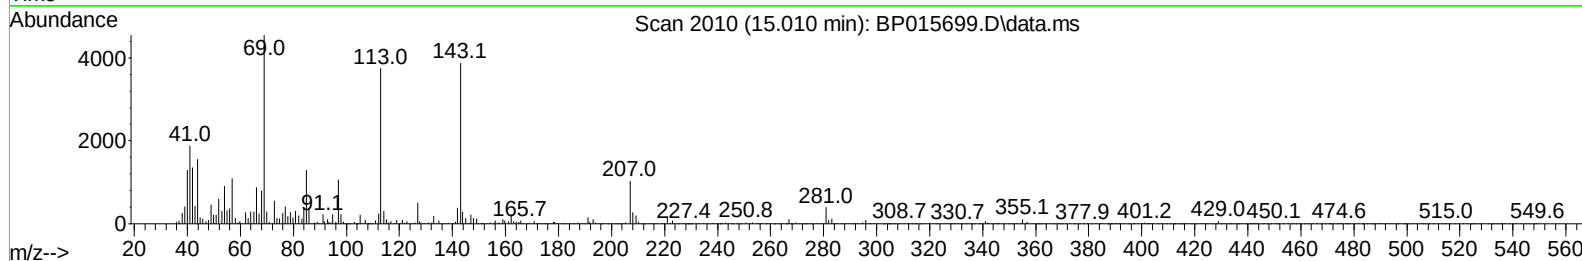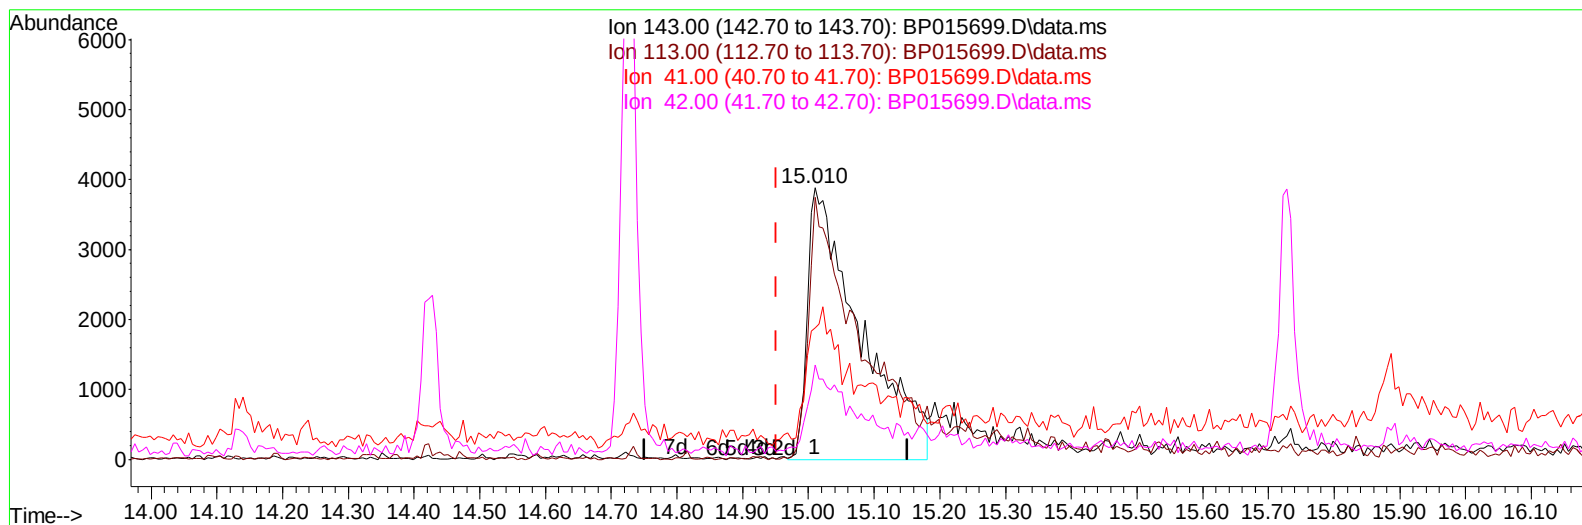

TIC: BP015699.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.010min (+ 0.059) 4.69 ng/ul m

response 21706

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	96.47
41.00	42.20	48.40
42.00	29.40	34.90

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015699.D
 Acq On : 24 Jun 2023 07:50
 Operator : MA/JU
 Sample : 03085-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFP6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023

Quant Time: Jun 24 23:00:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 22 22:01:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	150479	20.000	ng/ul	0.00
20) Naphthalene-d8	10.904	136	574451	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.728	164	327880	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.492	188	686265	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	665612	20.000	ng/ul	0.00
88) Perylene-d12	24.139	264	797537	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	6040	1.486	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.252	99	94148	6.791	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.399	67	68957	8.329	ng/ul	0.00
11) 2-Chlorophenol-d4	7.610	132	83556	8.313	ng/ul	0.00
15) 4-Methylphenol-d8	8.816	113	45591	4.007	ng/ul	0.01
21) Nitrobenzene-d5	9.269	128	40004	8.870	ng/ul	0.01
24) 2-Nitrophenol-d4	9.998	143	44345	8.610	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.569	165	65398	6.961	ng/ul	0.04
31) 4-Chloroaniline-d4	11.087	131	62997m	4.671	ng/ul	0.04
46) Dimethylphthalate-d6	14.134	166	244533	9.458	ng/ul	0.00
49) Acenaphthylene-d8	14.422	160	275530	9.746	ng/ul	0.00
54) 4-Nitrophenol-d4	15.010	143	21706m	4.688	ng/ul	0.06
60) Fluorene-d10	15.728	176	201376	9.236	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.886	200	21491	4.943	ng/ul	0.02
73) Anthracene-d10	17.592	188	293139	9.388	ng/ul	0.00
81) Pyrene-d10	19.822	212	392072	11.006	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	402713	10.064	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015699.D
Acq On : 24 Jun 2023 07:50
Operator : MA/JU
Sample : 03085-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFP6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023

Quant Time: Jun 24 23:00:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 22:01:49 2023
Response via : Initial Calibration

