

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015669.D
 Acq On : 23 Jun 2023 13:49
 Operator : MA/JU
 Sample : PB153415BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK415

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	44	rVB	48367	67997	2.31%	0.211%
2	3.840	108	111	128	rBV	516002	793897	27.02%	2.464%
3	4.175	165	168	171	rVB3	9098	11186	0.38%	0.035%
4	7.246	684	690	708	rBV	584430	1079644	36.75%	3.351%
5	7.405	710	717	730	rVV	496944	811913	27.63%	2.520%
6	7.611	744	752	770	rBV	673179	1147598	39.06%	3.562%
7	8.081	825	832	849	rBV	439121	746461	25.41%	2.317%
8	8.805	948	955	968	rBV	732220	1361471	46.34%	4.226%
9	9.263	1025	1033	1044	rBV	617019	1103839	37.57%	3.426%
10	9.993	1150	1157	1171	rVV	535207	983191	33.46%	3.052%
11	10.540	1242	1250	1272	rBV	634782	1339711	45.60%	4.158%
12	10.910	1305	1313	1328	rBV	591023	1008869	34.34%	3.132%
13	11.057	1330	1338	1366	rBV	587704	1348287	45.89%	4.185%
14	11.234	1366	1368	1371	rVB4	3665	3870	0.13%	0.012%
15	11.334	1384	1385	1390	rVB5	2383	2978	0.10%	0.009%
16	11.463	1405	1407	1414	rVB8	1680	2942	0.10%	0.009%
17	11.516	1414	1416	1421	rVB5	2446	3838	0.13%	0.012%
18	12.316	1547	1552	1556	rBV8	1642	3033	0.10%	0.009%
19	12.522	1577	1587	1594	rBV5	7603	21021	0.72%	0.065%
20	13.610	1767	1772	1775	rBV5	5696	8482	0.29%	0.026%
21	14.134	1854	1861	1878	rBV	1218312	1854769	63.13%	5.757%
22	14.428	1903	1911	1929	rBV2	1400138	2177065	74.10%	6.758%
23	14.734	1956	1963	1971	rBV	790979	1184626	40.32%	3.677%
24	14.916	1990	1994	1997	rBV6	2744	3967	0.14%	0.012%
25	14.969	1997	2003	2028	rBV2	183207	634048	21.58%	1.968%
26	15.669	2115	2122	2124	rBV8	1902	3357	0.11%	0.010%
27	15.728	2124	2132	2149	rBV	1581785	2429211	82.68%	7.540%
28	15.875	2151	2157	2170	rBV	351554	634439	21.59%	1.969%
29	16.310	2227	2231	2235	rVB7	2968	3824	0.13%	0.012%
30	17.492	2425	2432	2443	rBV	794659	1201470	40.89%	3.729%
31	17.598	2443	2450	2466	rVV	1420532	2300922	78.32%	7.142%
32	18.369	2577	2581	2583	rBV4	7252	9972	0.34%	0.031%
33	19.404	2753	2757	2759	rBV3	19996	25406	0.86%	0.079%
34	19.822	2823	2828	2841	rBV	1765054	2496904	84.99%	7.750%
35	21.586	3124	3128	3137	rVB	791729	1131367	38.51%	3.512%
36	23.980	3528	3535	3547	rVB2	1353230	2937990	100.00%	9.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015669.D
Acq On : 23 Jun 2023 13:49
Operator : MA/JU
Sample : PB153415BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK415

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	24.151	3558	3564	3575	rVB2	599193	1337062	45.51%	4.150%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 32216627

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015669.D
Acq On : 23 Jun 2023 13:49
Operator : MA/JU
Sample : PB153415BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK415

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

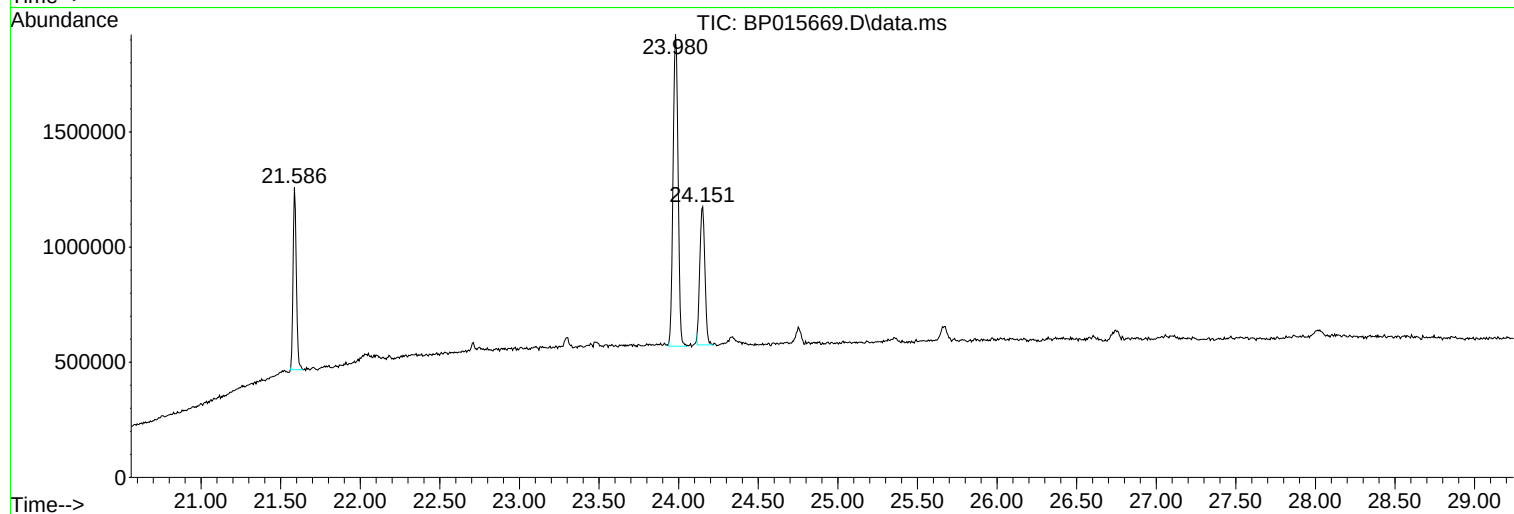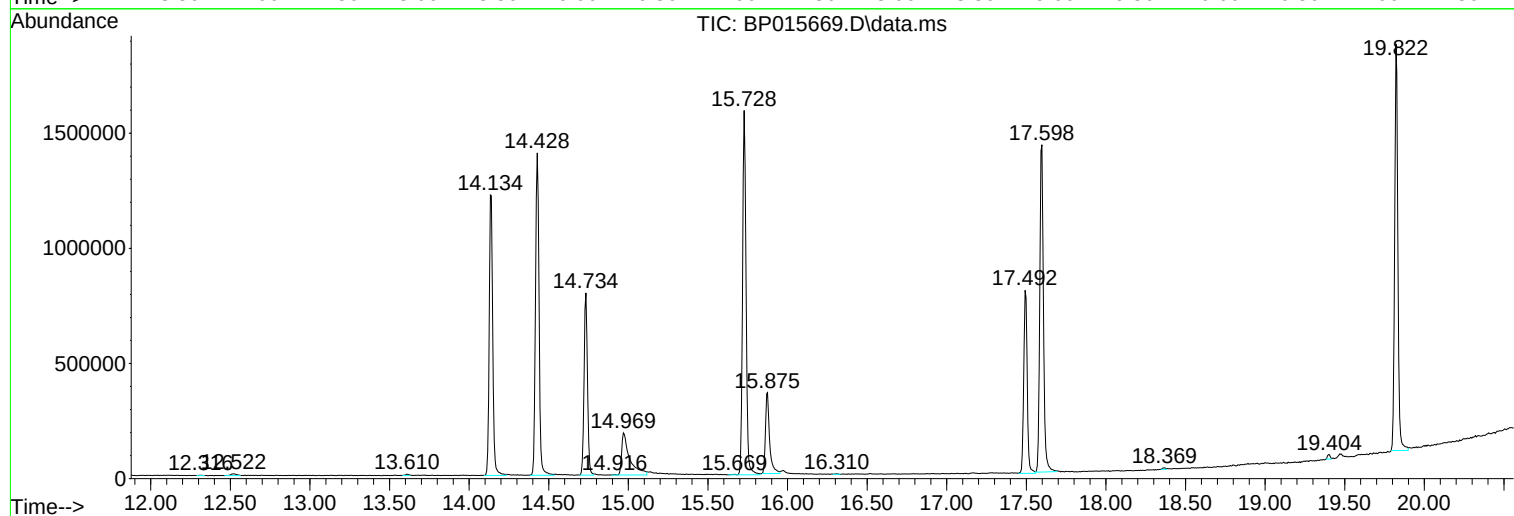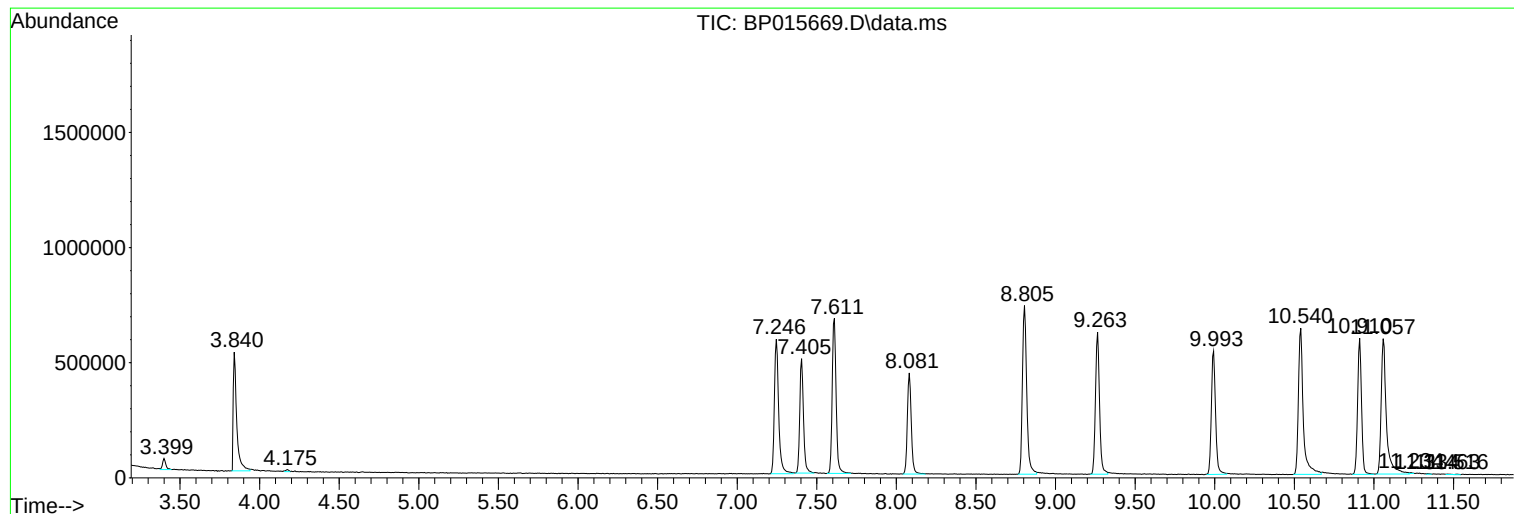

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015669.D
Acq On : 23 Jun 2023 13:49
Operator : MA/JU
Sample : PB153415BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK415

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015669.D
Acq On : 23 Jun 2023 13:49
Operator : MA/JU
Sample : PB153415BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK415

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc